

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019658.D
 Acq On : 15 Dec 2020 18:47
 Operator : SY/MD
 Sample : L5024-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	374933	367676	15.41%	2.057%
2	1.570	142	149	164	rVB	286975	323905	13.57%	1.812%
3	2.110	308	317	334	rBV	587018	870601	36.48%	4.870%
4	2.824	537	539	541	rBV	311	137	0.01%	0.001%
5	3.004	592	595	598	rBV3	418	362	0.02%	0.002%
6	3.139	633	637	638	rBV	708	367	0.02%	0.002%
7	3.184	643	651	655	rBV4	620	796	0.03%	0.004%
8	3.232	663	666	667	rBV	269	171	0.01%	0.001%
9	3.309	688	690	691	rBV2	389	185	0.01%	0.001%
10	3.521	750	756	758	rBV4	444	387	0.02%	0.002%
11	3.544	761	763	764	rVV2	368	130	0.01%	0.001%
12	3.560	764	768	773	rVB5	759	676	0.03%	0.004%
13	3.634	789	791	795	rVB3	415	273	0.01%	0.002%
14	3.656	795	798	800	rBV2	524	367	0.02%	0.002%
15	3.695	807	810	814	rBV2	433	325	0.01%	0.002%
16	3.775	832	835	837	rBV2	302	173	0.01%	0.001%
17	3.798	840	842	845	rBV3	410	196	0.01%	0.001%
18	3.830	849	852	854	rBV2	395	231	0.01%	0.001%
19	3.885	858	869	898	rBV	172490	490754	20.56%	2.745%
20	4.354	999	1015	1047	rBV	373682	917493	38.44%	5.133%
21	4.717	1126	1128	1129	rBV	421	153	0.01%	0.001%
22	4.788	1148	1150	1153	rBV3	421	289	0.01%	0.002%
23	4.875	1175	1177	1180	rBV2	322	158	0.01%	0.001%
24	4.904	1183	1186	1187	rBV	333	187	0.01%	0.001%
25	4.984	1207	1211	1214	rBV3	652	550	0.02%	0.003%
26	5.052	1214	1232	1260	rBV2	923838	2386628	100.00%	13.351%
27	5.463	1357	1360	1361	rBV2	636	295	0.01%	0.002%
28	5.621	1396	1409	1438	rBV	715485	1423611	59.65%	7.964%
29	5.849	1476	1480	1482	rBV4	850	591	0.02%	0.003%
30	5.913	1489	1500	1520	rVB3	12815	28836	1.21%	0.161%
31	6.074	1536	1550	1576	rBV	531133	1075314	45.06%	6.015%
32	6.405	1650	1653	1657	rBV3	686	563	0.02%	0.003%
33	6.457	1667	1669	1671	rBV2	564	350	0.01%	0.002%
34	6.505	1680	1684	1685	rBV3	597	414	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019658.D
 Acq On : 15 Dec 2020 18:47
 Operator : SY/MD
 Sample : L5024-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.602	1712	1714	1715	rVB	213	66	0.00%	0.000%
36	6.624	1715	1721	1722	rBV2	843	706	0.03%	0.004%
37	6.704	1744	1746	1748	rBV2	323	142	0.01%	0.001%
38	6.733	1753	1755	1757	rBV	333	160	0.01%	0.001%
39	6.782	1764	1770	1777	rVB5	868	1098	0.05%	0.006%
40	6.811	1777	1779	1780	rBV5	495	187	0.01%	0.001%
41	6.929	1814	1816	1818	rBV4	567	342	0.01%	0.002%
42	6.991	1822	1835	1863	rBV	310513	568078	23.80%	3.178%
43	7.274	1921	1923	1924	rBV	385	182	0.01%	0.001%
44	7.319	1925	1937	1969	rVV	1108939	1911765	80.10%	10.695%
45	7.624	2022	2032	2058	rBV	214269	369935	15.50%	2.069%
46	7.942	2124	2131	2136	rBV4	1855	2734	0.11%	0.015%
47	8.090	2164	2177	2207	rBV	593474	1055702	44.23%	5.906%
48	8.765	2385	2387	2388	rVB	329	79	0.00%	0.000%
49	8.781	2388	2392	2393	rBV2	443	284	0.01%	0.002%
50	8.855	2403	2415	2442	rBV	1066181	1723981	72.24%	9.644%
51	9.068	2480	2481	2483	rBV2	880	402	0.02%	0.002%
52	9.193	2517	2520	2524	rBV2	590	470	0.02%	0.003%
53	9.235	2531	2533	2537	rBV3	483	361	0.02%	0.002%
54	9.354	2565	2570	2571	rBV2	669	422	0.02%	0.002%
55	9.421	2588	2591	2592	rBV2	538	244	0.01%	0.001%
56	9.524	2621	2623	2625	rBV2	325	144	0.01%	0.001%
57	9.553	2630	2632	2634	rVB2	378	179	0.01%	0.001%
58	9.611	2646	2650	2652	rVB3	378	220	0.01%	0.001%
59	9.640	2657	2659	2660	rBV3	449	175	0.01%	0.001%
60	9.672	2667	2669	2671	rBV	229	133	0.01%	0.001%
61	9.711	2677	2681	2686	rBV3	595	613	0.03%	0.003%
62	9.810	2708	2712	2716	rBV3	616	649	0.03%	0.004%
63	9.859	2722	2727	2734	rVB3	726	836	0.04%	0.005%
64	9.888	2734	2736	2737	rBV	360	131	0.01%	0.001%
65	9.900	2737	2740	2741	rBV	489	208	0.01%	0.001%
66	9.984	2763	2766	2769	rBV2	554	393	0.02%	0.002%
67	10.222	2827	2840	2857	rBV	641103	1010726	42.35%	5.654%
68	10.425	2901	2903	2905	rBV	362	129	0.01%	0.001%
69	10.476	2917	2919	2921	rBV	303	136	0.01%	0.001%
70	10.489	2921	2923	2926	rVV2	346	191	0.01%	0.001%
71	10.524	2932	2934	2935	rBV	241	104	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019658.D
 Acq On : 15 Dec 2020 18:47
 Operator : SY/MD
 Sample : L5024-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.537	2935	2938	2940	rVV3	645	431	0.02%	0.002%
73	10.569	2946	2948	2949	rBV	423	110	0.00%	0.001%
74	10.913	3052	3055	3058	rBV2	619	393	0.02%	0.002%
75	10.929	3058	3060	3064	rVV4	707	480	0.02%	0.003%
76	11.019	3086	3088	3094	rVB3	527	442	0.02%	0.002%
77	11.055	3097	3099	3100	rBV3	314	120	0.01%	0.001%
78	11.132	3120	3123	3126	rBV3	613	368	0.02%	0.002%
79	11.177	3133	3137	3145	rVB6	1002	905	0.04%	0.005%
80	11.254	3149	3161	3181	rBV	1072165	1648607	69.08%	9.223%
81	11.476	3228	3230	3236	rVB4	1019	842	0.04%	0.005%
82	11.531	3243	3247	3250	rBV2	1207	1216	0.05%	0.007%
83	11.630	3265	3278	3299	rBV	1064290	1672491	70.08%	9.356%
84	11.961	3378	3381	3384	rBV2	534	339	0.01%	0.002%
85	12.006	3389	3395	3399	rBV4	568	818	0.03%	0.005%
86	12.103	3422	3425	3430	rBV3	759	768	0.03%	0.004%
87	12.212	3457	3459	3460	rBV	306	142	0.01%	0.001%
88	12.563	3565	3568	3570	rBV2	638	363	0.02%	0.002%
89	12.701	3609	3611	3612	rBV	498	166	0.01%	0.001%
90	13.042	3713	3717	3718	rBV	417	288	0.01%	0.002%
91	13.334	3806	3808	3810	rBV	350	201	0.01%	0.001%
92	13.582	3881	3885	3886	rBV	385	269	0.01%	0.002%
93	13.653	3905	3907	3908	rBV3	502	223	0.01%	0.001%
94	13.945	3995	3998	3999	rBV	627	332	0.01%	0.002%


Sum of corrected areas: 17875765

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019658.D
Acq On : 15 Dec 2020 18:47
Operator : SY/MD
Sample : L5024-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

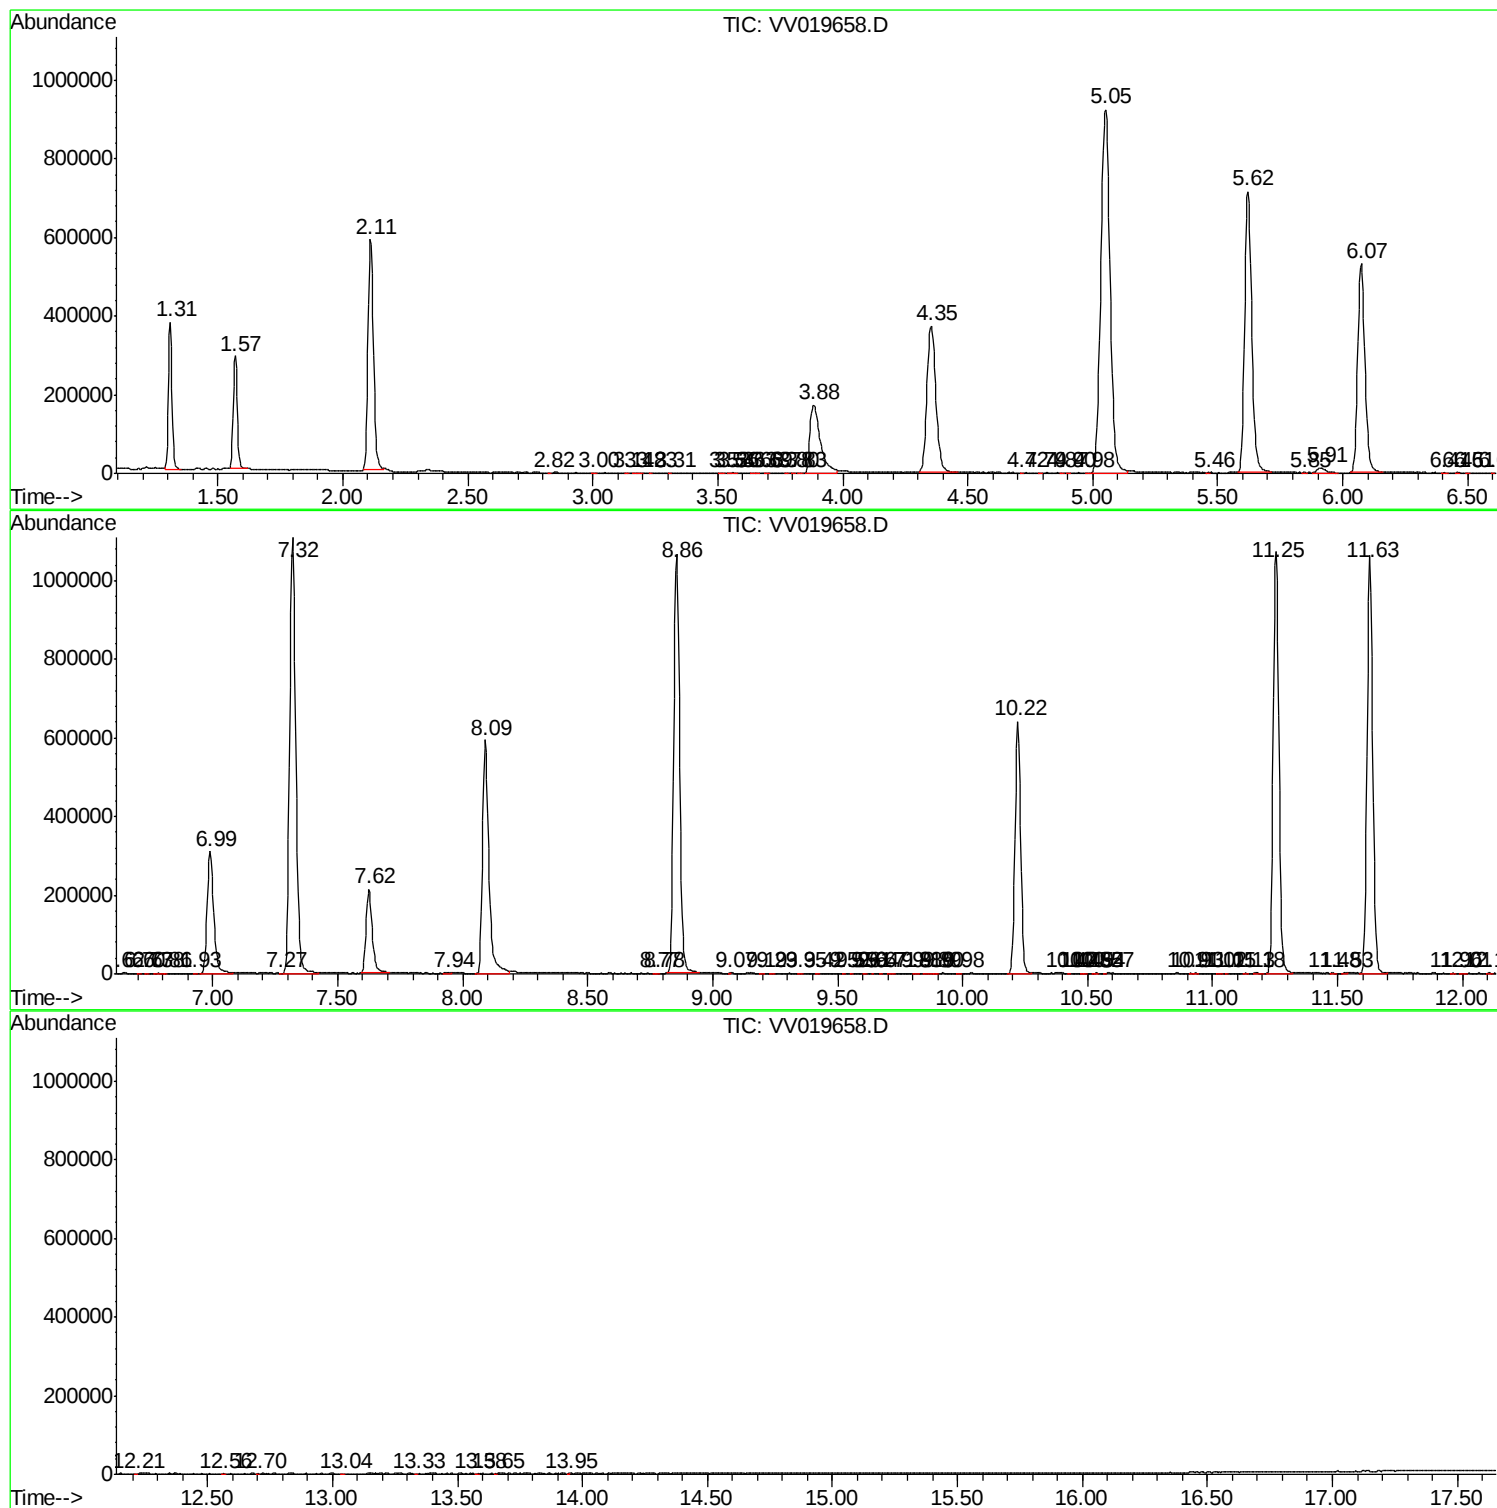

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019658.D
Acq On : 15 Dec 2020 18:47
Operator : SY/MD
Sample : L5024-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121520\
Data File : VV019658.D
Acq On : 15 Dec 2020 18:47
Operator : SY/MD
Sample : L5024-19
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AZ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc