




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023985.D
 Acq On : 15 Dec 2021 16:51
 Operator : SY/MD
 Sample : M4971-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D8

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:50:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
 Supervised By :Mahesh Dadoda 12/22/2021

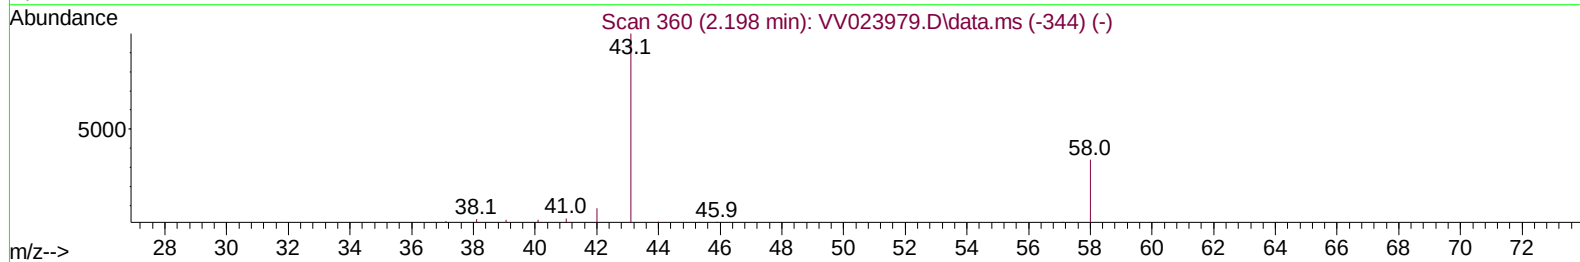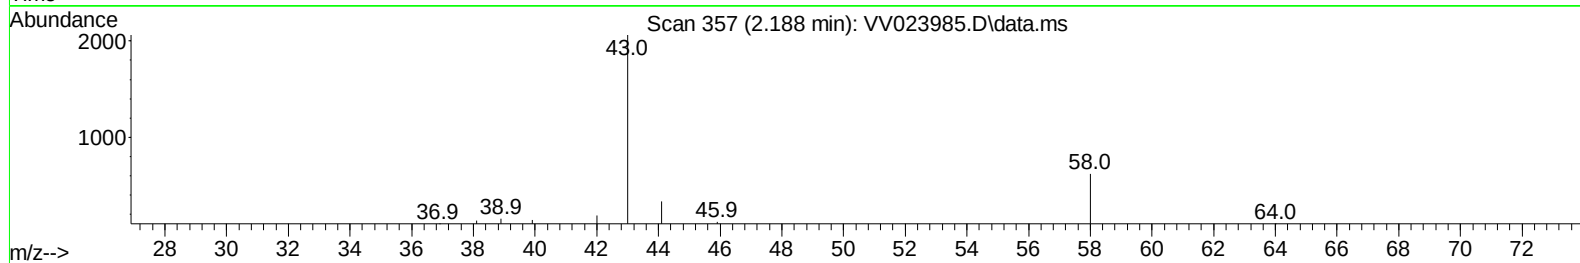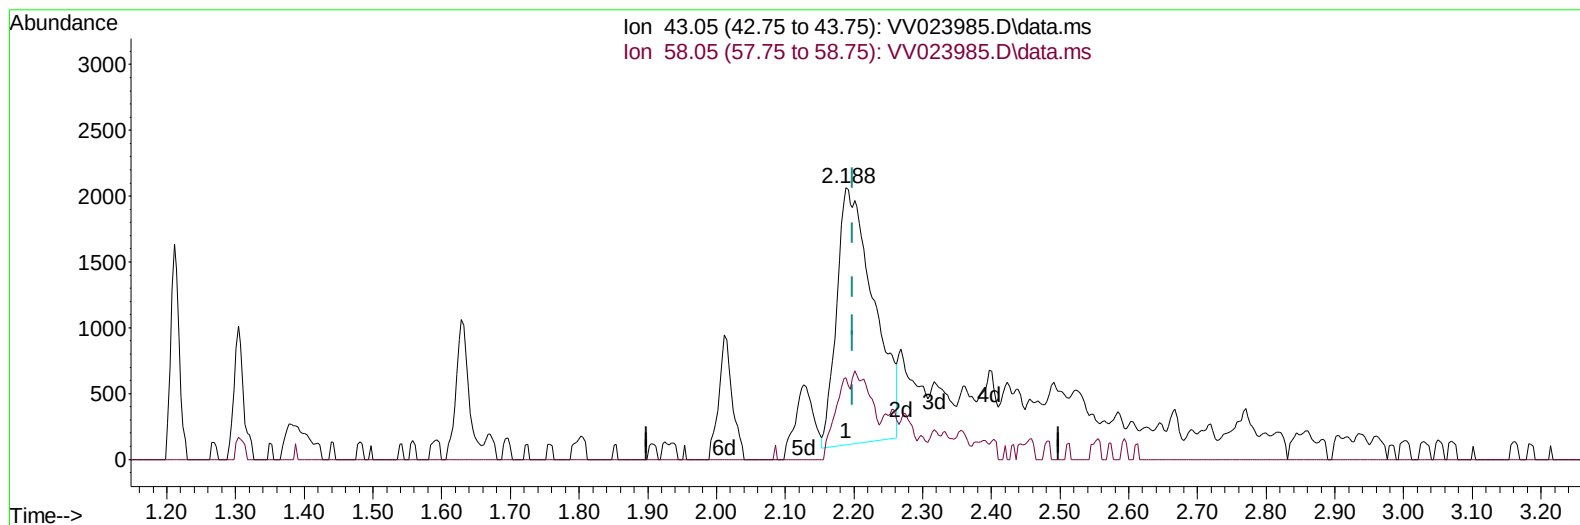

TIC: VV023985.D\data.ms

(13) Acetone (T)

2.188min (-0.010) 9.22 ug/L

response 7264

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	13.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023985.D
 Acq On : 15 Dec 2021 16:51
 Operator : SY/MD
 Sample : M4971-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D8

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:50:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
 Supervised By :Mahesh Dadoda 12/22/2021

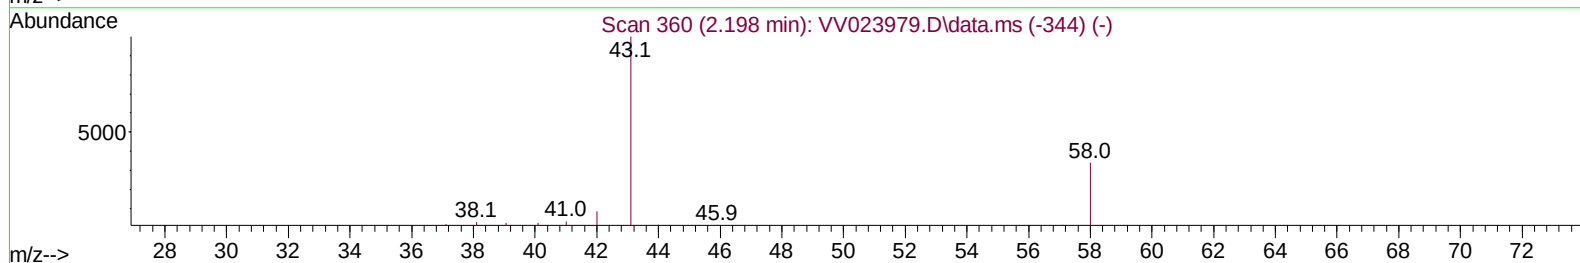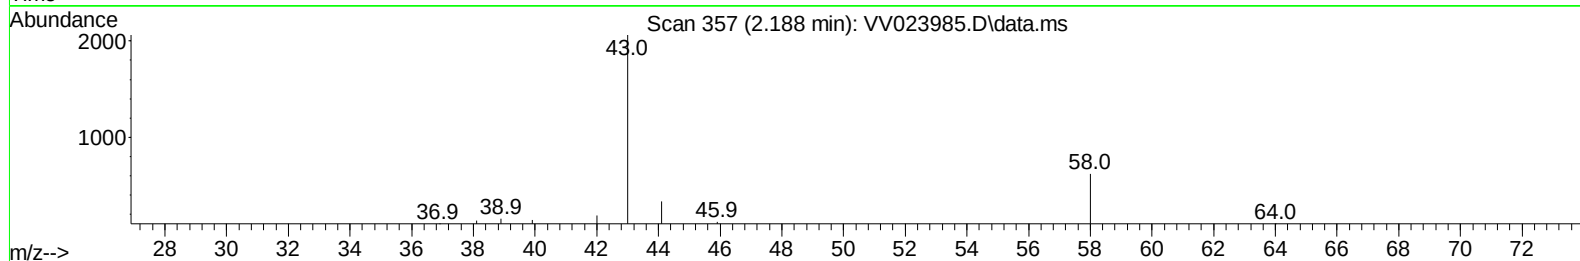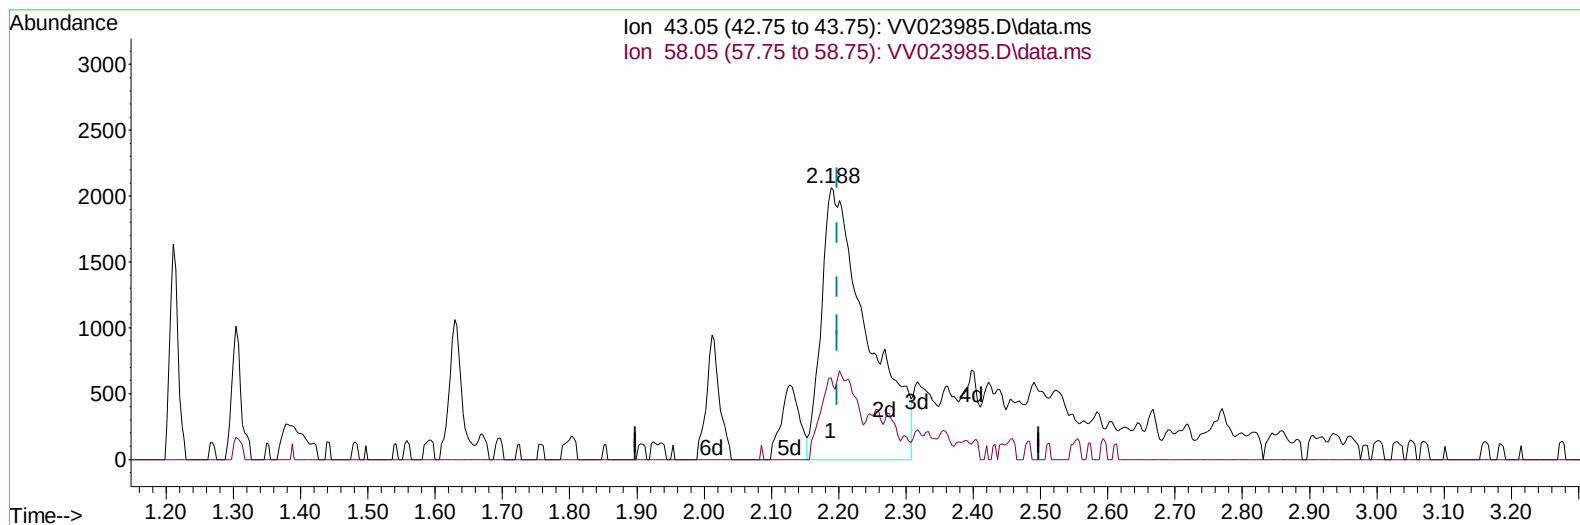

TIC: VV023985.D\data.ms

(13) Acetone (T)

2.188min (-0.010) 12.38 ug/L m

response 9755

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	9.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023985.D
 Acq On : 15 Dec 2021 16:51
 Operator : SY/MD
 Sample : M4971-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D8

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:50:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 12/16/2021
 Supervised By : Mahesh Dadoda 12/22/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	93780	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	99759	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50104	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	16753	3.323	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	66.400%	
7) Chloroethane-d5	1.565	69	17809	4.234	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	84.600%	
11) 1,1-Dichloroethene-d2	2.105	63	24027	2.442	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	48.800%#	
20) 2-Butanone-d5	3.902	46	44019	44.691	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	89.380%	
24) Chloroform-d	4.349	84	53263	4.664	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	93.200%	
26) 1,2-Dichloroethane-d4	5.034	65	26382	4.962	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.200%	
32) Benzene-d6	5.050	84	80153	4.057	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	81.200%	
36) 1,2-Dichloropropane-d6	6.069	67	27355	4.589	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	91.800%	
41) Toluene-d8	7.317	98	59156	3.325	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	66.600%#	
43) trans-1,3-Dichloroprop...	7.625	79	10437	4.220	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	84.400%	
46) 2-Hexanone-d5	8.092	63	53611	48.426	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	96.860%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24324	4.919	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	98.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	32426	4.845	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	96.800%	
Target Compounds						
						Qvalue
3) Chloromethane	1.237	50	1251	0.179	ug/L	83
13) Acetone	2.188	43	9755m	12.379	ug/L	
33) Benzene	5.101	78	27587	0.978	ug/L	100
42) Toluene	7.391	91	49706	1.565	ug/L	99
52) Ethylbenzene	9.021	91	3768	0.112	ug/L	99
53) m,p-xylene	9.140	106	4833	0.365	ug/L	85
54) o-xylene	9.545	106	4179	0.326	ug/L	91
62) 1,3,5-Trimethylbenzene	10.542	105	1721	0.071	ug/L	94
63) 1,2,4-Trimethylbenzene	10.915	105	7668	0.315	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023985.D
Acq On : 15 Dec 2021 16:51
Operator : SY/MD
Sample : M4971-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3D8

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:50:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
Supervised By :Mahesh Dadoda 12/22/2021

