




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023995.D
 Acq On : 15 Dec 2021 20:49
 Operator : SY/MD
 Sample : M5090-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3E2

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:53:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
 Supervised By :Mahesh Dadoda 12/22/2021

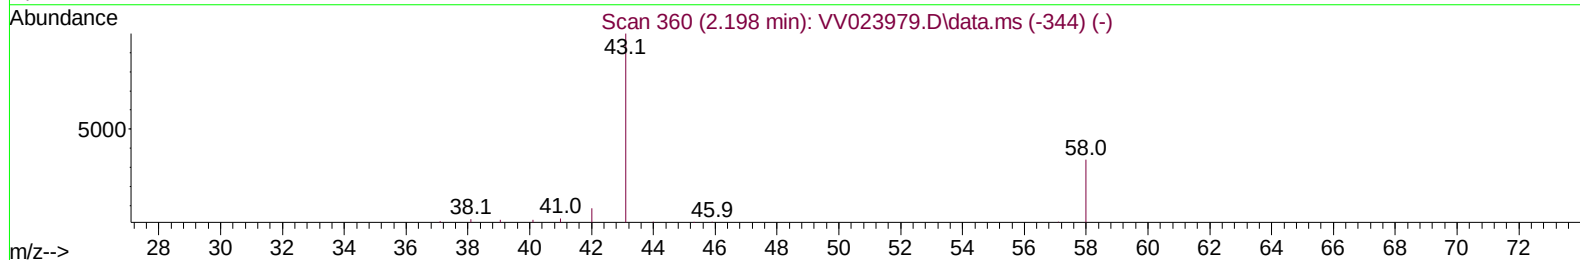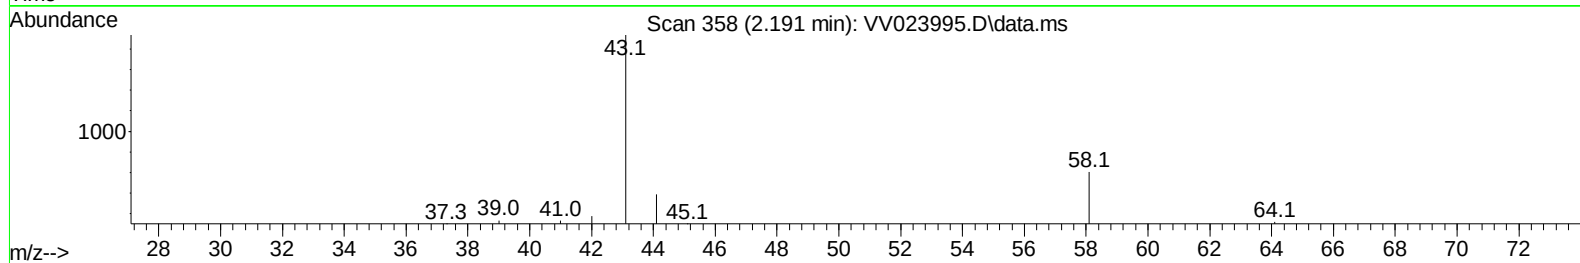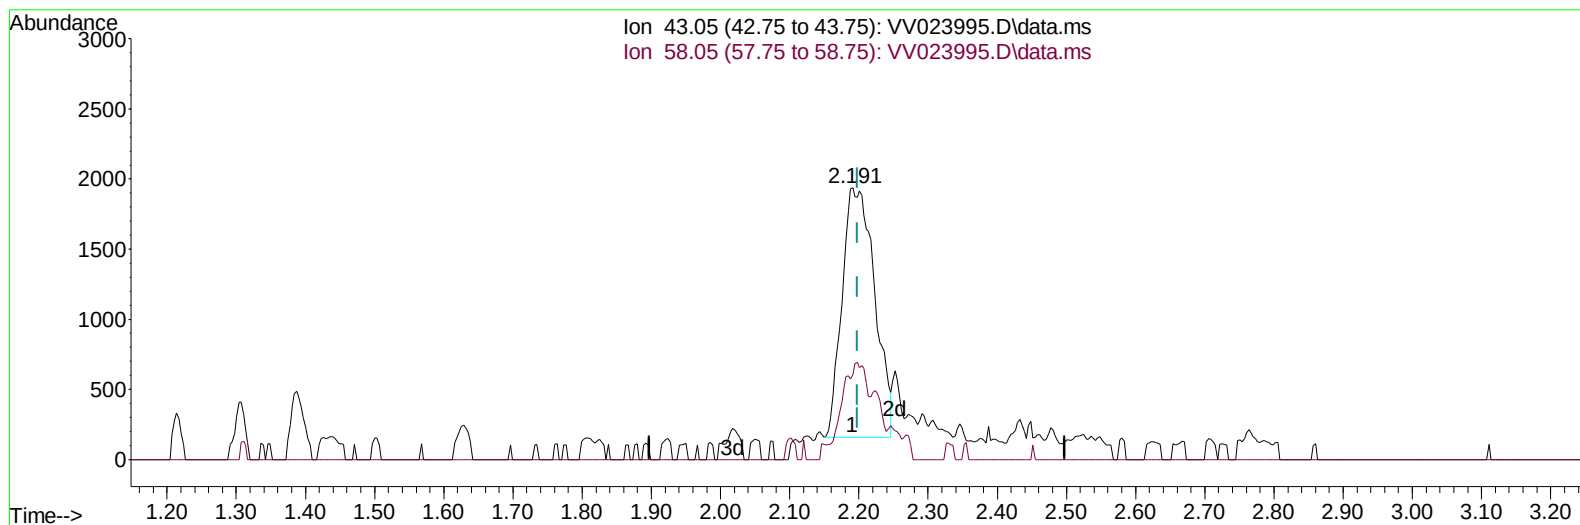

TIC: VV023995.D\data.ms

(13) Acetone (T)

2.191min (-0.007) 7.07 ug/L

response 5807

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	23.51
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023995.D
 Acq On : 15 Dec 2021 20:49
 Operator : SY/MD
 Sample : M5090-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3E2

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:53:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
 Supervised By :Mahesh Dadoda 12/22/2021

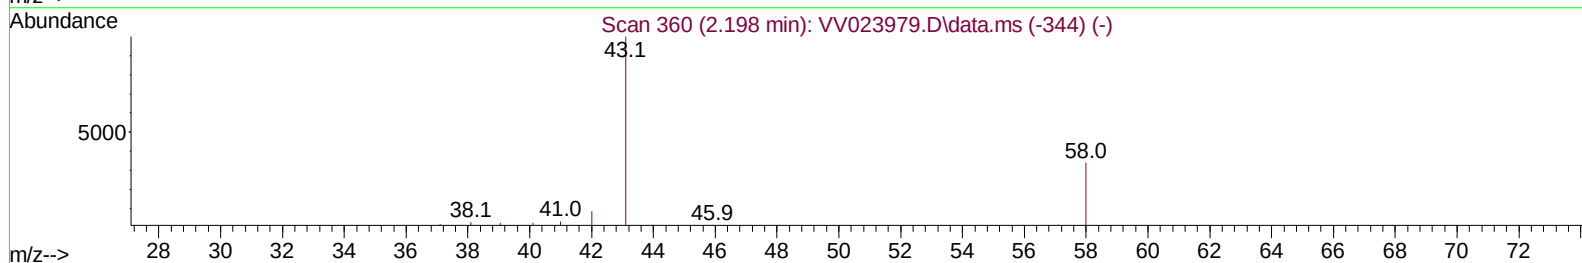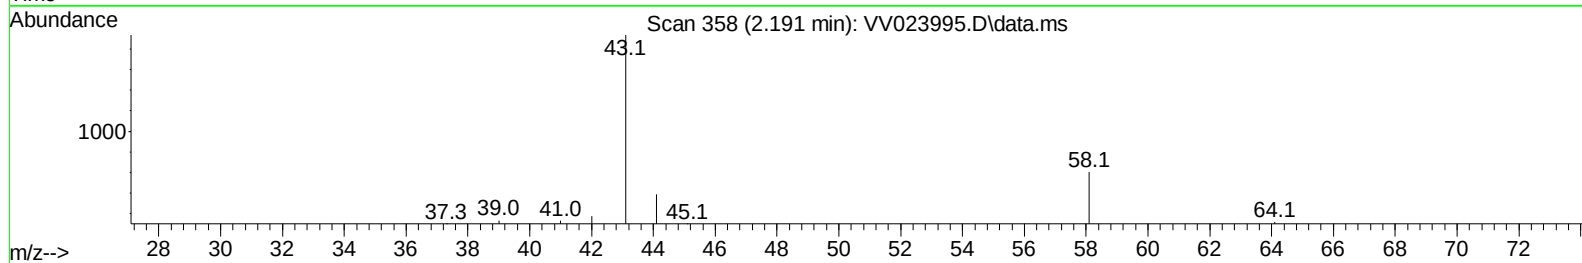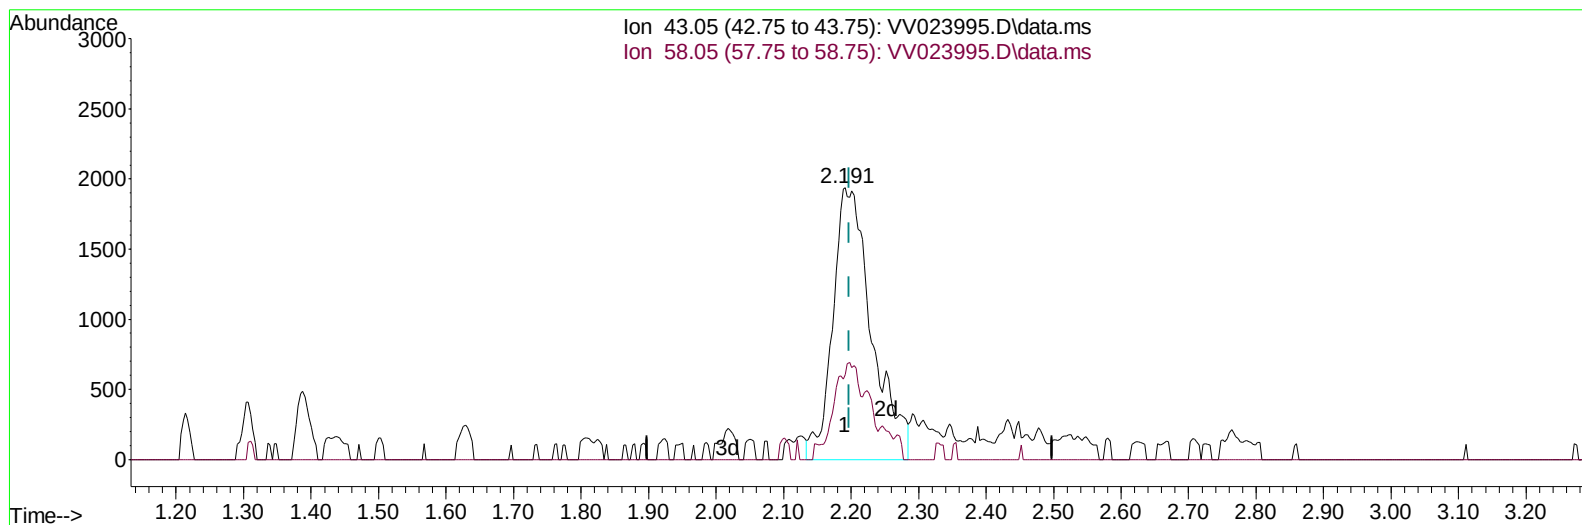

TIC: VV023995.D\data.ms

(13) Acetone (T)

2.191min (-0.007) 9.48 ug/L m

response 7778

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	17.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023995.D
 Acq On : 15 Dec 2021 20:49
 Operator : SY/MD
 Sample : M5090-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3E2

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:53:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 16 04:44:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	97684	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	102195	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51067	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15880	3.024	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery =	60.400%		
7) Chloroethane-d5	1.567	69	17249	3.937	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery =	78.800%		
11) 1,1-Dichloroethene-d2	2.108	63	23696	2.312	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery =	46.200%#		
20) 2-Butanone-d5	3.902	46	63964	62.345	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery =	124.700%		
24) Chloroform-d	4.346	84	50911	4.280	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	85.600%		
26) 1,2-Dichloroethane-d4	5.034	65	25701	4.641	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	92.800%		
32) Benzene-d6	5.050	84	79278	3.917	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	78.400%		
36) 1,2-Dichloropropane-d6	6.069	67	27093	4.437	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery =	88.800%		
41) Toluene-d8	7.320	98	58405	3.205	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	64.200%#		
43) trans-1,3-Dichloroprop...	7.628	79	9555	3.772	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery =	75.400%		
46) 2-Hexanone-d5	8.091	63	49861	43.965	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery =	87.920%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	23032	4.546	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery =	91.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	31227	4.578	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery =	91.600%		
Target Compounds						
					Qvalue	
13) Acetone	2.191	43	7778m	9.476	ug/L	
33) Benzene	5.108	78	9481	0.328	ug/L	100
42) Toluene	7.394	91	9428	0.290	ug/L	98
54) o-xylene	9.551	106	918	0.070	ug/L	92
63) 1,2,4-Trimethylbenzene	10.918	105	2782	0.112	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023995.D
Acq On : 15 Dec 2021 20:49
Operator : SY/MD
Sample : M5090-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3E2

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:53:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 16 04:44:29 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2021
Supervised By :Mahesh Dadoda 12/22/2021

