

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023980.D
 Acq On : 15 Dec 2021 12:02
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK278

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	48349	49914	15.86%	1.885%
2	1.568	155	164	172	rBV	41822	48004	15.25%	1.813%
3	2.105	319	331	351	rVB	86267	123295	39.17%	4.657%
4	2.507	447	456	475	rVB2	7649	12486	3.97%	0.472%
5	3.905	881	891	914	rBV2	12632	47366	15.05%	1.789%
6	4.346	1011	1028	1053	rVB	60260	145213	46.13%	5.485%
7	5.043	1230	1245	1271	rBV3	124129	310188	98.54%	11.716%
8	5.613	1410	1422	1444	rBV2	112419	230976	73.37%	8.724%
9	5.912	1504	1515	1525	rBV5	2799	5735	1.82%	0.217%
10	6.066	1548	1563	1590	rBV2	68895	149264	47.42%	5.638%
11	6.985	1836	1849	1866	rBV	31935	61165	19.43%	2.310%
12	7.313	1935	1951	1967	rBV	148753	262209	83.30%	9.903%
13	7.622	2037	2047	2068	rBV2	18766	37232	11.83%	1.406%
14	8.088	2182	2192	2223	rBV	91481	226377	71.91%	8.550%
15	8.850	2417	2429	2457	rBV	189762	314789	100.00%	11.889%
16	10.217	2842	2854	2866	rBV	45513	73824	23.45%	2.788%
17	10.381	2896	2905	2915	rBV3	2340	3665	1.16%	0.138%
18	11.246	3164	3174	3191	rBV	195363	308305	97.94%	11.645%
19	11.622	3279	3291	3312	rBV	148147	232712	73.93%	8.789%
20	12.252	3475	3487	3496	rBV3	3140	4922	1.56%	0.186%




Sum of corrected areas: 2647641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023980.D
Acq On : 15 Dec 2021 12:02
Operator : SY/MD
Sample : VV1215WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

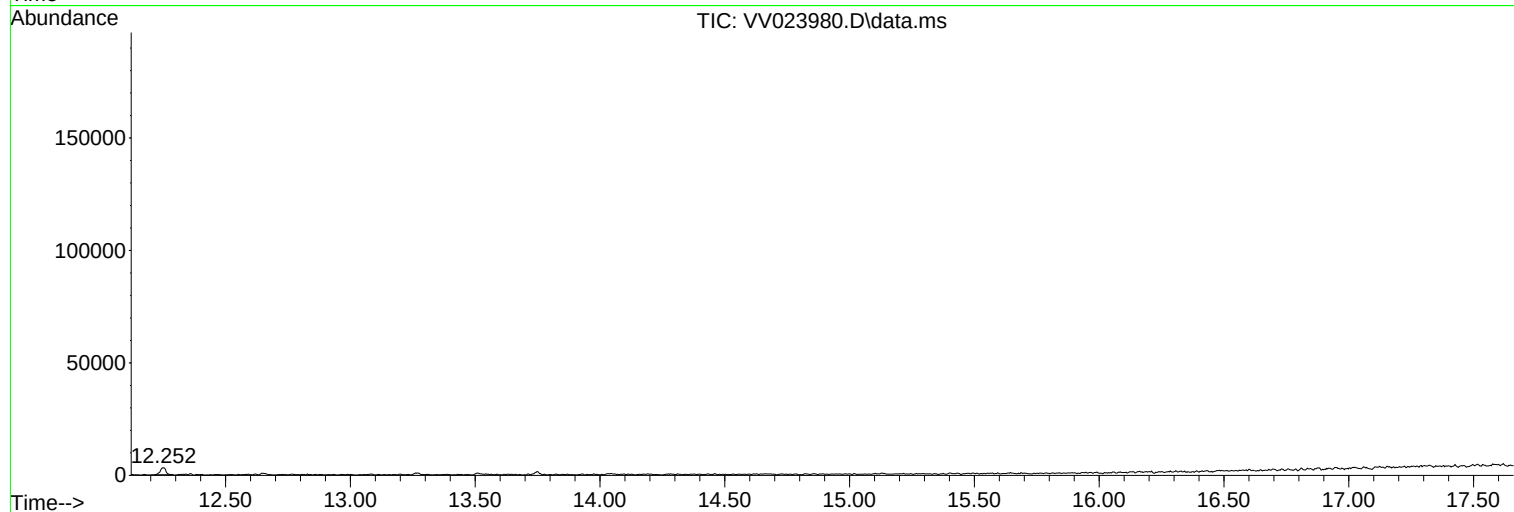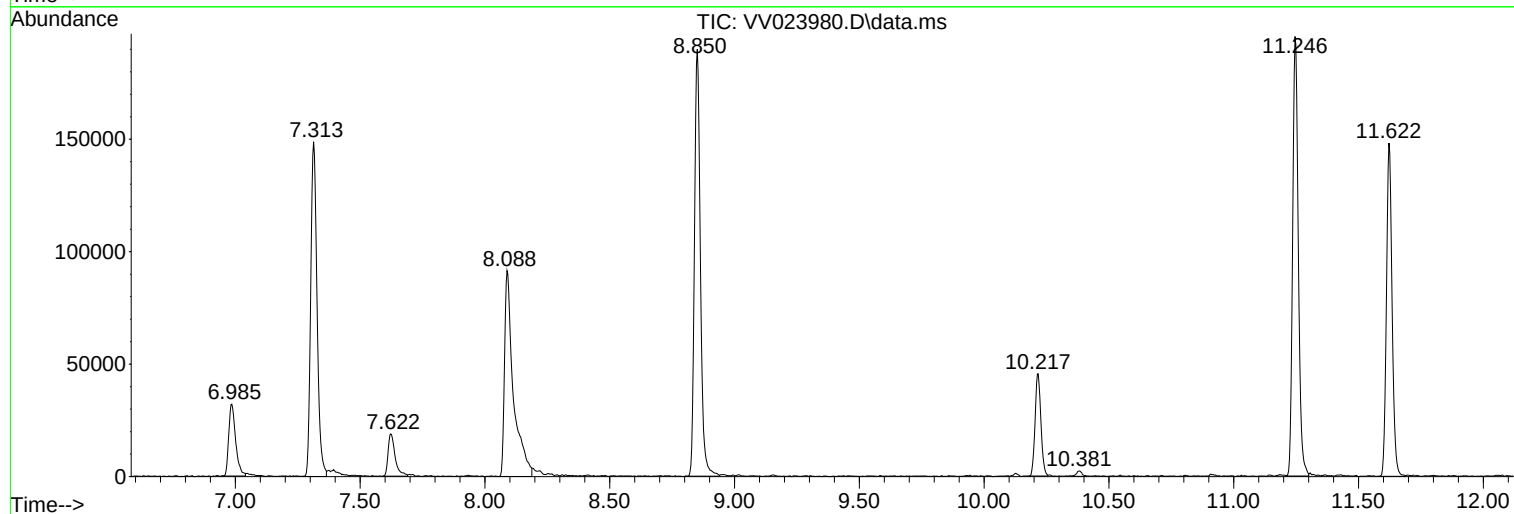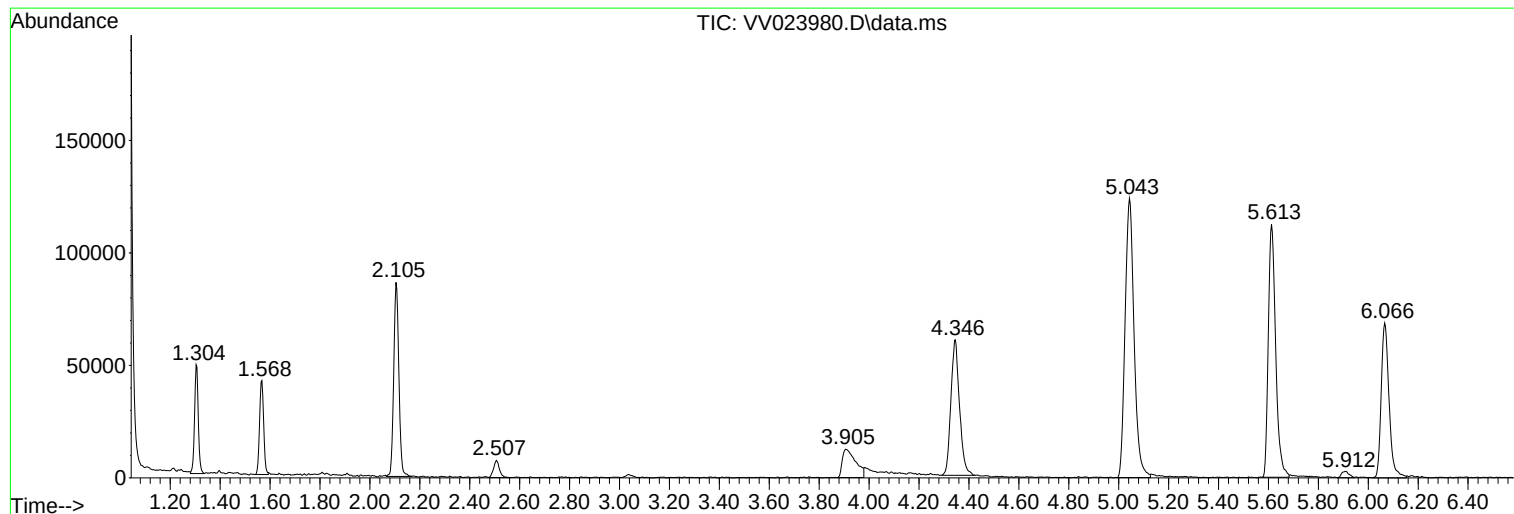

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023980.D
Acq On : 15 Dec 2021 12:02
Operator : SY/MD
Sample : VV1215WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023980.D
Acq On : 15 Dec 2021 12:02
Operator : SY/MD
Sample : VV1215WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
