

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023984.D
 Acq On : 15 Dec 2021 16:27
 Operator : SY/MD
 Sample : M4971-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	28675	29999	9.81%	1.216%
2	1.417	109	117	132	rVB	42670	49680	16.25%	2.014%
3	1.568	148	164	171	rBV	34634	49979	16.34%	2.026%
4	2.108	323	332	345	rVB	51568	75892	24.82%	3.076%
5	2.185	345	356	359	rBV2	3990	5792	1.89%	0.235%
6	2.510	450	457	466	rVB8	1933	3162	1.03%	0.128%
7	3.905	877	891	926	rBV3	39789	173668	56.79%	7.039%
8	4.346	1013	1028	1049	rBV2	48041	120603	39.44%	4.888%
9	5.047	1232	1246	1276	rBV3	89971	228469	74.71%	9.261%
10	5.619	1411	1424	1456	rBV	108041	224354	73.37%	9.094%
11	6.072	1552	1565	1584	rBV2	58139	120042	39.26%	4.866%
12	6.989	1838	1850	1871	rBV3	25304	47731	15.61%	1.935%
13	7.317	1941	1952	1970	rBV	84859	151723	49.62%	6.150%
14	7.625	2039	2048	2065	rBV2	14545	27226	8.90%	1.104%
15	7.940	2137	2146	2156	rVB4	1891	3423	1.12%	0.139%
16	8.092	2182	2193	2232	rBV	142500	289109	94.54%	11.719%
17	8.854	2418	2430	2450	rBV	182639	305790	100.00%	12.395%
18	10.217	2842	2854	2872	rVB2	53417	82121	26.86%	3.329%
19	10.381	2894	2905	2916	rBV5	2895	4545	1.49%	0.184%
20	11.249	3163	3175	3200	rBV	186128	294283	96.24%	11.928%
21	11.625	3277	3292	3314	rBV	110112	179488	58.70%	7.275%




Sum of corrected areas: 2467079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023984.D
Acq On : 15 Dec 2021 16:27
Operator : SY/MD
Sample : M4971-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3D5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

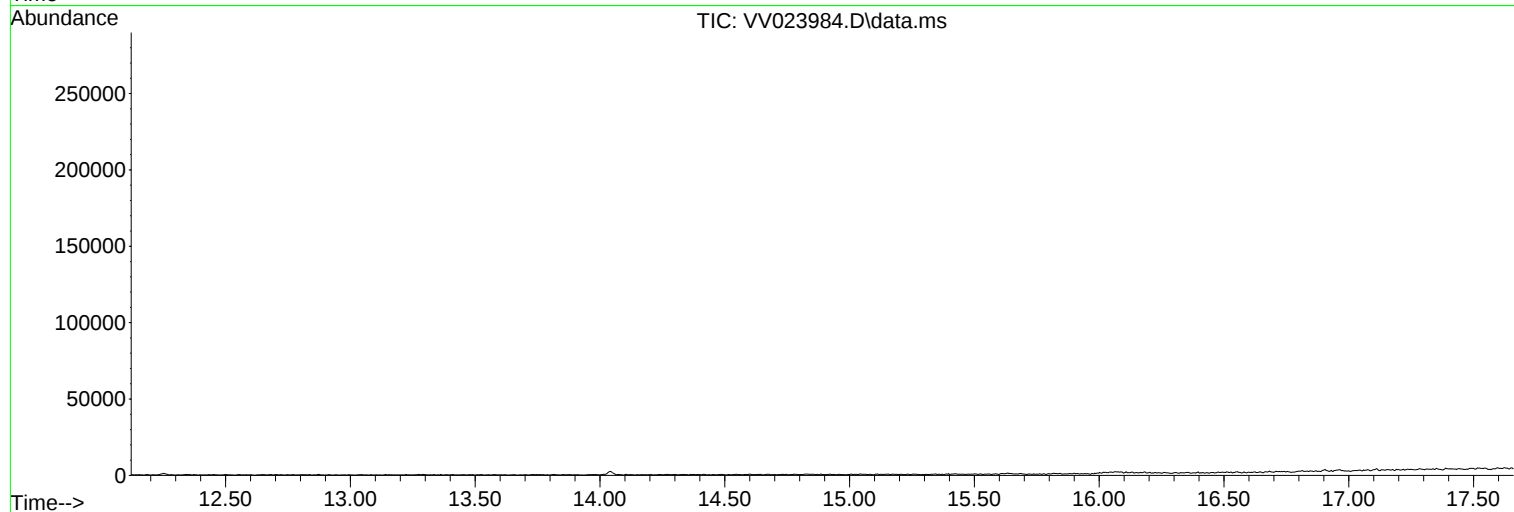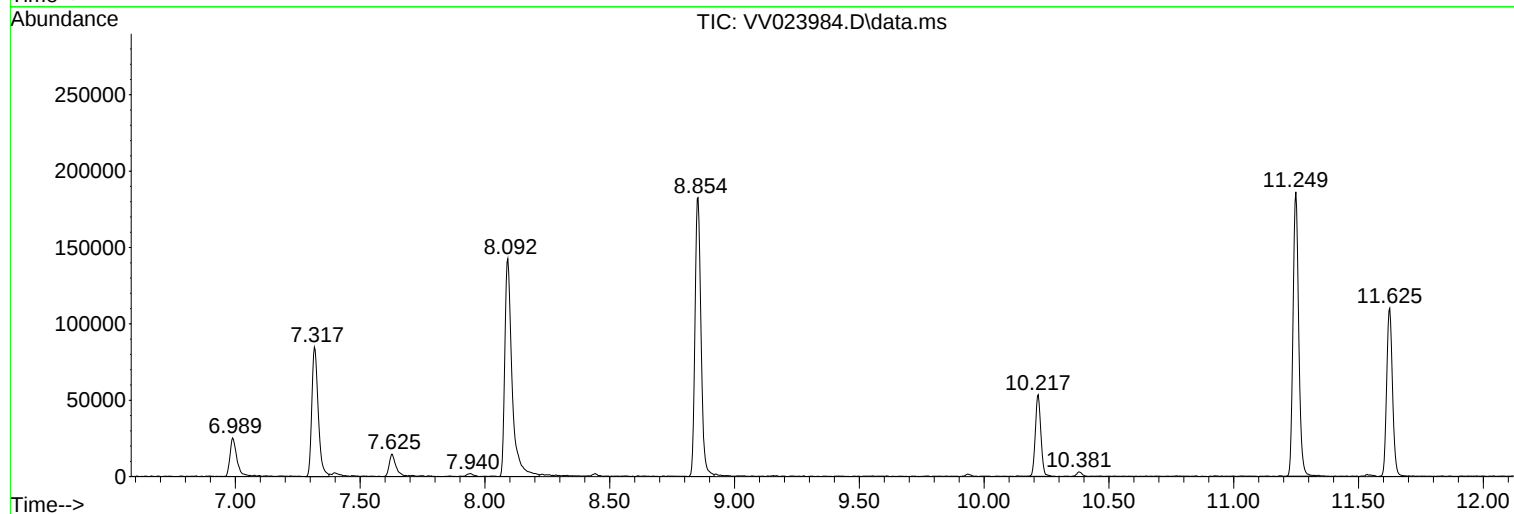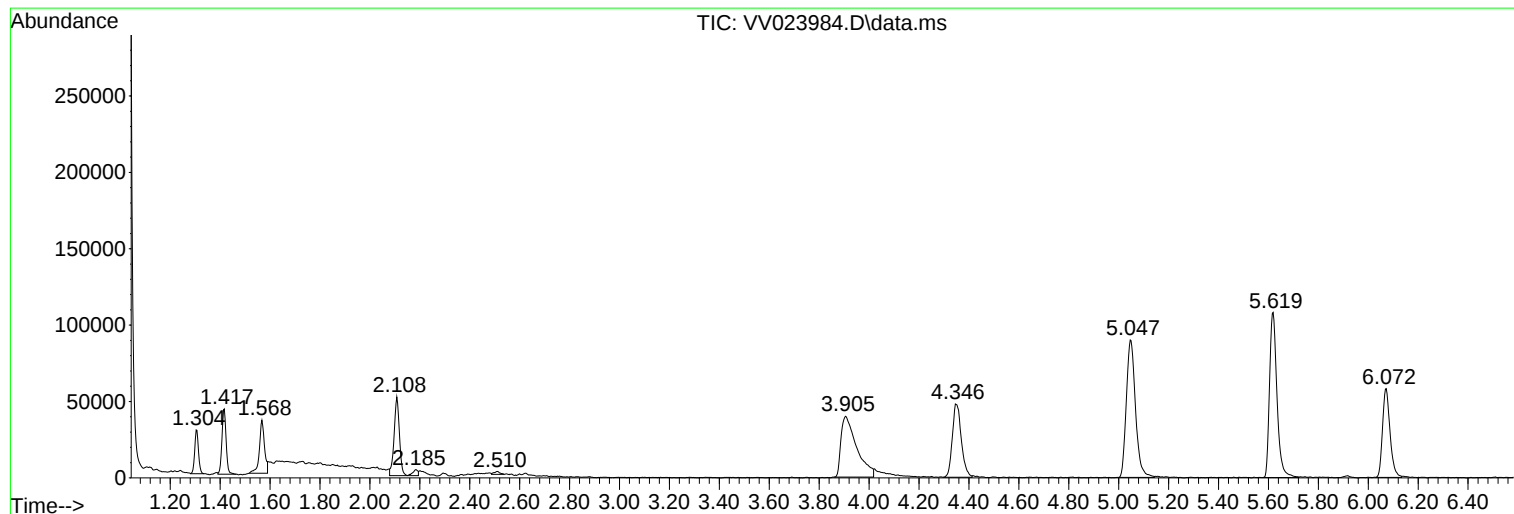

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023984.D
Acq On : 15 Dec 2021 16:27
Operator : SY/MD
Sample : M4971-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3D5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
Data File : VV023984.D
Acq On : 15 Dec 2021 16:27
Operator : SY/MD
Sample : M4971-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3D5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc