
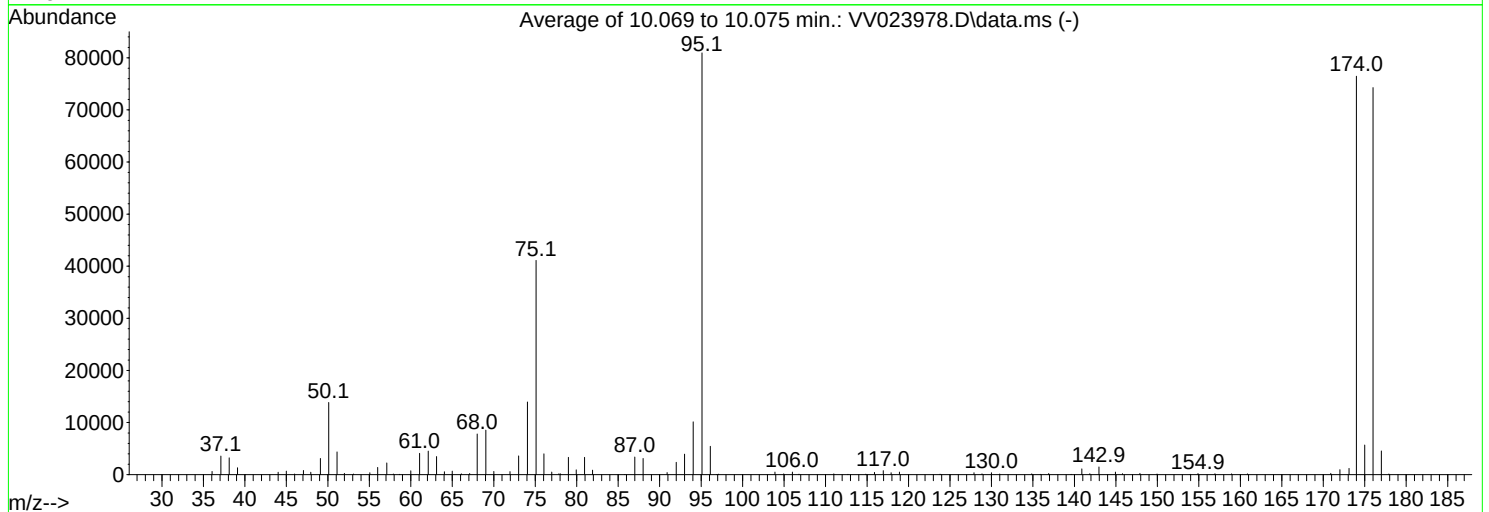


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121521\
 Data File : VV023978.D
 Acq On : 15 Dec 2021 10:54
 Operator : SY/MD
 Sample : BFB252
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB252

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Dec 20 04:04:22 2021

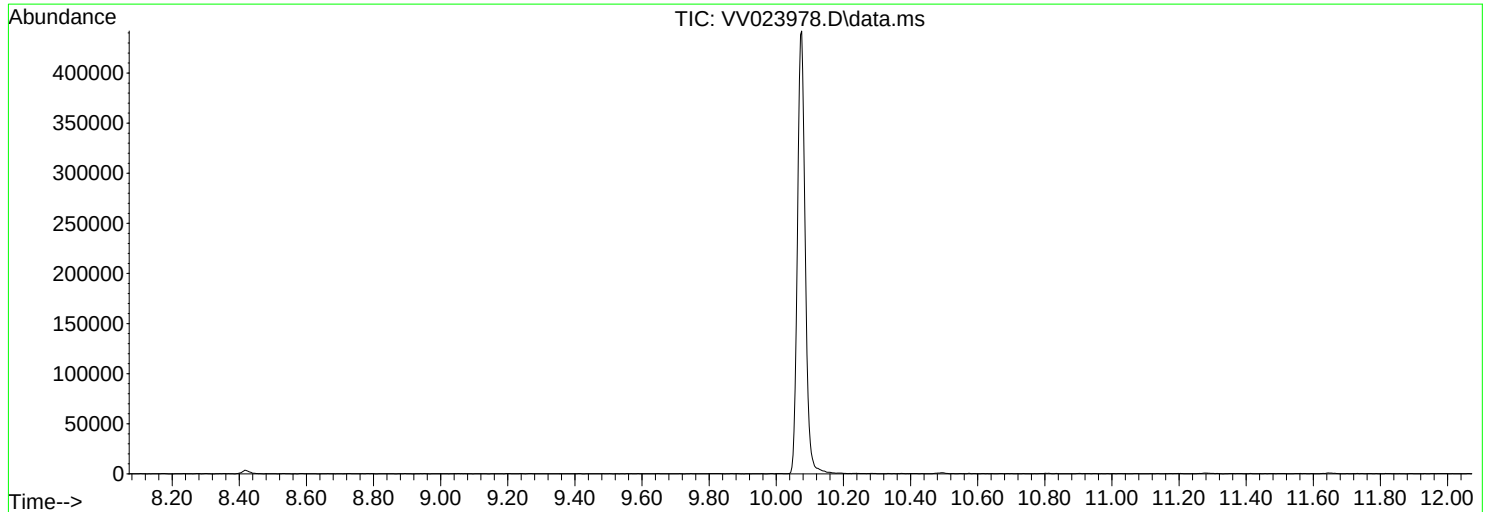

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	13840	PASS
75	95	30	80	50.8	41115	PASS
95	95	100	100	100.0	80949	PASS
96	95	5	9	6.7	5450	PASS
173	174	0.00	2	1.6	1199	PASS
174	95	50	120	94.4	76453	PASS
175	174	5	9	7.4	5671	PASS
176	174	95	105	97.2	74291	PASS
177	176	5	10	6.1	4553	PASS

m/z	Abundance
40.10	107.0
43.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
36.00	636.0
37.10	3389.0
38.10	3024.0
39.10	1240.0
40.10	118.0
44.10	514.0
45.00	695.0
46.00	133.0
47.10	849.0
48.00	421.0
49.10	3037.0
50.10	12854.0
51.10	4125.0
51.90	205.0
53.10	123.0
55.10	360.0
56.00	1386.0
57.10	2029.0
57.90	109.0
60.00	769.0
61.10	3820.0
62.10	4260.0
63.10	3219.0
64.10	561.0
65.00	685.0
66.10	146.0
67.10	233.0
68.00	7077.0
69.10	8136.0
70.00	537.0
72.00	548.0
73.00	3285.0
74.00	13594.0
75.10	38728.0
76.10	3843.0
77.00	458.0
77.80	283.0
78.10	221.0
79.00	3108.0
80.00	842.0
81.00	3130.0
81.90	698.0
85.80	119.0
87.00	3331.0
88.00	2698.0
90.90	427.0
92.00	2240.0
93.00	3518.0
94.00	9719.0
95.10	75808.0
96.10	5395.0
96.90	139.0
103.90	474.0
105.00	190.0
106.00	435.0
106.80	134.0
111.10	131.0
112.70	106.0
115.90	440.0
117.00	700.0
117.90	344.0
118.90	482.0
123.90	107.0
127.90	319.0
128.90	178.0
130.00	363.0
131.00	117.0
134.90	127.0
136.90	202.0
140.90	1044.0
141.90	177.0
143.00	1333.0
144.90	493.0
145.80	133.0
147.90	223.0
150.00	107.0
154.90	204.0
157.00	179.0
159.00	178.0
161.00	102.0
170.90	189.0
172.10	829.0
173.10	1100.0
174.00	68704.0
175.00	5141.0
176.00	67312.0
177.00	4171.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
36.10	624.0
37.10	3690.0
38.10	3330.0
39.10	1396.0
40.10	126.0
44.00	574.0
45.00	713.0
46.00	133.0
47.10	840.0
48.00	447.0
49.10	3130.0
50.10	14253.0
51.10	4445.0
52.00	236.0
53.10	132.0
55.10	386.0
56.00	1409.0
57.10	2366.0
57.90	123.0
58.60	116.0
60.00	758.0
61.10	4251.0
62.10	4827.0
63.10	3608.0
64.10	587.0
65.00	722.0
66.10	156.0
67.10	244.0
68.00	8054.0
69.10	8892.0
70.00	640.0
71.90	591.0
73.00	3684.0
74.10	14455.0
75.10	42456.0
76.10	4140.0
77.00	532.0
77.90	232.0
79.00	3446.0
79.90	963.0
80.90	3384.0
81.90	894.0
87.00	3509.0
88.00	3235.0
90.90	414.0
92.00	2402.0
93.00	4015.0
94.00	10380.0
95.10	83552.0
96.10	5612.0
97.10	148.0
103.90	502.0
105.00	178.0
106.00	503.0
106.80	114.0
111.00	167.0
112.70	106.0
114.80	129.0
115.90	447.0
117.00	756.0
117.90	397.0
118.90	515.0
123.70	114.0
127.90	379.0
128.80	156.0
130.00	395.0
131.00	124.0
134.80	180.0
135.90	113.0
136.90	224.0
139.60	102.0
140.90	1130.0
141.90	203.0
142.90	1530.0
144.90	493.0
145.80	170.0
147.90	252.0
150.00	136.0
154.00	111.0
154.90	230.0
157.00	198.0
158.90	168.0
160.80	157.0
170.90	233.0
172.00	973.0
173.10	1250.0
174.00	78896.0
175.00	5786.0
176.00	76664.0
177.00	4674.0
177.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
36.00	601.0
37.10	3655.0
38.10	3359.0
39.10	1368.0
40.00	142.0
44.00	606.0
45.00	624.0
46.00	139.0
47.00	755.0
47.90	489.0
49.10	3184.0
50.10	14413.0
51.10	4507.0
52.10	257.0
53.10	133.0
55.00	322.0
56.00	1321.0
57.10	2337.0
57.90	111.0
58.70	118.0
60.00	661.0
61.00	4217.0
62.10	4462.0
63.10	3608.0
64.00	515.0
65.00	656.0
66.10	126.0
67.10	210.0
68.00	8254.0
69.00	8553.0
70.00	681.0
71.90	577.0
73.00	3812.0
74.10	13824.0
75.10	42160.0
76.00	4012.0
77.00	519.0
78.00	241.0
79.00	3449.0
80.00	974.0
81.00	3463.0
81.90	977.0
87.00	3339.0
88.00	3353.0
90.90	368.0
92.00	2505.0
93.00	4237.0
94.10	10276.0
95.10	83488.0
96.10	5344.0
97.10	157.0
103.90	467.0
104.90	134.0
106.00	531.0
110.90	177.0
114.90	127.0
115.90	394.0
116.90	814.0
117.90	384.0
118.90	520.0
123.80	104.0
127.90	386.0
128.80	155.0
130.00	372.0
131.00	121.0
134.80	197.0
135.90	104.0
136.90	258.0
139.60	105.0
140.90	1118.0
141.80	197.0
143.00	1611.0
145.00	483.0
145.80	221.0
147.90	274.0
149.90	161.0
153.90	107.0
154.90	224.0
156.90	194.0
158.90	128.0
160.80	192.0
170.90	286.0
171.90	1066.0
173.10	1247.0
174.00	81760.0
175.00	6085.0
176.00	78896.0
177.00	4815.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252