

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033411.D
 Acq On : 16 Dec 2023 04:51
 Operator : SY/MD
 Sample : 05802-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 16 06:46:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 01:35:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	228259	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	238771	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	100461	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	79675	45.327	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.660%
7) Chloroethane-d5	1.532	69	73786	46.775	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.540%
11) 1,1-Dichloroethene-d2	2.060	65	38764	44.300	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.600%
21) 2-Butanone-d5	3.786	46	86471	97.607	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.610%
24) Chloroform-d	4.249	84	160853	46.261	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.520%
26) 1,2-Dichloroethane-d4	4.940	65	105003	49.159	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.320%
32) Benzene-d6	4.960	84	299846	46.626	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.260%
36) 1,2-Dichloropropane-d6	5.989	67	91587	46.925	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.860%
41) Toluene-d8	7.243	98	255010	43.337	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.680%
43) trans-1,3-Dichloroprop...	7.551	79	41031	42.895	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.800%
47) 2-Hexanone-d5	8.027	63	58491	89.099	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.100%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	128518	45.814	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.620%
66) 1,2-Dichlorobenzene-d4	11.561	152	105895	56.094	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.180%
Target Compounds						
44) trans-1,3-Dichloropropene	7.551	75	1844	0.732	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033411.D
Acq On : 16 Dec 2023 04:51
Operator : SY/MD
Sample : 05802-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 16 06:46:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 01:35:53 2023
Response via : Initial Calibration

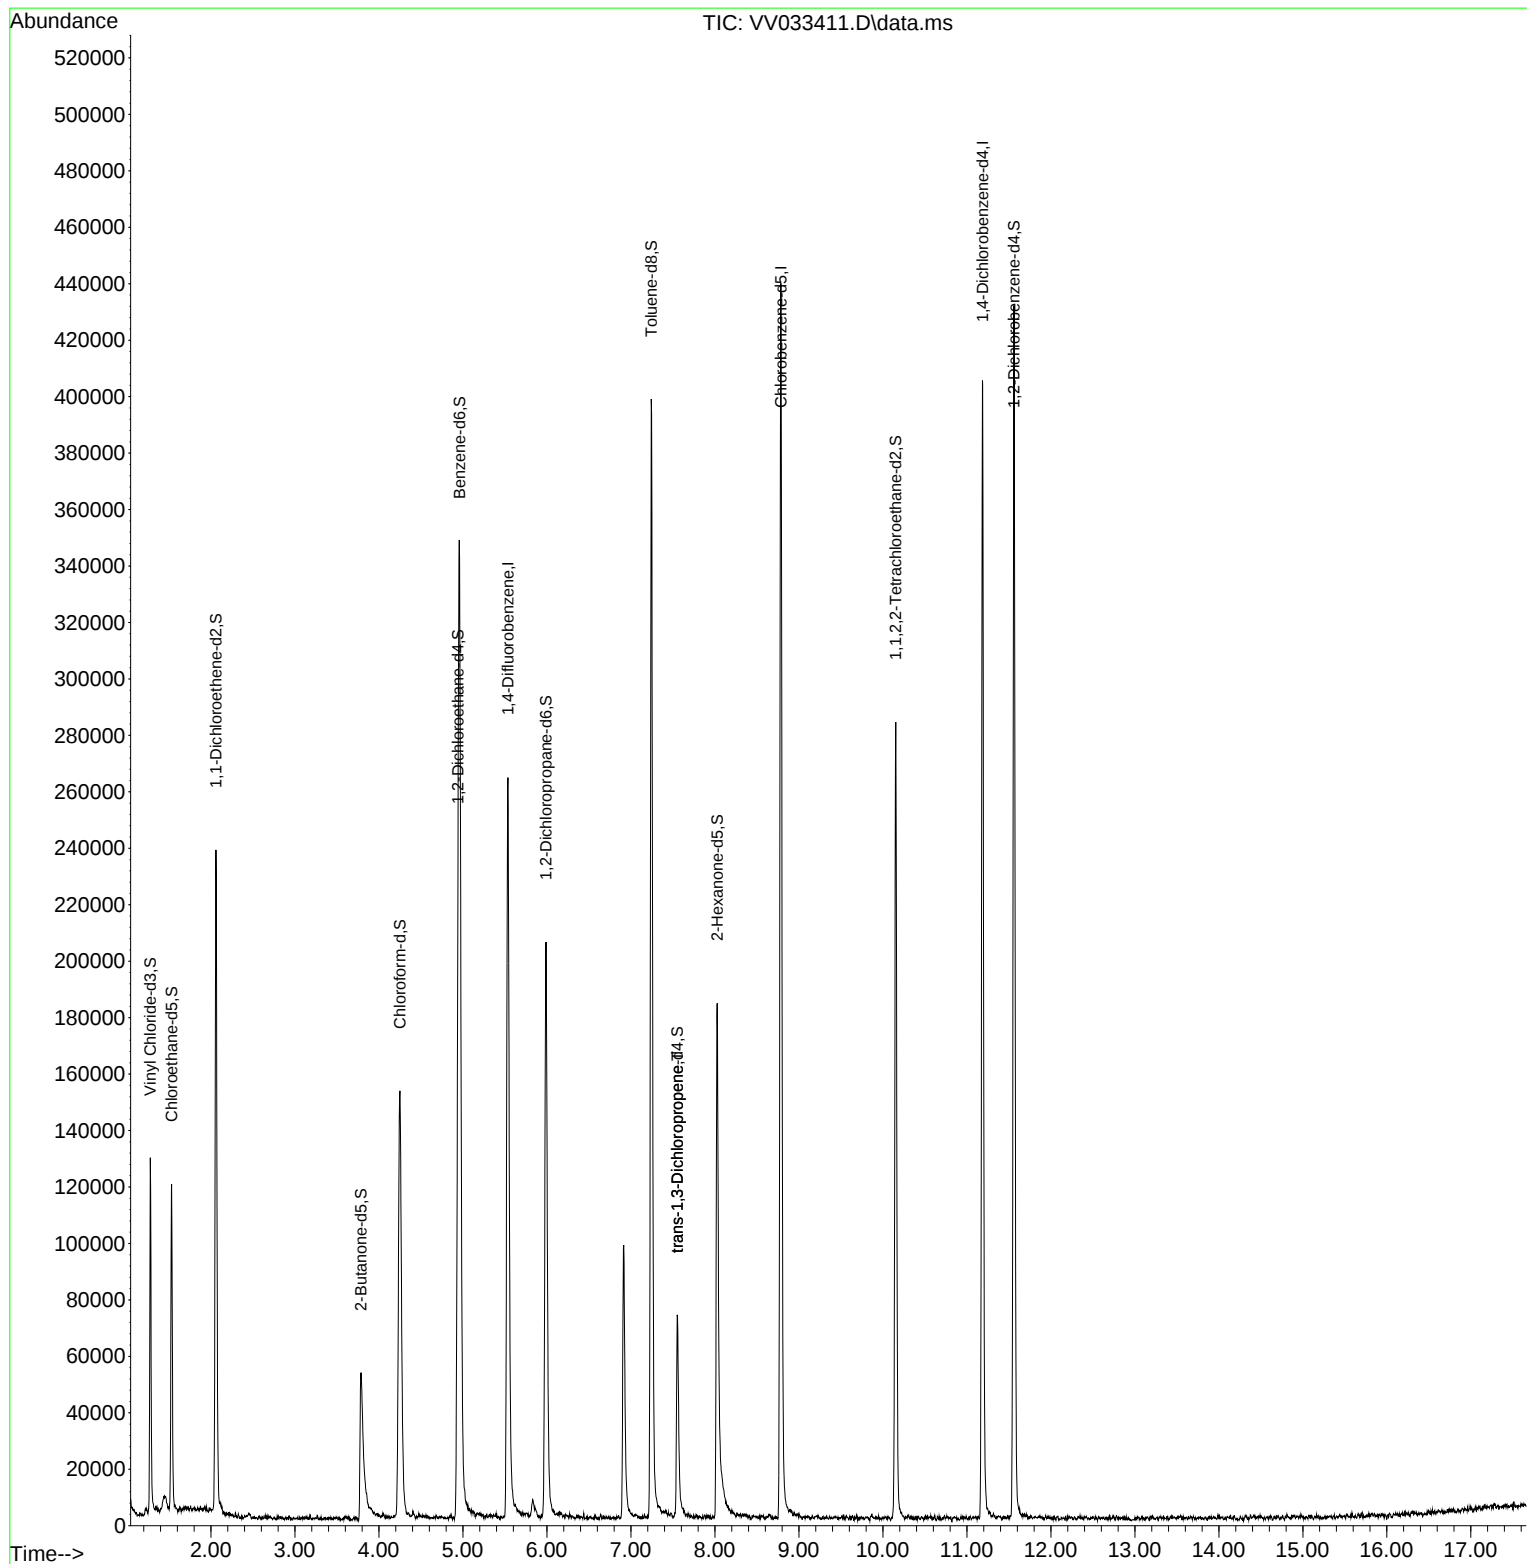

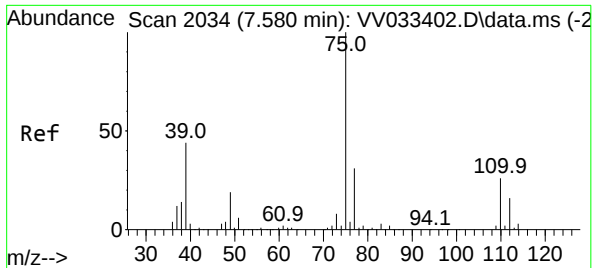

#44
 trans-1,3-Dichloropropene
 Concen: 0.732 ug/L
 RT: 7.551 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: VV033411.D
 Acq: 16 Dec 2023 04:51

Instrument :
 MSVOA_V
 ClientSampleId :

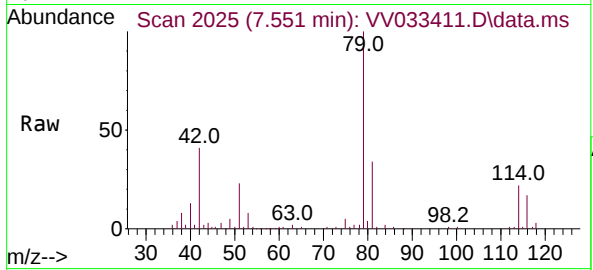

Tgt Ion: 75 Resp: 1844
 Ion Ratio Lower Upper
 75 100
 77 39.9 22.4 41.6

