

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033413.D
 Acq On : 16 Dec 2023 05:37
 Operator : SY/MD
 Sample : 05802-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 16 06:46:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 01:35:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	219196	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	230123	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	98546	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	76281	45.190	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.380%		
7) Chloroethane-d5	1.529	69	70628	46.624	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.240%		
11) 1,1-Dichloroethene-d2	2.060	65	37714	44.883	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.760%		
21) 2-Butanone-d5	3.786	46	80359	94.458	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.460%		
24) Chloroform-d	4.246	84	157659	47.217	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.440%		
26) 1,2-Dichloroethane-d4	4.941	65	99769	48.639	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.280%		
32) Benzene-d6	4.960	84	289237	46.667	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.340%		
36) 1,2-Dichloropropane-d6	5.986	67	89333	47.490	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.980%		
41) Toluene-d8	7.243	98	249781	44.044	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.080%		
43) trans-1,3-Dichloroprop...	7.555	79	39181	42.501	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.000%		
47) 2-Hexanone-d5	8.024	63	54162	85.605	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.610%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	122491	45.307	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.620%		
66) 1,2-Dichlorobenzene-d4	11.561	152	101327	54.717	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	109.440%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.066	96	1387	0.898	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033413.D
Acq On : 16 Dec 2023 05:37
Operator : SY/MD
Sample : 05802-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 16 06:46:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 01:35:53 2023
Response via : Initial Calibration

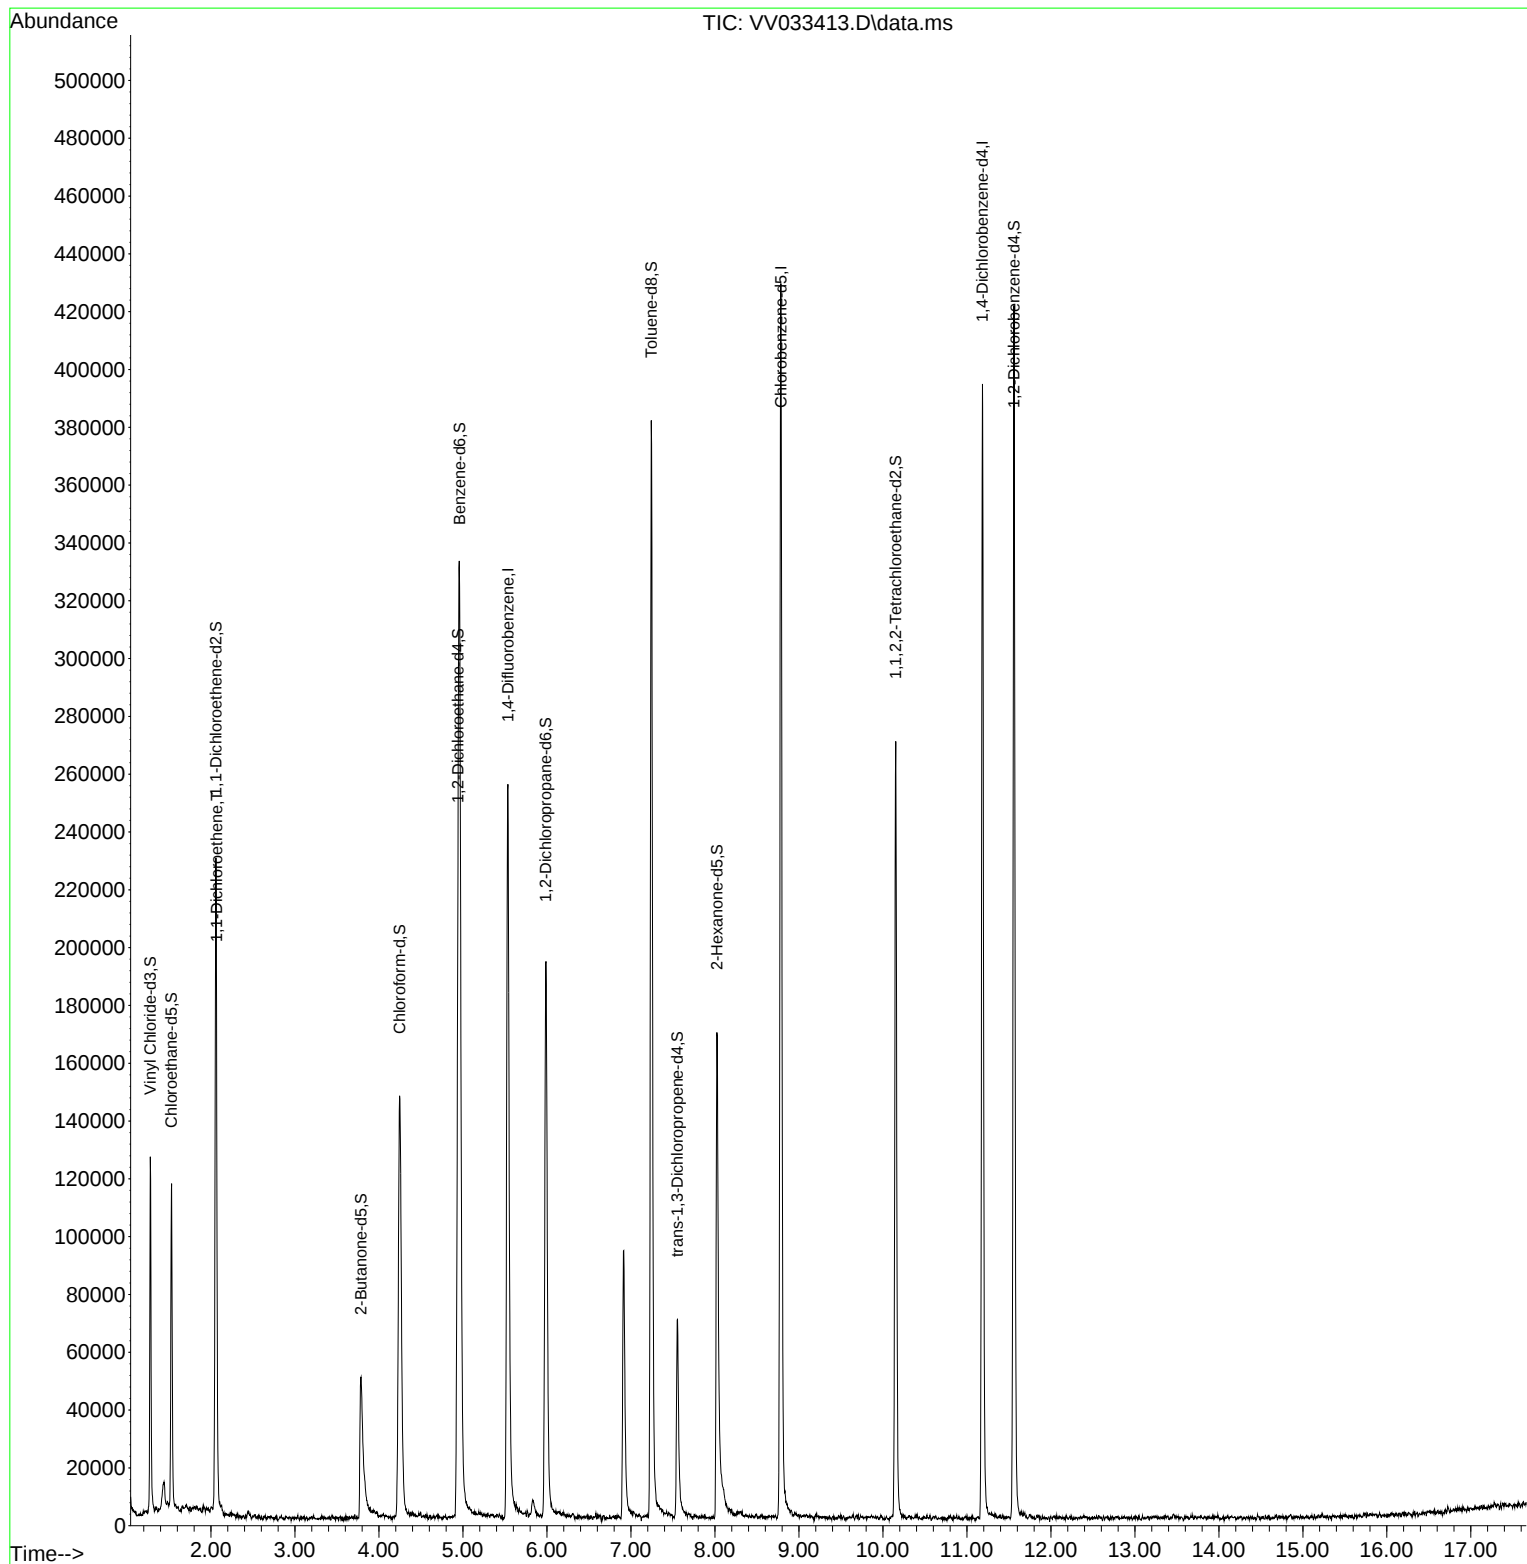

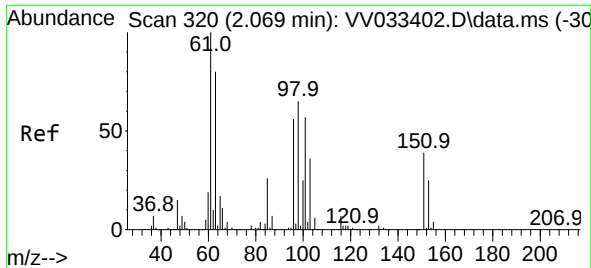

#12
 1,1-Dichloroethene
 Concen: 0.898 ug/L
 RT: 2.066 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV033413.D
 Acq: 16 Dec 2023 05:37

Instrument :
 MSVOA_V
 ClientSampleId :

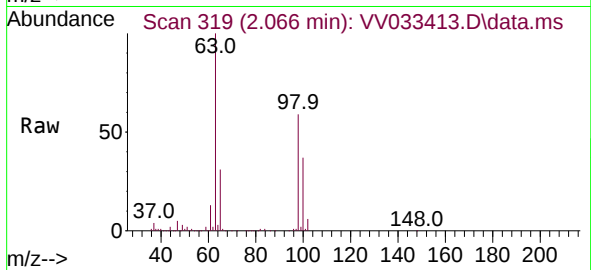

Tgt Ion:	96	Resp:	1387
Ion	Ratio	Lower	Upper
96	100		
61	1034.6	124.3	230.8#
63	8248.6	108.1	200.7#

