




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033388.D
 Acq On : 15 Dec 2023 19:33
 Operator : SY/MD
 Sample : 05846-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:18:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

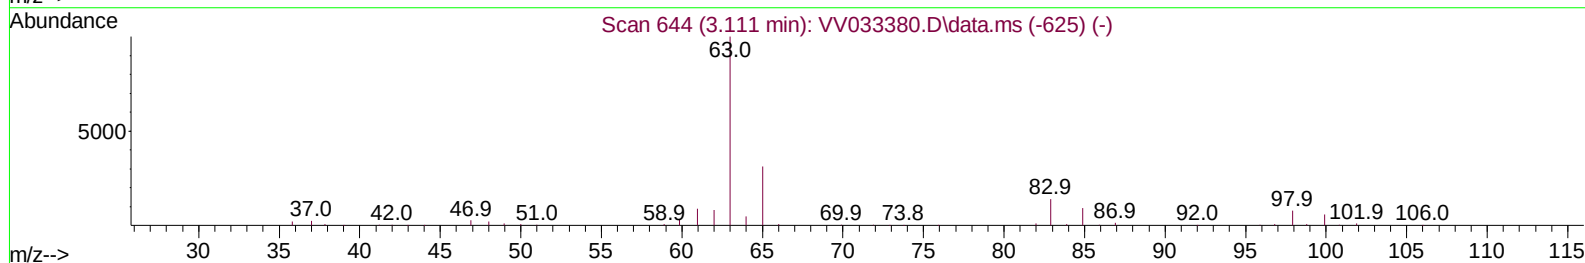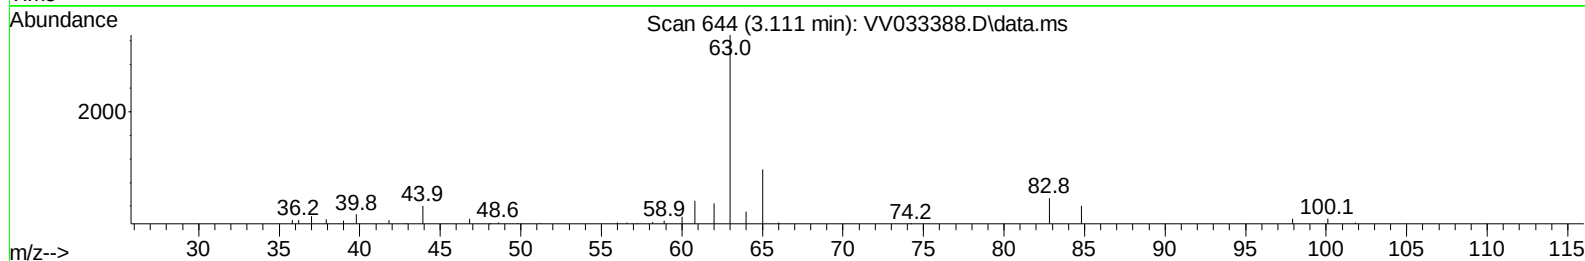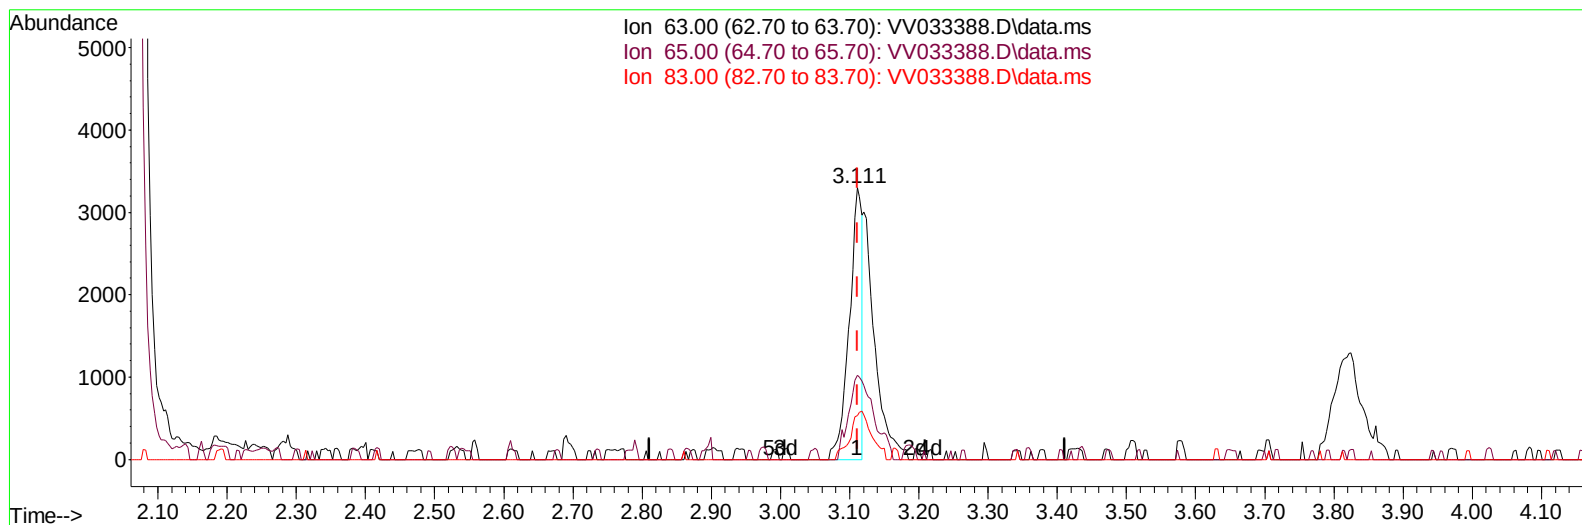

TIC: VV033388.D\data.ms

(19) 1,1-Dichloroethane (T)

3.111min (-0.000) 1.43 ug/L

response 4189

Ion	Exp%	Act%
63.00	100.00	100.00
65.00	30.20	31.09
83.00	13.80	16.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033388.D
Acq On : 15 Dec 2023 19:33
Operator : SY/MD
Sample : 05846-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD0

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:18:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 15 23:24:47 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

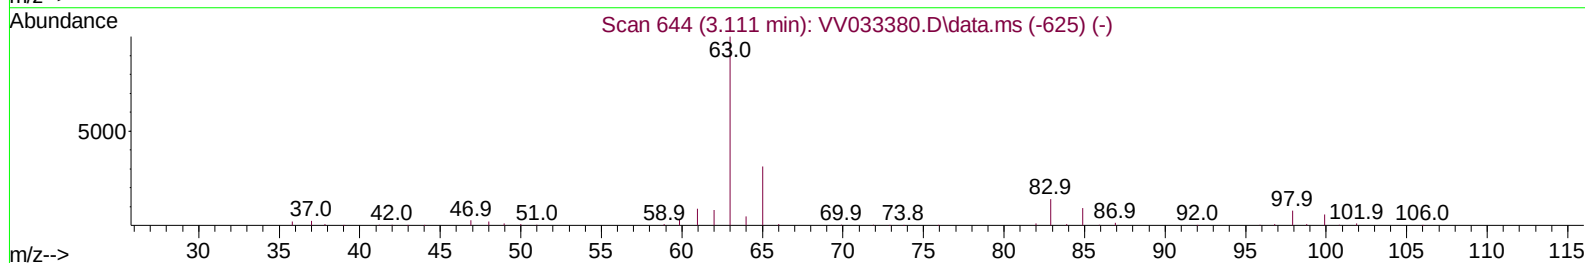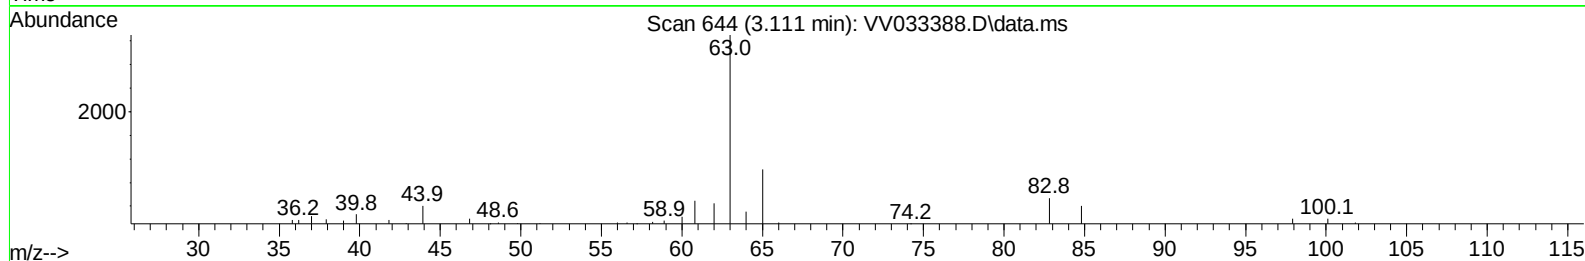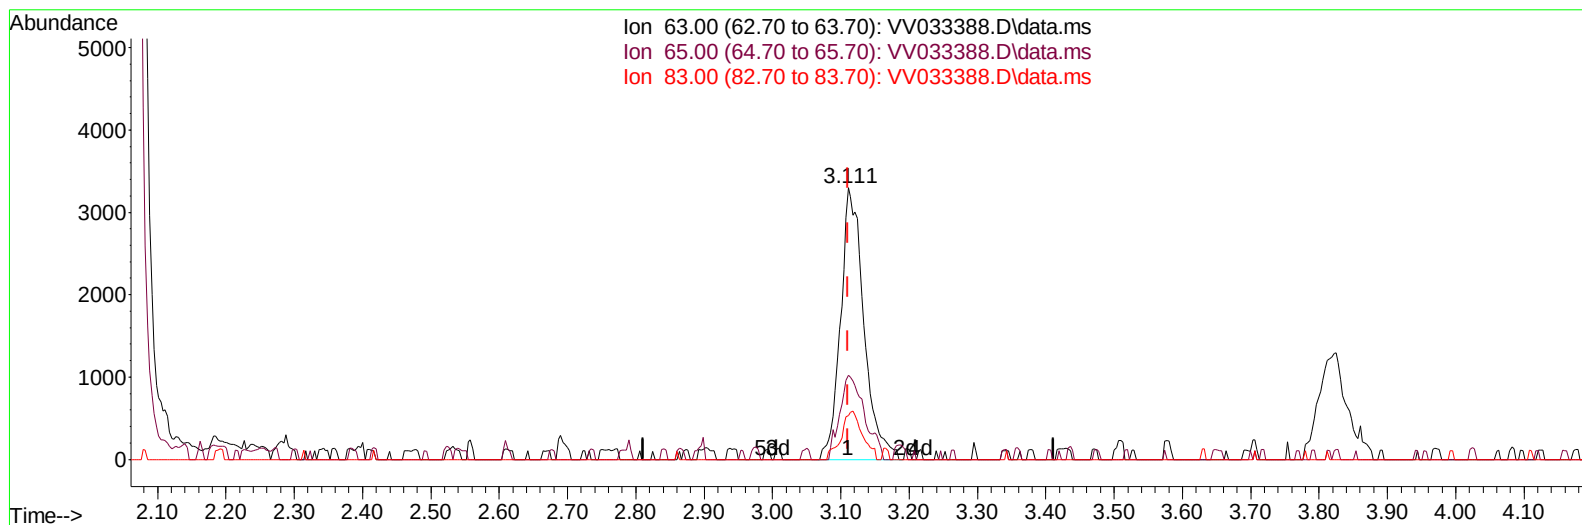

TIC: VV033388.D\data.ms

(19) 1,1-Dichloroethane (T)

3.111min (-0.000) 2.65 ug/L m

response 7773

Ion	Exp%	Act%
63.00	100.00	100.00
65.00	30.20	31.09
83.00	13.80	16.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033388.D
 Acq On : 15 Dec 2023 19:33
 Operator : SY/MD
 Sample : 05846-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:18:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

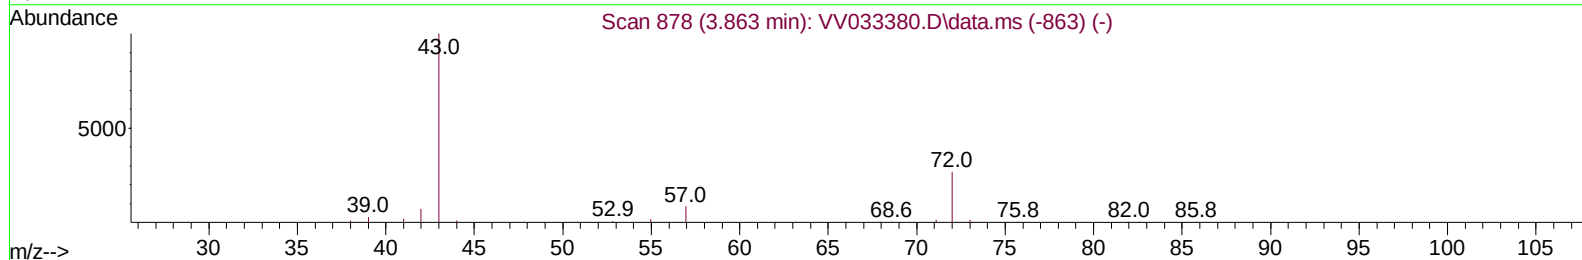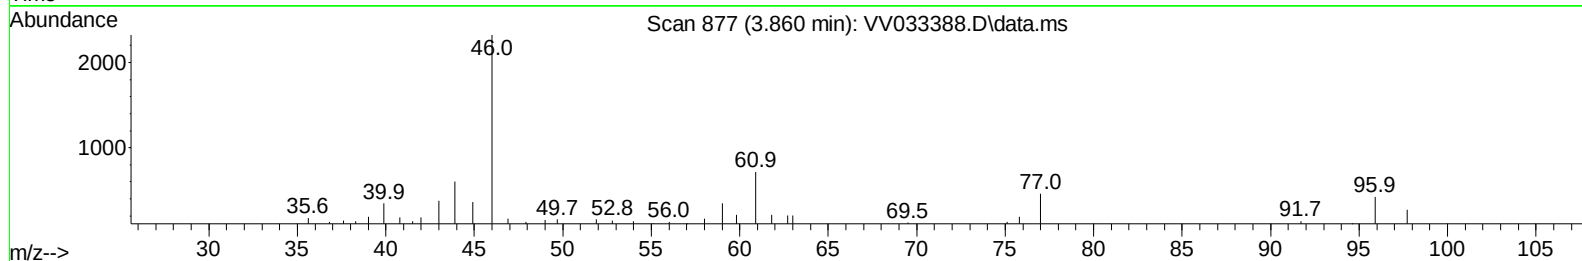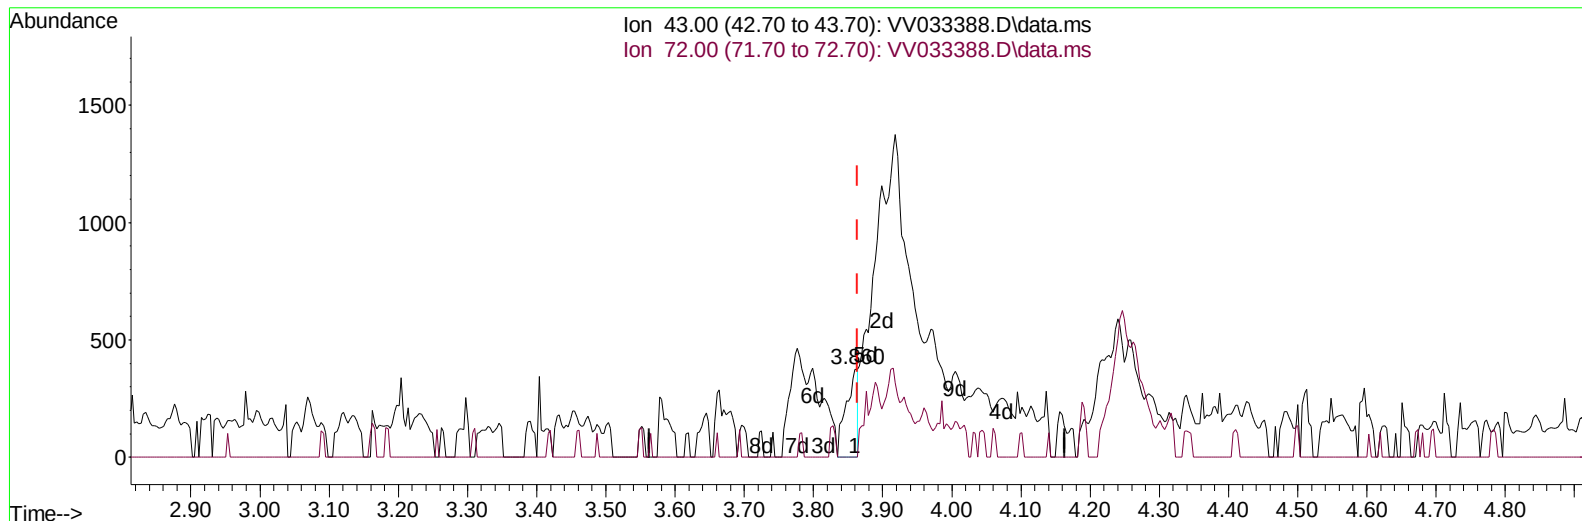

TIC: VV033388.D\data.ms

(22) 2-Butanone (T)

3.860min (-0.003) 0.44 ug/L

response 445

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	17.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033388.D
 Acq On : 15 Dec 2023 19:33
 Operator : SY/MD
 Sample : 05846-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD0

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:18:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

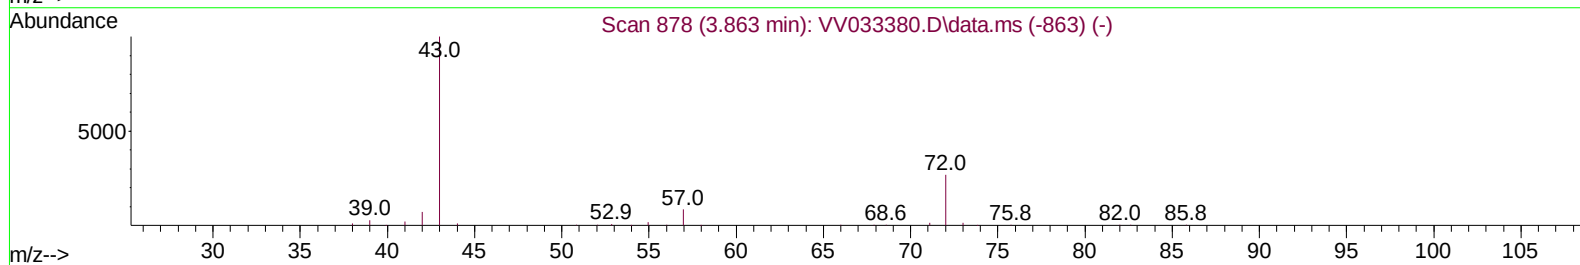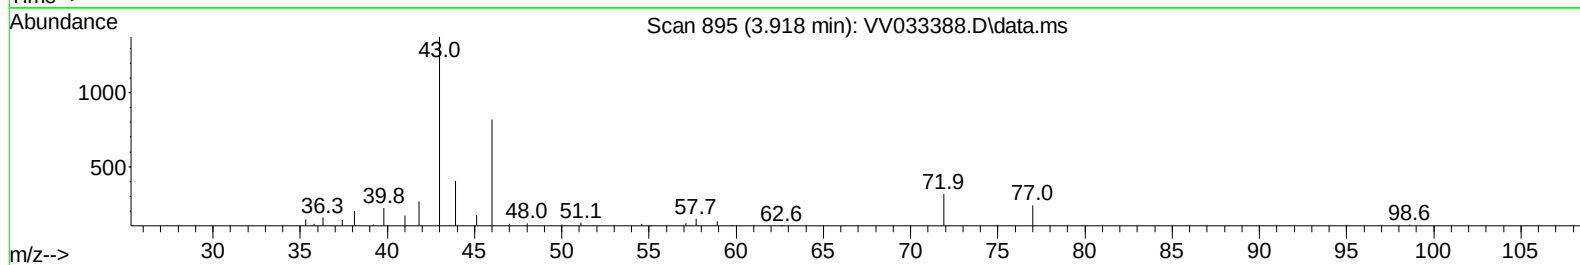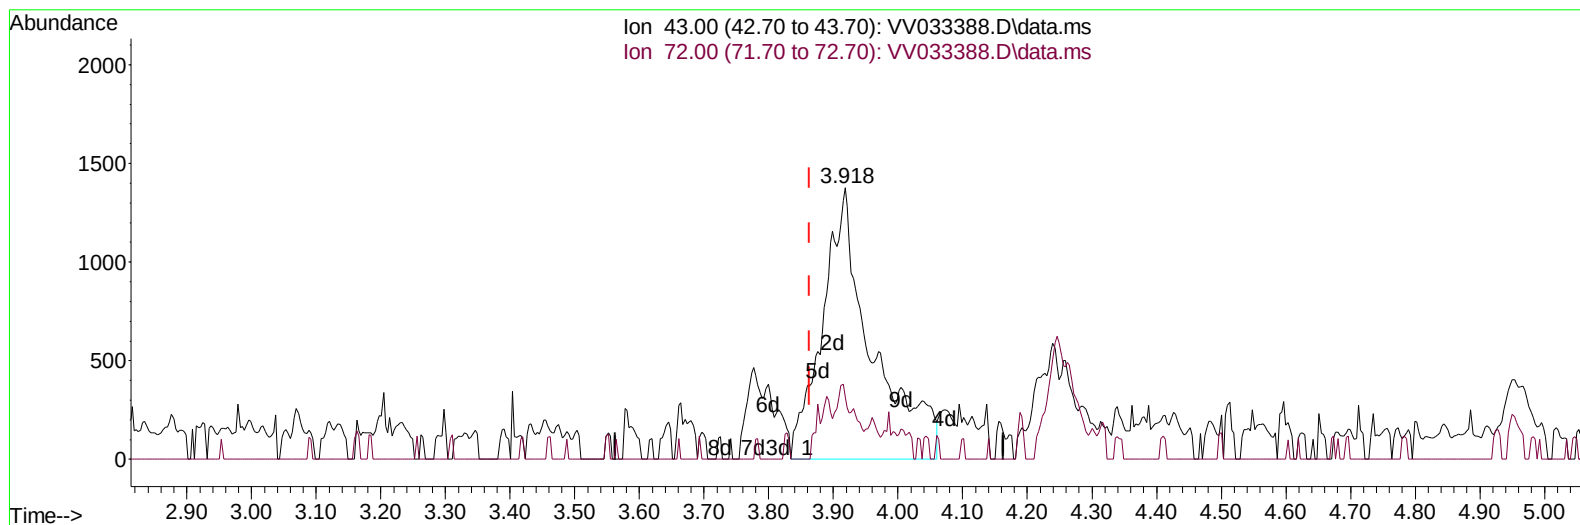

TIC: VV033388.D\data.ms

(22) 2-Butanone (T)

3.918min (+ 0.055) 7.15 ug/L m

response 7283

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	1.04#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033388.D
 Acq On : 15 Dec 2023 19:33
 Operator : SY/MD
 Sample : 05846-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD0

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:18:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	229437	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	233229	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	97954	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	83930	47.502	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	95.000%	
7) Chloroethane-d5	1.532	69	74761	47.149	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	94.300%	
11) 1,1-Dichloroethene-d2	2.060	65	40573	46.130	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	92.260%	
21) 2-Butanone-d5	3.783	46	88601	99.498	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	99.500%	
24) Chloroform-d	4.249	84	163158	46.683	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.360%	
26) 1,2-Dichloroethane-d4	4.941	65	105674	49.219	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	98.440%	
32) Benzene-d6	4.960	84	305666	48.660	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.320%	
36) 1,2-Dichloropropane-d6	5.989	67	94571	49.606	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	99.220%	
41) Toluene-d8	7.243	98	259667	45.177	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.360%	
43) trans-1,3-Dichloroprop...	7.555	79	39700	42.490	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	84.980%	
47) 2-Hexanone-d5	8.024	63	59111	92.183	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	92.180%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	131477	47.983	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	95.960%	
66) 1,2-Dichlorobenzene-d4	11.561	152	105079	57.086	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	114.180%	
Target Compounds						
13) Acetone	2.111	43	44603	43.151	ug/L	98
19) 1,1-Dichloroethane	3.111	63	7773m	2.654	ug/L	
20) cis-1,2-Dichloroethene	3.822	96	9108	5.256	ug/L	97
22) 2-Butanone	3.918	43	7283m	7.152	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033388.D
Acq On : 15 Dec 2023 19:33
Operator : SY/MD
Sample : 05846-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD0

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:18:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 15 23:24:47 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

