




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

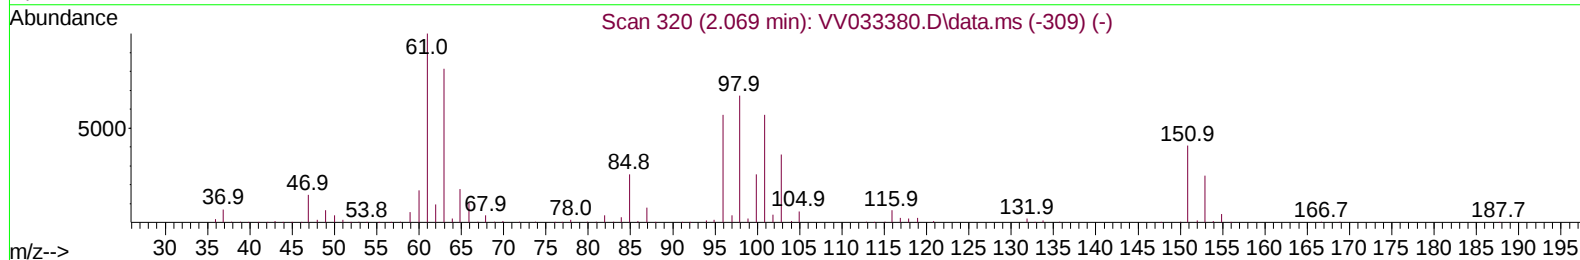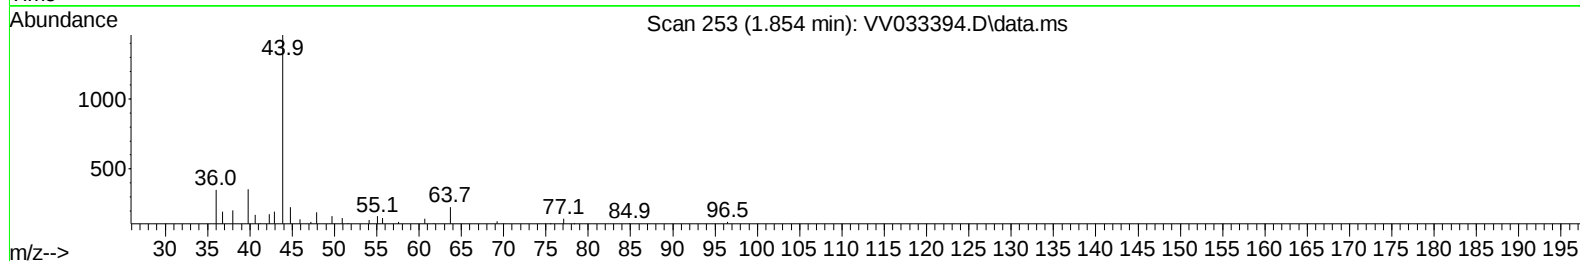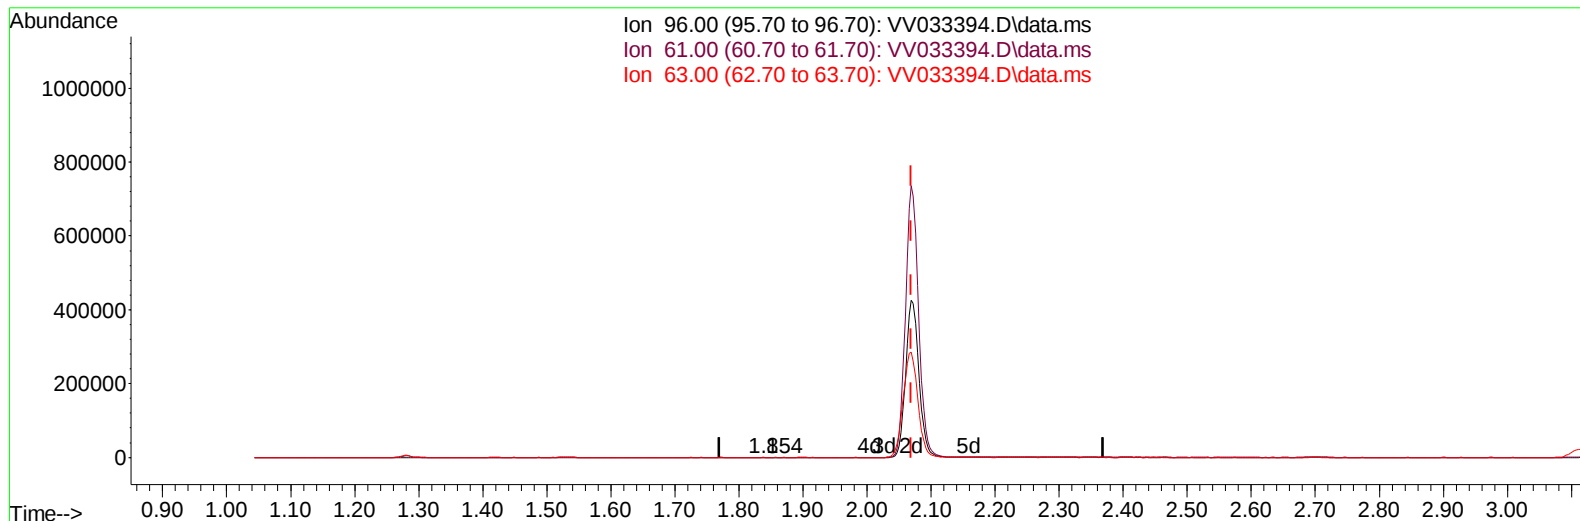

TIC: VV033394.D\data.ms

(12) 1,1-Dichloroethene (T)

1.854min (-0.216) 0.03 ug/L

response 45

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	177.50	205.69
63.00	154.40	184.55
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

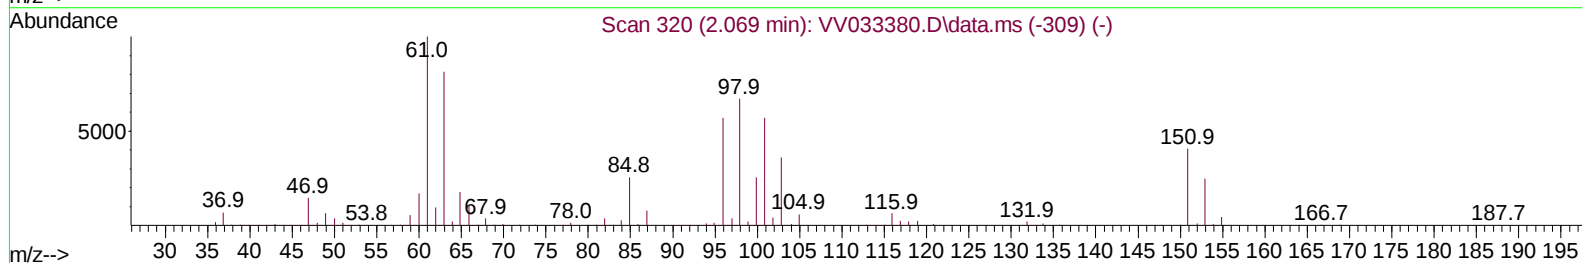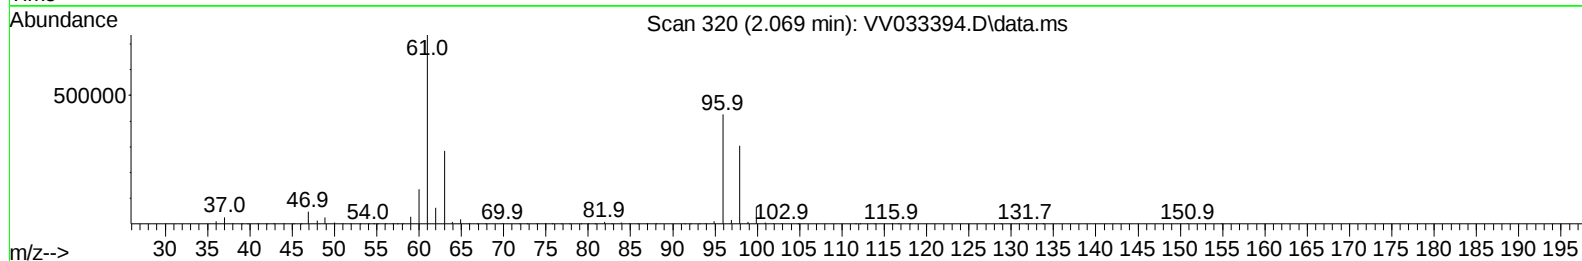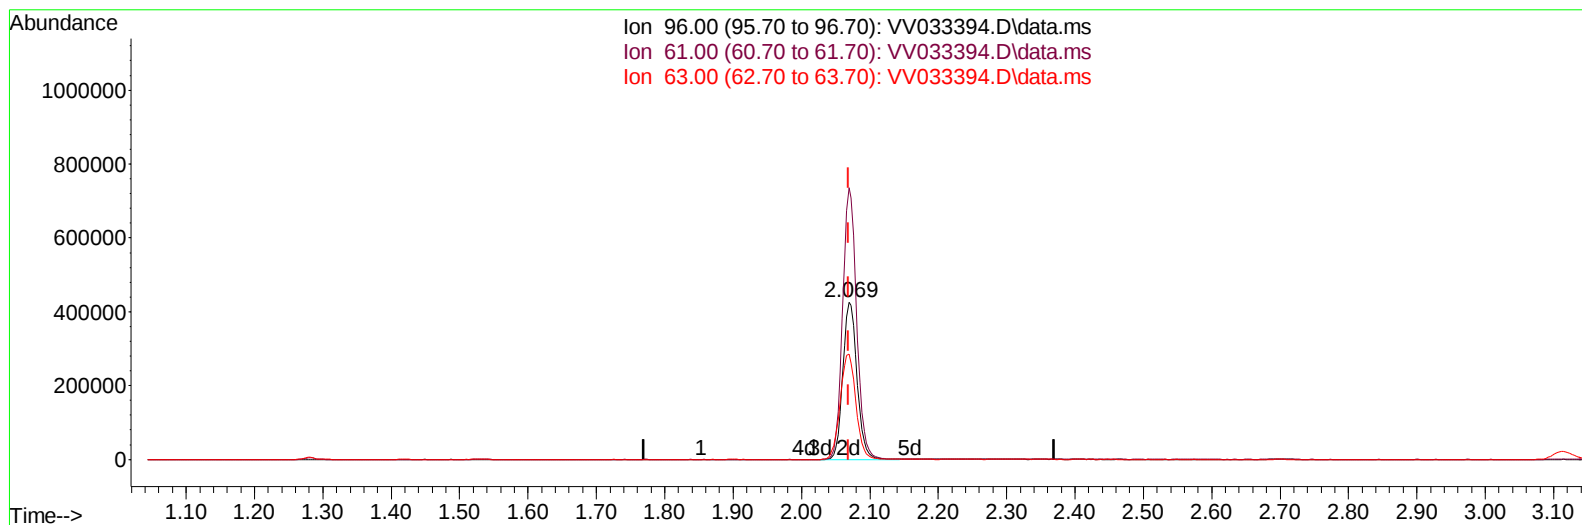

TIC: VV033394.D\data.ms

(12) 1,1-Dichloroethene (T)

2.069min (-0.000) 390.15 ug/L m

response 614721

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	177.50	172.59
63.00	154.40	66.86#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

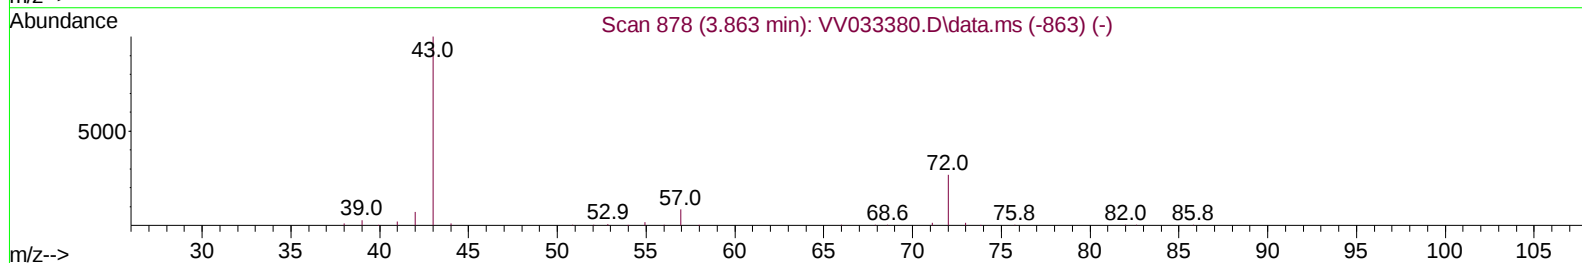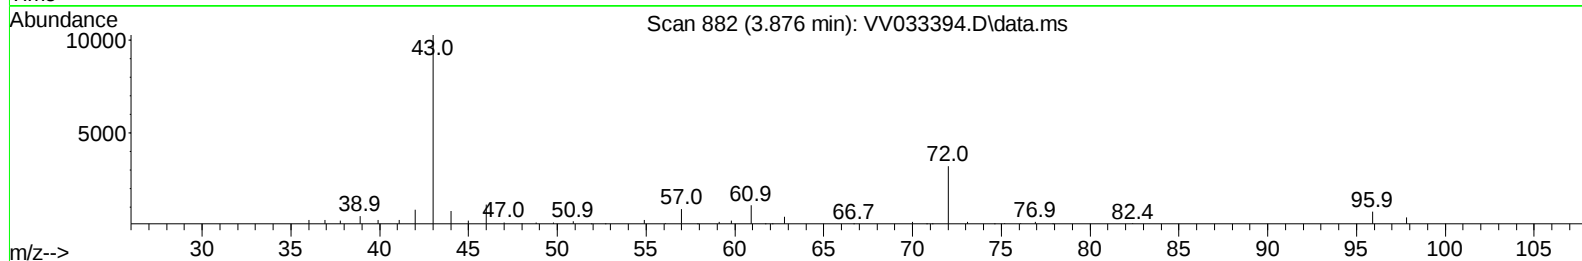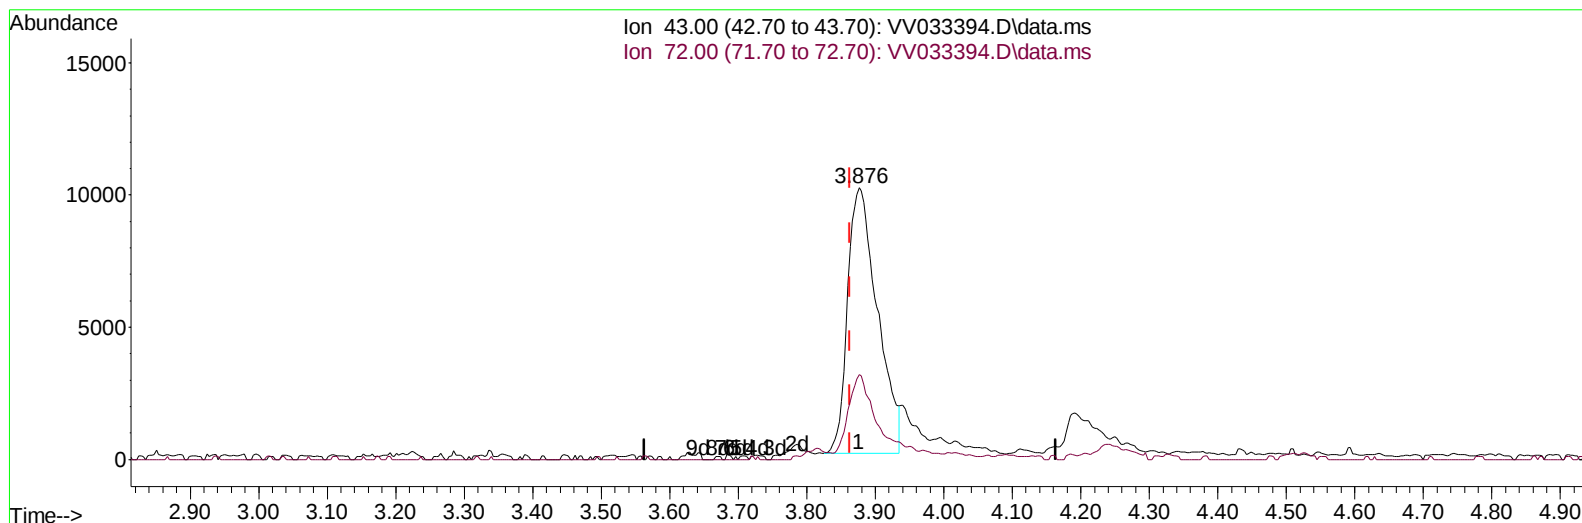

TIC: VV033394.D\data.ms

(22) 2-Butanone (T)

3.876min (+ 0.013) 30.67 ug/L

response 30438

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	26.44
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

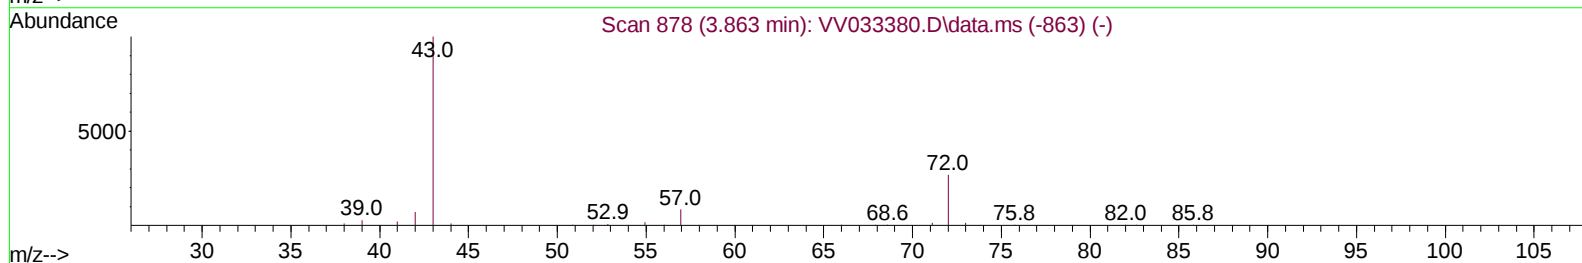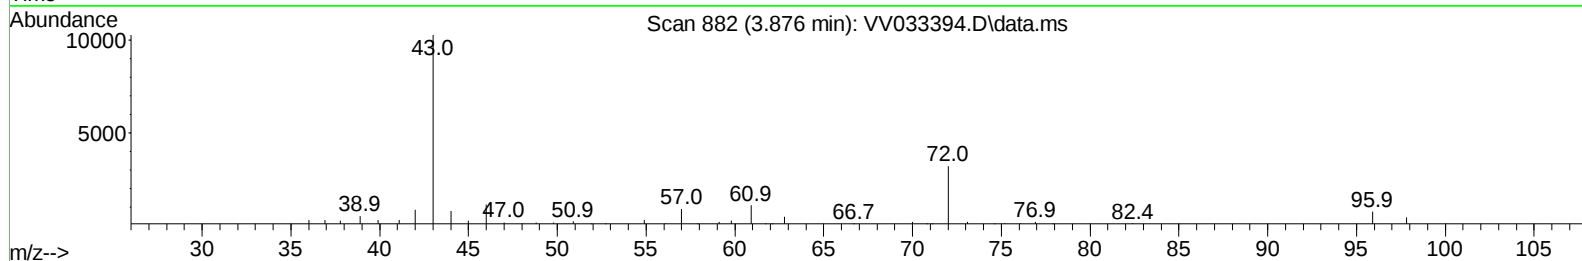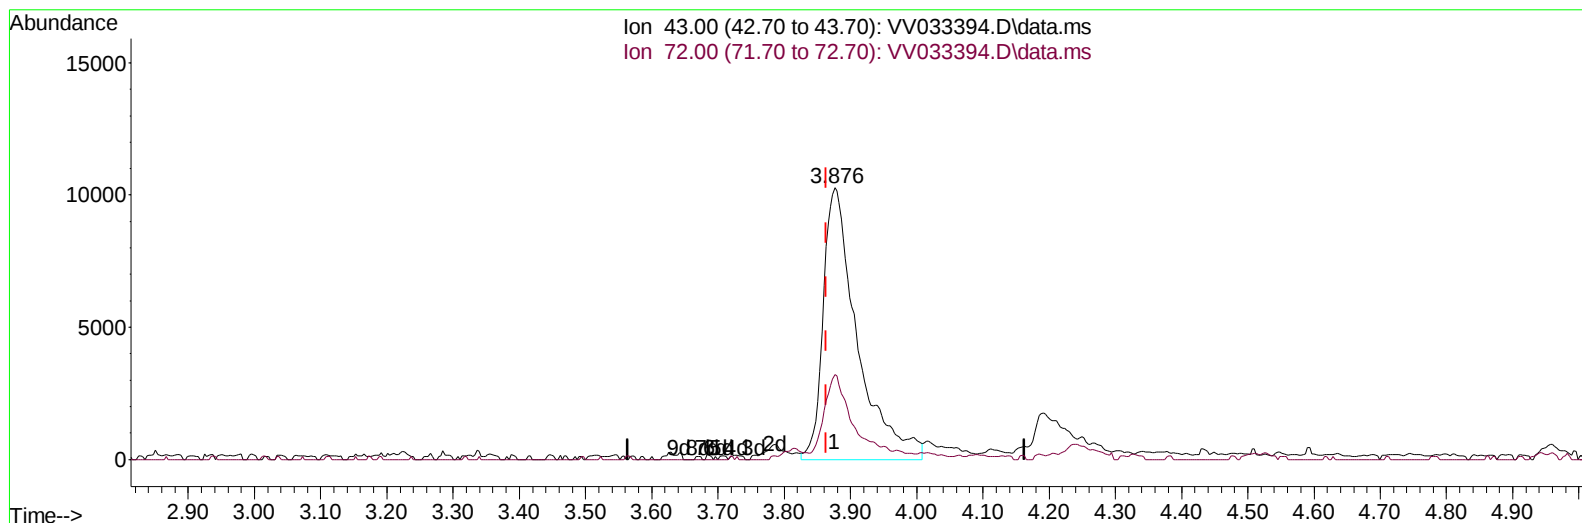

TIC: VV033394.D\data.ms

(22) 2-Butanone (T)

3.876min (+ 0.013) 37.04 ug/L m

response 36761

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	21.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

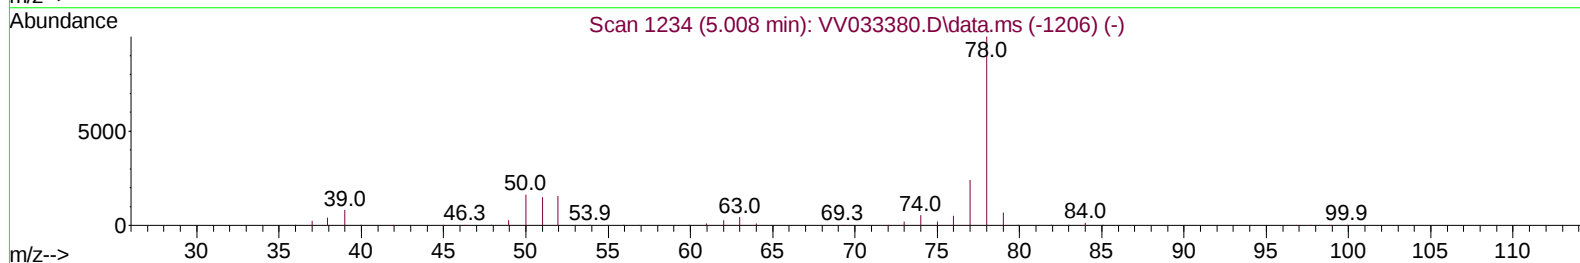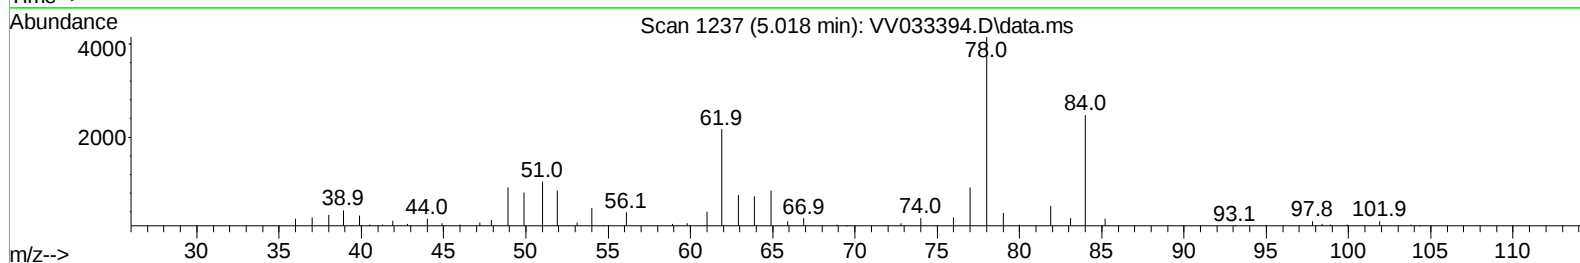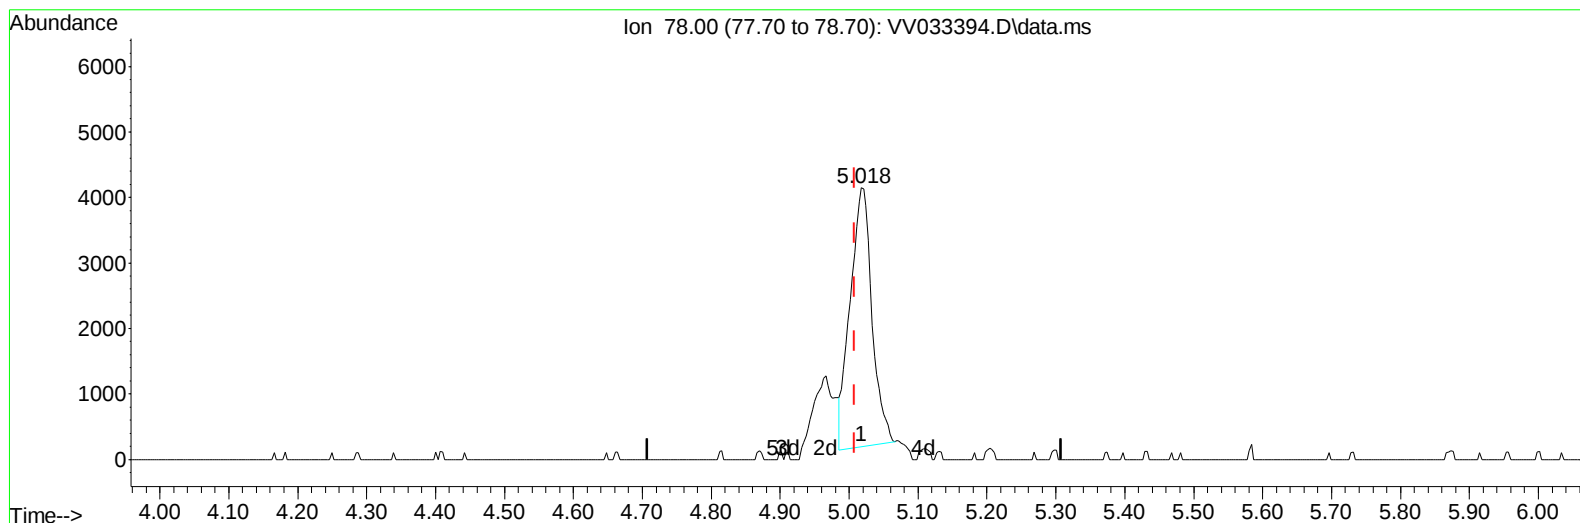

TIC: VV033394.D\data.ms

(33) Benzene (T)

5.018min (+ 0.010) 1.40 ug/L

response 8658

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

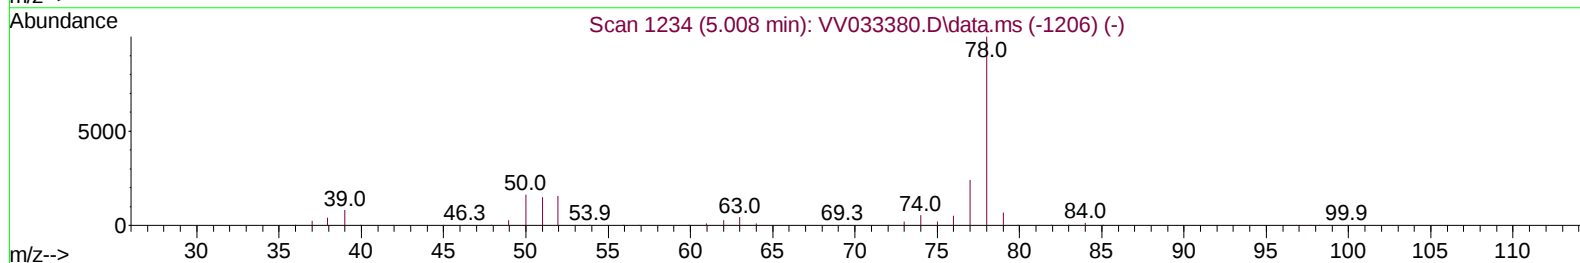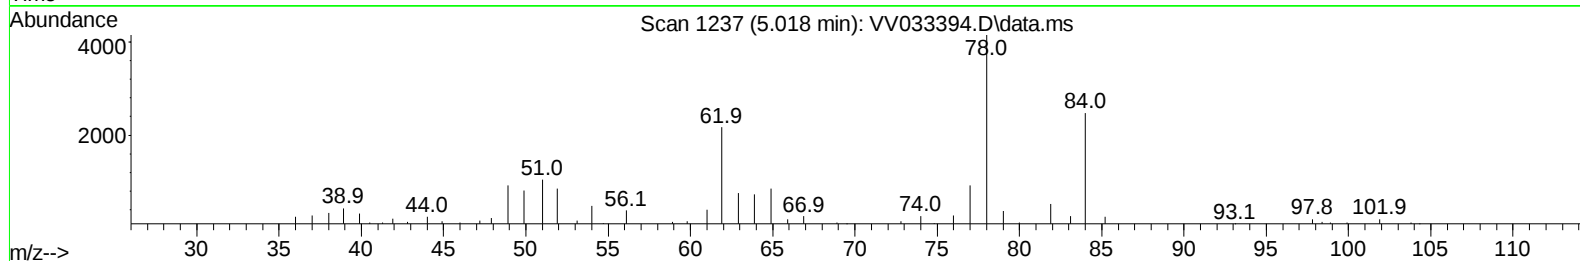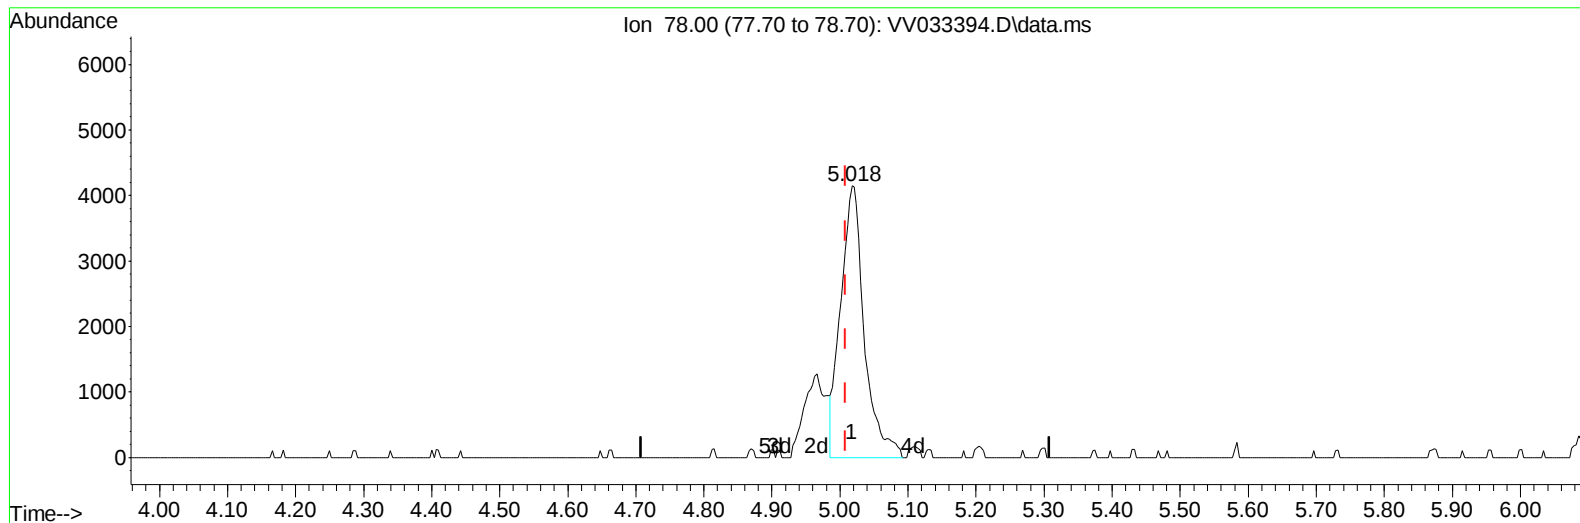

TIC: VV033394.D\data.ms

(33) Benzene (T)

5.018min (+ 0.010) 1.61 ug/L m

response 9945

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

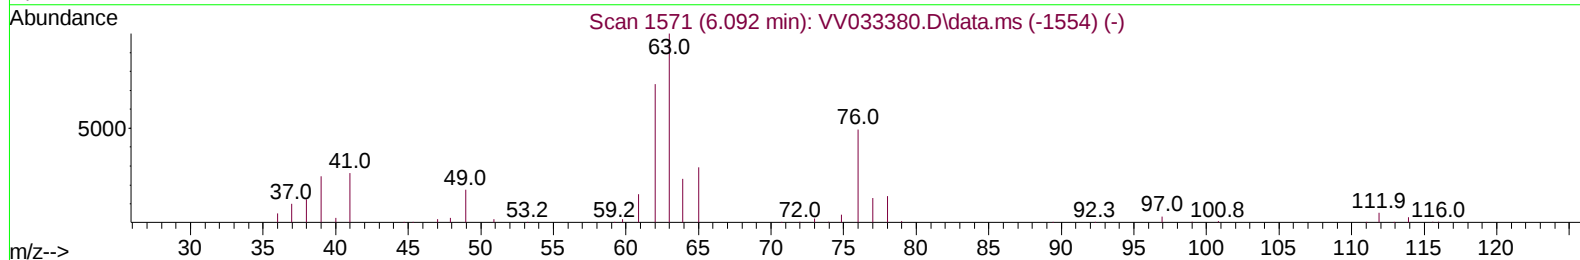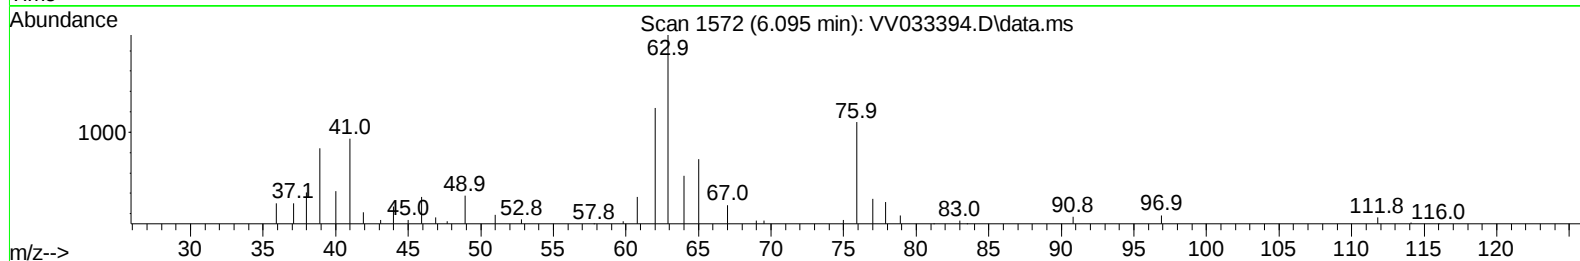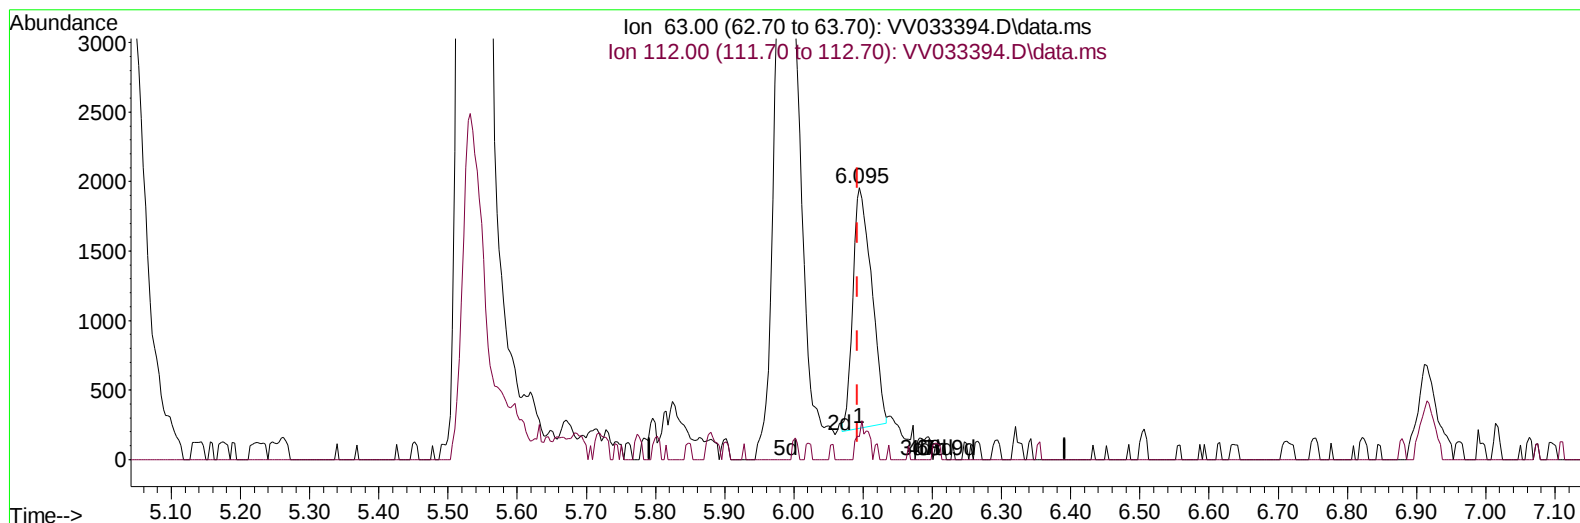

TIC: VV033394.D\data.ms

(37) 1,2-Dichloropropane (T)

6.095min (+ 0.003) 1.94 ug/L

response 3250

Ion	Exp%	Act%
63.00	100.00	100.00
112.00	4.60	2.74#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

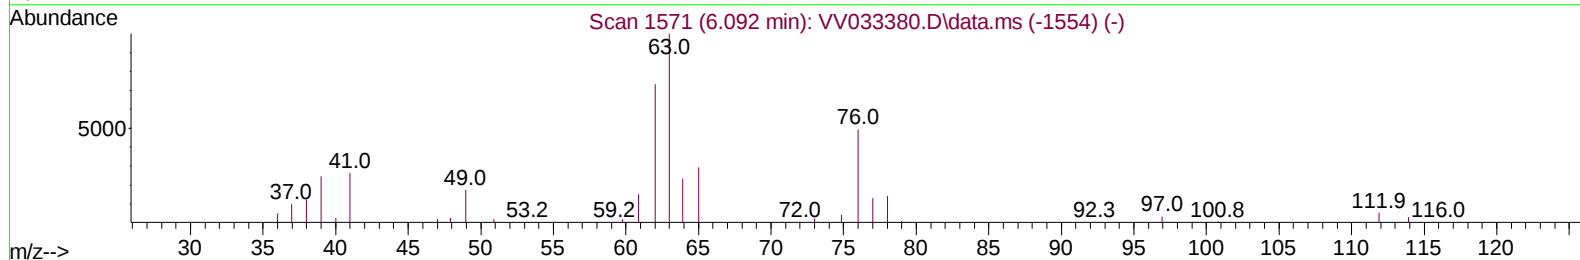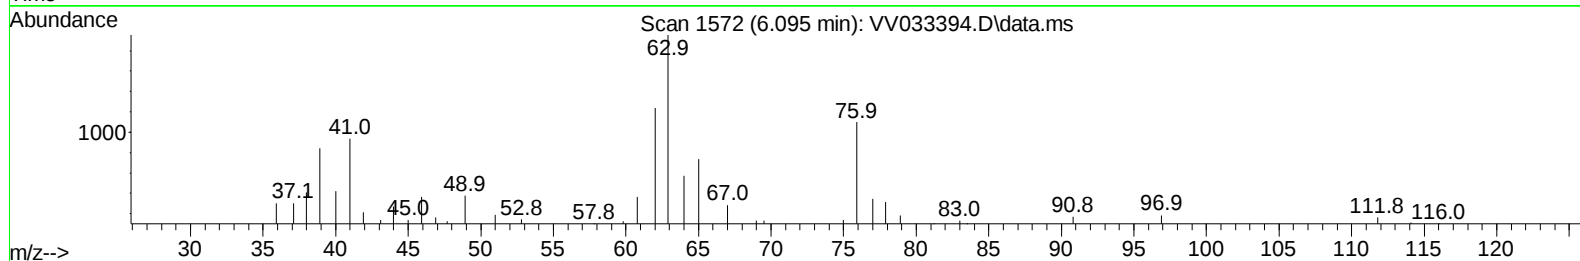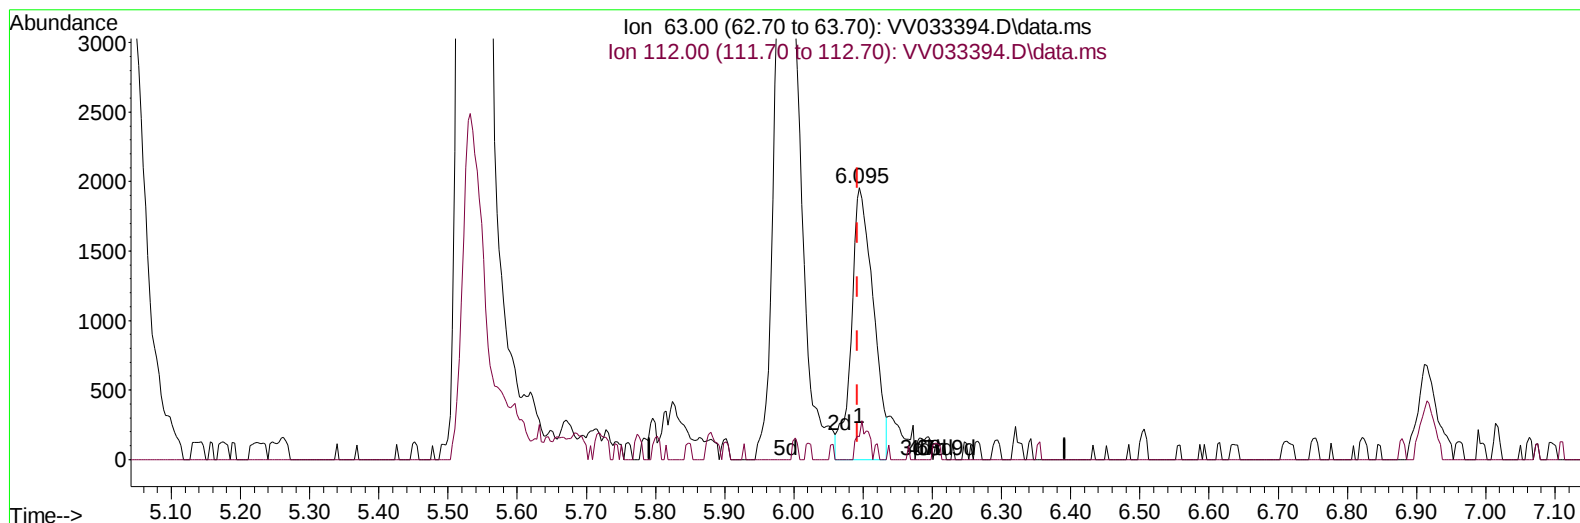

TIC: VV033394.D\data.ms

(37) 1,2-Dichloropropane (T)

6.095min (+ 0.003) 2.55 ug/L m

response 4284

Ion	Exp%	Act%
63.00	100.00	100.00
112.00	4.60	2.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	223589	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	231977	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	95663	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	81137	47.122	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	94.240%	
7) Chloroethane-d5	1.532	69	71420	46.220	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	92.440%	
11) 1,1-Dichloroethene-d2	2.060	65	39925	46.580	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	93.160%	
21) 2-Butanone-d5	3.783	46	86585	99.777	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	99.780%	
24) Chloroform-d	4.249	84	157630	46.281	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.560%	
26) 1,2-Dichloroethane-d4	4.941	65	101945	48.724	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.440%	
32) Benzene-d6	4.960	84	296466	47.451	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.900%	
36) 1,2-Dichloropropane-d6	5.986	67	90707	47.836	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	95.680%	
41) Toluene-d8	7.243	98	252096	44.096	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	88.200%	
43) trans-1,3-Dichloroprop...	7.555	79	40881	43.990	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.980%	
47) 2-Hexanone-d5	8.024	63	54985	86.212	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	86.210%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	124801	45.792	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.580%	
66) 1,2-Dichlorobenzene-d4	11.561	152	99382	55.284	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	110.560%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.285	62	21821	12.036	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.069	101	8388	4.523	ug/L #	82
12) 1,1-Dichloroethene	2.069	96	614721m	390.149	ug/L	
13) Acetone	2.111	43	40657	40.362	ug/L	98
14) Carbon disulfide	2.240	76	4588	1.139	ug/L	97
18) Methyl tert-butyl Ether	2.703	73	2845	0.629	ug/L #	81
19) 1,1-Dichloroethane	3.111	63	46794	16.394	ug/L	99
20) cis-1,2-Dichloroethene	3.815	96	81591	48.320	ug/L	95
22) 2-Butanone	3.876	43	36761m	37.042	ug/L	
25) Chloroform	4.278	83	8285	2.579	ug/L	97
27) 1,2-Dichloroethane	5.043	62	48159	19.450	ug/L	98
30) 1,1,1-Trichloroethane	4.513	97	108155	37.762	ug/L	98
33) Benzene	5.018	78	9945m	1.608	ug/L	
34) Trichloroethene	5.834	95	62787	37.014	ug/L	98
37) 1,2-Dichloropropane	6.095	63	4284m	2.555	ug/L	
46) Tetrachloroethene	7.912	164	2786	2.102	ug/L	92

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:21:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 15 23:24:47 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed								

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033394.D
Acq On : 15 Dec 2023 21:53
Operator : SY/MD
Sample : 05846-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 00:21:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 15 23:24:47 2023
Response via : Initial Calibration

