




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033424.D
 Acq On : 16 Dec 2023 11:02
 Operator : SY/MD
 Sample : 05846-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:26:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

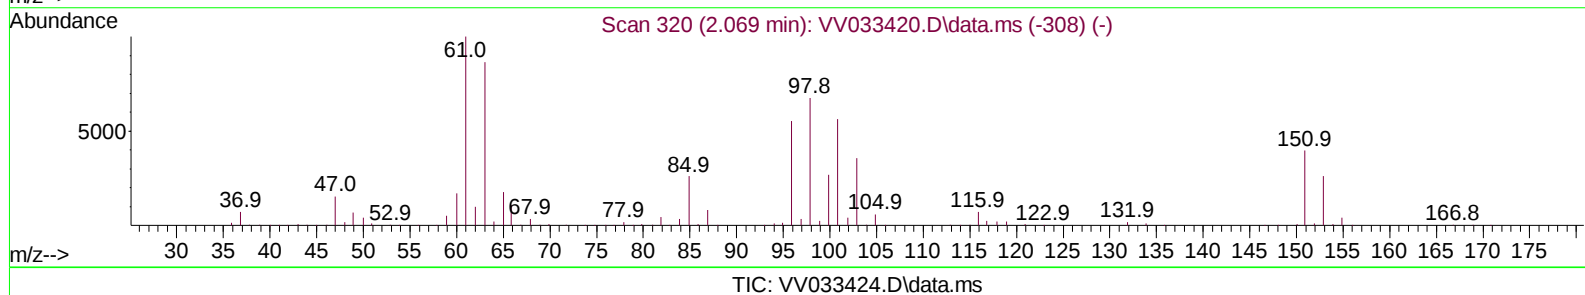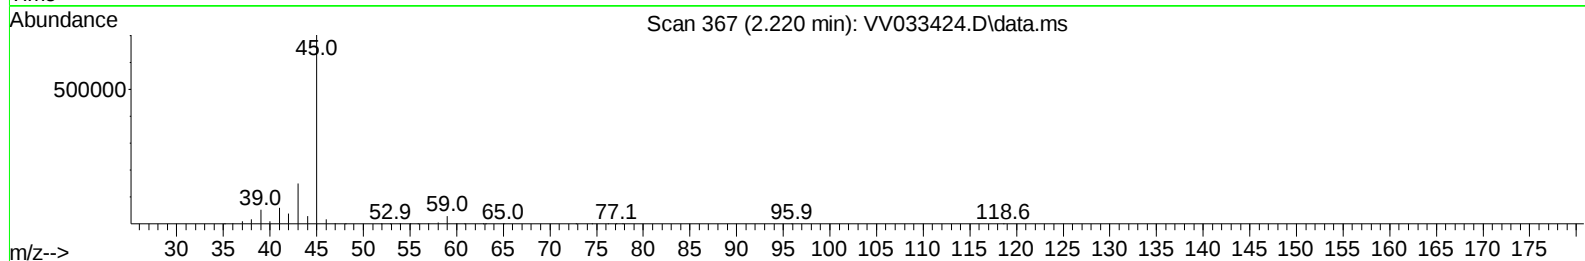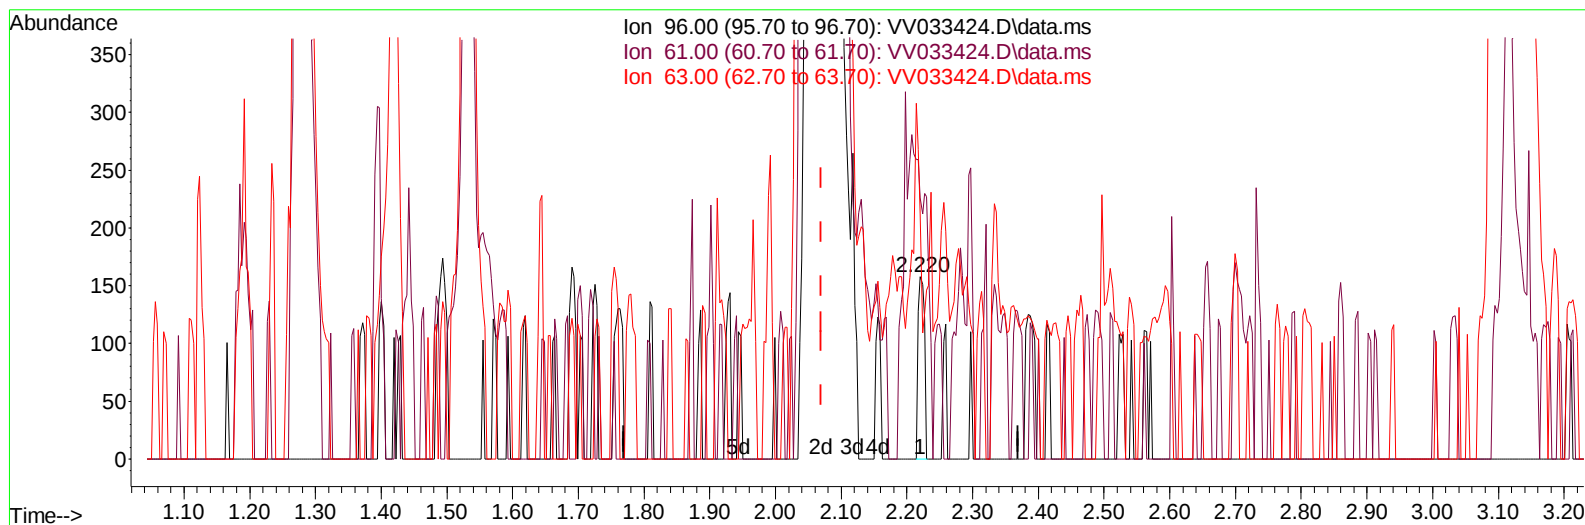

(12) 1,1-Dichloroethene (T)

2.220min (+ 0.151) 0.07 ug/L

response 108

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	177.50	143.04
63.00	154.40	134.18
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033424.D
 Acq On : 16 Dec 2023 11:02
 Operator : SY/MD
 Sample : 05846-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:26:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

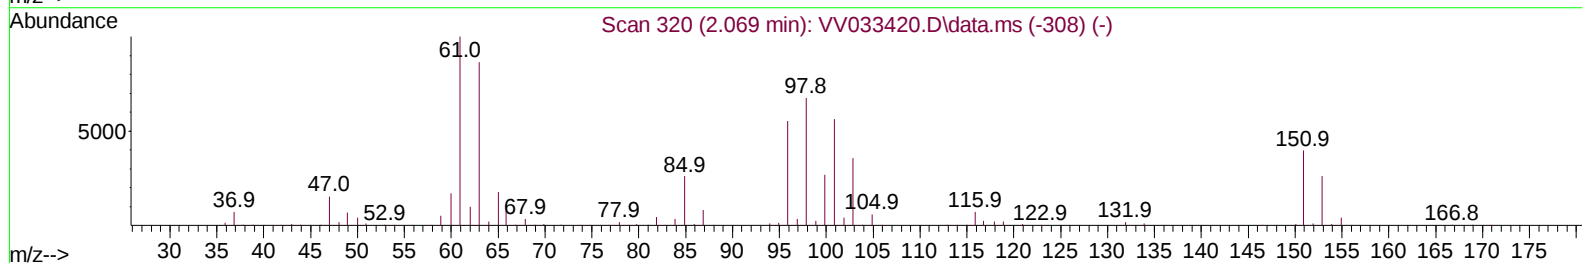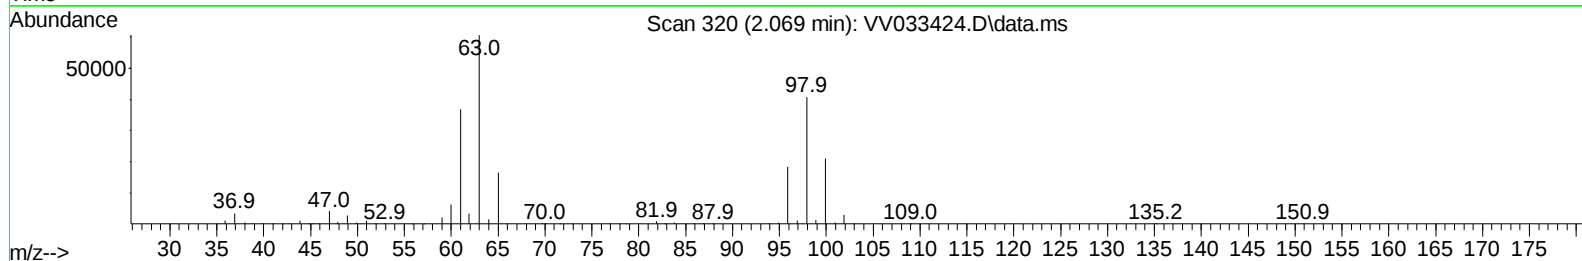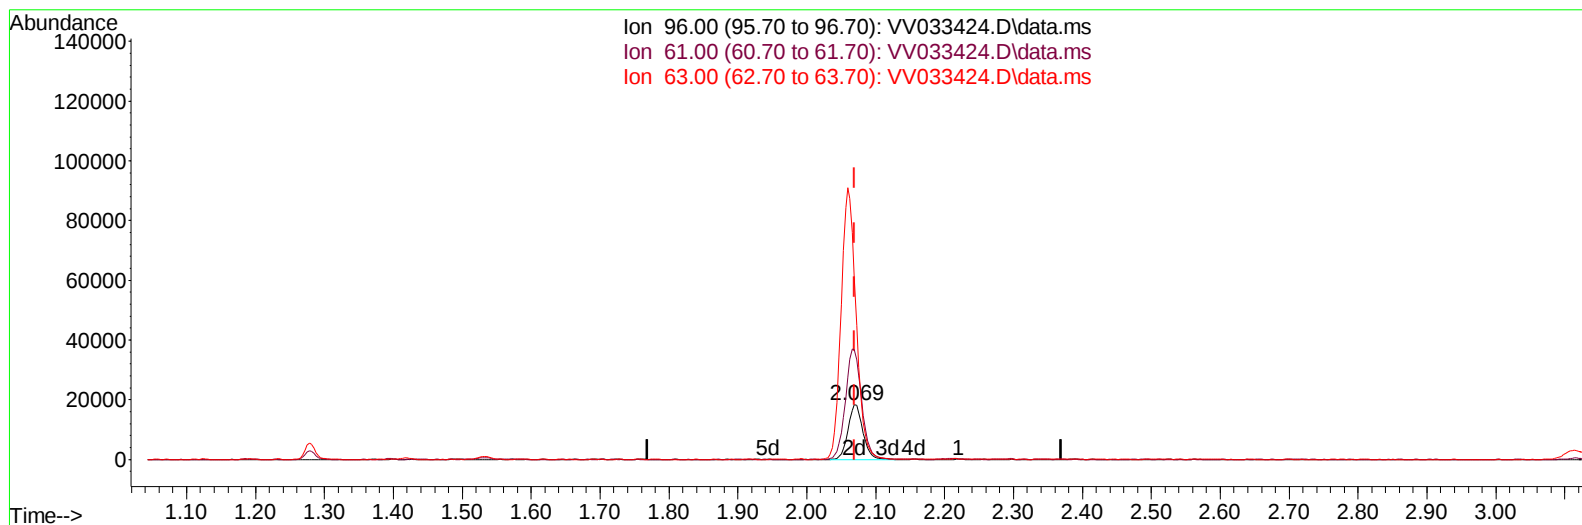

TIC: VV033424.D\data.ms

(12) 1,1-Dichloroethene (T)

2.069min (-0.000) 17.26 ug/L m

response 27289

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	177.50	200.09
63.00	154.40	330.13#
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033424.D
 Acq On : 16 Dec 2023 11:02
 Operator : SY/MD
 Sample : 05846-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:26:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

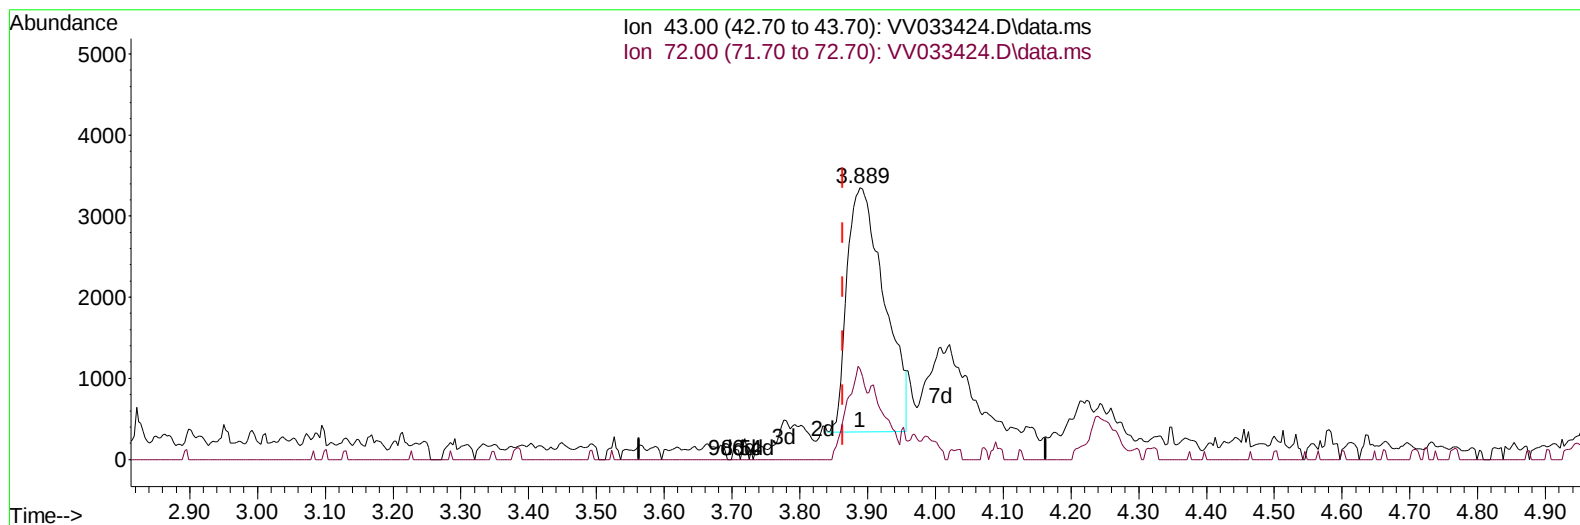




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033424.D
 Acq On : 16 Dec 2023 11:02
 Operator : SY/MD
 Sample : 05846-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:26:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

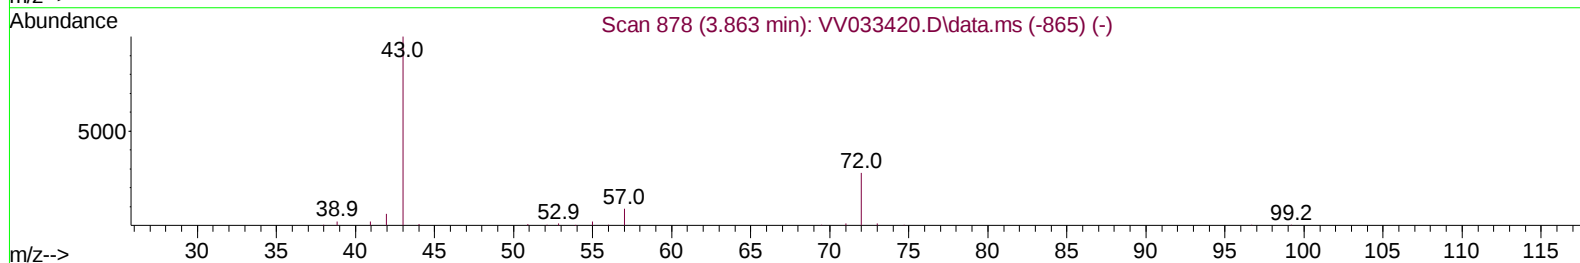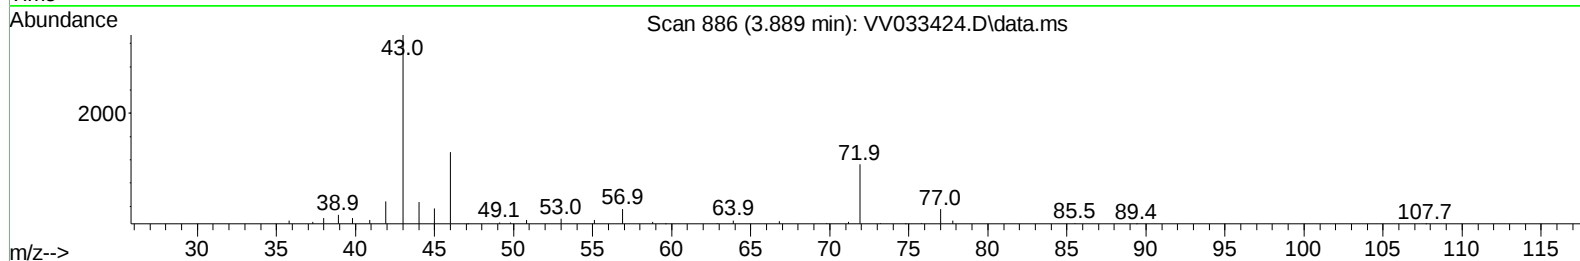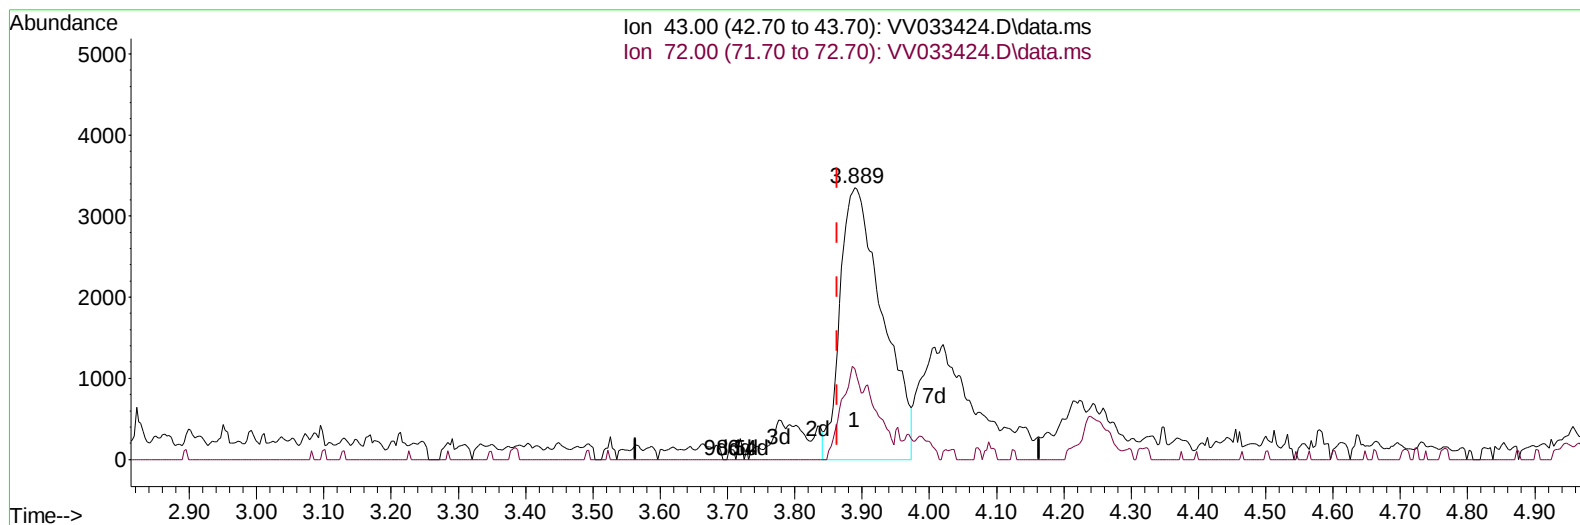

TIC: VV033424.D\data.ms

(22) 2-Butanone (T)

3.889min (+ 0.026) 14.70 ug/L m

response 14635

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.90	14.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033424.D
 Acq On : 16 Dec 2023 11:02
 Operator : SY/MD
 Sample : 05846-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:26:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	224331	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	233236	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	99643	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	80769	46.753	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	93.500%	
7) Chloroethane-d5	1.532	69	73388	47.337	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	94.680%	
11) 1,1-Dichloroethene-d2	2.060	65	38954	45.297	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	90.600%	
21) 2-Butanone-d5	3.783	46	88305	101.422	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	101.420%	
24) Chloroform-d	4.249	84	162689	47.608	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.220%	
26) 1,2-Dichloroethane-d4	4.940	65	107573	51.244	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.480%	
32) Benzene-d6	4.960	84	305112	48.571	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.140%	
36) 1,2-Dichloropropane-d6	5.989	67	94704	49.674	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	99.340%	
41) Toluene-d8	7.243	98	260047	45.242	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.480%	
43) trans-1,3-Dichloroprop...	7.551	79	40968	43.846	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.700%	
47) 2-Hexanone-d5	8.024	63	56462	88.049	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	88.050%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	129506	47.262	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.520%	
66) 1,2-Dichlorobenzene-d4	11.561	152	104308	55.707	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	111.420%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.069	96	27289m	17.262	ug/L	
13) Acetone	2.108	43	144350	142.829	ug/L	99
19) 1,1-Dichloroethane	3.114	63	7339	2.563	ug/L	96
22) 2-Butanone	3.889	43	14635m	14.698	ug/L	
30) 1,1,1-Trichloroethane	4.513	97	9347	3.246	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033424.D
Acq On : 16 Dec 2023 11:02
Operator : SY/MD
Sample : 05846-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHJ3

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:26:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

