




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033439.D
Acq On : 16 Dec 2023 16:50
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

Quant Time: Dec 16 20:29:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

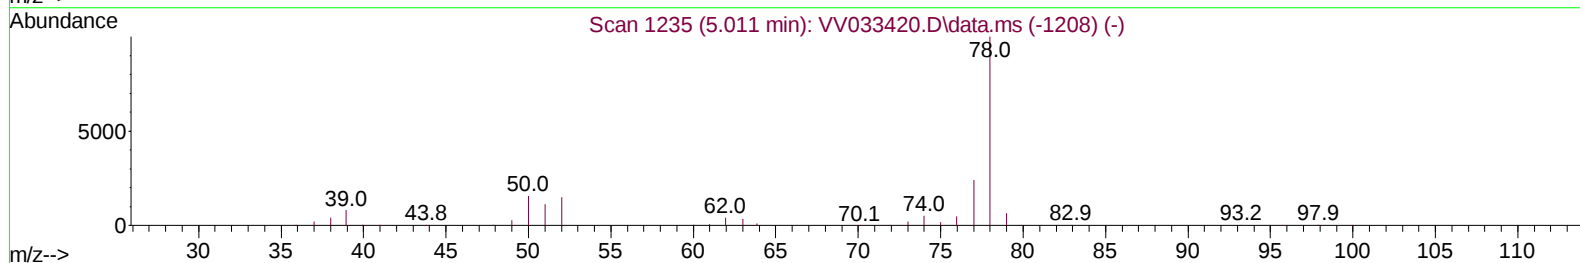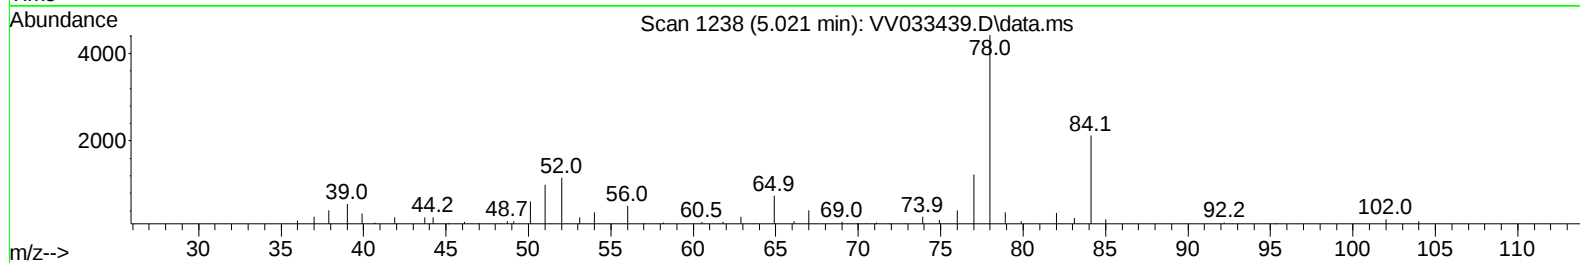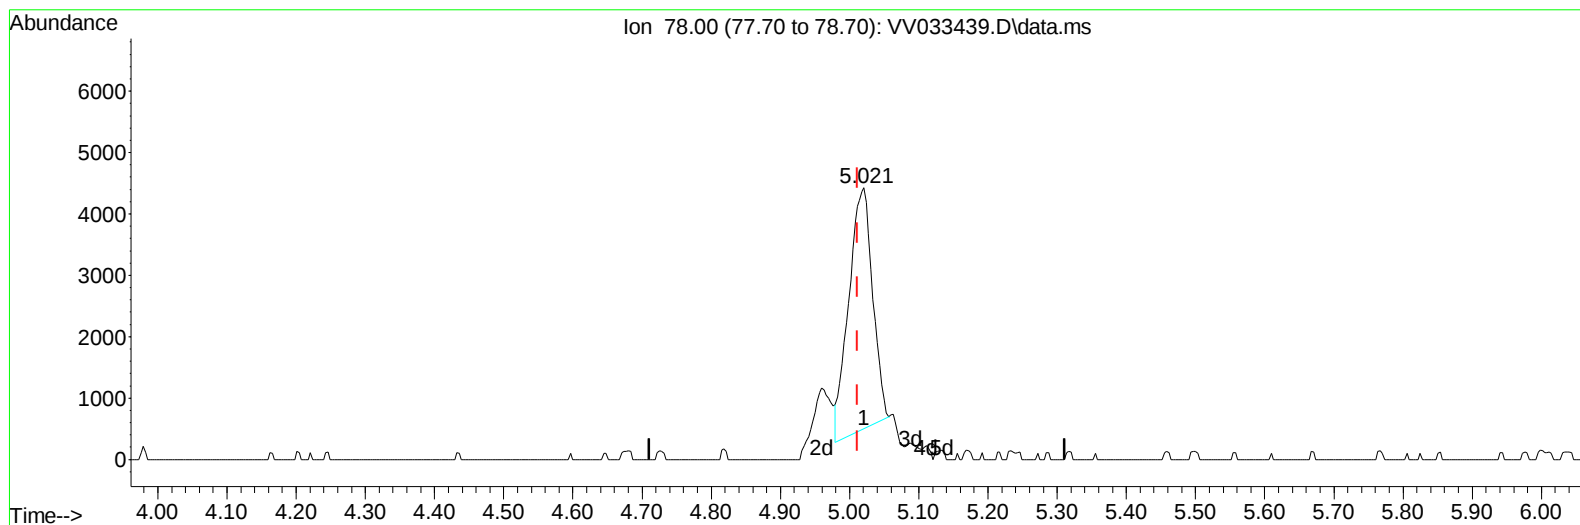

TIC: VV033439.D\data.ms

(33) Benzene (T)

5.021min (+ 0.010) 1.55 ug/L

response 9475

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033439.D
Acq On : 16 Dec 2023 16:50
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:29:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

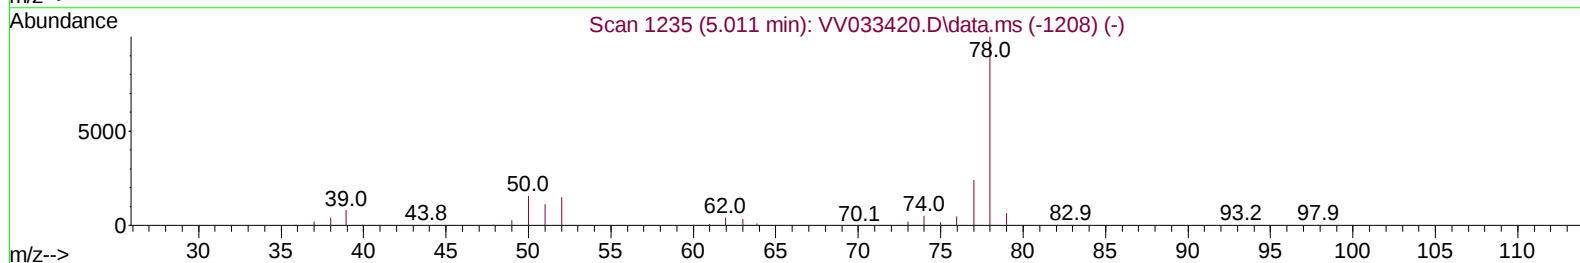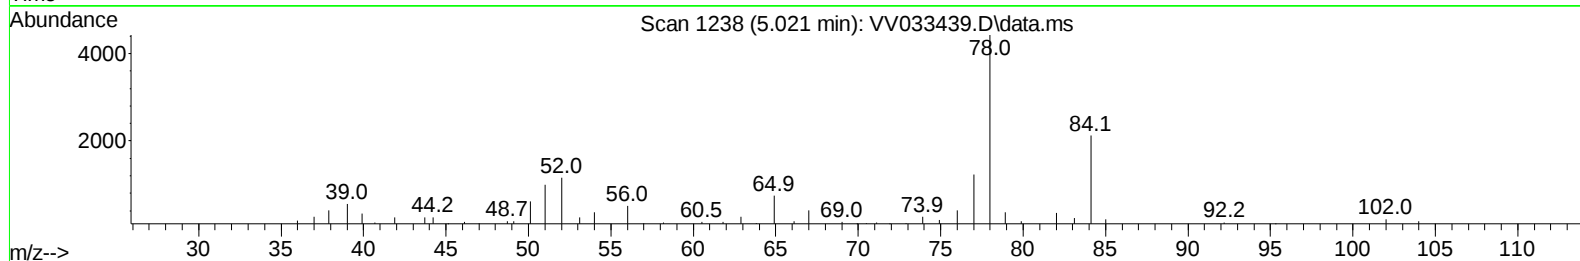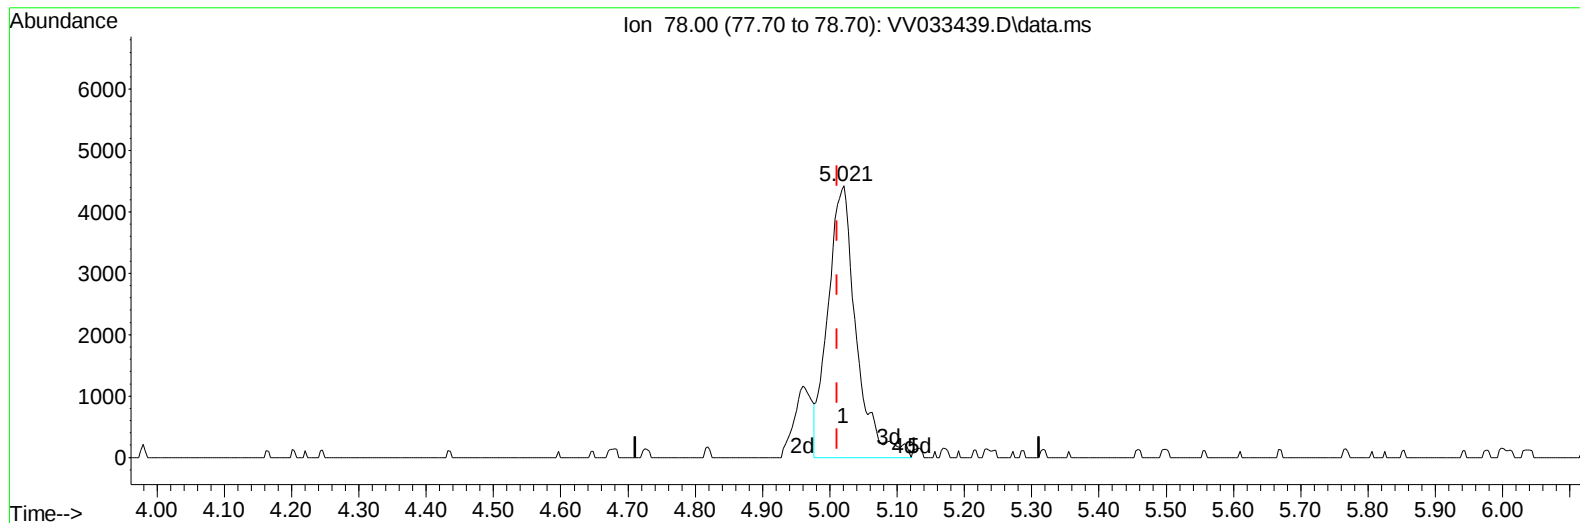

TIC: VV033439.D\data.ms

(33) Benzene (T)

5.021min (+ 0.010) 2.13 ug/L m

response 12978

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033439.D
 Acq On : 16 Dec 2023 16:50
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:29:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

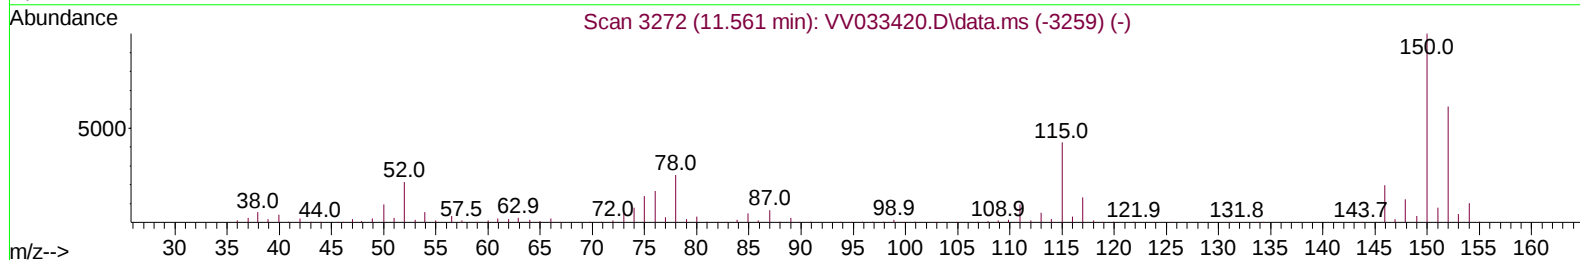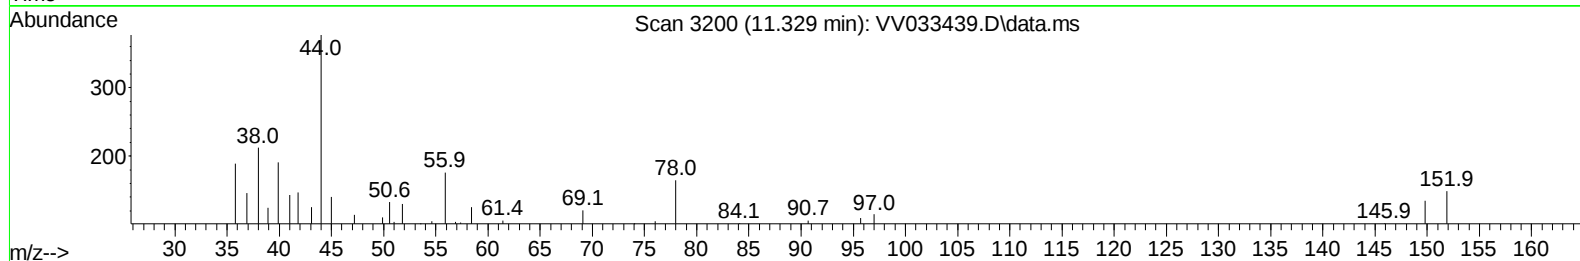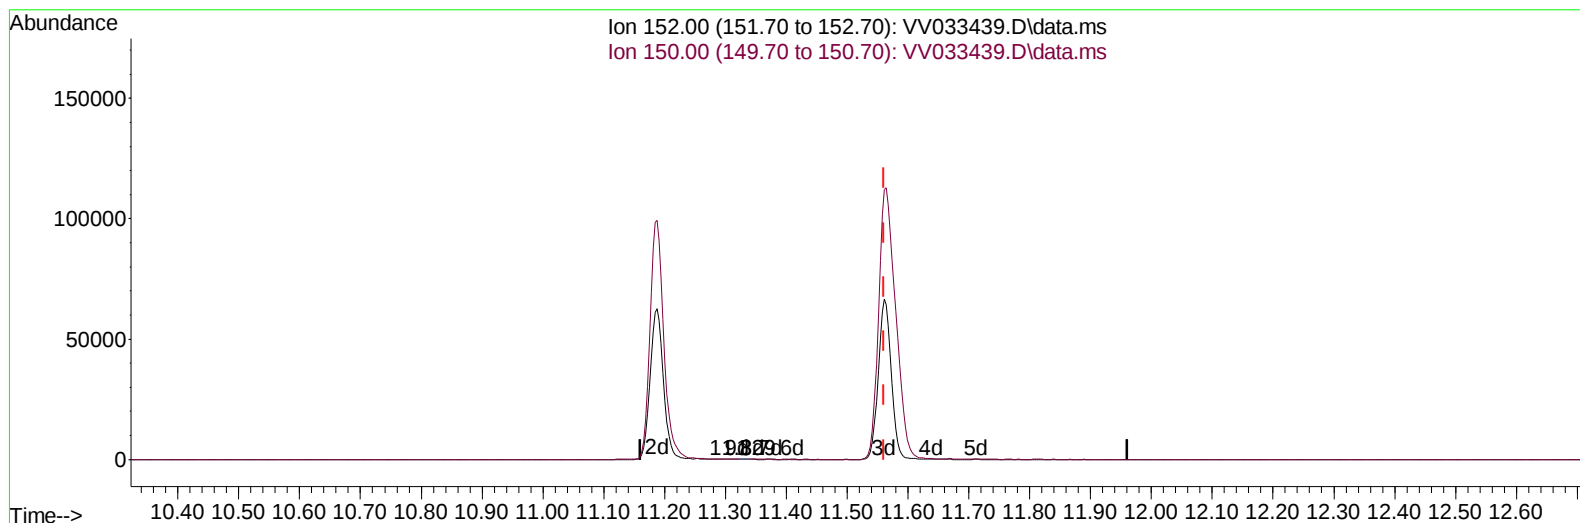

TIC: VV033439.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.329min (-0.231) 0.03 ug/L

response 59

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	171.50	120.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033439.D
 Acq On : 16 Dec 2023 16:50
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:29:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

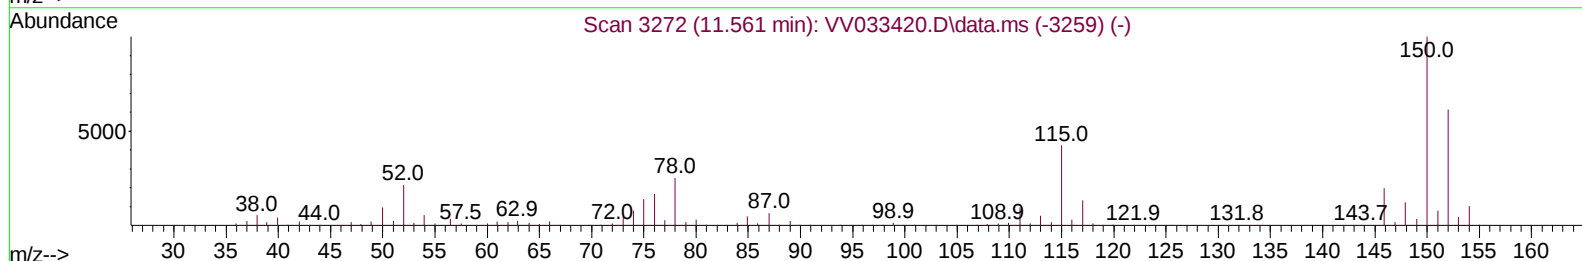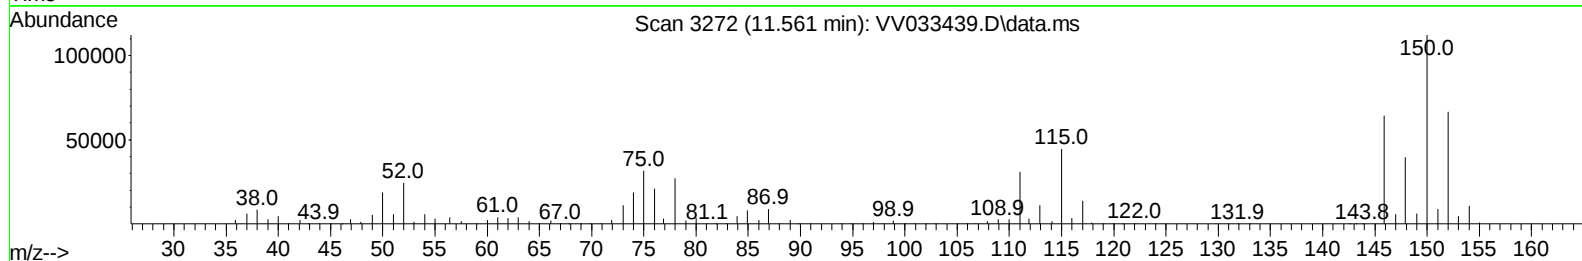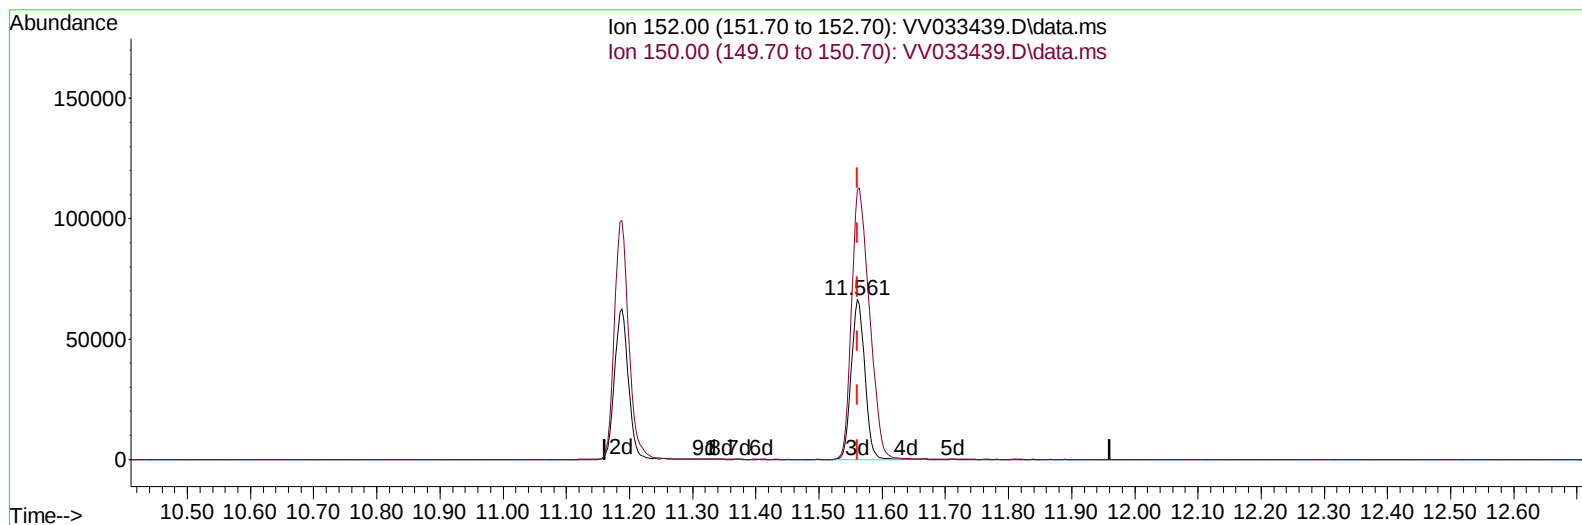

TIC: VV033439.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.561min (+ 0.000) 54.96 ug/L m

response 98921

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	171.50	0.07#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033439.D
 Acq On : 16 Dec 2023 16:50
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:29:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	214681	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	228837	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	95780	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	67133	40.607	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	81.220%	
7) Chloroethane-d5	1.532	69	64399	43.406	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	86.820%	
11) 1,1-Dichloroethene-d2	2.060	65	33645	40.882	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.760%	
21) 2-Butanone-d5	3.783	46	75764	90.930	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	90.930%	
24) Chloroform-d	4.249	84	150850	46.128	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.260%	
26) 1,2-Dichloroethane-d4	4.944	65	97607	48.586	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.180%	
32) Benzene-d6	4.960	84	273172	44.322	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.640%	
36) 1,2-Dichloropropane-d6	5.989	67	85398	45.654	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	91.300%	
41) Toluene-d8	7.246	98	225898	40.056	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	80.120%	
43) trans-1,3-Dichloroprop...	7.555	79	38479	41.974	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	83.940%	
47) 2-Hexanone-d5	8.024	63	55701	88.532	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	88.530%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	123659	45.996	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	92.000%	
66) 1,2-Dichlorobenzene-d4	11.561	152	98921m	54.960	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	109.920%	
Target Compounds						
					Qvalue	
33) Benzene	5.021	78	12978m	2.128	ug/L	
51) Chlorobenzene	8.815	112	138184	29.660	ug/L	99
64) 1,3-Dichlorobenzene	11.127	146	2445	0.865	ug/L	96
65) 1,4-Dichlorobenzene	11.210	146	56301	18.505	ug/L	98
67) 1,2-Dichlorobenzene	11.580	146	616505	209.533	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033439.D
Acq On : 16 Dec 2023 16:50
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Manual IntegrationsAPPROVED

Quant Time: Dec 16 20:29:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

