

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033414.D
 Acq On : 16 Dec 2023 06:01
 Operator : SY/MD
 Sample : 05802-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B29

Quant Time: Dec 16 06:46:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 01:35:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	227635	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	236223	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	101211	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	76455	43.614	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.220%
7) Chloroethane-d5	1.529	69	71831	45.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.320%
11) 1,1-Dichloroethene-d2	2.060	65	37736	43.244	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.480%
21) 2-Butanone-d5	3.783	46	83321	94.309	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.310%
24) Chloroform-d	4.249	84	159209	45.913	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.820%
26) 1,2-Dichloroethane-d4	4.940	65	104487	49.051	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.100%
32) Benzene-d6	4.960	84	293440	46.122	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.240%
36) 1,2-Dichloropropane-d6	5.989	67	92914	48.119	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.240%
41) Toluene-d8	7.243	98	253079	43.473	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.940%
43) trans-1,3-Dichloroprop...	7.551	79	40025	42.295	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.600%
47) 2-Hexanone-d5	8.024	63	54426	83.801	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.800%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	124888	45.000	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	101324	53.275	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.540%
Target Compounds						
12) 1,1-Dichloroethene	2.069	96	65285	40.698	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033414.D
Acq On : 16 Dec 2023 06:01
Operator : SY/MD
Sample : 05802-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B29


Quant Time: Dec 16 06:46:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 01:35:53 2023
Response via : Initial Calibration

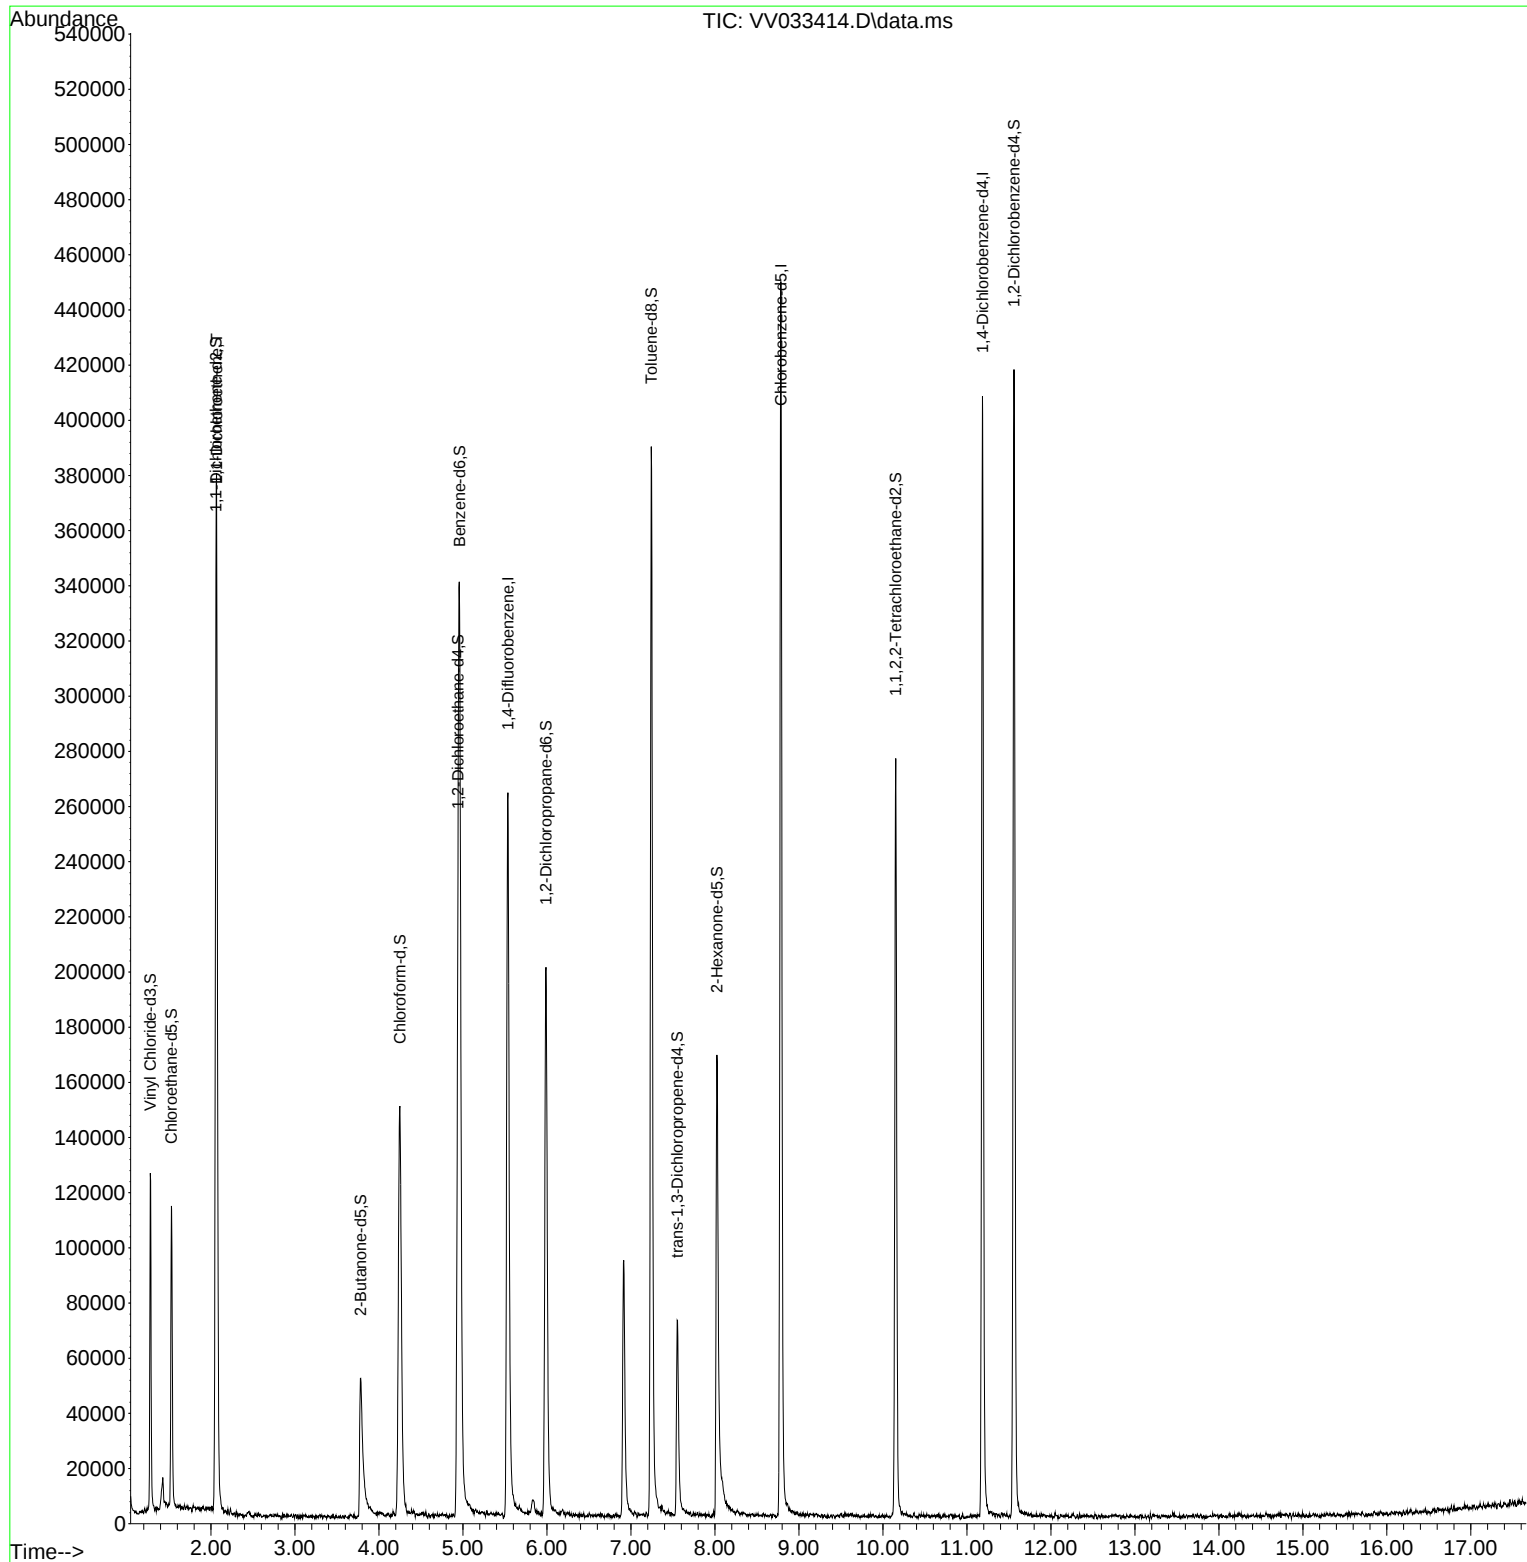

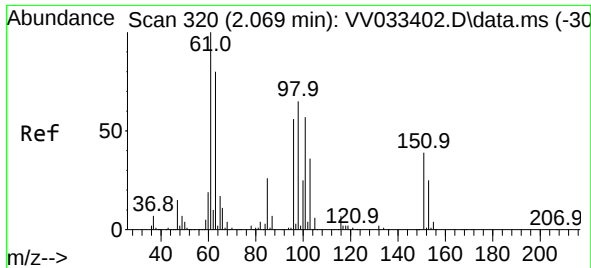

#12
 1,1-Dichloroethene
 Concen: 40.698 ug/L
 RT: 2.069 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV033414.D
 Acq: 16 Dec 2023 06:01

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B29

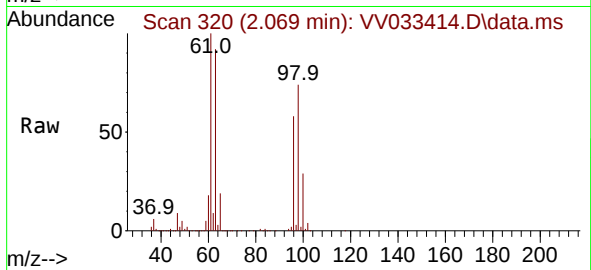

Tgt Ion:	96	Resp:	65285
Ion	Ratio	Lower	Upper
96	100		
61	171.7	124.3	230.8
63	158.6	108.1	200.7

