

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033432.D
 Acq On : 16 Dec 2023 14:06
 Operator : SY/MD
 Sample : 05846-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD2

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

Quant Time: Dec 16 20:28:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 16 20:24:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	217415	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	225437	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	95090	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	72161	43.099	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.200%		
7) Chloroethane-d5	1.532	69	67846	45.154	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.300%		
11) 1,1-Dichloroethene-d2	2.060	65	36243	43.485	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.980%		
21) 2-Butanone-d5	3.783	46	88628	105.031	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	105.030%		
24) Chloroform-d	4.249	84	154372	46.611	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.220%		
26) 1,2-Dichloroethane-d4	4.941	65	100327	49.312	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.620%		
32) Benzene-d6	4.960	84	283629	46.713	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.420%		
36) 1,2-Dichloropropane-d6	5.989	67	90601	49.166	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.340%		
41) Toluene-d8	7.246	98	240832	43.348	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.700%		
43) trans-1,3-Dichloroprop...	7.555	79	38807	42.970	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.940%		
47) 2-Hexanone-d5	8.024	63	56531	91.207	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.210%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	125848	47.516	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.040%		
66) 1,2-Dichlorobenzene-d4	11.561	152	97243	54.420	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.840%		
Target Compounds					Qvalue	
13) Acetone	2.111	43	71880	73.385	ug/L	99
19) 1,1-Dichloroethane	3.118	63	3430	1.236	ug/L	98
20) cis-1,2-Dichloroethene	3.825	96	2801m	1.706	ug/L	
22) 2-Butanone	3.873	43	42329	43.864	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033432.D
Acq On : 16 Dec 2023 14:06
Operator : SY/MD
Sample : 05846-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 63 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
YCHD2

Quant Time: Dec 16 20:28:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 16 20:24:09 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

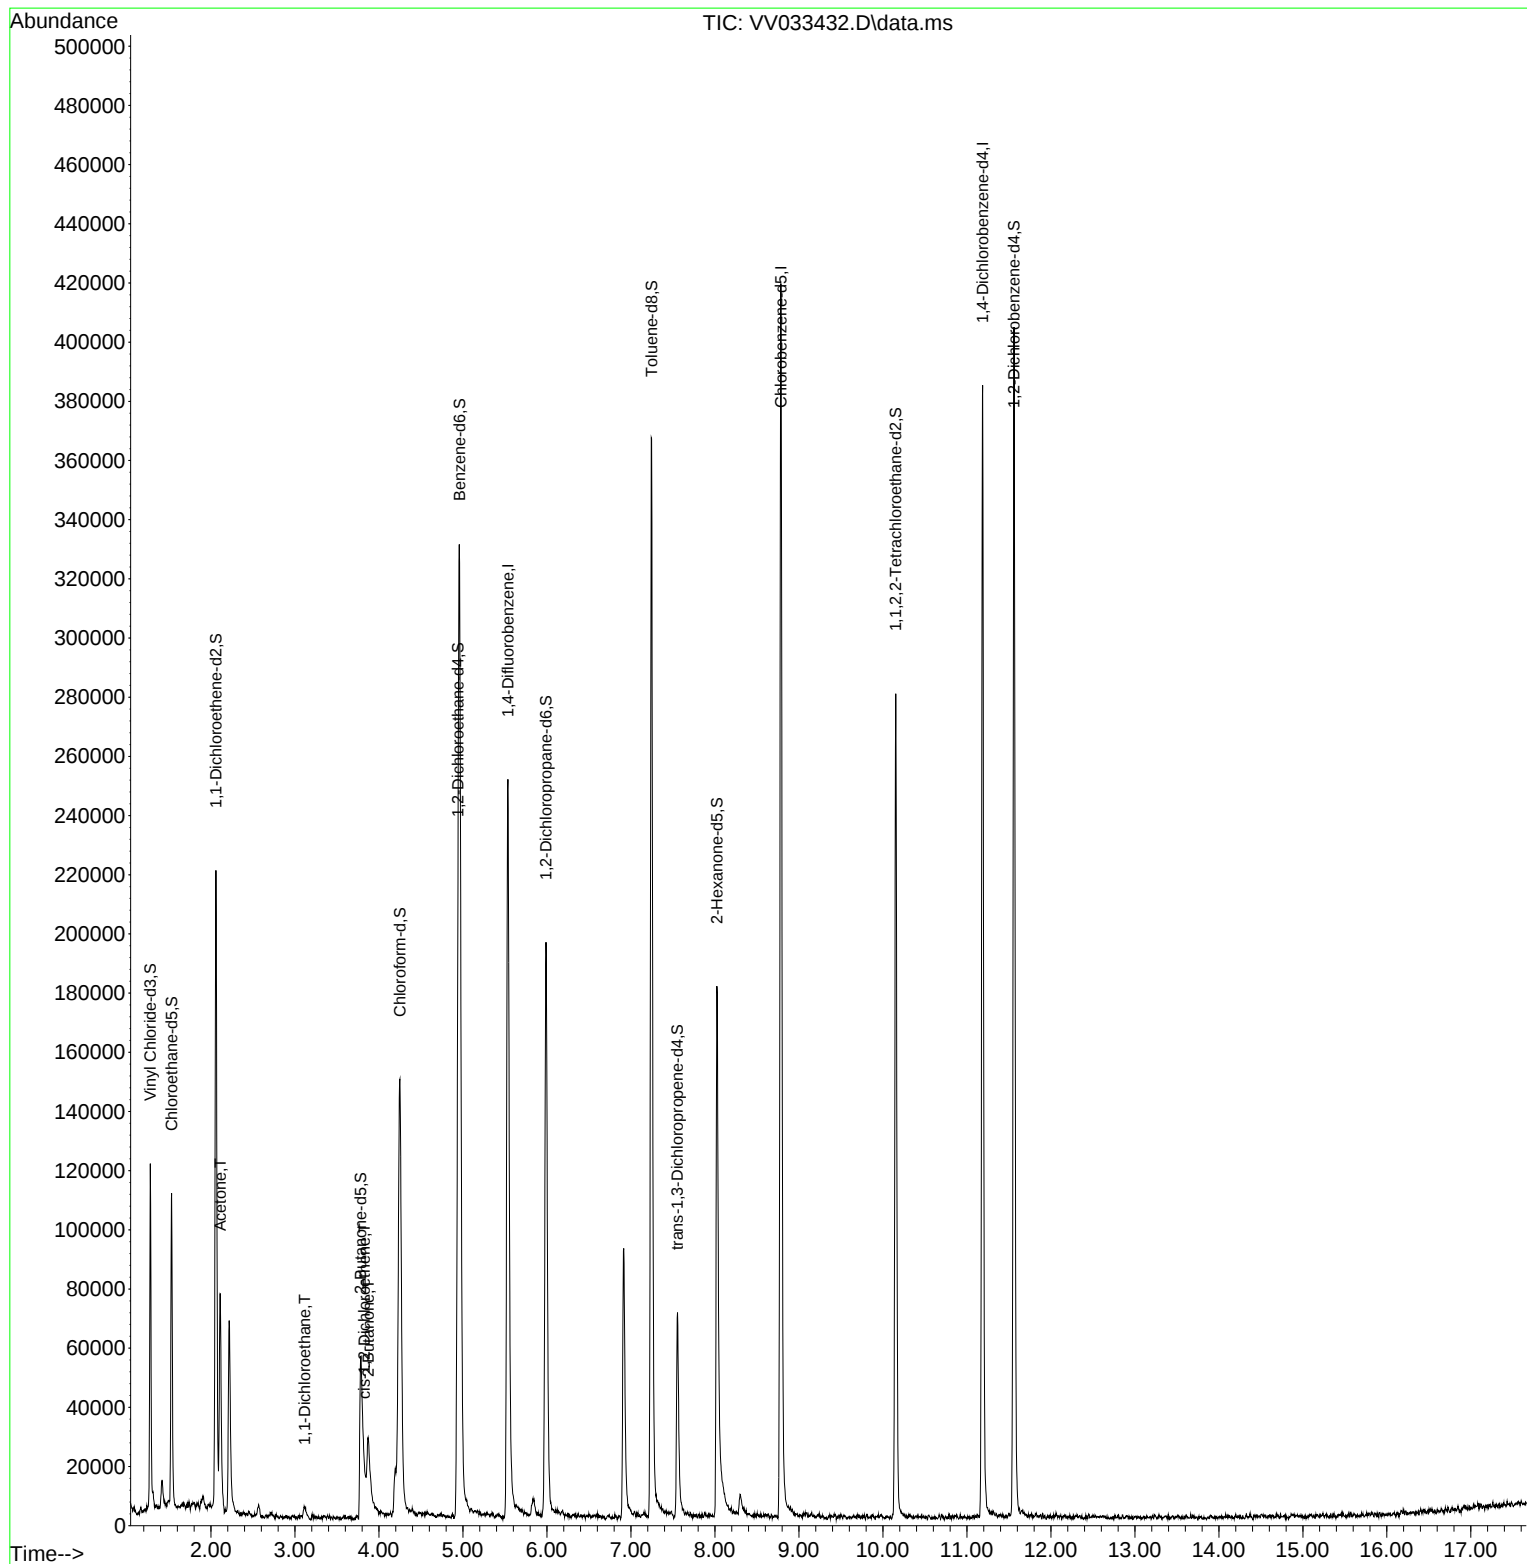

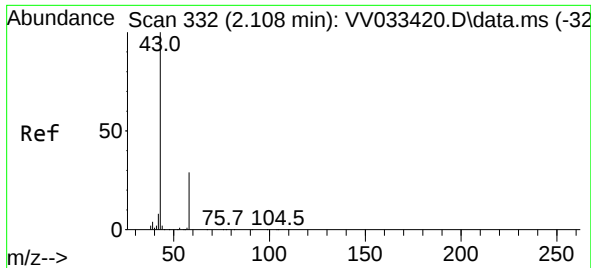

#13

Acetone

Concen: 73.385 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV033432.D

Acq: 16 Dec 2023 14:06

Instrument :

MSVOA_V

ClientSampleId :

YCHD2

Tgt Ion: 43 Resp: 71880

Ion Ratio Lower Upper

43 100





58 30.0 0.0 59.2

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023

Supervised By :Semsettin Yesilyurt 12/18/2023

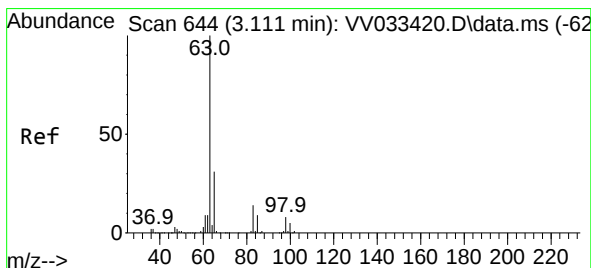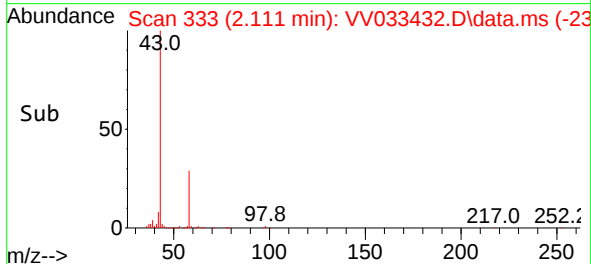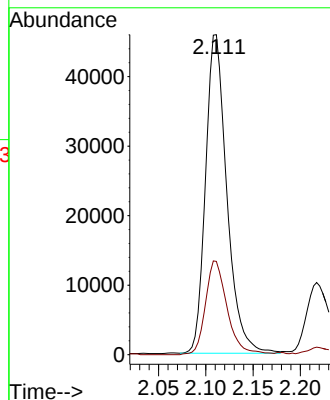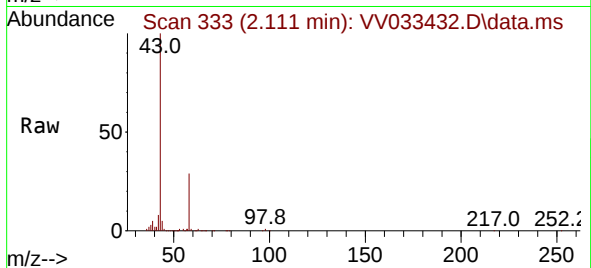

#19

1,1-Dichloroethane

Concen: 1.236 ug/L

RT: 3.118 min Scan# 646

Delta R.T. 0.007 min

Lab File: VV033432.D

Acq: 16 Dec 2023 14:06




Tgt Ion: 63 Resp: 3430


Ion Ratio Lower Upper

63 100

65 30.4 21.1 39.3

83 11.8 9.7 17.9

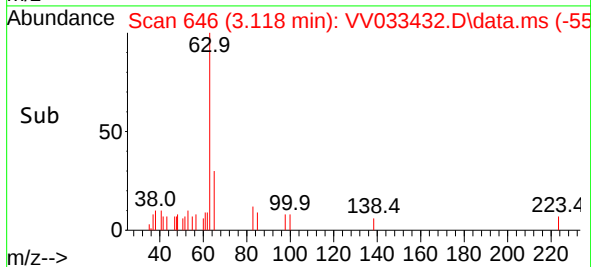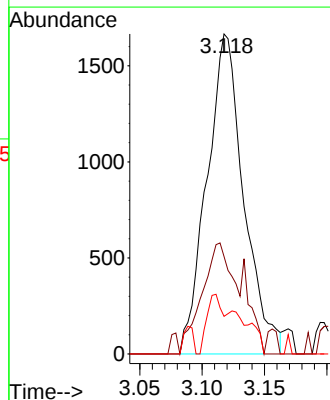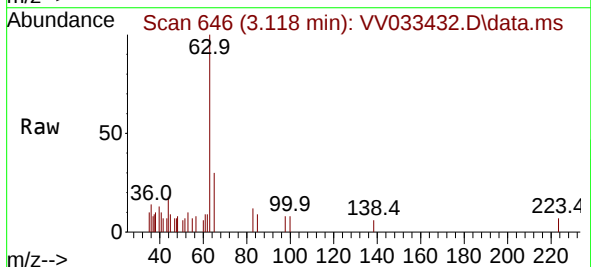

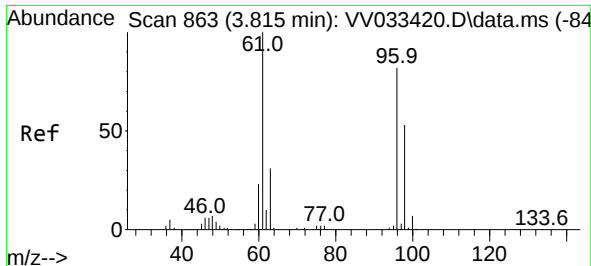





#20
cis-1,2-Dichloroethene
Concen: 1.706 ug/L m
RT: 3.825 min Scan# 80
Delta R.T. 0.010 min
Lab File: VV033432.D
Acq: 16 Dec 2023 14:06

Instrument :
MSVOA_V
ClientSampleId :
YCHD2

Tgt Ion: 96 Resp: 280
Ion Ratio Lower Upper
96 100
61 112.7 81.9 152.1
98 57.6 44.3 82.3

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

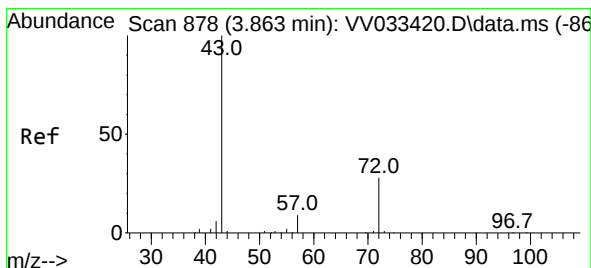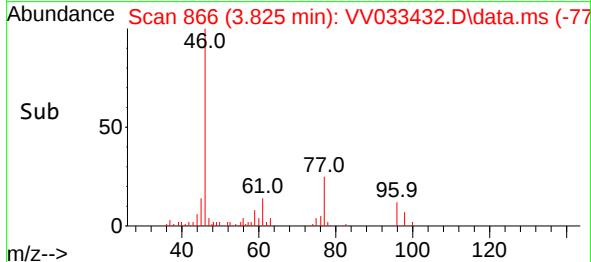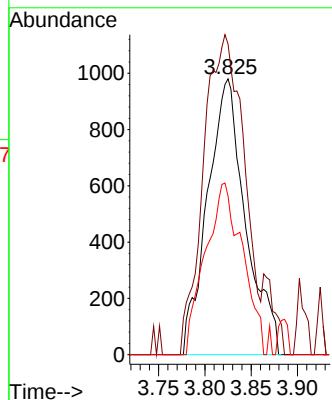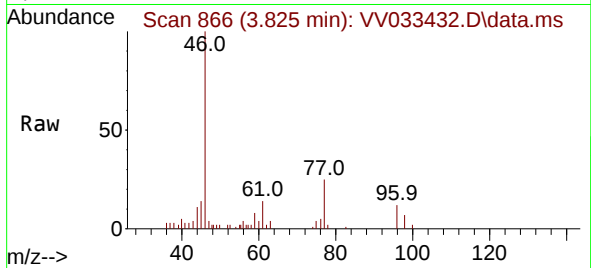

#22
2-Butanone
Concen: 43.864 ug/L
RT: 3.873 min Scan# 881
Delta R.T. 0.010 min
Lab File: VV033432.D
Acq: 16 Dec 2023 14:06

Tgt Ion: 43 Resp: 42329
Ion Ratio Lower Upper
43 100
72 23.7 12.4 37.4

