

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033381.D
 Acq On : 15 Dec 2023 16:49
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	138288	145579	15.19%	2.015%
2	1.532	146	153	168	rVB	127654	147831	15.42%	2.046%
3	2.060	308	317	337	rVB	256760	372135	38.82%	5.151%
4	2.429	429	432	434	rBV4	1350	904	0.09%	0.013%
5	2.706	514	518	521	rBV6	1427	1268	0.13%	0.018%
6	2.809	546	550	554	rBV7	898	854	0.09%	0.012%
7	2.854	562	564	566	rBV3	966	550	0.06%	0.008%
8	2.973	596	601	604	rBV4	1392	1242	0.13%	0.017%
9	3.008	610	612	617	rVB5	819	595	0.06%	0.008%
10	3.047	621	624	626	rVB3	1502	903	0.09%	0.012%
11	3.092	634	638	642	rBV7	1485	1485	0.15%	0.021%
12	3.195	666	670	671	rVB4	963	546	0.06%	0.008%
13	3.320	707	709	712	rVB4	1456	779	0.08%	0.011%
14	3.359	716	721	722	rBV4	1121	714	0.07%	0.010%
15	3.455	747	751	754	rBV4	764	565	0.06%	0.008%
16	3.587	789	792	795	rVB5	1378	897	0.09%	0.012%
17	3.610	795	799	801	rBV5	1249	813	0.08%	0.011%
18	3.693	824	825	831	rVB5	851	620	0.06%	0.009%
19	3.783	841	853	882	rBV	56504	165706	17.29%	2.294%
20	4.108	951	954	958	rBV4	1160	1078	0.11%	0.015%
21	4.249	984	998	1027	rVB	157794	398925	41.62%	5.522%
22	4.757	1155	1156	1160	rBV4	1119	537	0.06%	0.007%
23	4.812	1170	1173	1179	rVB5	1918	1577	0.16%	0.022%
24	4.844	1179	1183	1184	rBV5	820	602	0.06%	0.008%
25	4.957	1202	1218	1243	rBV3	360360	958514	100.00%	13.268%
26	5.310	1325	1328	1331	rBV5	1348	1241	0.13%	0.017%
27	5.535	1385	1398	1419	rBV	270756	565459	58.99%	7.827%
28	5.989	1527	1539	1555	rBV	209517	429863	44.85%	5.950%
29	6.191	1599	1602	1606	rBV6	1617	1362	0.14%	0.019%
30	6.269	1624	1626	1629	rBV4	1334	754	0.08%	0.010%
31	6.497	1695	1697	1701	rVB5	1510	1033	0.11%	0.014%
32	6.590	1725	1726	1731	rBV5	959	648	0.07%	0.009%
33	6.616	1731	1734	1735	rBV3	864	523	0.05%	0.007%
34	6.651	1742	1745	1748	rBV4	829	767	0.08%	0.011%
35	6.719	1763	1766	1770	rBV7	1785	1589	0.17%	0.022%
36	6.912	1816	1826	1845	rBV	108415	202821	21.16%	2.808%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033381.D
 Acq On : 15 Dec 2023 16:49
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.159	1902	1903	1906	rBV3	838	599	0.06%	0.008%
38	7.243	1918	1929	1952	rBV	426368	742208	77.43%	10.274%
39	7.551	2017	2025	2042	rBV	76956	136583	14.25%	1.891%
40	7.899	2131	2133	2137	rBV5	1313	939	0.10%	0.013%
41	8.024	2163	2172	2199	rBV	191514	361939	37.76%	5.010%
42	8.654	2365	2368	2369	rBV2	1442	676	0.07%	0.009%
43	8.699	2379	2382	2389	rBV7	1895	1855	0.19%	0.026%
44	8.728	2389	2391	2396	rBV6	1538	1198	0.12%	0.017%
45	8.783	2396	2408	2437	rBV	430856	724772	75.61%	10.033%
46	9.130	2514	2516	2520	rBV5	1417	983	0.10%	0.014%
47	9.320	2573	2575	2578	rBV4	1425	1005	0.10%	0.014%
48	9.368	2584	2590	2594	rBV7	1847	2315	0.24%	0.032%
49	9.612	2663	2666	2668	rVB4	1163	647	0.07%	0.009%
50	9.719	2696	2699	2703	rBV5	1263	1154	0.12%	0.016%
51	10.153	2817	2834	2849	rBV	288023	463885	48.40%	6.421%
52	10.342	2890	2893	2898	rBV6	1018	1058	0.11%	0.015%
53	10.371	2900	2902	2904	rBV3	989	562	0.06%	0.008%
54	10.654	2987	2990	2992	rBV4	1905	1123	0.12%	0.016%
55	10.767	3020	3025	3027	rBV8	1303	1075	0.11%	0.015%
56	10.879	3058	3060	3063	rVB3	1760	835	0.09%	0.012%
57	11.059	3115	3116	3119	rBV4	960	595	0.06%	0.008%
58	11.111	3130	3132	3134	rBV2	1324	712	0.07%	0.010%
59	11.185	3145	3155	3180	rVB	391387	620049	64.69%	8.583%
60	11.349	3202	3206	3209	rBV6	1678	1626	0.17%	0.023%
61	11.432	3229	3232	3233	rBV3	1023	706	0.07%	0.010%
62	11.561	3259	3272	3295	rBV	426047	685858	71.55%	9.494%
63	11.722	3319	3322	3324	rBV4	1315	790	0.08%	0.011%
64	12.011	3409	3412	3415	rBV5	686	558	0.06%	0.008%
65	12.117	3442	3445	3448	rBV5	1514	1010	0.11%	0.014%
66	12.188	3464	3467	3472	rBV6	1254	1275	0.13%	0.018%
67	12.458	3549	3551	3556	rBV6	1127	1097	0.11%	0.015%
68	12.577	3584	3588	3589	rBV4	1742	1232	0.13%	0.017%
69	12.638	3604	3607	3610	rVB3	955	601	0.06%	0.008%
70	12.738	3637	3638	3644	rVB6	778	691	0.07%	0.010%
71	12.927	3694	3697	3700	rVV5	1323	898	0.09%	0.012%
72	12.989	3714	3716	3721	rBV5	1174	912	0.10%	0.013%
73	13.098	3748	3750	3753	rVB4	1622	918	0.10%	0.013%
74	13.120	3753	3757	3759	rBV4	1570	1122	0.12%	0.016%
75	13.169	3771	3772	3775	rVV2	951	573	0.06%	0.008%
76	13.204	3778	3783	3792	rVV8	4342	6911	0.72%	0.096%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033381.D
 Acq On : 15 Dec 2023 16:49
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.371	3831	3835	3839	rBV6	993	1029	0.11%	0.014%
78	13.445	3852	3858	3866	rBV	9882	15138	1.58%	0.210%
79	13.590	3901	3903	3908	rBV4	1695	1196	0.12%	0.017%
80	13.673	3925	3929	3930	rBV3	3977	2346	0.24%	0.032%
81	13.735	3946	3948	3954	rVB5	1339	1081	0.11%	0.015%
82	13.767	3954	3958	3961	rBV6	846	745	0.08%	0.010%
83	13.796	3961	3967	3968	rBV4	776	780	0.08%	0.011%
84	13.818	3972	3974	3976	rBV3	1034	609	0.06%	0.008%
85	13.870	3987	3990	3992	rBV4	1227	797	0.08%	0.011%
86	13.947	4012	4014	4017	rVB4	1112	526	0.05%	0.007%
87	13.989	4023	4027	4030	rBV5	1284	1032	0.11%	0.014%
88	14.239	4101	4105	4107	rVV4	1382	1129	0.12%	0.016%
89	14.252	4107	4109	4111	rVV2	1540	576	0.06%	0.008%
90	14.390	4150	4152	4158	rVB6	1664	1483	0.15%	0.021%
91	14.551	4199	4202	4204	rBV2	1397	816	0.09%	0.011%
92	14.599	4213	4217	4219	rBV5	1029	930	0.10%	0.013%
93	14.751	4261	4264	4268	rBV4	2008	1437	0.15%	0.020%
94	14.911	4312	4314	4317	rBV4	1163	812	0.08%	0.011%
95	15.072	4362	4364	4372	rVB6	1745	1686	0.18%	0.023%
96	15.236	4413	4415	4418	rBV4	1738	1257	0.13%	0.017%
97	15.316	4437	4440	4441	rBV2	1238	759	0.08%	0.011%
98	15.461	4482	4485	4486	rBV3	1161	821	0.09%	0.011%
99	15.934	4629	4632	4635	rBV5	1205	943	0.10%	0.013%
100	16.117	4687	4689	4693	rBV5	1734	1405	0.15%	0.019%




Sum of corrected areas: 7224157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033381.D
Acq On : 15 Dec 2023 16:49
Operator : SY/MD
Sample : VV1215WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

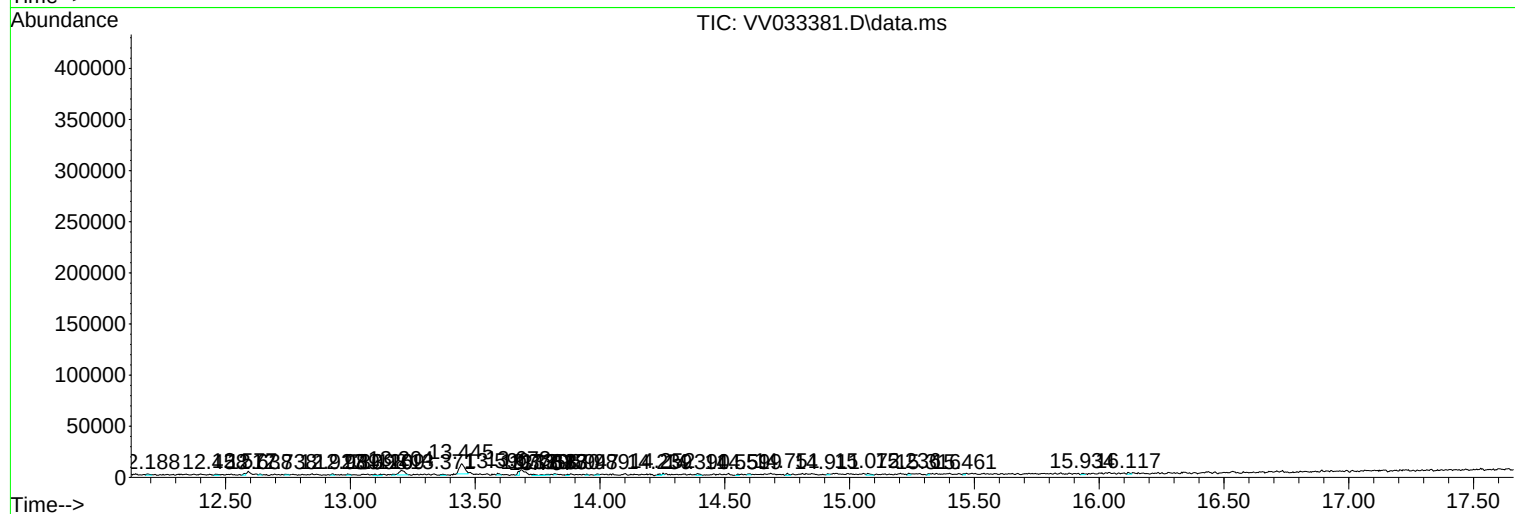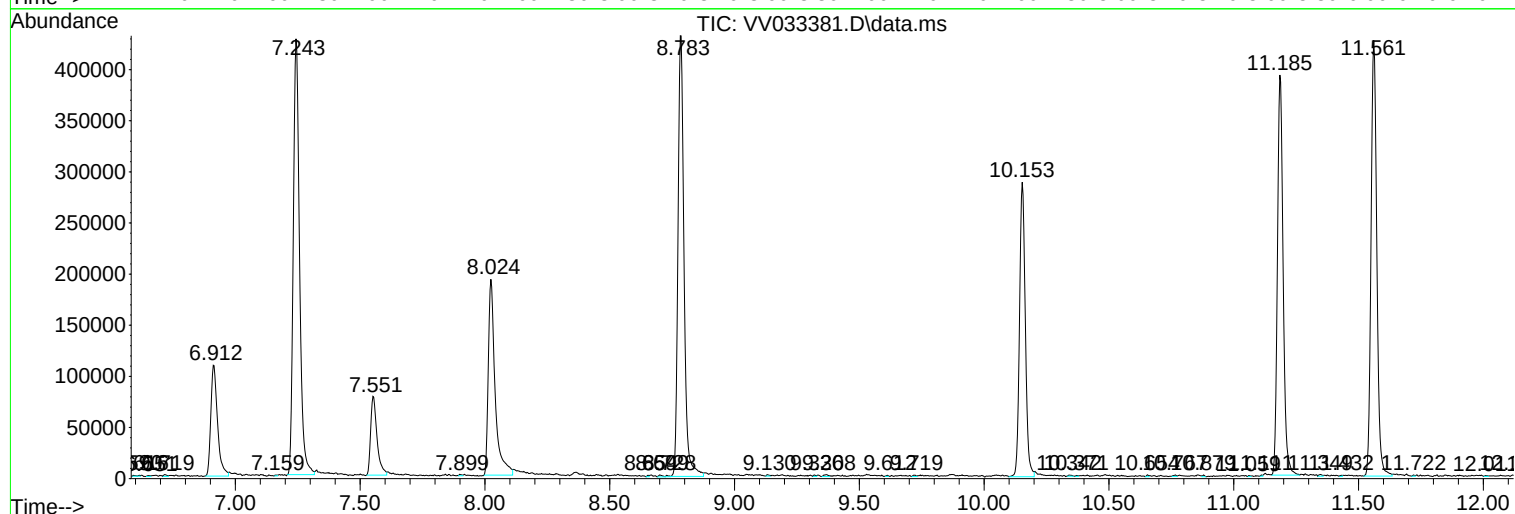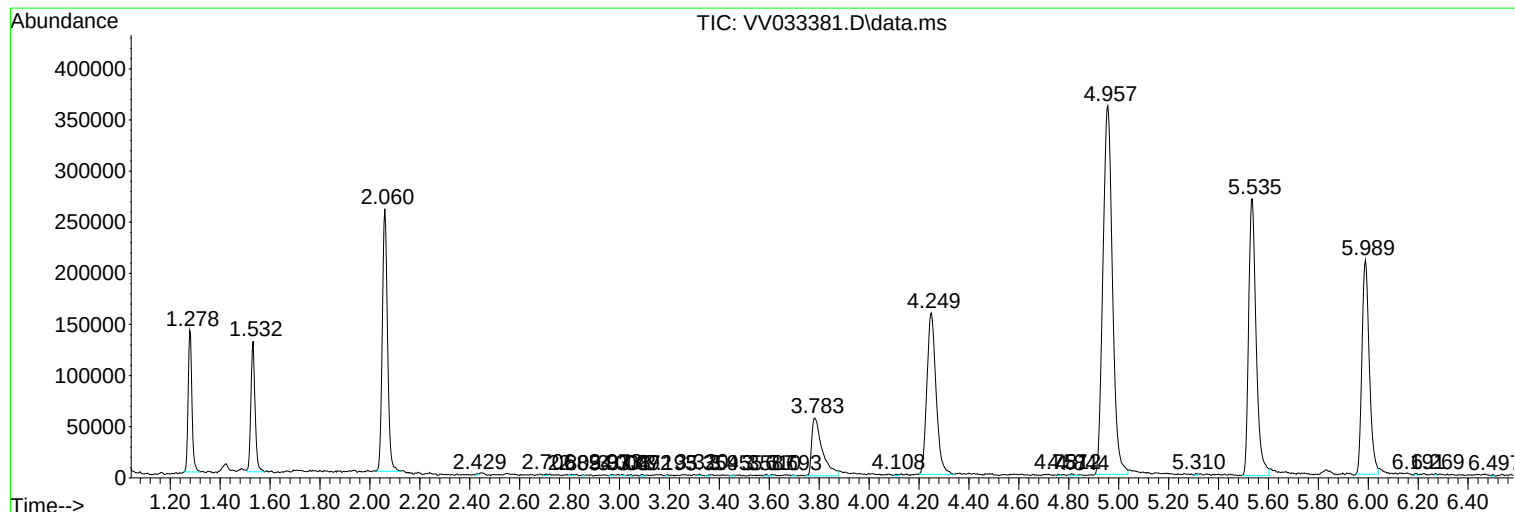

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033381.D
Acq On : 15 Dec 2023 16:49
Operator : SY/MD
Sample : VV1215WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033381.D
Acq On : 15 Dec 2023 16:49
Operator : SY/MD
Sample : VV1215WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------