

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033391.D
 Acq On : 15 Dec 2023 20:43
 Operator : SY/MD
 Sample : 05846-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	67	75	93	rVB2	379286	422802	4.86%	2.581%
2	1.532	146	153	163	rVB	112500	131965	1.52%	0.806%
3	2.069	308	320	352	rVB	6026000	8697796	100.00%	53.093%
4	2.214	357	365	384	rVV	190435	328292	3.77%	2.004%
5	3.111	632	644	667	rVB	174388	360534	4.15%	2.201%
6	3.346	715	717	718	rBV2	1200	551	0.01%	0.003%
7	3.503	762	766	767	rBV3	697	454	0.01%	0.003%
8	3.539	775	777	780	rVB3	973	463	0.01%	0.003%
9	3.561	782	784	787	rVV3	957	589	0.01%	0.004%
10	3.574	787	788	791	rVB3	1033	495	0.01%	0.003%
11	3.664	813	816	817	rBV3	1042	539	0.01%	0.003%
12	3.748	840	842	843	rBV2	897	464	0.01%	0.003%
13	3.812	844	862	876	rBV4	83230	301630	3.47%	1.841%
14	4.246	980	997	1030	rBV2	145296	414224	4.76%	2.529%
15	4.957	1202	1218	1232	rBV2	336255	892968	10.27%	5.451%
16	5.535	1386	1398	1422	rBV	255016	532498	6.12%	3.250%
17	5.838	1482	1492	1514	rVB3	63692	134238	1.54%	0.819%
18	5.989	1527	1539	1560	rBV	193832	397508	4.57%	2.426%
19	6.416	1668	1672	1677	rBV6	1586	1777	0.02%	0.011%
20	6.503	1695	1699	1702	rVB5	1521	979	0.01%	0.006%
21	6.825	1797	1799	1804	rVB6	1214	880	0.01%	0.005%
22	6.912	1816	1826	1846	rBV	96662	182500	2.10%	1.114%
23	7.059	1869	1872	1875	rVB3	1772	1027	0.01%	0.006%
24	7.243	1914	1929	1949	rBV	379542	675860	7.77%	4.126%
25	7.555	2017	2026	2047	rBV	70985	126037	1.45%	0.769%
26	7.773	2093	2094	2096	rBV2	1269	624	0.01%	0.004%
27	7.863	2120	2122	2124	rBV3	1107	484	0.01%	0.003%
28	7.879	2124	2127	2129	rVV5	1639	766	0.01%	0.005%
29	7.992	2160	2162	2163	rBV2	1097	538	0.01%	0.003%
30	8.024	2163	2172	2205	rVV	177440	355316	4.09%	2.169%
31	8.490	2314	2317	2321	rBV4	1660	1091	0.01%	0.007%
32	8.513	2322	2324	2326	rVB3	1150	448	0.01%	0.003%
33	8.635	2360	2362	2364	rBV2	1698	845	0.01%	0.005%
34	8.786	2398	2409	2431	rBV	416974	689196	7.92%	4.207%
35	9.223	2538	2545	2546	rBV6	1307	1235	0.01%	0.008%
36	9.278	2560	2562	2565	rBV3	1200	660	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033391.D
 Acq On : 15 Dec 2023 20:43
 Operator : SY/MD
 Sample : 05846-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.387	2593	2596	2598	rBV2	1324	803	0.01%	0.005%
38	9.458	2615	2618	2621	rBV3	703	608	0.01%	0.004%
39	9.474	2621	2623	2625	rBV2	1024	641	0.01%	0.004%
40	9.719	2697	2699	2701	rBV3	930	406	0.00%	0.002%
41	9.796	2719	2723	2724	rBV4	942	664	0.01%	0.004%
42	9.883	2747	2750	2751	rBV2	1271	617	0.01%	0.004%
43	9.918	2759	2761	2763	rBV3	1282	670	0.01%	0.004%
44	10.024	2792	2794	2795	rBV2	1311	482	0.01%	0.003%
45	10.153	2823	2834	2852	rBV	273778	438288	5.04%	2.675%
46	10.249	2862	2864	2868	rBV4	1426	937	0.01%	0.006%
47	10.529	2945	2951	2953	rBV6	1193	1155	0.01%	0.007%
48	10.555	2957	2959	2962	rVB3	1420	597	0.01%	0.004%
49	10.587	2968	2969	2973	rBV3	1137	755	0.01%	0.005%
50	10.612	2973	2977	2979	rBV5	1215	1015	0.01%	0.006%
51	10.641	2982	2986	2990	rBV5	938	740	0.01%	0.005%
52	10.725	3010	3012	3014	rBV3	982	384	0.00%	0.002%
53	10.751	3017	3020	3022	rBV3	1903	985	0.01%	0.006%
54	10.918	3068	3072	3073	rBV4	1232	781	0.01%	0.005%
55	10.928	3073	3075	3078	rVV4	1132	555	0.01%	0.003%
56	10.979	3089	3091	3093	rBV4	1448	719	0.01%	0.004%
57	11.104	3128	3130	3133	rBV4	888	594	0.01%	0.004%
58	11.185	3145	3155	3169	rBV	382002	594498	6.84%	3.629%
59	11.413	3223	3226	3229	rBV4	1242	1200	0.01%	0.007%
60	11.490	3244	3250	3254	rBV5	1758	2023	0.02%	0.012%
61	11.561	3261	3272	3290	rBV	401827	639534	7.35%	3.904%
62	11.834	3353	3357	3360	rBV5	759	530	0.01%	0.003%
63	11.854	3360	3363	3365	rBV3	1123	811	0.01%	0.005%
64	12.162	3456	3459	3461	rBV3	1566	874	0.01%	0.005%
65	12.198	3468	3470	3473	rBV4	855	431	0.00%	0.003%
66	12.262	3487	3490	3496	rBV5	1751	1352	0.02%	0.008%
67	12.445	3541	3547	3548	rBV4	1253	1215	0.01%	0.007%
68	12.564	3582	3584	3586	rBV2	975	449	0.01%	0.003%
69	12.590	3590	3592	3594	rBV3	1117	562	0.01%	0.003%
70	12.635	3601	3606	3607	rBV3	1621	1390	0.02%	0.008%
71	12.693	3621	3624	3627	rVB4	2217	1207	0.01%	0.007%
72	12.715	3627	3631	3633	rBV5	1302	808	0.01%	0.005%
73	13.001	3718	3720	3723	rBV3	1174	727	0.01%	0.004%
74	13.104	3747	3752	3753	rBV5	1053	979	0.01%	0.006%
75	13.133	3759	3761	3762	rBV2	1102	542	0.01%	0.003%
76	13.226	3788	3790	3793	rBV4	1223	807	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033391.D
 Acq On : 15 Dec 2023 20:43
 Operator : SY/MD
 Sample : 05846-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.339	3822	3825	3827	rBV3	798	565	0.01%	0.003%
78	13.384	3837	3839	3842	rBV4	902	624	0.01%	0.004%
79	13.567	3891	3896	3900	rBV6	1358	1608	0.02%	0.010%
80	13.596	3903	3905	3908	rVB4	1483	819	0.01%	0.005%
81	13.709	3936	3940	3942	rVB3	1143	602	0.01%	0.004%
82	13.731	3944	3947	3948	rBV3	784	448	0.01%	0.003%
83	13.763	3955	3957	3960	rVB4	1482	819	0.01%	0.005%
84	13.889	3994	3996	3999	rBV4	840	602	0.01%	0.004%
85	13.953	4013	4016	4019	rVB5	1218	719	0.01%	0.004%
86	14.152	4074	4078	4079	rBV3	1164	613	0.01%	0.004%
87	14.191	4086	4090	4091	rBV4	920	690	0.01%	0.004%
88	14.249	4102	4108	4110	rBV6	1561	1182	0.01%	0.007%
89	14.262	4110	4112	4117	rVB4	1715	1393	0.02%	0.009%
90	14.288	4117	4120	4121	rBV2	1098	663	0.01%	0.004%
91	14.384	4147	4150	4151	rBV2	1169	711	0.01%	0.004%
92	14.513	4187	4190	4191	rBV3	1373	794	0.01%	0.005%
93	14.866	4298	4300	4302	rVB3	1447	610	0.01%	0.004%
94	15.037	4349	4353	4357	rBV7	1988	1930	0.02%	0.012%
95	15.120	4377	4379	4381	rBV3	955	470	0.01%	0.003%
96	15.178	4394	4397	4399	rBV3	1938	1132	0.01%	0.007%
97	15.220	4407	4410	4414	rBV4	1270	957	0.01%	0.006%
98	15.712	4559	4563	4567	rBV6	1365	1226	0.01%	0.007%
99	15.895	4618	4620	4625	rVB5	2384	1406	0.02%	0.009%
100	16.011	4652	4656	4657	rBV4	1418	902	0.01%	0.006%




Sum of corrected areas: 16382093

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033391.D
Acq On : 15 Dec 2023 20:43
Operator : SY/MD
Sample : 05846-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

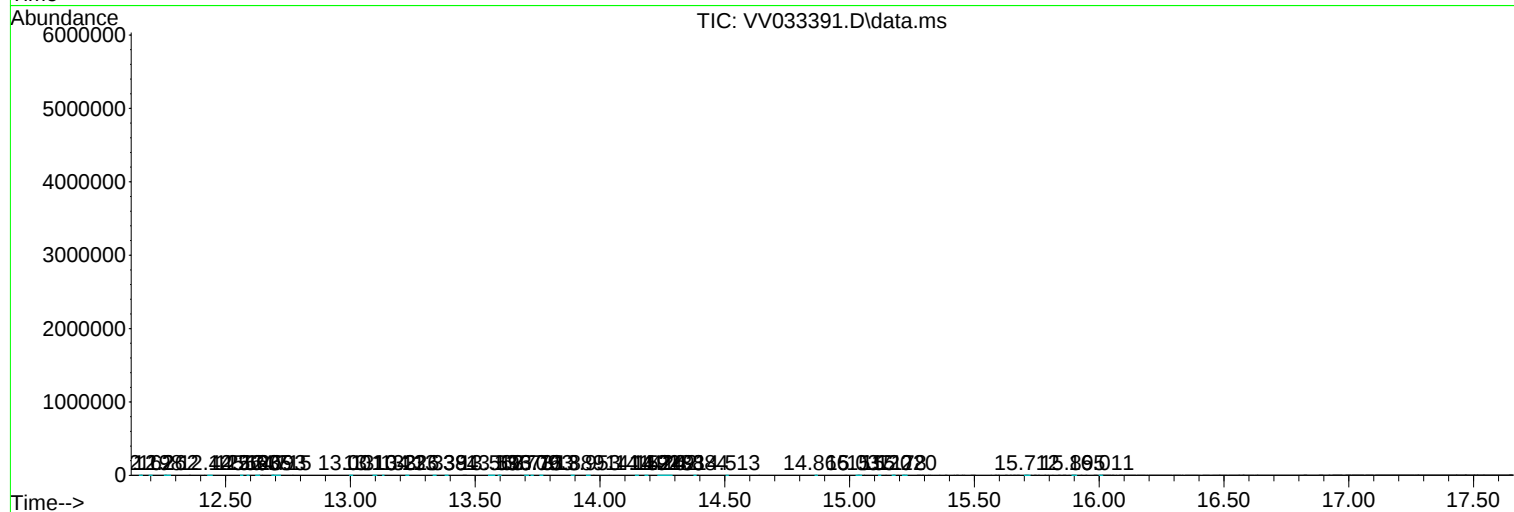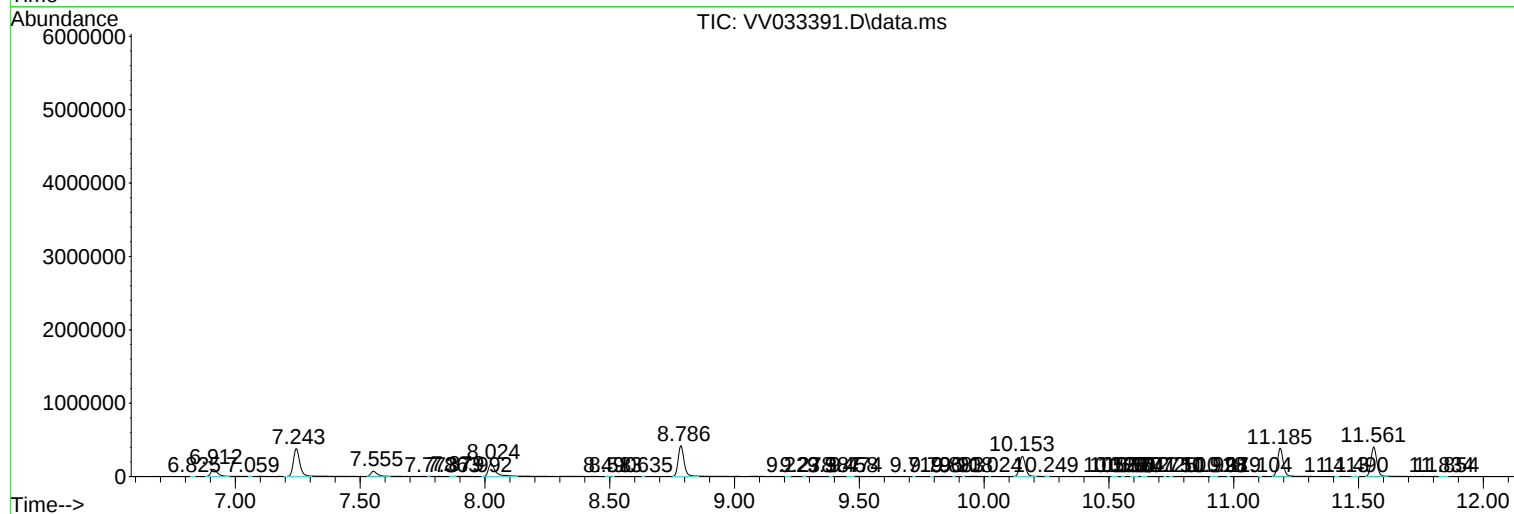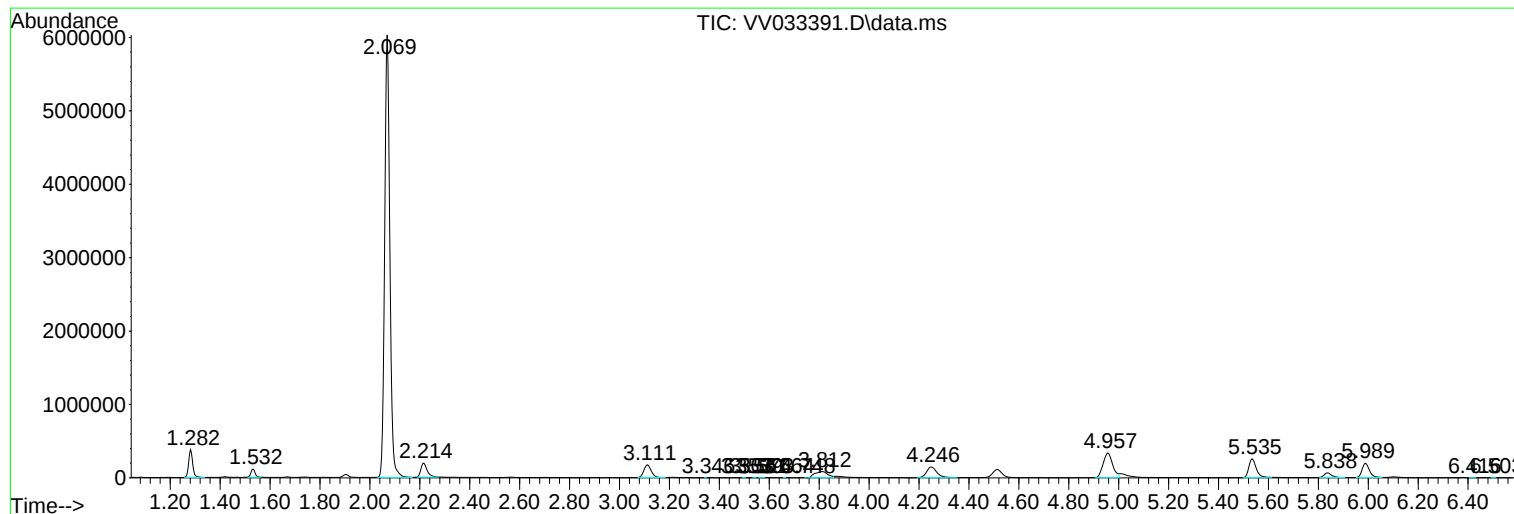

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033391.D
Acq On : 15 Dec 2023 20:43
Operator : SY/MD
Sample : 05846-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033391.D
Acq On : 15 Dec 2023 20:43
Operator : SY/MD
Sample : 05846-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------