

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033393.D
 Acq On : 15 Dec 2023 21:30
 Operator : SY/MD
 Sample : 05846-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rBV2	157287	176440	5.16%	1.626%
2	1.532	146	153	169	rVB	115591	135680	3.97%	1.250%
3	2.069	308	320	349	rVB	2231277	3417377	100.00%	31.486%
4	2.217	358	366	386	rVB	72212	129429	3.79%	1.192%
5	2.825	551	555	557	rBV4	1469	1121	0.03%	0.010%
6	2.899	574	578	580	rBV4	1189	1016	0.03%	0.009%
7	3.072	628	632	634	rBV5	1596	1150	0.03%	0.011%
8	3.114	634	645	661	rVV	48051	103276	3.02%	0.952%
9	3.301	699	703	704	rBV5	1303	748	0.02%	0.007%
10	3.368	721	724	727	rBV4	1025	612	0.02%	0.006%
11	3.387	727	730	732	rVB3	1120	568	0.02%	0.005%
12	3.403	732	735	739	rBV7	1170	1035	0.03%	0.010%
13	3.532	773	775	778	rVB4	1211	540	0.02%	0.005%
14	3.731	832	837	838	rBV3	855	736	0.02%	0.007%
15	3.812	844	862	894	rBV5	158312	551349	16.13%	5.080%
16	4.191	972	980	982	rBV2	15584	20094	0.59%	0.185%
17	4.513	1068	1080	1105	rVB	122161	308256	9.02%	2.840%
18	4.841	1177	1182	1184	rBV6	1480	1202	0.04%	0.011%
19	4.889	1195	1197	1199	rBV3	1265	648	0.02%	0.006%
20	4.956	1202	1218	1237	rBV2	337945	914787	26.77%	8.428%
21	5.535	1387	1398	1423	rBV	256842	537182	15.72%	4.949%
22	5.834	1479	1491	1509	rBV	158706	325578	9.53%	3.000%
23	5.989	1528	1539	1563	rVB	200050	407883	11.94%	3.758%
24	6.272	1625	1627	1630	rBV4	1389	727	0.02%	0.007%
25	6.590	1724	1726	1728	rBV3	1204	585	0.02%	0.005%
26	6.677	1749	1753	1754	rBV3	842	729	0.02%	0.007%
27	6.860	1808	1810	1812	rBV3	1337	636	0.02%	0.006%
28	6.915	1816	1827	1847	rBV2	99197	189936	5.56%	1.750%
29	7.243	1919	1929	1948	rBV	382364	672145	19.67%	6.193%
30	7.554	2017	2026	2044	rBV	72065	130450	3.82%	1.202%
31	7.757	2086	2089	2090	rBV2	1570	987	0.03%	0.009%
32	7.972	2154	2156	2158	rBV3	1251	515	0.02%	0.005%
33	8.024	2163	2172	2198	rBV	180248	353757	10.35%	3.259%
34	8.300	2252	2258	2273	rVB3	8862	17957	0.53%	0.165%
35	8.519	2323	2326	2329	rBV4	1486	1238	0.04%	0.011%
36	8.738	2392	2394	2397	rBV4	1122	625	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033393.D
 Acq On : 15 Dec 2023 21:30
 Operator : SY/MD
 Sample : 05846-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.786	2398	2409	2428	rVV	419571	695704	20.36%	6.410%
38	9.271	2557	2560	2562	rBV5	1209	784	0.02%	0.007%
39	9.381	2592	2594	2600	rVB6	1648	980	0.03%	0.009%
40	9.455	2615	2617	2619	rBV3	977	567	0.02%	0.005%
41	9.525	2633	2639	2643	rBV9	1695	2118	0.06%	0.020%
42	9.596	2659	2661	2664	rVB3	1379	498	0.01%	0.005%
43	9.635	2669	2673	2676	rBV6	1241	1083	0.03%	0.010%
44	9.696	2687	2692	2696	rBV8	1772	2053	0.06%	0.019%
45	10.017	2789	2792	2797	rVB5	1200	982	0.03%	0.009%
46	10.043	2798	2800	2803	rVB3	1467	743	0.02%	0.007%
47	10.152	2824	2834	2849	rBV	278307	436476	12.77%	4.021%
48	10.300	2876	2880	2882	rBV4	1590	1106	0.03%	0.010%
49	10.390	2904	2908	2910	rBV4	1459	1007	0.03%	0.009%
50	10.615	2976	2978	2980	rBV2	1374	729	0.02%	0.007%
51	10.683	2995	2999	3001	rBV4	1344	1009	0.03%	0.009%
52	10.783	3026	3030	3034	rBV5	1023	1340	0.04%	0.012%
53	10.966	3085	3087	3090	rBV4	870	499	0.01%	0.005%
54	11.188	3144	3156	3176	rBV	385947	608541	17.81%	5.607%
55	11.509	3252	3256	3259	rBV5	1283	1007	0.03%	0.009%
56	11.561	3259	3272	3289	rBV	414866	656080	19.20%	6.045%
57	11.815	3348	3351	3353	rBV3	1158	658	0.02%	0.006%
58	11.866	3363	3367	3368	rVV4	1005	627	0.02%	0.006%
59	11.876	3368	3370	3373	rVV3	716	544	0.02%	0.005%
60	11.892	3373	3375	3378	rVB2	1883	781	0.02%	0.007%
61	11.937	3387	3389	3391	rBV3	1079	529	0.02%	0.005%
62	12.030	3415	3418	3421	rBV4	1058	934	0.03%	0.009%
63	12.281	3493	3496	3498	rBV3	1094	489	0.01%	0.005%
64	12.294	3498	3500	3502	rBV3	1438	870	0.03%	0.008%
65	12.326	3508	3510	3513	rVB4	1021	597	0.02%	0.006%
66	12.352	3513	3518	3520	rBV5	1520	1444	0.04%	0.013%
67	12.545	3576	3578	3582	rVB5	1535	894	0.03%	0.008%
68	12.574	3584	3587	3591	rVV4	917	710	0.02%	0.007%
69	12.705	3626	3628	3631	rBV4	729	461	0.01%	0.004%
70	12.754	3640	3643	3644	rBV2	809	499	0.01%	0.005%
71	12.779	3650	3651	3653	rBV2	848	459	0.01%	0.004%
72	12.802	3656	3658	3660	rBV3	755	467	0.01%	0.004%
73	12.937	3698	3700	3703	rVV3	1290	759	0.02%	0.007%
74	12.959	3705	3707	3709	rVV4	966	502	0.01%	0.005%
75	12.985	3712	3715	3718	rVB5	1684	1098	0.03%	0.010%
76	13.094	3747	3749	3753	rVB5	1428	1034	0.03%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033393.D
 Acq On : 15 Dec 2023 21:30
 Operator : SY/MD
 Sample : 05846-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.123	3753	3758	3759	rBV4	1287	1175	0.03%	0.011%
78	13.175	3772	3774	3777	rBV3	1800	721	0.02%	0.007%
79	13.242	3793	3795	3798	rBV4	1291	694	0.02%	0.006%
80	13.400	3840	3844	3848	rBV7	1118	1210	0.04%	0.011%
81	13.628	3911	3915	3916	rBV4	1434	929	0.03%	0.009%
82	13.651	3920	3922	3927	rVB5	1586	767	0.02%	0.007%
83	13.683	3931	3932	3935	rVV3	1495	662	0.02%	0.006%
84	13.789	3962	3965	3967	rBV3	1104	632	0.02%	0.006%
85	13.853	3983	3985	3987	rBV4	1282	542	0.02%	0.005%
86	14.008	4031	4033	4035	rBV3	1293	646	0.02%	0.006%
87	14.213	4095	4097	4100	rBV3	791	440	0.01%	0.004%
88	14.252	4108	4109	4114	rBV5	1286	841	0.02%	0.008%
89	14.278	4114	4117	4119	rBV2	1122	675	0.02%	0.006%
90	14.519	4187	4192	4195	rBV5	1674	1661	0.05%	0.015%
91	14.606	4217	4219	4221	rBV2	1170	477	0.01%	0.004%
92	14.667	4236	4238	4240	rBV3	799	501	0.01%	0.005%
93	14.725	4253	4256	4257	rBV2	750	505	0.01%	0.005%
94	14.779	4270	4273	4274	rBV4	1310	689	0.02%	0.006%
95	14.853	4294	4296	4299	rBV4	1194	919	0.03%	0.008%
96	15.014	4341	4346	4348	rBV6	1385	1241	0.04%	0.011%
97	15.053	4354	4358	4361	rBV6	1245	1050	0.03%	0.010%
98	15.229	4411	4413	4416	rBV3	1020	628	0.02%	0.006%
99	15.329	4442	4444	4446	rBV2	1179	523	0.02%	0.005%
100	15.638	4538	4540	4543	rBV4	1273	855	0.03%	0.008%




Sum of corrected areas: 10853639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033393.D
Acq On : 15 Dec 2023 21:30
Operator : SY/MD
Sample : 05846-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

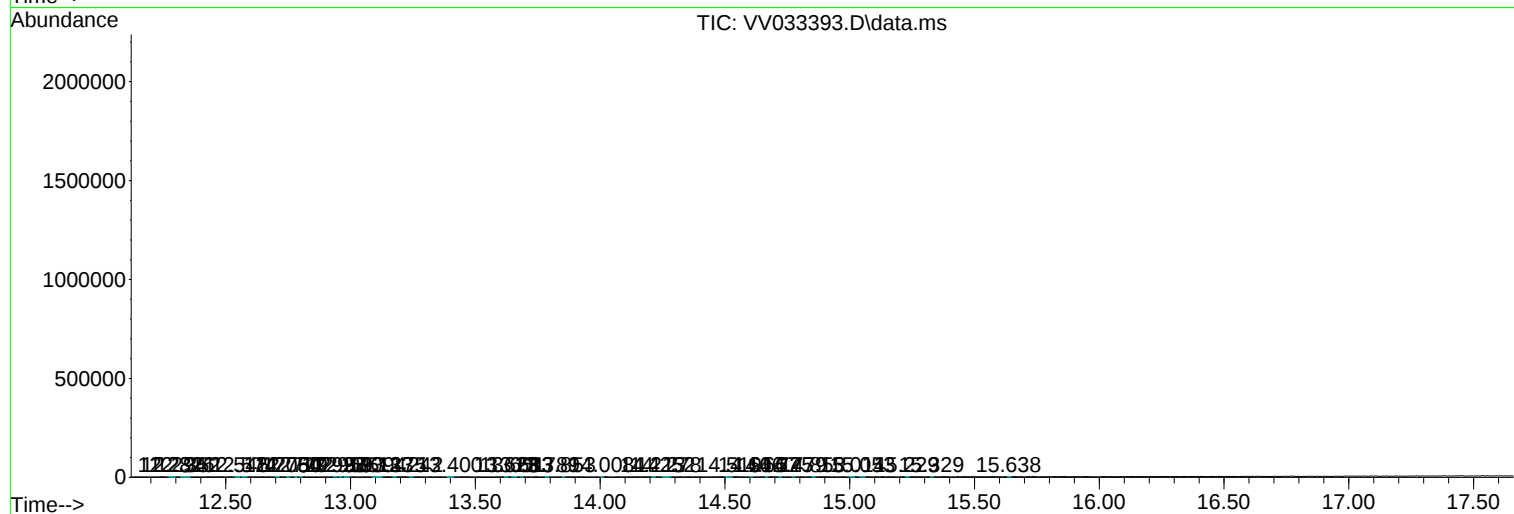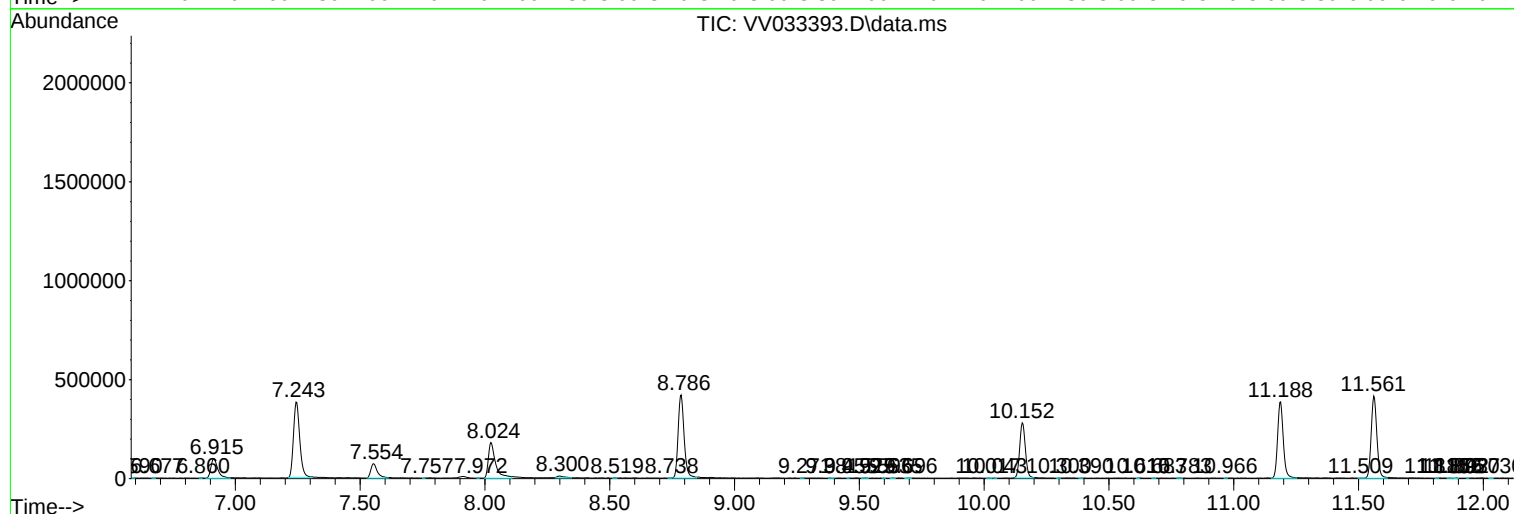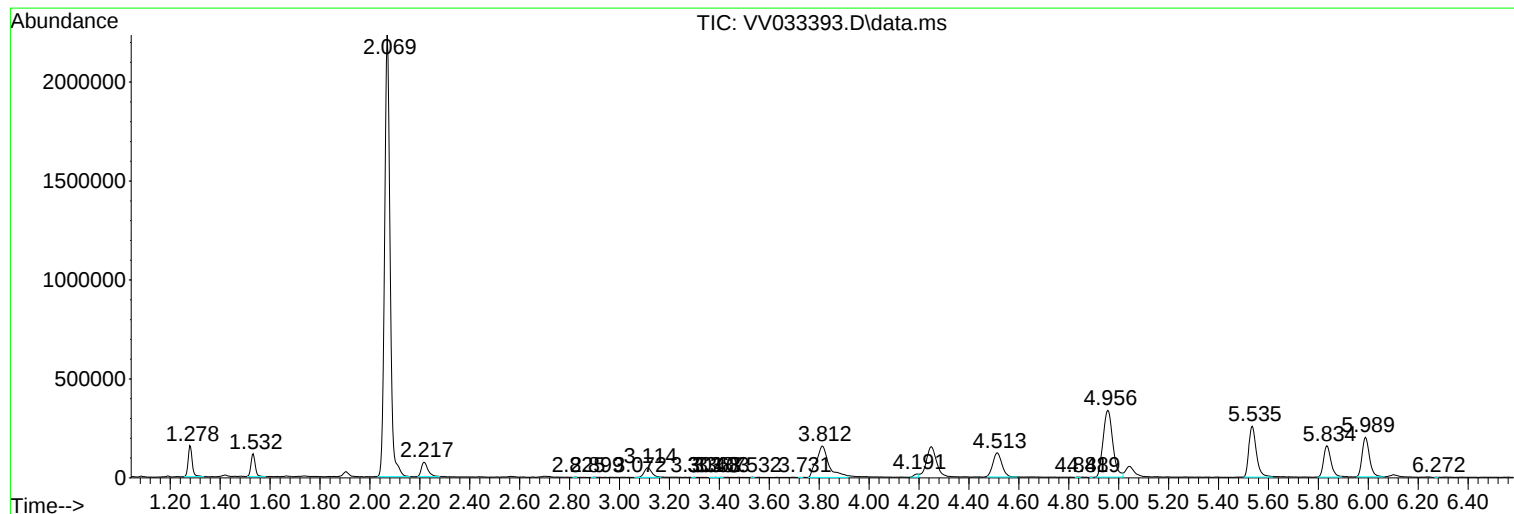

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033393.D
Acq On : 15 Dec 2023 21:30
Operator : SY/MD
Sample : 05846-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033393.D
Acq On : 15 Dec 2023 21:30
Operator : SY/MD
Sample : 05846-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------