

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	43	47	52	rVB	6645	5776	0.17%	0.053%
2	1.282	67	75	91	rBV2	157802	177564	5.12%	1.631%
3	1.532	146	153	165	rVB	112398	131459	3.79%	1.207%
4	2.069	308	320	348	rVB	2271429	3466978	100.00%	31.840%
5	2.217	358	366	391	rVB	76055	141437	4.08%	1.299%
6	3.056	625	627	629	rBV3	984	643	0.02%	0.006%
7	3.114	634	645	660	rVV	47207	100477	2.90%	0.923%
8	3.320	707	709	710	rBV2	1408	637	0.02%	0.006%
9	3.378	726	727	732	rBV5	691	576	0.02%	0.005%
10	3.465	752	754	759	rVB5	1252	948	0.03%	0.009%
11	3.516	765	770	771	rBV4	1377	835	0.02%	0.008%
12	3.815	844	863	878	rBV3	157942	497737	14.36%	4.571%
13	4.188	973	979	982	rBV2	13810	17074	0.49%	0.157%
14	4.513	1065	1080	1103	rVB2	127033	330396	9.53%	3.034%
15	4.687	1130	1134	1135	rBV3	1880	1044	0.03%	0.010%
16	4.802	1167	1170	1171	rBV3	961	610	0.02%	0.006%
17	4.957	1201	1218	1235	rBV2	339975	898196	25.91%	8.249%
18	5.535	1386	1398	1422	rBV	258010	536797	15.48%	4.930%
19	5.834	1480	1491	1516	rBV	180203	356040	10.27%	3.270%
20	5.989	1528	1539	1561	rBV	198315	401266	11.57%	3.685%
21	6.375	1654	1659	1661	rBV4	2423	1982	0.06%	0.018%
22	6.468	1686	1688	1691	rBV4	1022	812	0.02%	0.007%
23	6.587	1721	1725	1728	rBV4	1030	902	0.03%	0.008%
24	6.857	1806	1809	1811	rBV3	1077	573	0.02%	0.005%
25	6.915	1817	1827	1850	rBV	95423	178574	5.15%	1.640%
26	7.243	1917	1929	1950	rBV	388254	682639	19.69%	6.269%
27	7.555	2017	2026	2046	rBV	70636	127711	3.68%	1.173%
28	7.738	2080	2083	2084	rBV3	1477	729	0.02%	0.007%
29	7.908	2129	2136	2149	rVB6	13185	21920	0.63%	0.201%
30	8.024	2163	2172	2207	rBV	173747	351482	10.14%	3.228%
31	8.690	2374	2379	2380	rBV4	1410	1022	0.03%	0.009%
32	8.786	2397	2409	2432	rBV	420169	701622	20.24%	6.444%
33	9.011	2476	2479	2481	rBV5	1388	881	0.03%	0.008%
34	9.391	2594	2597	2605	rVB7	1709	1845	0.05%	0.017%
35	9.429	2605	2609	2611	rBV4	1089	966	0.03%	0.009%
36	9.439	2611	2612	2619	rVB6	1366	1134	0.03%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.493	2627	2629	2635	rBV8	938	637	0.02%	0.006%
38	9.580	2652	2656	2660	rBV5	1467	1581	0.05%	0.015%
39	9.619	2664	2668	2673	rBV7	1122	1364	0.04%	0.013%
40	9.731	2697	2703	2704	rBV5	998	905	0.03%	0.008%
41	9.767	2712	2714	2718	rBV5	737	696	0.02%	0.006%
42	9.860	2741	2743	2747	rVB5	1256	786	0.02%	0.007%
43	9.931	2763	2765	2769	rBV5	989	753	0.02%	0.007%
44	10.011	2787	2790	2791	rBV3	1466	686	0.02%	0.006%
45	10.153	2823	2834	2852	rBV	272396	436099	12.58%	4.005%
46	10.371	2896	2902	2903	rBV5	931	872	0.03%	0.008%
47	10.407	2910	2913	2917	rBV5	1603	1259	0.04%	0.012%
48	10.484	2934	2937	2939	rBV3	1746	1289	0.04%	0.012%
49	10.526	2946	2950	2952	rBV4	1137	910	0.03%	0.008%
50	10.670	2991	2995	2997	rBV4	1657	1127	0.03%	0.010%
51	10.722	3008	3011	3012	rBV4	1249	623	0.02%	0.006%
52	10.960	3082	3085	3087	rBV4	1304	599	0.02%	0.006%
53	11.011	3097	3101	3102	rBV4	1069	647	0.02%	0.006%
54	11.066	3116	3118	3120	rBV3	1228	590	0.02%	0.005%
55	11.082	3120	3123	3126	rVB3	1106	558	0.02%	0.005%
56	11.124	3133	3136	3140	rBV5	883	645	0.02%	0.006%
57	11.185	3143	3155	3174	rBV	387871	609691	17.59%	5.599%
58	11.509	3254	3256	3259	rBV4	983	640	0.02%	0.006%
59	11.561	3259	3272	3287	rBV	411162	648103	18.69%	5.952%
60	11.731	3324	3325	3327	rBV2	1539	604	0.02%	0.006%
61	12.053	3423	3425	3429	rBV5	830	780	0.02%	0.007%
62	12.088	3435	3436	3443	rVB6	1070	858	0.02%	0.008%
63	12.117	3443	3445	3447	rBV3	1231	742	0.02%	0.007%
64	12.188	3464	3467	3470	rBV5	1502	1038	0.03%	0.010%
65	12.288	3496	3498	3500	rBV3	1132	581	0.02%	0.005%
66	12.352	3516	3518	3521	rBV4	1709	1037	0.03%	0.010%
67	12.426	3538	3541	3545	rBV4	1068	845	0.02%	0.008%
68	12.452	3545	3549	3551	rBV4	1141	824	0.02%	0.008%
69	12.632	3600	3605	3607	rBV5	1395	1319	0.04%	0.012%
70	12.644	3607	3609	3614	rVB6	1087	687	0.02%	0.006%
71	12.689	3620	3623	3629	rVB5	1369	1030	0.03%	0.009%
72	12.718	3629	3632	3635	rBV5	1096	868	0.03%	0.008%
73	12.808	3658	3660	3663	rBV3	1375	806	0.02%	0.007%
74	12.931	3695	3698	3700	rBV4	877	621	0.02%	0.006%
75	13.050	3731	3735	3737	rBV4	1200	838	0.02%	0.008%
76	13.104	3750	3752	3755	rBV4	1224	993	0.03%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033394.D
 Acq On : 15 Dec 2023 21:53
 Operator : SY/MD
 Sample : 05846-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.146	3760	3765	3767	rBV4	991	811	0.02%	0.007%
78	13.162	3767	3770	3774	rBV6	1394	955	0.03%	0.009%
79	13.204	3780	3783	3789	rBV7	1223	1174	0.03%	0.011%
80	13.230	3789	3791	3794	rVB3	1580	929	0.03%	0.009%
81	13.287	3806	3809	3815	rVB6	1333	1019	0.03%	0.009%
82	13.316	3815	3818	3820	rBV4	1032	709	0.02%	0.007%
83	13.329	3820	3822	3826	rVB5	1039	635	0.02%	0.006%
84	13.384	3836	3839	3842	rBV4	943	801	0.02%	0.007%
85	13.529	3878	3884	3886	rBV6	1294	1363	0.04%	0.013%
86	13.577	3894	3899	3903	rBV7	1433	1339	0.04%	0.012%
87	13.615	3907	3911	3916	rVB7	1394	1305	0.04%	0.012%
88	13.931	4005	4009	4010	rBV4	1173	649	0.02%	0.006%
89	14.056	4045	4048	4051	rVB5	1020	617	0.02%	0.006%
90	14.101	4060	4062	4066	rBV3	949	768	0.02%	0.007%
91	14.146	4073	4076	4077	rBV3	1185	633	0.02%	0.006%
92	14.188	4088	4089	4095	rVB4	882	806	0.02%	0.007%
93	14.259	4109	4111	4114	rBV3	1127	636	0.02%	0.006%
94	14.387	4149	4151	4153	rBV2	1168	681	0.02%	0.006%
95	14.493	4181	4184	4187	rBV5	1323	996	0.03%	0.009%
96	14.641	4228	4230	4234	rVB4	1417	925	0.03%	0.008%
97	15.181	4395	4398	4399	rBV3	1418	858	0.02%	0.008%
98	15.419	4468	4472	4475	rBV6	1164	1002	0.03%	0.009%
99	15.586	4521	4524	4528	rBV5	1327	1149	0.03%	0.011%
100	15.609	4528	4531	4534	rBV5	1497	1072	0.03%	0.010%




Sum of corrected areas: 10888647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033394.D
Acq On : 15 Dec 2023 21:53
Operator : SY/MD
Sample : 05846-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

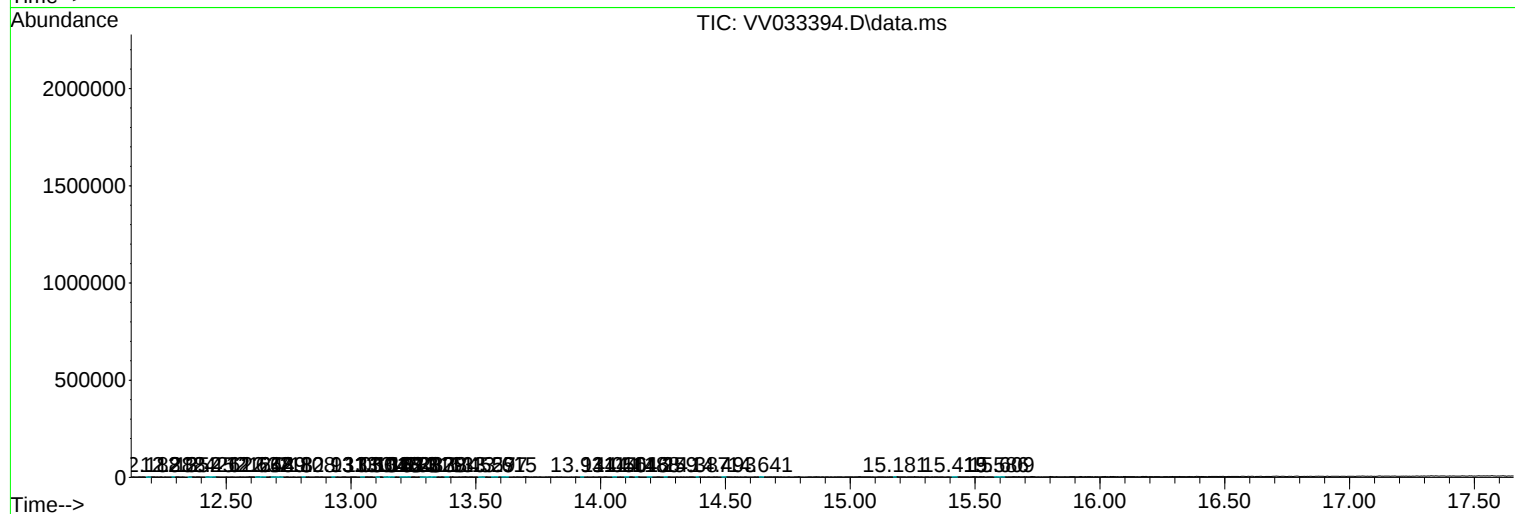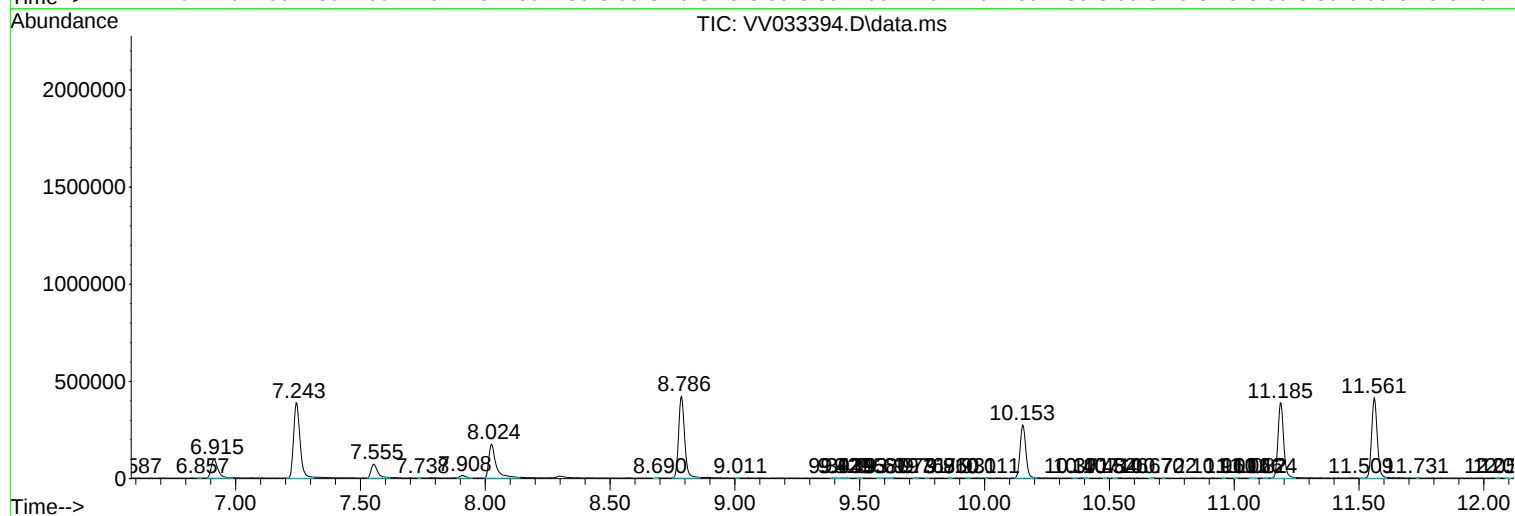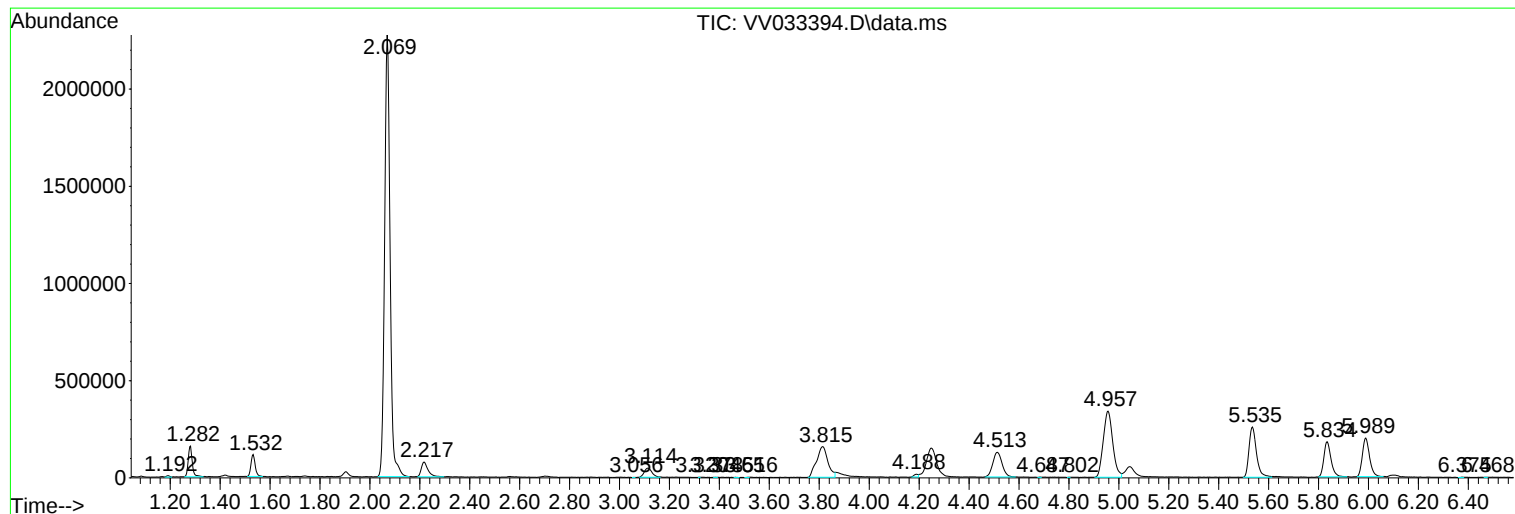

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033394.D
Acq On : 15 Dec 2023 21:53
Operator : SY/MD
Sample : 05846-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033394.D
Acq On : 15 Dec 2023 21:53
Operator : SY/MD
Sample : 05846-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------