

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033399.D
 Acq On : 15 Dec 2023 23:49
 Operator : SY/MD
 Sample : 05846-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	49	53	55	rBV4	2471	1974	0.23%	0.031%
2	1.278	68	74	85	rBV	121009	123858	14.56%	1.953%
3	1.532	146	153	167	rVB	109341	130222	15.31%	2.053%
4	2.059	308	317	330	rBV	213978	306649	36.06%	4.835%
5	2.281	384	386	387	rBV2	1571	579	0.07%	0.009%
6	2.404	422	424	426	rVB3	1311	484	0.06%	0.008%
7	2.439	432	435	437	rBV4	1998	1126	0.13%	0.018%
8	2.529	458	463	465	rBV5	1449	1192	0.14%	0.019%
9	2.635	492	496	497	rBV3	1632	1015	0.12%	0.016%
10	2.712	518	520	522	rBV3	826	479	0.06%	0.008%
11	2.973	598	601	604	rBV3	938	604	0.07%	0.010%
12	3.072	629	632	634	rBV3	1348	861	0.10%	0.014%
13	3.143	651	654	657	rBV5	1479	1074	0.13%	0.017%
14	3.262	690	691	694	rVB4	1058	421	0.05%	0.007%
15	3.330	707	712	717	rVB7	1790	1724	0.20%	0.027%
16	3.371	720	725	727	rBV6	1197	1107	0.13%	0.017%
17	3.468	750	755	758	rVV8	982	1127	0.13%	0.018%
18	3.545	776	779	781	rBV5	1065	748	0.09%	0.012%
19	3.574	784	788	791	rBV6	1197	1041	0.12%	0.016%
20	3.641	806	809	813	rBV6	941	710	0.08%	0.011%
21	3.703	826	828	830	rBV3	1244	759	0.09%	0.012%
22	3.786	846	854	873	rBV	50252	132657	15.60%	2.092%
23	4.249	985	998	1021	rVB3	139522	354897	41.73%	5.596%
24	4.667	1126	1128	1130	rBV4	1018	454	0.05%	0.007%
25	4.799	1167	1169	1174	rBV5	901	848	0.10%	0.013%
26	4.956	1202	1218	1242	rBV2	319710	850499	100.00%	13.410%
27	5.468	1374	1377	1379	rBV3	941	572	0.07%	0.009%
28	5.535	1386	1398	1422	rBV	238196	500206	58.81%	7.887%
29	5.989	1527	1539	1562	rBV	187933	390874	45.96%	6.163%
30	6.407	1667	1669	1671	rBV3	962	543	0.06%	0.009%
31	6.609	1725	1732	1738	rBV9	1712	2670	0.31%	0.042%
32	6.654	1743	1746	1748	rBV3	1130	683	0.08%	0.011%
33	6.715	1763	1765	1769	rBV4	1063	882	0.10%	0.014%
34	6.796	1788	1790	1797	rBV6	1247	819	0.10%	0.013%
35	6.854	1807	1808	1814	rVB4	2261	1341	0.16%	0.021%
36	6.915	1814	1827	1842	rBV	91481	175991	20.69%	2.775%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033399.D
 Acq On : 15 Dec 2023 23:49
 Operator : SY/MD
 Sample : 05846-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.243	1919	1929	1946	rBV	350010	616205	72.45%	9.716%
38	7.554	2017	2026	2042	rBV	66723	120511	14.17%	1.900%
39	7.976	2155	2157	2160	rBV4	1008	538	0.06%	0.008%
40	8.027	2163	2173	2210	rBV	170518	356436	41.91%	5.620%
41	8.503	2317	2321	2324	rBV6	1449	987	0.12%	0.016%
42	8.661	2368	2370	2372	rBV3	1455	783	0.09%	0.012%
43	8.686	2376	2378	2379	rBV2	858	403	0.05%	0.006%
44	8.786	2398	2409	2431	rBV	386152	643302	75.64%	10.143%
45	9.008	2474	2478	2479	rBV3	1949	1189	0.14%	0.019%
46	9.304	2567	2570	2573	rBV5	1237	762	0.09%	0.012%
47	9.484	2621	2626	2629	rBV6	1586	1157	0.14%	0.018%
48	9.564	2649	2651	2655	rBV4	1659	1380	0.16%	0.022%
49	9.644	2674	2676	2679	rBV3	1057	663	0.08%	0.010%
50	9.709	2694	2696	2697	rBV2	1109	582	0.07%	0.009%
51	9.950	2767	2771	2774	rBV5	1221	1160	0.14%	0.018%
52	10.152	2824	2834	2855	rVB	263269	422587	49.69%	6.663%
53	10.371	2901	2902	2905	rBV2	741	516	0.06%	0.008%
54	10.625	2979	2981	2988	rVB7	1485	965	0.11%	0.015%
55	10.651	2988	2989	2993	rVB2	1138	470	0.06%	0.007%
56	10.683	2997	2999	3001	rBV	1239	723	0.09%	0.011%
57	10.802	3033	3036	3042	rVB7	1707	1426	0.17%	0.022%
58	10.828	3042	3044	3047	rBV4	855	437	0.05%	0.007%
59	10.863	3051	3055	3057	rBV3	1304	735	0.09%	0.012%
60	10.879	3057	3060	3063	rBV3	1652	1004	0.12%	0.016%
61	10.959	3082	3085	3087	rBV4	936	738	0.09%	0.012%
62	11.188	3144	3156	3173	rBV	348192	548519	64.49%	8.649%
63	11.349	3204	3206	3209	rVB3	1960	846	0.10%	0.013%
64	11.381	3209	3216	3219	rBV9	1209	1675	0.20%	0.026%
65	11.471	3242	3244	3247	rVB3	1727	631	0.07%	0.010%
66	11.561	3261	3272	3289	rBV	378439	598960	70.42%	9.444%
67	11.776	3335	3339	3344	rBV7	1541	1408	0.17%	0.022%
68	12.008	3409	3411	3413	rBV3	1041	516	0.06%	0.008%
69	12.037	3418	3420	3424	rVB4	1187	951	0.11%	0.015%
70	12.059	3425	3427	3431	rBV3	1277	862	0.10%	0.014%
71	12.287	3497	3498	3501	rVB2	1588	532	0.06%	0.008%
72	12.310	3501	3505	3509	rBV4	1559	1473	0.17%	0.023%
73	12.397	3530	3532	3533	rBV2	883	457	0.05%	0.007%
74	12.500	3560	3564	3566	rBV3	888	716	0.08%	0.011%
75	12.641	3606	3608	3610	rBV2	1110	517	0.06%	0.008%
76	12.702	3625	3627	3630	rBV4	1139	753	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033399.D
 Acq On : 15 Dec 2023 23:49
 Operator : SY/MD
 Sample : 05846-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.802	3656	3658	3661	rBV3	1019	494	0.06%	0.008%
78	12.821	3661	3664	3665	rBV2	1239	659	0.08%	0.010%
79	12.930	3695	3698	3700	rBV2	1060	721	0.08%	0.011%
80	13.194	3778	3780	3783	rBV4	1215	500	0.06%	0.008%
81	13.348	3824	3828	3829	rBV4	826	493	0.06%	0.008%
82	13.403	3843	3845	3850	rBV7	1183	1153	0.14%	0.018%
83	13.538	3882	3887	3891	rBV7	1452	1220	0.14%	0.019%
84	13.628	3913	3915	3918	rBV4	776	404	0.05%	0.006%
85	13.651	3919	3922	3923	rBV2	899	404	0.05%	0.006%
86	13.699	3935	3937	3938	rBV3	1010	518	0.06%	0.008%
87	13.718	3942	3943	3946	rVB2	1132	404	0.05%	0.006%
88	13.737	3946	3949	3952	rBV6	1067	491	0.06%	0.008%
89	13.934	4007	4010	4011	rBV2	1124	653	0.08%	0.010%
90	14.110	4063	4065	4068	rVB4	1285	720	0.08%	0.011%
91	14.136	4068	4073	4076	rBV7	1208	1069	0.13%	0.017%
92	14.271	4112	4115	4120	rBV5	1089	900	0.11%	0.014%
93	14.326	4128	4132	4133	rBV3	1050	671	0.08%	0.011%
94	14.429	4162	4164	4167	rVB3	1031	411	0.05%	0.006%
95	14.493	4180	4184	4185	rBV3	1116	751	0.09%	0.012%
96	14.519	4190	4192	4194	rBV2	1092	753	0.09%	0.012%
97	14.567	4205	4207	4209	rBV3	1110	394	0.05%	0.006%
98	14.638	4226	4229	4230	rBV3	1162	681	0.08%	0.011%
99	14.708	4248	4251	4255	rBV5	1173	1041	0.12%	0.016%
100	14.728	4255	4257	4258	rBV2	939	461	0.05%	0.007%




Sum of corrected areas: 6342131

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033399.D
Acq On : 15 Dec 2023 23:49
Operator : SY/MD
Sample : 05846-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

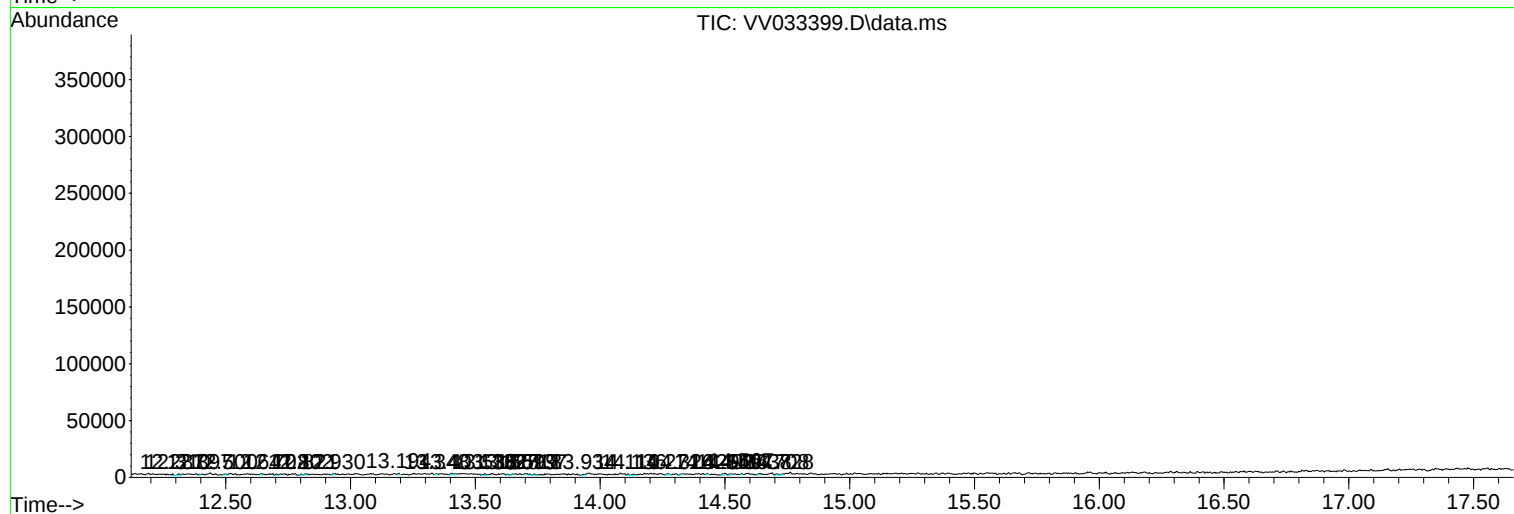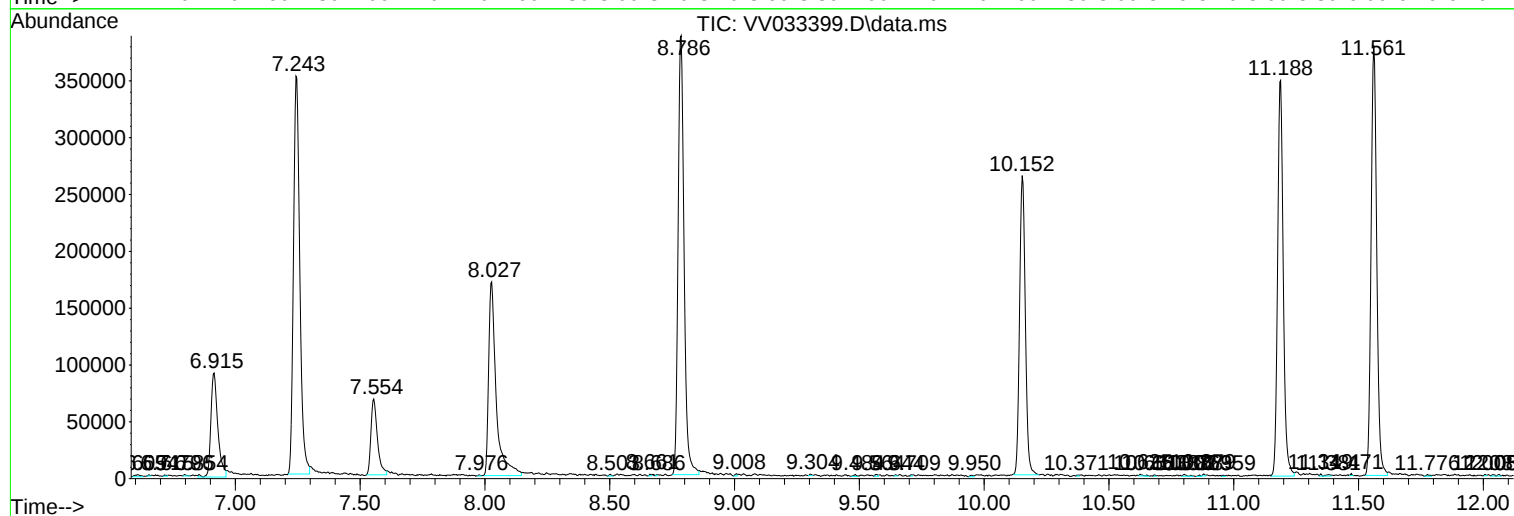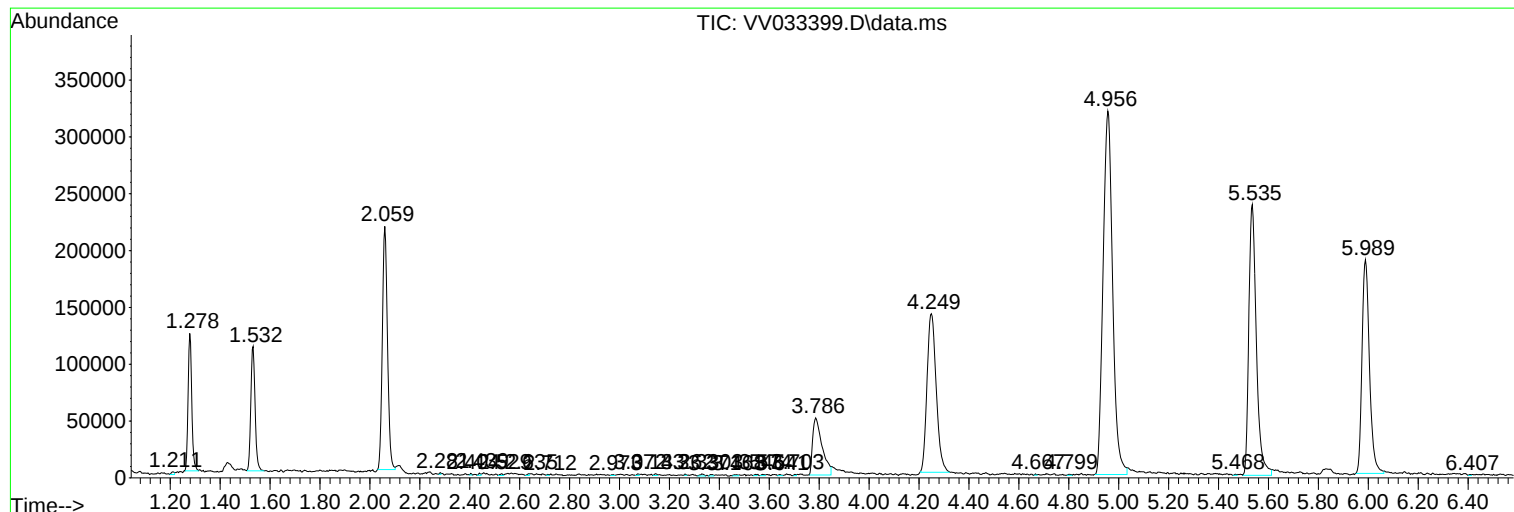

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033399.D
Acq On : 15 Dec 2023 23:49
Operator : SY/MD
Sample : 05846-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033399.D
Acq On : 15 Dec 2023 23:49
Operator : SY/MD
Sample : 05846-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------