

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033404.D
 Acq On : 16 Dec 2023 02:09
 Operator : SY/MD
 Sample : VV1215WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	133534	139257	14.88%	1.971%
2	1.532	146	153	167	rVB	118476	139694	14.93%	1.977%
3	2.060	307	317	336	rBV	243625	358023	38.25%	5.066%
4	2.507	451	456	459	rBV6	1335	1148	0.12%	0.016%
5	2.587	478	481	482	rBV3	1228	695	0.07%	0.010%
6	2.831	554	557	560	rBV4	884	758	0.08%	0.011%
7	2.854	560	564	568	rVB6	1058	1060	0.11%	0.015%
8	2.880	568	572	574	rBV4	1340	961	0.10%	0.014%
9	2.950	590	594	598	rBV6	1134	1048	0.11%	0.015%
10	2.992	605	607	610	rBV3	1546	894	0.10%	0.013%
11	3.082	632	635	636	rBV3	919	595	0.06%	0.008%
12	3.568	782	786	791	rBV6	1467	1359	0.15%	0.019%
13	3.786	846	854	885	rBV	55015	156091	16.68%	2.209%
14	4.143	961	965	969	rBV6	1604	1250	0.13%	0.018%
15	4.249	981	998	1020	rBV2	150830	392530	41.94%	5.554%
16	4.812	1170	1173	1175	rBV4	1178	859	0.09%	0.012%
17	4.831	1177	1179	1182	rVV4	1014	674	0.07%	0.010%
18	4.957	1201	1218	1251	rBV3	346726	935968	100.00%	13.244%
19	5.535	1386	1398	1422	rBV	255055	536437	57.31%	7.591%
20	5.838	1481	1492	1496	rBV10	6253	11920	1.27%	0.169%
21	5.989	1525	1539	1565	rBV	202957	431192	46.07%	6.101%
22	6.304	1635	1637	1640	rVB3	1508	753	0.08%	0.011%
23	6.365	1654	1656	1660	rVB4	1442	701	0.07%	0.010%
24	6.523	1703	1705	1707	rBV2	1068	601	0.06%	0.009%
25	6.542	1709	1711	1715	rVB5	1261	687	0.07%	0.010%
26	6.577	1719	1722	1725	rBV5	1209	856	0.09%	0.012%
27	6.915	1811	1827	1846	rBV	97830	192247	20.54%	2.720%
28	7.143	1892	1898	1901	rBV7	1759	1567	0.17%	0.022%
29	7.243	1918	1929	1948	rBV	390893	701520	74.95%	9.927%
30	7.516	2011	2014	2015	rBV3	1230	814	0.09%	0.012%
31	7.555	2017	2026	2040	rVV	71906	127375	13.61%	1.802%
32	8.027	2160	2173	2202	rBV	186437	379572	40.55%	5.371%
33	8.555	2336	2337	2343	rVB5	1091	631	0.07%	0.009%
34	8.596	2349	2350	2352	rBV2	1156	617	0.07%	0.009%
35	8.667	2370	2372	2377	rVB5	1997	1509	0.16%	0.021%
36	8.696	2377	2381	2385	rBV7	1427	1400	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033404.D
 Acq On : 16 Dec 2023 02:09
 Operator : SY/MD
 Sample : VV1215WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.712	2385	2386	2390	rVB4	1310	645	0.07%	0.009%
38	8.735	2390	2393	2396	rBV3	1351	1036	0.11%	0.015%
39	8.786	2398	2409	2431	rBV	430112	715401	76.43%	10.123%
40	9.021	2479	2482	2486	rBB5	1082	830	0.09%	0.012%
41	9.198	2534	2537	2538	rBV3	1117	694	0.07%	0.010%
42	9.272	2558	2560	2564	rVB5	1130	672	0.07%	0.010%
43	9.294	2564	2567	2570	rBV5	1248	1081	0.12%	0.015%
44	9.371	2587	2591	2596	rBV6	1341	1172	0.13%	0.017%
45	9.400	2596	2600	2602	rVB5	1272	784	0.08%	0.011%
46	9.419	2602	2606	2608	rBV4	1167	597	0.06%	0.008%
47	9.432	2608	2610	2614	rBV5	1015	902	0.10%	0.013%
48	9.680	2683	2687	2688	rBV4	1147	647	0.07%	0.009%
49	9.693	2688	2691	2692	rBV3	1326	620	0.07%	0.009%
50	9.725	2698	2701	2702	rBV3	1357	832	0.09%	0.012%
51	9.854	2738	2741	2742	rBV4	1840	752	0.08%	0.011%
52	10.153	2823	2834	2851	rBV	276588	445692	47.62%	6.307%
53	10.307	2880	2882	2884	rBV3	1636	817	0.09%	0.012%
54	10.333	2886	2890	2892	rVV4	1236	884	0.09%	0.013%
55	10.413	2913	2915	2918	rBV4	1023	683	0.07%	0.010%
56	10.490	2936	2939	2941	rVB3	2093	1122	0.12%	0.016%
57	10.516	2941	2947	2948	rBV5	1320	952	0.10%	0.013%
58	10.815	3038	3040	3042	rVB2	1611	660	0.07%	0.009%
59	10.831	3042	3045	3048	rBV2	1228	1078	0.12%	0.015%
60	10.982	3090	3092	3094	rVB3	1794	735	0.08%	0.010%
61	11.030	3101	3107	3109	rBV7	1358	1287	0.14%	0.018%
62	11.098	3125	3128	3129	rBV3	1129	630	0.07%	0.009%
63	11.136	3133	3140	3144	rBV9	1841	2708	0.29%	0.038%
64	11.185	3145	3155	3173	rBV	404128	624863	66.76%	8.842%
65	11.352	3204	3207	3210	rBV4	1292	836	0.09%	0.012%
66	11.561	3260	3272	3292	rBV	427157	686795	73.38%	9.718%
67	11.963	3394	3397	3404	rVB7	1087	1140	0.12%	0.016%
68	12.008	3407	3411	3416	rBV6	1994	2194	0.23%	0.031%
69	12.156	3454	3457	3460	rVB4	1300	895	0.10%	0.013%
70	12.178	3460	3464	3466	rBV4	1532	1003	0.11%	0.014%
71	12.262	3487	3490	3492	rBV4	1009	596	0.06%	0.008%
72	12.307	3502	3504	3508	rBV4	1040	767	0.08%	0.011%
73	12.503	3560	3565	3567	rBV4	1973	1564	0.17%	0.022%
74	12.561	3581	3583	3586	rBV4	935	610	0.07%	0.009%
75	12.738	3635	3638	3642	rVB6	1249	806	0.09%	0.011%
76	12.760	3642	3645	3649	rVB5	1138	800	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033404.D
 Acq On : 16 Dec 2023 02:09
 Operator : SY/MD
 Sample : VV1215WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.828	3660	3666	3668	rBV7	1394	1334	0.14%	0.019%
78	12.866	3672	3678	3679	rBV6	1369	1326	0.14%	0.019%
79	12.921	3692	3695	3699	rBV5	858	646	0.07%	0.009%
80	13.037	3729	3731	3735	rVB5	1219	599	0.06%	0.008%
81	13.165	3769	3771	3774	rVB4	1344	653	0.07%	0.009%
82	13.204	3774	3783	3791	rBV4	3638	6721	0.72%	0.095%
83	13.361	3828	3832	3835	rVB5	1005	662	0.07%	0.009%
84	13.381	3835	3838	3843	rBV5	1267	1259	0.13%	0.018%
85	13.448	3847	3859	3867	rBV4	4922	9681	1.03%	0.137%
86	13.529	3882	3884	3888	rVV5	946	676	0.07%	0.010%
87	13.654	3920	3923	3925	rBV4	1258	630	0.07%	0.009%
88	13.783	3959	3963	3966	rVB4	1307	1037	0.11%	0.015%
89	13.828	3975	3977	3980	rBV4	1282	642	0.07%	0.009%
90	14.030	4037	4040	4041	rBV3	1434	734	0.08%	0.010%
91	14.056	4045	4048	4053	rVB4	1749	1324	0.14%	0.019%
92	14.361	4137	4143	4147	rBV8	1759	1764	0.19%	0.025%
93	14.432	4162	4165	4167	rBV4	878	608	0.06%	0.009%
94	14.522	4190	4193	4197	rBV4	1309	950	0.10%	0.013%
95	14.808	4278	4282	4286	rBV7	1142	1238	0.13%	0.018%
96	14.879	4301	4304	4305	rBV2	1354	779	0.08%	0.011%
97	14.918	4314	4316	4320	rBV5	1335	1051	0.11%	0.015%
98	15.133	4380	4383	4384	rBV3	1112	728	0.08%	0.010%
99	15.185	4396	4399	4402	rBV4	1608	996	0.11%	0.014%
100	15.352	4449	4451	4456	rBV5	1022	947	0.10%	0.013%




Sum of corrected areas: 7067030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033404.D
Acq On : 16 Dec 2023 02:09
Operator : SY/MD
Sample : VV1215WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

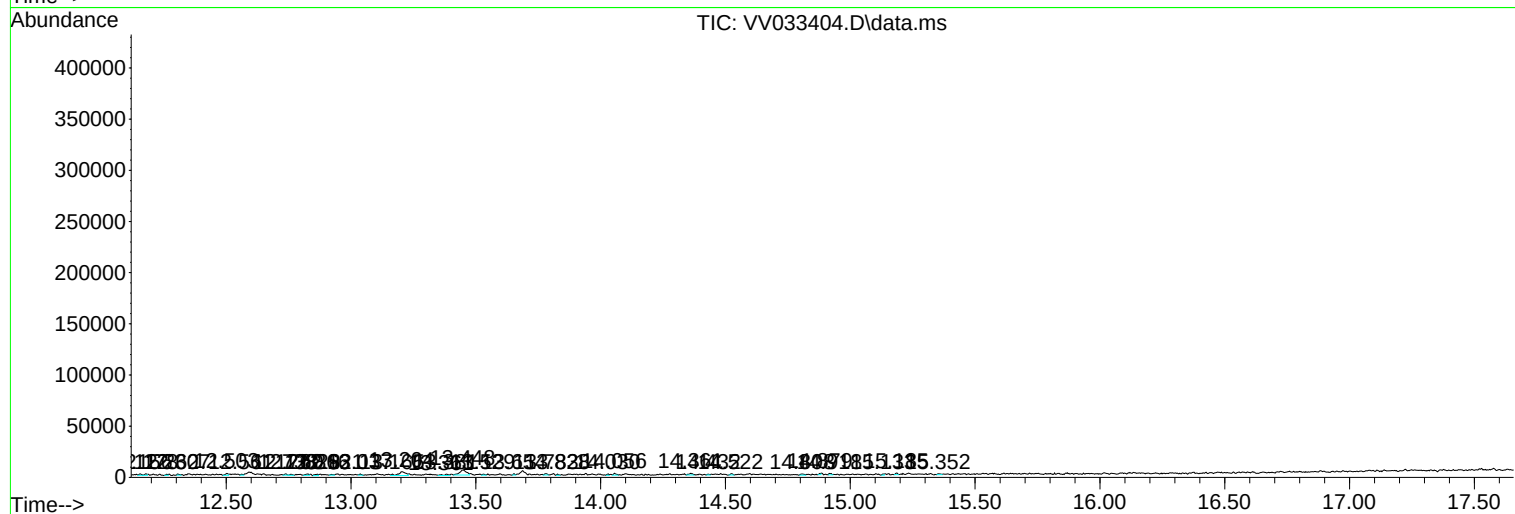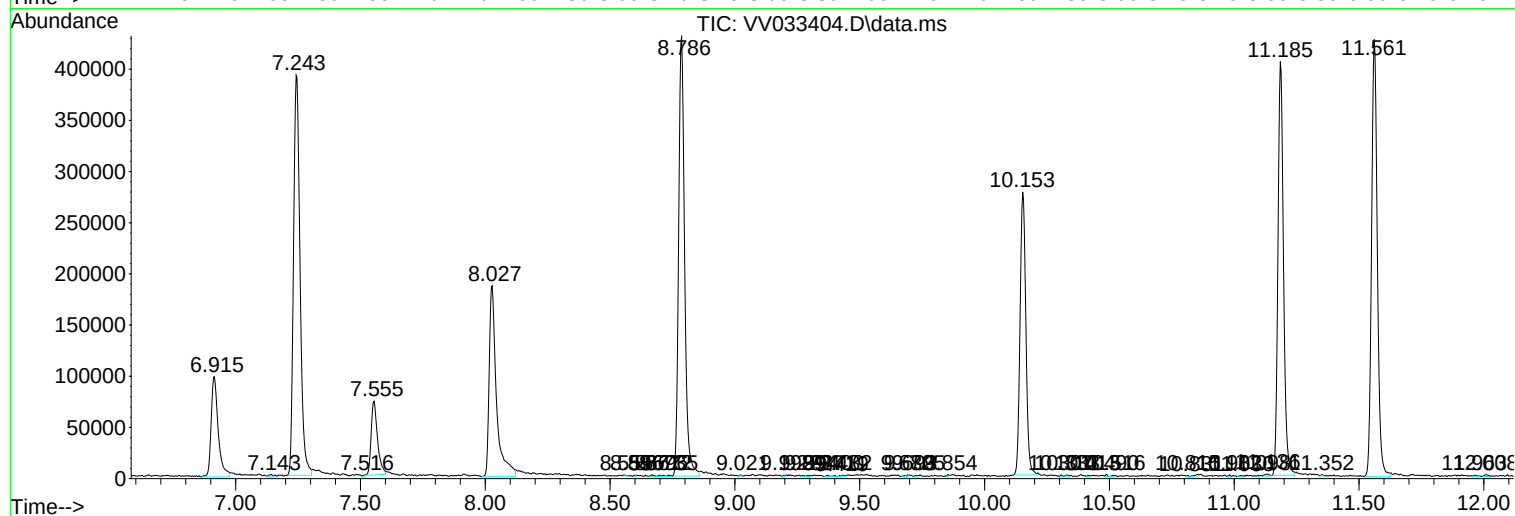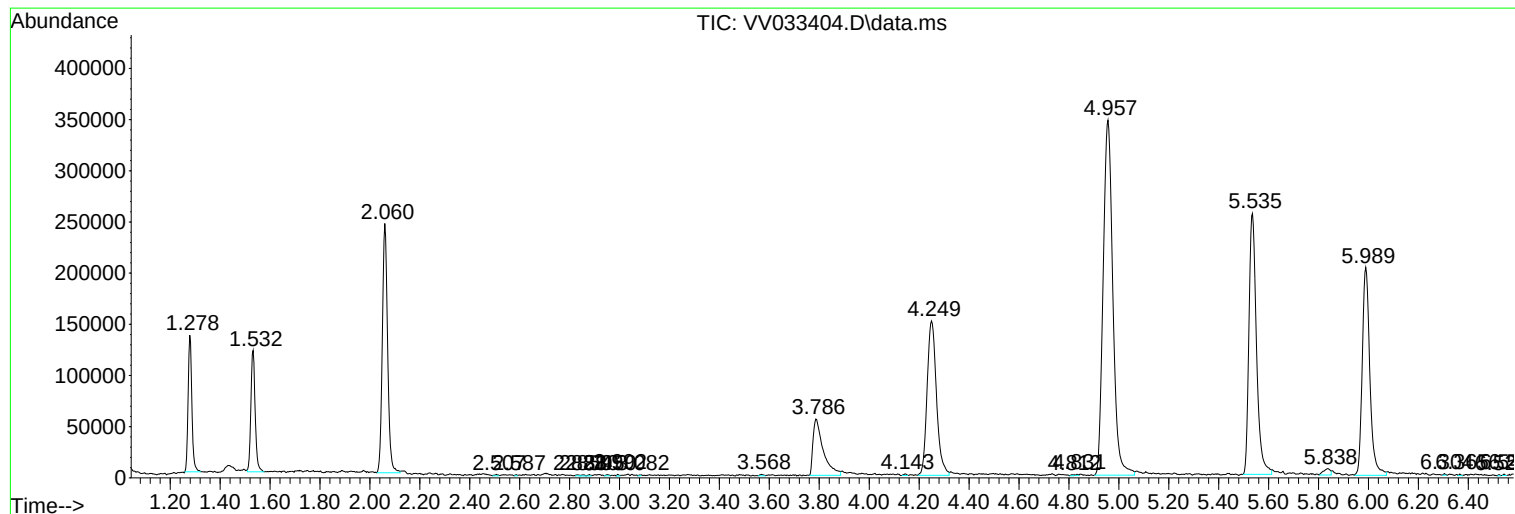

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033404.D
Acq On : 16 Dec 2023 02:09
Operator : SY/MD
Sample : VV1215WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033404.D
Acq On : 16 Dec 2023 02:09
Operator : SY/MD
Sample : VV1215WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------