

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033405.D
 Acq On : 16 Dec 2023 02:32
 Operator : SY/MD
 Sample : 05802-17DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	48	rBV5	1629	1233	0.13%	0.017%
2	1.278	68	74	84	rBV	126013	129960	14.16%	1.826%
3	1.529	146	152	166	rVB	116419	136140	14.83%	1.912%
4	2.060	308	317	341	rVB	231052	348544	37.98%	4.896%
5	2.404	421	424	427	rVB5	1430	821	0.09%	0.012%
6	2.442	427	436	441	rBV5	3454	5184	0.56%	0.073%
7	2.507	451	456	458	rBV5	912	662	0.07%	0.009%
8	2.539	462	466	467	rBV4	1114	750	0.08%	0.011%
9	2.703	504	517	528	rBV3	17667	37496	4.09%	0.527%
10	2.912	579	582	586	rBV5	1235	1099	0.12%	0.015%
11	3.111	637	644	646	rBV6	5188	5939	0.65%	0.083%
12	3.253	686	688	691	rBV3	1128	673	0.07%	0.009%
13	3.323	706	710	712	rBV5	764	643	0.07%	0.009%
14	3.439	743	746	749	rBV3	1172	871	0.09%	0.012%
15	3.474	755	757	760	rBV5	984	670	0.07%	0.009%
16	3.516	767	770	775	rBV6	1024	840	0.09%	0.012%
17	3.609	795	799	804	rBV5	703	829	0.09%	0.012%
18	3.725	832	835	836	rBV3	1530	903	0.10%	0.013%
19	3.786	844	854	885	rBV3	52938	211553	23.05%	2.972%
20	4.246	984	997	1020	rBV	148771	378036	41.19%	5.310%
21	4.783	1162	1164	1169	rVV6	986	714	0.08%	0.010%
22	4.809	1169	1172	1176	rVB6	1207	705	0.08%	0.010%
23	4.957	1202	1218	1253	rBV2	336278	917728	100.00%	12.892%
24	5.275	1313	1317	1318	rBV3	1264	951	0.10%	0.013%
25	5.449	1368	1371	1372	rBV3	1686	934	0.10%	0.013%
26	5.535	1387	1398	1424	rBV2	261498	543252	59.20%	7.631%
27	5.989	1528	1539	1562	rVB	196619	401303	43.73%	5.637%
28	6.346	1647	1650	1652	rBV4	1687	1240	0.14%	0.017%
29	6.687	1752	1756	1759	rBV6	1529	1454	0.16%	0.020%
30	6.912	1816	1826	1846	rVV	94152	179915	19.60%	2.527%
31	7.143	1896	1898	1901	rBV4	1020	660	0.07%	0.009%
32	7.243	1918	1929	1950	rBV	386463	686427	74.80%	9.643%
33	7.551	2016	2025	2046	rBV	69759	128772	14.03%	1.809%
34	7.683	2062	2066	2070	rBV4	1799	1370	0.15%	0.019%
35	7.950	2145	2149	2151	rBV5	1317	1060	0.12%	0.015%
36	8.024	2163	2172	2191	rBV	168645	323487	35.25%	4.544%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033405.D
 Acq On : 16 Dec 2023 02:32
 Operator : SY/MD
 Sample : 05802-17DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.522	2324	2327	2331	rBV7	1416	1078	0.12%	0.015%
38	8.786	2398	2409	2413	rBV	454949	708906	77.25%	9.958%
39	9.133	2515	2517	2520	rBV4	1034	732	0.08%	0.010%
40	9.198	2535	2537	2541	rBV5	1041	659	0.07%	0.009%
41	9.320	2573	2575	2578	rBV3	1221	665	0.07%	0.009%
42	9.371	2588	2591	2593	rBV4	1138	644	0.07%	0.009%
43	9.481	2623	2625	2628	rBV3	1324	636	0.07%	0.009%
44	9.667	2679	2683	2688	rBV8	885	941	0.10%	0.013%
45	9.719	2696	2699	2702	rBV4	1710	950	0.10%	0.013%
46	9.866	2740	2745	2746	rBV4	2315	1747	0.19%	0.025%
47	9.928	2760	2764	2766	rBV4	1286	898	0.10%	0.013%
48	9.950	2768	2771	2776	rBV7	1290	1086	0.12%	0.015%
49	10.063	2803	2806	2809	rBV5	1237	768	0.08%	0.011%
50	10.092	2813	2815	2818	rVB4	1470	766	0.08%	0.011%
51	10.153	2818	2834	2851	rBV	270167	441004	48.05%	6.195%
52	10.333	2887	2890	2891	rBV3	1537	692	0.08%	0.010%
53	10.371	2898	2902	2906	rBV6	1114	934	0.10%	0.013%
54	10.529	2948	2951	2953	rBV4	1031	620	0.07%	0.009%
55	10.603	2970	2974	2976	rBV5	997	792	0.09%	0.011%
56	10.670	2992	2995	2998	rVB4	1523	902	0.10%	0.013%
57	10.696	2998	3003	3005	rBV5	1365	1169	0.13%	0.016%
58	10.789	3028	3032	3035	rBV5	2001	1916	0.21%	0.027%
59	10.860	3050	3054	3061	rBV8	1805	2297	0.25%	0.032%
60	10.937	3076	3078	3081	rBV3	1328	957	0.10%	0.013%
61	10.963	3084	3086	3091	rVB5	971	768	0.08%	0.011%
62	11.027	3104	3106	3112	rVB4	1413	994	0.11%	0.014%
63	11.120	3125	3135	3145	rBV	19552	32040	3.49%	0.450%
64	11.185	3145	3155	3180	rVB2	412845	721864	78.66%	10.140%
65	11.378	3210	3215	3216	rBV5	1247	832	0.09%	0.012%
66	11.561	3260	3272	3295	rBV	424468	694990	75.73%	9.763%
67	11.828	3352	3355	3356	rBV3	1374	658	0.07%	0.009%
68	11.863	3362	3366	3369	rBV6	1732	1205	0.13%	0.017%
69	11.882	3369	3372	3375	rVB4	1702	1279	0.14%	0.018%
70	11.921	3379	3384	3385	rBV5	1036	693	0.08%	0.010%
71	12.091	3433	3437	3438	rBV4	1161	679	0.07%	0.010%
72	12.156	3454	3457	3461	rVB4	1162	803	0.09%	0.011%
73	12.191	3466	3468	3475	rVV6	1333	1074	0.12%	0.015%
74	12.304	3497	3503	3507	rBV7	1643	1452	0.16%	0.020%
75	12.374	3522	3525	3531	rBV7	1807	1487	0.16%	0.021%
76	12.464	3550	3553	3557	rVB6	1262	916	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033405.D
 Acq On : 16 Dec 2023 02:32
 Operator : SY/MD
 Sample : 05802-17DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.487	3557	3560	3563	rBV4	748	655	0.07%	0.009%
78	12.506	3563	3566	3569	rBV4	1140	848	0.09%	0.012%
79	12.648	3606	3610	3612	rBV5	1103	722	0.08%	0.010%
80	12.796	3652	3656	3658	rBV5	967	638	0.07%	0.009%
81	12.950	3700	3704	3706	rBV5	1020	800	0.09%	0.011%
82	13.040	3729	3732	3735	rBV5	1205	1108	0.12%	0.016%
83	13.088	3744	3747	3748	rBV3	1558	792	0.09%	0.011%
84	13.153	3765	3767	3772	rVB5	1347	786	0.09%	0.011%
85	13.204	3778	3783	3789	rBV9	3263	4640	0.51%	0.065%
86	13.410	3838	3847	3851	rBV9	1999	2450	0.27%	0.034%
87	13.455	3853	3861	3865	rBV8	2663	4175	0.45%	0.059%
88	13.538	3884	3887	3892	rBV7	755	788	0.09%	0.011%
89	13.686	3927	3933	3936	rBV8	3047	3689	0.40%	0.052%
90	13.792	3964	3966	3968	rBV3	1117	623	0.07%	0.009%
91	14.005	4028	4032	4033	rBV5	1304	744	0.08%	0.010%
92	14.082	4052	4056	4057	rBV4	1080	681	0.07%	0.010%
93	14.207	4092	4095	4098	rBV3	830	777	0.08%	0.011%
94	14.439	4162	4167	4172	rBV8	1292	1571	0.17%	0.022%
95	14.532	4194	4196	4200	rBV4	1692	1124	0.12%	0.016%
96	14.590	4212	4214	4219	rVV5	1505	1189	0.13%	0.017%
97	14.805	4278	4281	4284	rBV5	1255	1210	0.13%	0.017%
98	15.033	4349	4352	4354	rBV4	1010	651	0.07%	0.009%
99	15.255	4418	4421	4424	rBV5	1333	764	0.08%	0.011%
100	15.686	4552	4555	4559	rBV4	1199	982	0.11%	0.014%




Sum of corrected areas: 7118718

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033405.D
Acq On : 16 Dec 2023 02:32
Operator : SY/MD
Sample : 05802-17DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

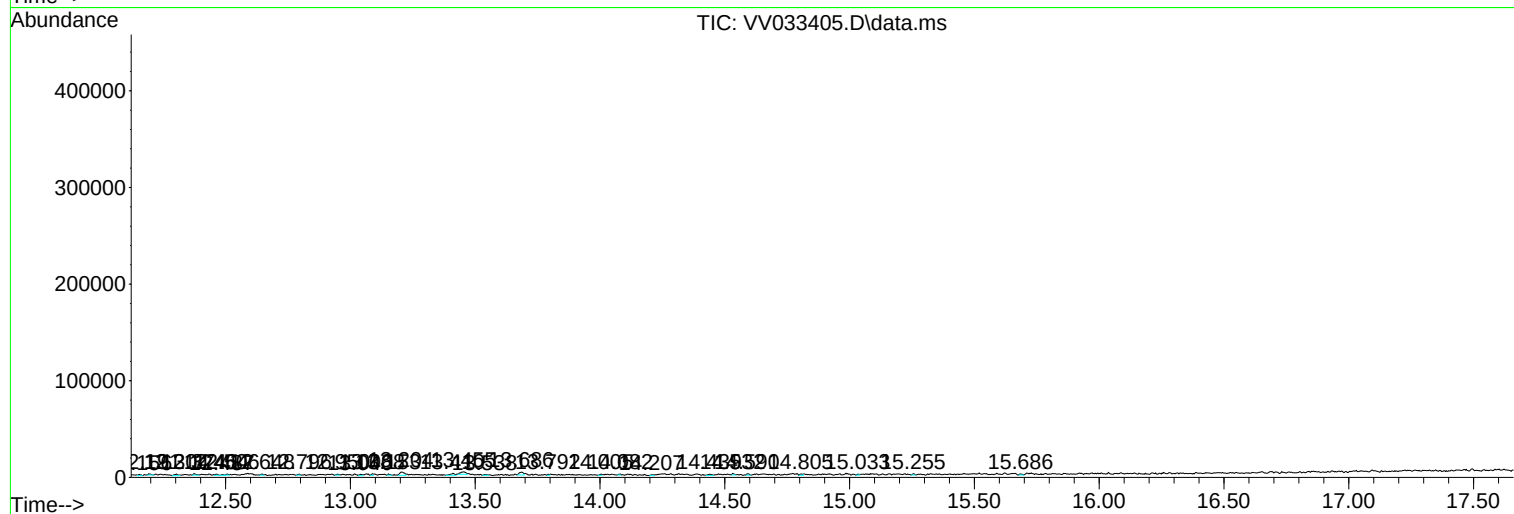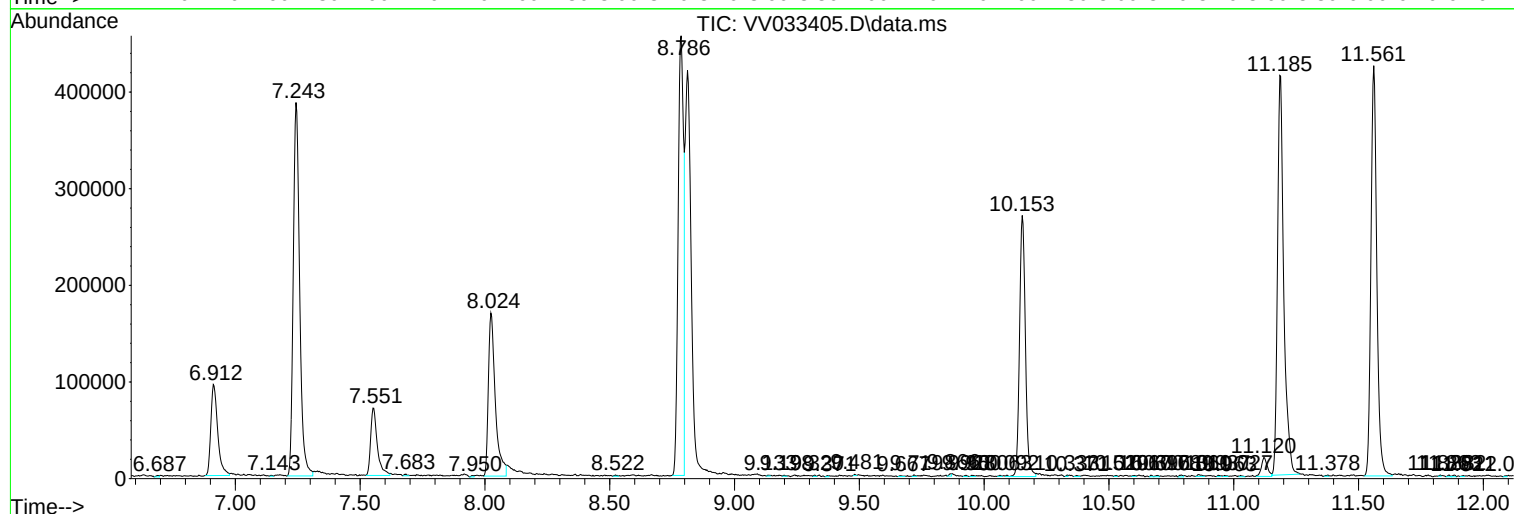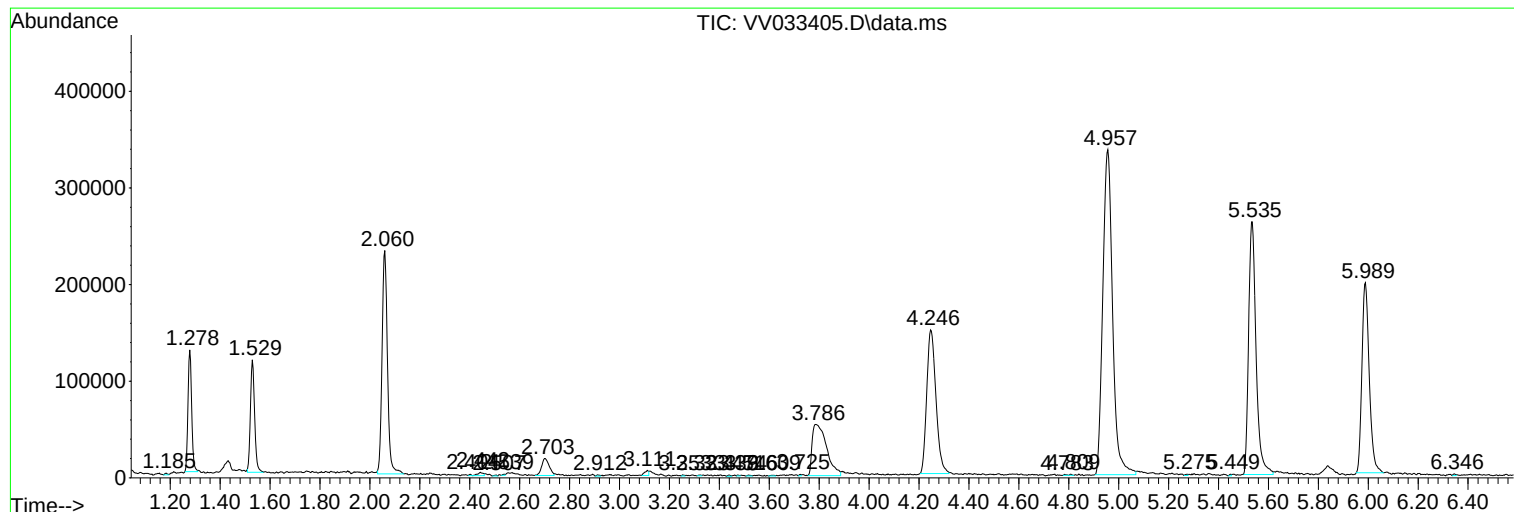

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033405.D
Acq On : 16 Dec 2023 02:32
Operator : SY/MD
Sample : 05802-17DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033405.D
Acq On : 16 Dec 2023 02:32
Operator : SY/MD
Sample : 05802-17DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------