

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033406.D
 Acq On : 16 Dec 2023 02:55
 Operator : SY/MD
 Sample : 05802-02DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	133193	137459	14.75%	1.881%
2	1.532	146	153	165	rVB	116140	136793	14.68%	1.872%
3	2.066	308	319	334	rBV3	383474	649147	69.67%	8.885%
4	2.536	461	465	468	rBV4	1753	1461	0.16%	0.020%
5	2.603	483	486	490	rVV5	746	634	0.07%	0.009%
6	2.674	505	508	510	rBV3	930	675	0.07%	0.009%
7	2.815	549	552	554	rBV4	1256	608	0.07%	0.008%
8	2.986	600	605	606	rBV5	1153	969	0.10%	0.013%
9	3.085	633	636	637	rBV2	1530	859	0.09%	0.012%
10	3.117	644	646	649	rVB4	1170	606	0.07%	0.008%
11	3.256	687	689	691	rBV3	1370	627	0.07%	0.009%
12	3.471	750	756	759	rBV7	1481	1514	0.16%	0.021%
13	3.542	775	778	780	rBV4	880	599	0.06%	0.008%
14	3.635	802	807	808	rBV3	893	672	0.07%	0.009%
15	3.741	838	840	845	rBV5	1081	686	0.07%	0.009%
16	3.786	845	854	876	rBV	51676	142618	15.31%	1.952%
17	4.063	936	940	942	rBV4	1117	960	0.10%	0.013%
18	4.108	949	954	955	rBV4	1264	927	0.10%	0.013%
19	4.249	984	998	1024	rBV2	150540	380521	40.84%	5.208%
20	4.680	1129	1132	1134	rBV4	1240	599	0.06%	0.008%
21	4.799	1167	1169	1172	rBV3	1180	803	0.09%	0.011%
22	4.844	1178	1183	1184	rBV5	1341	891	0.10%	0.012%
23	4.957	1200	1218	1249	rBV2	350012	931682	100.00%	12.753%
24	5.404	1354	1357	1359	rBV4	1608	1053	0.11%	0.014%
25	5.535	1386	1398	1425	rBV2	266263	554727	59.54%	7.593%
26	5.989	1524	1539	1565	rBV	205950	431325	46.30%	5.904%
27	6.121	1578	1580	1583	rBV3	1729	925	0.10%	0.013%
28	6.407	1665	1669	1671	rBV4	1421	1118	0.12%	0.015%
29	6.452	1681	1683	1688	rVB6	2420	1550	0.17%	0.021%
30	6.484	1688	1693	1698	rBV8	1429	1911	0.21%	0.026%
31	6.535	1707	1709	1711	rBV3	1431	721	0.08%	0.010%
32	6.619	1730	1735	1736	rBV4	1495	1125	0.12%	0.015%
33	6.683	1752	1755	1756	rBV3	1302	772	0.08%	0.011%
34	6.728	1765	1769	1772	rBV6	1506	1069	0.11%	0.015%
35	6.751	1772	1776	1778	rBV5	1488	1018	0.11%	0.014%
36	6.912	1814	1826	1845	rBV	99210	190992	20.50%	2.614%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033406.D
 Acq On : 16 Dec 2023 02:55
 Operator : SY/MD
 Sample : 05802-02DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.194	1912	1914	1916	rBV2	1122	685	0.07%	0.009%
38	7.243	1918	1929	1950	rBV	397028	701249	75.27%	9.598%
39	7.555	2017	2026	2039	rBV2	72438	127397	13.67%	1.744%
40	7.908	2133	2136	2138	rBV4	1651	920	0.10%	0.013%
41	8.027	2164	2173	2197	rBV	180730	350357	37.60%	4.796%
42	8.574	2341	2343	2345	rBV3	1064	681	0.07%	0.009%
43	8.606	2351	2353	2360	rVB7	1553	1275	0.14%	0.017%
44	8.654	2363	2368	2370	rBV4	1162	998	0.11%	0.014%
45	8.715	2383	2387	2390	rBV5	1032	946	0.10%	0.013%
46	8.786	2397	2409	2432	rBV	436514	732364	78.61%	10.024%
47	9.387	2593	2596	2597	rBV2	1053	669	0.07%	0.009%
48	9.439	2608	2612	2614	rBV4	1146	909	0.10%	0.012%
49	9.452	2614	2616	2620	rVB5	1320	834	0.09%	0.011%
50	9.471	2620	2622	2625	rBV3	1097	659	0.07%	0.009%
51	9.709	2693	2696	2698	rBV3	1930	856	0.09%	0.012%
52	9.741	2702	2706	2709	rBV6	1562	1267	0.14%	0.017%
53	9.940	2765	2768	2769	rBV	1009	612	0.07%	0.008%
54	10.153	2823	2834	2856	rVB	276849	442728	47.52%	6.060%
55	10.442	2921	2924	2925	rBV3	996	595	0.06%	0.008%
56	10.635	2981	2984	2989	rBV6	1582	1458	0.16%	0.020%
57	10.792	3031	3033	3036	rBV4	1028	663	0.07%	0.009%
58	10.915	3067	3071	3073	rVB4	1048	801	0.09%	0.011%
59	10.944	3075	3080	3084	rBV6	1712	1912	0.21%	0.026%
60	11.127	3130	3137	3141	rBV8	2050	2898	0.31%	0.040%
61	11.185	3144	3155	3174	rBV	403416	634762	68.13%	8.688%
62	11.342	3202	3204	3210	rVB8	2025	1269	0.14%	0.017%
63	11.445	3234	3236	3239	rVB3	1337	617	0.07%	0.008%
64	11.561	3257	3272	3292	rBV	425917	683607	73.37%	9.357%
65	11.837	3355	3358	3359	rBV3	1183	665	0.07%	0.009%
66	11.918	3381	3383	3385	rBV3	1134	672	0.07%	0.009%
67	12.069	3427	3430	3432	rBV3	1342	876	0.09%	0.012%
68	12.185	3464	3466	3470	rVV5	1242	767	0.08%	0.010%
69	12.281	3492	3496	3498	rBV5	1517	1160	0.12%	0.016%
70	12.413	3532	3537	3540	rBV5	1361	1193	0.13%	0.016%
71	12.432	3540	3543	3546	rBV3	1095	764	0.08%	0.010%
72	12.667	3612	3616	3620	rVB7	1371	1217	0.13%	0.017%
73	12.818	3660	3663	3666	rBV4	1887	1146	0.12%	0.016%
74	12.847	3669	3672	3674	rBV3	1387	735	0.08%	0.010%
75	12.882	3679	3683	3685	rBV3	1180	878	0.09%	0.012%
76	12.911	3688	3692	3695	rBV6	979	802	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033406.D
 Acq On : 16 Dec 2023 02:55
 Operator : SY/MD
 Sample : 05802-02DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.059	3734	3738	3740	rBV4	868	705	0.08%	0.010%
78	13.082	3743	3745	3747	rBV3	1481	1024	0.11%	0.014%
79	13.178	3773	3775	3779	rBV5	1097	776	0.08%	0.011%
80	13.304	3810	3814	3816	rVB4	1127	757	0.08%	0.010%
81	13.326	3816	3821	3828	rBV8	1744	1987	0.21%	0.027%
82	13.439	3853	3856	3857	rBV3	1670	995	0.11%	0.014%
83	13.680	3929	3931	3932	rBV2	1487	704	0.08%	0.010%
84	13.789	3962	3965	3969	rBV5	1324	879	0.09%	0.012%
85	13.805	3969	3970	3973	rBV3	1048	670	0.07%	0.009%
86	14.152	4073	4078	4079	rBV5	951	655	0.07%	0.009%
87	14.316	4127	4129	4133	rVB4	1643	657	0.07%	0.009%
88	14.336	4133	4135	4137	rBV2	1093	586	0.06%	0.008%
89	14.435	4163	4166	4170	rBV5	1712	1427	0.15%	0.020%
90	14.455	4170	4172	4175	rVV2	1778	964	0.10%	0.013%
91	14.548	4199	4201	4204	rVV3	1513	1037	0.11%	0.014%
92	14.635	4226	4228	4230	rBV2	1192	725	0.08%	0.010%
93	14.734	4256	4259	4262	rBV4	1205	800	0.09%	0.011%
94	14.750	4262	4264	4267	rVB4	1363	625	0.07%	0.009%
95	14.795	4276	4278	4281	rBV4	1030	631	0.07%	0.009%
96	14.953	4325	4327	4329	rBV3	1296	695	0.07%	0.010%
97	15.300	4433	4435	4438	rVB4	1198	772	0.08%	0.011%
98	15.326	4438	4443	4445	rBV5	1562	1069	0.11%	0.015%
99	15.532	4505	4507	4510	rBV4	1182	659	0.07%	0.009%
100	15.763	4577	4579	4581	rBV3	1303	589	0.06%	0.008%




Sum of corrected areas: 7305867

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033406.D
Acq On : 16 Dec 2023 02:55
Operator : SY/MD
Sample : 05802-02DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

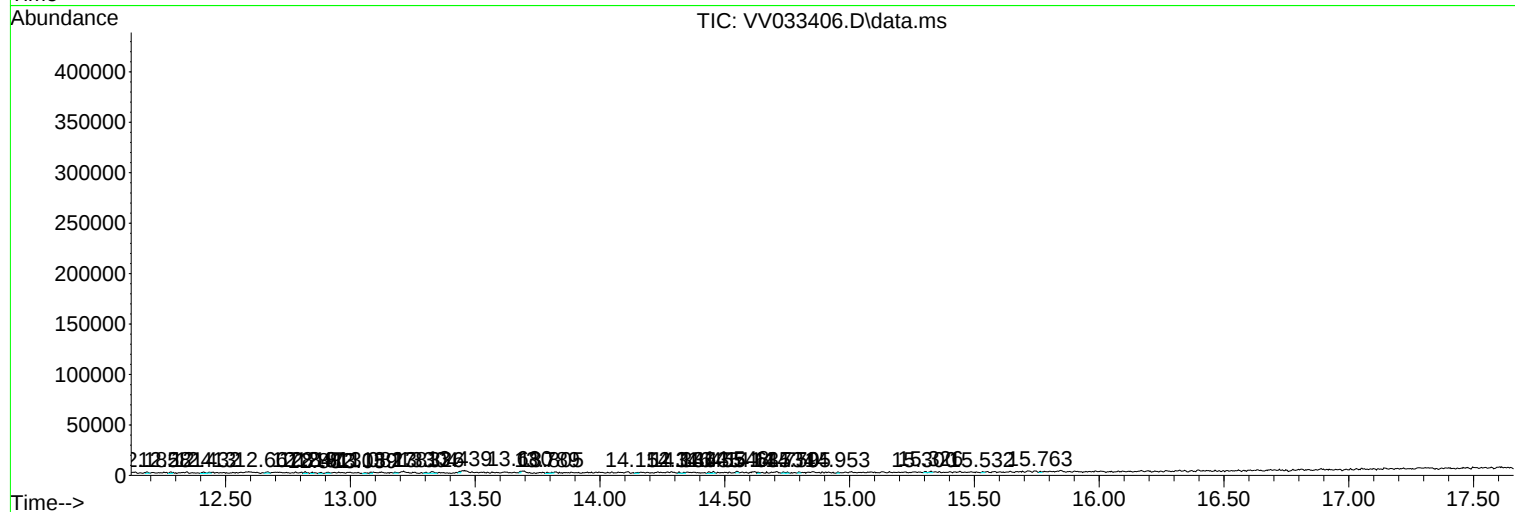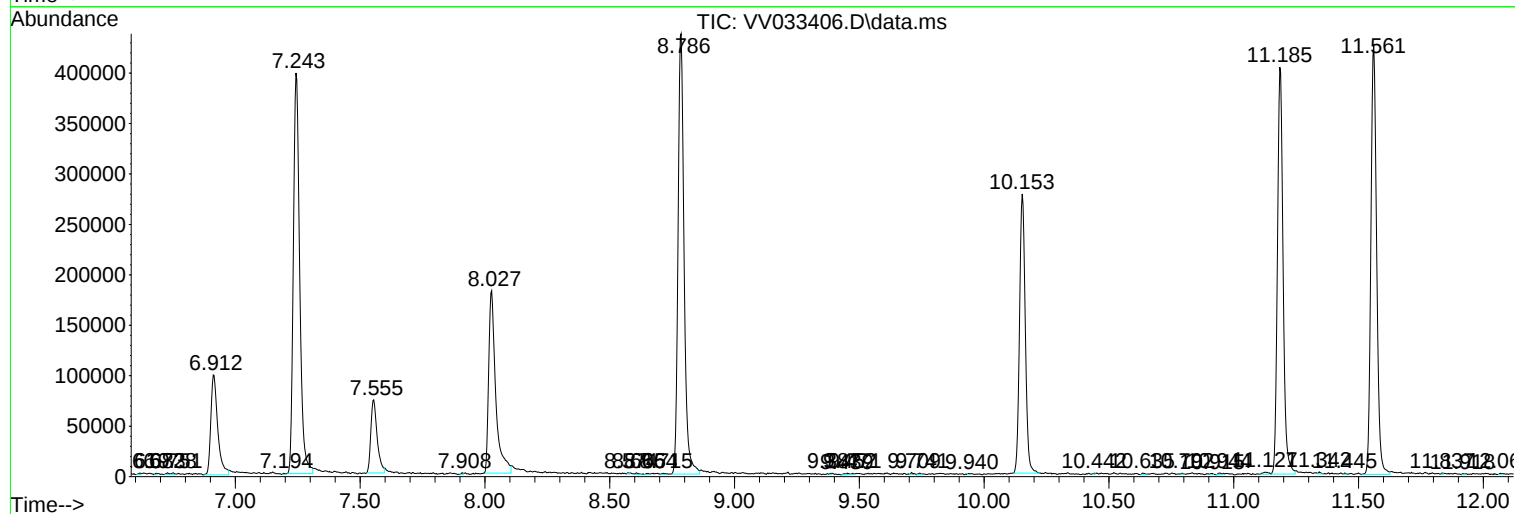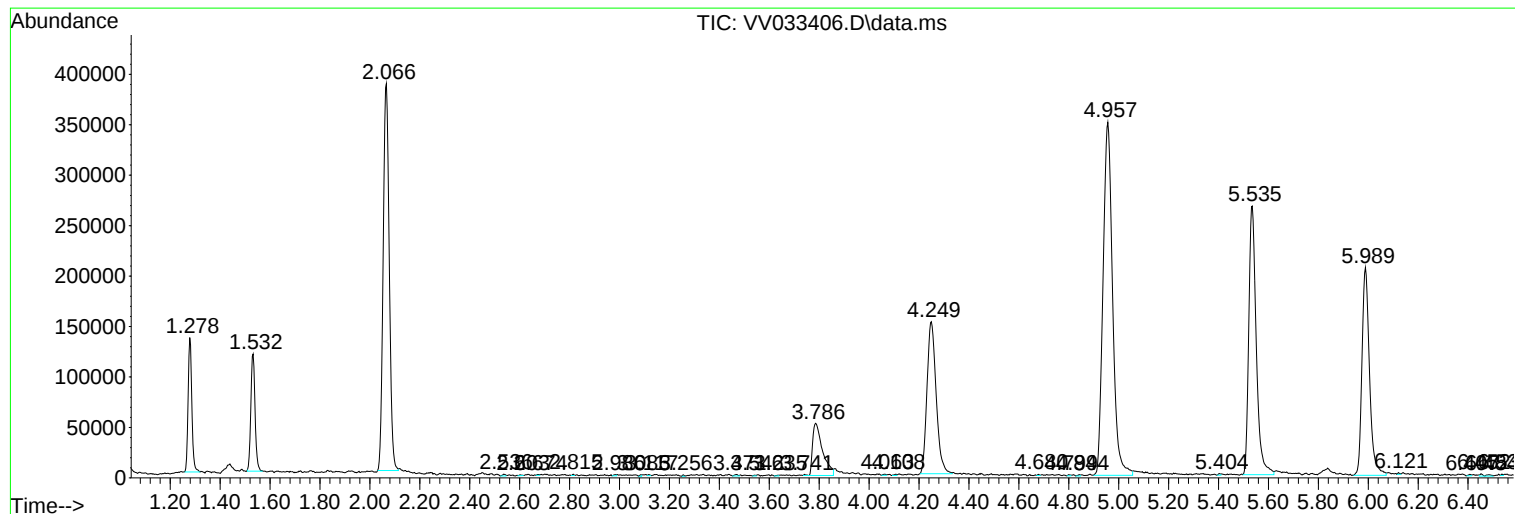

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033406.D
Acq On : 16 Dec 2023 02:55
Operator : SY/MD
Sample : 05802-02DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033406.D
Acq On : 16 Dec 2023 02:55
Operator : SY/MD
Sample : 05802-02DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc