

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033407.D
 Acq On : 16 Dec 2023 03:18
 Operator : SY/MD
 Sample : 05802-16DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B28DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	130188	135192	14.47%	1.896%
2	1.532	146	153	166	rVB	120405	136623	14.62%	1.916%
3	2.060	308	317	331	rBV	229085	331739	35.51%	4.653%
4	2.275	380	384	389	rBV6	1969	1954	0.21%	0.027%
5	2.561	470	473	479	rBV5	1310	1311	0.14%	0.018%
6	2.613	486	489	492	rVB4	830	611	0.07%	0.009%
7	2.658	500	503	505	rBV3	876	595	0.06%	0.008%
8	2.706	505	518	532	rVV2	15987	35227	3.77%	0.494%
9	2.870	565	569	572	rBV5	1187	978	0.10%	0.014%
10	2.896	575	577	580	rVB4	1072	633	0.07%	0.009%
11	2.960	595	597	599	rBV3	1375	747	0.08%	0.010%
12	3.095	637	639	640	rBV2	1754	786	0.08%	0.011%
13	3.204	667	673	674	rBV5	1216	936	0.10%	0.013%
14	3.288	697	699	703	rBV5	1095	694	0.07%	0.010%
15	3.690	822	824	826	rBV3	1224	643	0.07%	0.009%
16	3.754	841	844	846	rBV2	1507	999	0.11%	0.014%
17	3.786	846	854	878	rBV	50895	142162	15.22%	1.994%
18	4.159	968	970	972	rBV2	1198	570	0.06%	0.008%
19	4.188	978	979	982	rBV3	1109	726	0.08%	0.010%
20	4.249	984	998	1022	rVV2	151930	386396	41.36%	5.419%
21	4.654	1121	1124	1126	rBV4	975	681	0.07%	0.010%
22	4.796	1165	1168	1170	rBV4	839	557	0.06%	0.008%
23	4.825	1174	1177	1185	rBV7	1001	1374	0.15%	0.019%
24	4.957	1201	1218	1250	rBV3	347873	934211	100.00%	13.102%
25	5.535	1386	1398	1423	rBV	255450	534882	57.25%	7.502%
26	5.834	1478	1491	1505	rBV	6300	16813	1.80%	0.236%
27	5.989	1527	1539	1558	rBV	203647	417632	44.70%	5.857%
28	6.342	1647	1649	1652	rBV4	1161	574	0.06%	0.008%
29	6.645	1740	1743	1746	rVB5	1599	930	0.10%	0.013%
30	6.677	1750	1753	1758	rBV6	1374	1278	0.14%	0.018%
31	6.799	1784	1791	1793	rBV6	1267	1359	0.15%	0.019%
32	6.915	1817	1827	1850	rBV	95930	182500	19.54%	2.560%
33	7.195	1912	1914	1916	rBV3	1129	710	0.08%	0.010%
34	7.243	1918	1929	1956	rVV	399042	697209	74.63%	9.778%
35	7.551	2017	2025	2039	rBV	69134	120234	12.87%	1.686%
36	7.883	2125	2128	2132	rBV5	1049	1139	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033407.D
 Acq On : 16 Dec 2023 03:18
 Operator : SY/MD
 Sample : 05802-16DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B28DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.912	2135	2137	2141	rVB4	2264	1264	0.14%	0.018%
38	7.969	2153	2155	2158	rBV4	1202	647	0.07%	0.009%
39	7.989	2158	2161	2163	rBV3	1016	676	0.07%	0.009%
40	8.027	2163	2173	2203	rBV	176586	361258	38.67%	5.067%
41	8.564	2338	2340	2346	rVB6	2014	2056	0.22%	0.029%
42	8.596	2346	2350	2352	rBV4	1366	962	0.10%	0.013%
43	8.664	2369	2371	2374	rBV3	2170	1196	0.13%	0.017%
44	8.786	2398	2409	2414	rBV	448222	737871	78.98%	10.349%
45	9.185	2531	2533	2536	rBV3	1193	683	0.07%	0.010%
46	9.275	2558	2561	2564	rBV4	1096	691	0.07%	0.010%
47	9.500	2625	2631	2635	rBV7	1511	1671	0.18%	0.023%
48	9.628	2667	2671	2676	rVB8	1389	1184	0.13%	0.017%
49	9.651	2676	2678	2680	rBV3	1194	591	0.06%	0.008%
50	9.850	2734	2740	2745	rBV9	1778	2308	0.25%	0.032%
51	10.153	2823	2834	2852	rBV	275163	441553	47.26%	6.193%
52	10.333	2887	2890	2893	rBV5	1495	971	0.10%	0.014%
53	10.384	2903	2906	2907	rBV2	1209	685	0.07%	0.010%
54	10.481	2934	2936	2939	rVB3	1182	605	0.06%	0.008%
55	10.497	2939	2941	2942	rBV2	1068	565	0.06%	0.008%
56	10.571	2962	2964	2969	rVB6	1915	1296	0.14%	0.018%
57	10.641	2980	2986	2990	rVB7	1064	1147	0.12%	0.016%
58	10.828	3043	3044	3048	rBV4	1020	698	0.07%	0.010%
59	10.857	3050	3053	3057	rVB6	1694	1068	0.11%	0.015%
60	10.886	3060	3062	3066	rVB5	1099	601	0.06%	0.008%
61	10.927	3073	3075	3079	rBV4	1038	835	0.09%	0.012%
62	11.079	3118	3122	3126	rBV4	971	836	0.09%	0.012%
63	11.124	3126	3136	3144	rBV4	16436	26954	2.89%	0.378%
64	11.185	3145	3155	3179	rVV	398375	699376	74.86%	9.809%
65	11.317	3192	3196	3198	rBV5	2010	1550	0.17%	0.022%
66	11.464	3238	3242	3243	rBV3	1777	1227	0.13%	0.017%
67	11.561	3257	3272	3292	rBV	435846	714702	76.50%	10.024%
68	11.915	3380	3382	3385	rBV3	1284	770	0.08%	0.011%
69	12.278	3491	3495	3498	rBV4	1055	741	0.08%	0.010%
70	12.378	3522	3526	3528	rBV3	968	789	0.08%	0.011%
71	12.580	3588	3589	3593	rVB3	1333	636	0.07%	0.009%
72	12.599	3593	3595	3598	rVB3	1063	555	0.06%	0.008%
73	12.622	3598	3602	3603	rBV4	867	593	0.06%	0.008%
74	12.754	3637	3643	3647	rBV8	1496	1856	0.20%	0.026%
75	12.870	3675	3679	3680	rBV2	1025	677	0.07%	0.009%
76	13.037	3729	3731	3734	rVB4	1387	689	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033407.D
 Acq On : 16 Dec 2023 03:18
 Operator : SY/MD
 Sample : 05802-16DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B28DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.059	3736	3738	3743	rBV7	1004	891	0.10%	0.012%
78	13.207	3778	3784	3792	rBV7	1904	2677	0.29%	0.038%
79	13.345	3823	3827	3833	rBV9	944	1211	0.13%	0.017%
80	13.451	3856	3860	3861	rBV4	1748	1120	0.12%	0.016%
81	13.638	3916	3918	3923	rVB4	1345	1137	0.12%	0.016%
82	13.677	3928	3930	3931	rBV2	1369	581	0.06%	0.008%
83	13.860	3984	3987	3991	rBV5	1078	824	0.09%	0.012%
84	13.943	4007	4013	4015	rBV5	1159	1143	0.12%	0.016%
85	13.985	4023	4026	4030	rBV6	1328	1266	0.14%	0.018%
86	14.005	4030	4032	4035	rVV3	838	590	0.06%	0.008%
87	14.091	4055	4059	4060	rBV5	1076	794	0.08%	0.011%
88	14.252	4104	4109	4110	rBV4	1531	985	0.11%	0.014%
89	14.291	4117	4121	4124	rBV5	989	887	0.09%	0.012%
90	14.323	4129	4131	4135	rVB4	951	639	0.07%	0.009%
91	14.374	4144	4147	4150	rBV4	1322	987	0.11%	0.014%
92	14.532	4193	4196	4200	rBV4	1332	1259	0.13%	0.018%
93	14.654	4231	4234	4236	rBV3	1261	712	0.08%	0.010%
94	14.689	4241	4245	4246	rBV3	1059	685	0.07%	0.010%
95	14.908	4310	4313	4314	rBV2	1180	589	0.06%	0.008%
96	14.976	4332	4334	4337	rBV4	893	614	0.07%	0.009%
97	15.027	4349	4350	4353	rBV3	977	729	0.08%	0.010%
98	15.062	4357	4361	4366	rBV6	1402	1424	0.15%	0.020%
99	15.683	4552	4554	4555	rBV2	1403	596	0.06%	0.008%
100	16.069	4672	4674	4676	rBV3	1736	1091	0.12%	0.015%




Sum of corrected areas: 7130069

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033407.D
Acq On : 16 Dec 2023 03:18
Operator : SY/MD
Sample : 05802-16DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

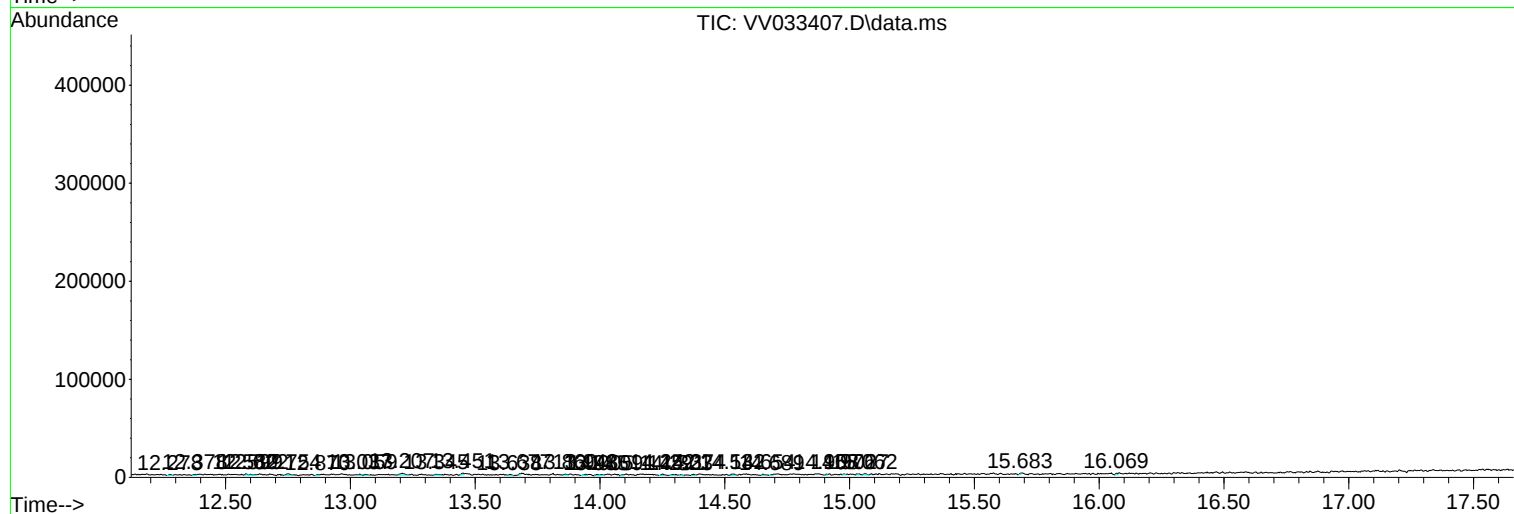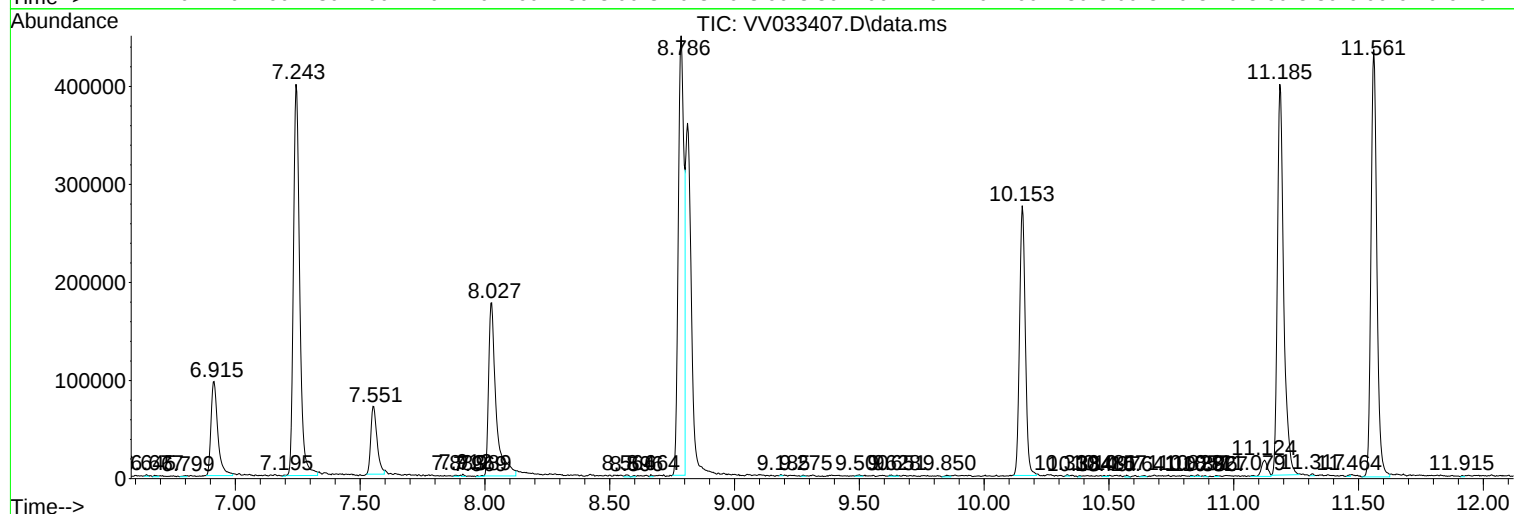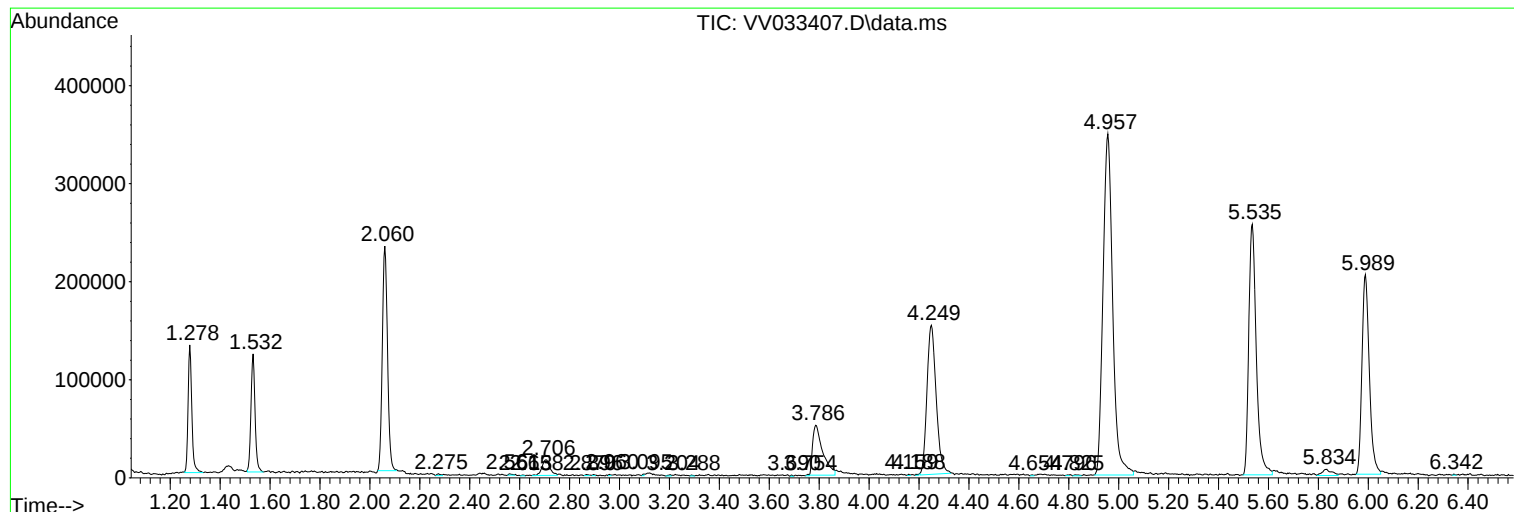

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033407.D
Acq On : 16 Dec 2023 03:18
Operator : SY/MD
Sample : 05802-16DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033407.D
Acq On : 16 Dec 2023 03:18
Operator : SY/MD
Sample : 05802-16DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------