

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033408.D
 Acq On : 16 Dec 2023 03:41
 Operator : SY/MD
 Sample : 05802-18DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B31DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV2	149909	160391	17.17%	2.096%
2	1.532	146	153	168	rVB	117849	140219	15.01%	1.833%
3	2.060	308	317	330	rBV	231463	332661	35.61%	4.348%
4	2.529	460	463	464	rBV3	1156	670	0.07%	0.009%
5	2.883	571	573	575	rBV4	1069	403	0.04%	0.005%
6	2.921	583	585	586	rBV2	1027	404	0.04%	0.005%
7	3.044	620	623	624	rBV2	908	452	0.05%	0.006%
8	3.056	625	627	629	rVV3	1045	444	0.05%	0.006%
9	3.204	669	673	674	rBV2	1474	1149	0.12%	0.015%
10	3.307	702	705	707	rBV4	739	413	0.04%	0.005%
11	3.439	744	746	750	rVB5	994	528	0.06%	0.007%
12	3.455	750	751	753	rBV2	855	349	0.04%	0.005%
13	3.478	756	758	759	rBV	1071	418	0.04%	0.005%
14	3.523	771	772	774	rBV2	812	351	0.04%	0.005%
15	3.700	826	827	830	rVB3	1162	361	0.04%	0.005%
16	3.716	830	832	834	rBV3	1238	604	0.06%	0.008%
17	3.728	834	836	839	rVV3	1062	532	0.06%	0.007%
18	3.812	845	862	891	rBV3	235435	681627	72.96%	8.909%
19	4.249	985	998	1027	rVB	148824	381327	40.82%	4.984%
20	4.484	1068	1071	1073	rBV4	1548	951	0.10%	0.012%
21	4.957	1202	1218	1248	rVV2	342611	934255	100.00%	12.211%
22	5.535	1387	1398	1427	rBV	263408	537861	57.57%	7.030%
23	5.989	1527	1539	1561	rBV	203175	415406	44.46%	5.430%
24	6.449	1680	1682	1685	rBV3	723	425	0.05%	0.006%
25	6.597	1726	1728	1732	rBV5	1298	1216	0.13%	0.016%
26	6.648	1741	1744	1749	rVB6	1220	1016	0.11%	0.013%
27	6.796	1785	1790	1793	rBV4	2103	1465	0.16%	0.019%
28	6.915	1815	1827	1848	rBV	97498	189103	20.24%	2.472%
29	7.243	1918	1929	1950	rBV	391996	699466	74.87%	9.142%
30	7.555	2017	2026	2042	rBV2	71154	125767	13.46%	1.644%
31	7.703	2070	2072	2075	rBV3	930	607	0.06%	0.008%
32	7.812	2104	2106	2108	rBV2	939	459	0.05%	0.006%
33	7.860	2119	2121	2123	rBV3	1284	546	0.06%	0.007%
34	7.963	2150	2153	2154	rBV4	944	572	0.06%	0.007%
35	8.027	2163	2173	2203	rBV	182095	357805	38.30%	4.677%
36	8.574	2341	2343	2345	rBV3	1112	672	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033408.D
 Acq On : 16 Dec 2023 03:41
 Operator : SY/MD
 Sample : 05802-18DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B31DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.693	2378	2380	2382	rVB2	1040	347	0.04%	0.005%
38	8.706	2382	2384	2386	rBV3	1144	535	0.06%	0.007%
39	8.735	2390	2393	2397	rVB5	877	706	0.08%	0.009%
40	8.786	2397	2409	2436	rBV	437106	762218	81.59%	9.963%
41	9.063	2492	2495	2496	rBV3	1089	638	0.07%	0.008%
42	9.140	2515	2519	2522	rBV4	1355	1284	0.14%	0.017%
43	9.301	2565	2569	2572	rVB6	1380	847	0.09%	0.011%
44	9.471	2618	2622	2626	rBV7	2025	1953	0.21%	0.026%
45	9.526	2636	2639	2642	rBV4	1412	976	0.10%	0.013%
46	9.574	2651	2654	2658	rBV5	1086	902	0.10%	0.012%
47	9.664	2680	2682	2687	rVB6	1645	1104	0.12%	0.014%
48	9.802	2722	2725	2726	rBV3	1183	652	0.07%	0.009%
49	9.828	2731	2733	2735	rBV2	777	404	0.04%	0.005%
50	9.924	2758	2763	2765	rBV5	1188	938	0.10%	0.012%
51	10.153	2819	2834	2857	rBV	279486	450819	48.25%	5.892%
52	10.284	2873	2875	2876	rBV	721	348	0.04%	0.005%
53	10.362	2897	2899	2904	rVB7	1367	985	0.11%	0.013%
54	10.455	2926	2928	2930	rVB2	1035	422	0.05%	0.006%
55	10.538	2953	2954	2958	rVB4	1367	747	0.08%	0.010%
56	10.564	2958	2962	2964	rBV4	1193	1127	0.12%	0.015%
57	10.664	2991	2993	2997	rBV5	1004	636	0.07%	0.008%
58	10.683	2997	2999	3001	rBV3	825	500	0.05%	0.007%
59	10.805	3032	3037	3041	rBV6	1494	1520	0.16%	0.020%
60	10.850	3049	3051	3054	rBV5	1051	599	0.06%	0.008%
61	10.953	3081	3083	3084	rBV2	991	455	0.05%	0.006%
62	11.079	3119	3122	3125	rBV4	1399	1140	0.12%	0.015%
63	11.124	3129	3136	3144	rVV3	13539	21720	2.32%	0.284%
64	11.185	3145	3155	3179	rVV	405733	675585	72.31%	8.830%
65	11.407	3221	3224	3225	rBV3	909	450	0.05%	0.006%
66	11.561	3260	3272	3293	rBV	438832	719737	77.04%	9.407%
67	11.828	3349	3355	3356	rBV4	1329	1275	0.14%	0.017%
68	11.895	3372	3376	3377	rBV4	1137	926	0.10%	0.012%
69	12.043	3416	3422	3428	rBV7	2175	3180	0.34%	0.042%
70	12.394	3526	3531	3534	rBV7	1437	1543	0.17%	0.020%
71	12.464	3551	3553	3555	rBV3	975	538	0.06%	0.007%
72	12.481	3557	3558	3560	rVV2	897	390	0.04%	0.005%
73	12.802	3655	3658	3660	rBV3	1006	542	0.06%	0.007%
74	12.863	3673	3677	3680	rBV6	1014	934	0.10%	0.012%
75	12.992	3713	3717	3719	rBV4	1434	897	0.10%	0.012%
76	13.008	3719	3722	3724	rBV3	659	423	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033408.D
 Acq On : 16 Dec 2023 03:41
 Operator : SY/MD
 Sample : 05802-18DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B31DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.034	3727	3730	3732	rBV3	1181	579	0.06%	0.008%
78	13.062	3735	3739	3741	rBV4	1316	930	0.10%	0.012%
79	13.191	3777	3779	3782	rBV3	975	490	0.05%	0.006%
80	13.381	3835	3838	3842	rBV5	1276	980	0.10%	0.013%
81	13.419	3849	3850	3851	rBV2	944	350	0.04%	0.005%
82	13.500	3874	3875	3877	rBV2	1088	427	0.05%	0.006%
83	13.564	3892	3895	3896	rBV2	1130	585	0.06%	0.008%
84	13.622	3911	3913	3915	rBV3	742	530	0.06%	0.007%
85	13.763	3954	3957	3963	rBV5	1472	1074	0.11%	0.014%
86	13.789	3963	3965	3967	rVB3	1489	613	0.07%	0.008%
87	13.802	3967	3969	3970	rVB2	979	351	0.04%	0.005%
88	13.815	3970	3973	3976	rBV5	1539	904	0.10%	0.012%
89	13.886	3992	3995	3998	rBV4	1239	1025	0.11%	0.013%
90	14.117	4065	4067	4069	rVB3	811	359	0.04%	0.005%
91	14.133	4069	4072	4074	rBV4	1686	1004	0.11%	0.013%
92	14.230	4100	4102	4105	rBV3	1096	697	0.07%	0.009%
93	14.259	4107	4111	4113	rVV3	1466	941	0.10%	0.012%
94	14.307	4121	4126	4127	rBV5	1516	1402	0.15%	0.018%
95	14.345	4136	4138	4141	rBV4	1085	753	0.08%	0.010%
96	14.718	4252	4254	4260	rVB6	1103	959	0.10%	0.013%
97	14.882	4302	4305	4309	rBV6	1942	1540	0.16%	0.020%
98	15.159	4389	4391	4393	rBV2	932	479	0.05%	0.006%
99	15.300	4433	4435	4437	rBV2	1227	567	0.06%	0.007%
100	15.892	4615	4619	4621	rBV5	1720	1382	0.15%	0.018%




Sum of corrected areas: 7650758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033408.D
Acq On : 16 Dec 2023 03:41
Operator : SY/MD
Sample : 05802-18DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

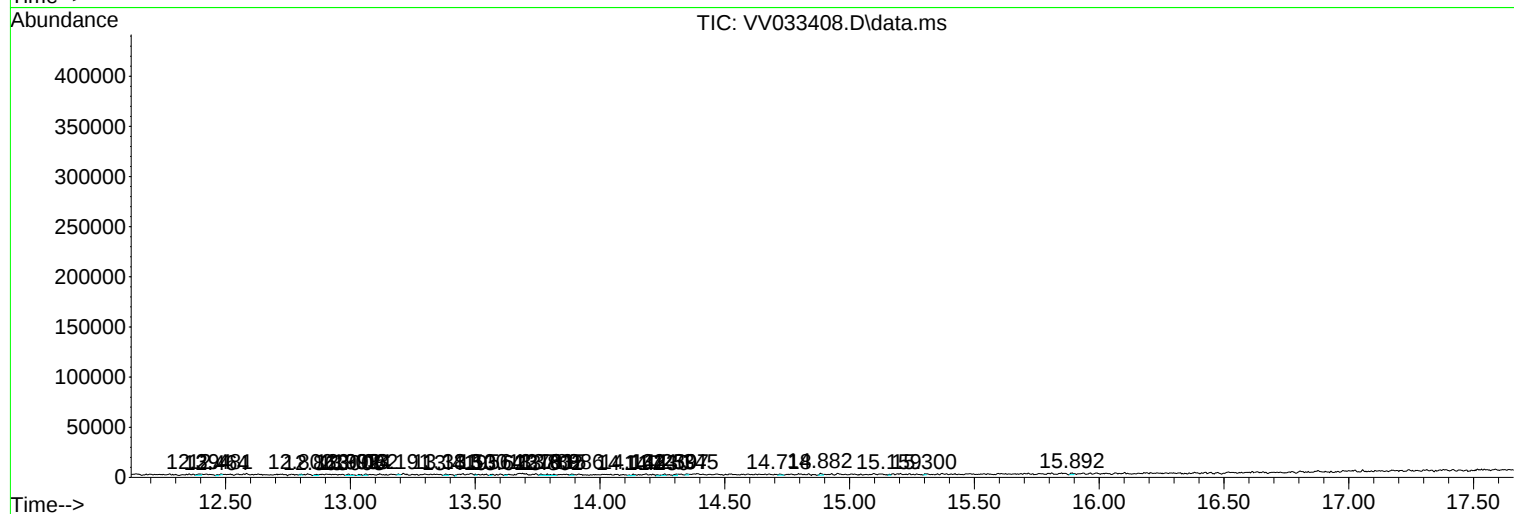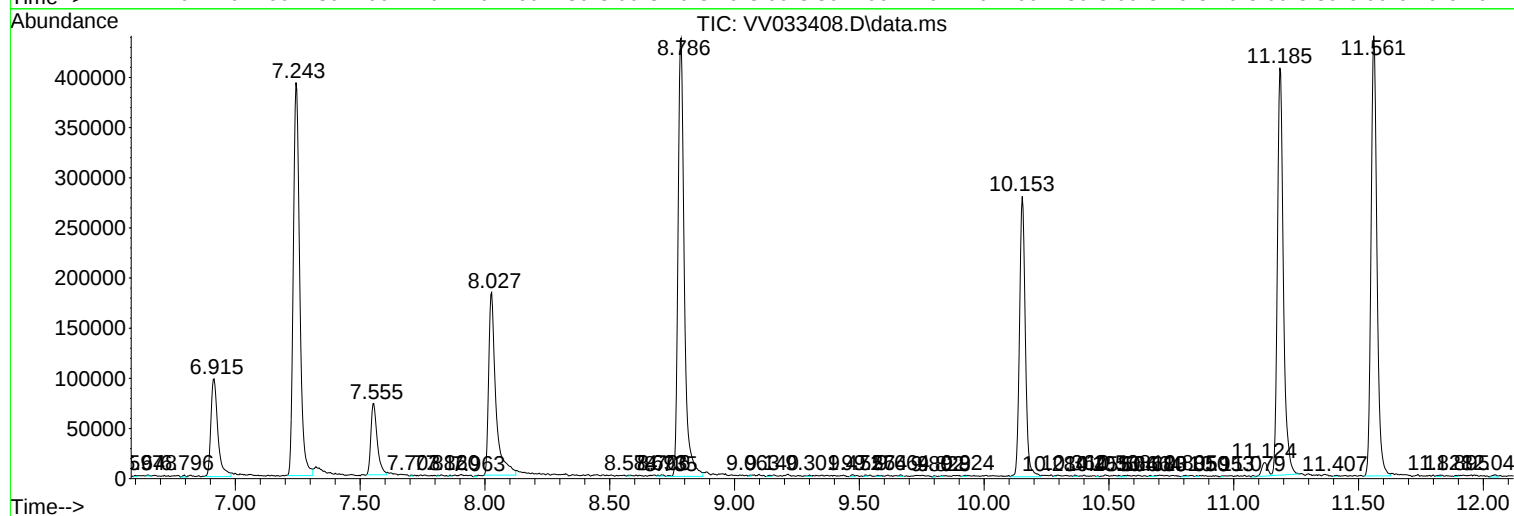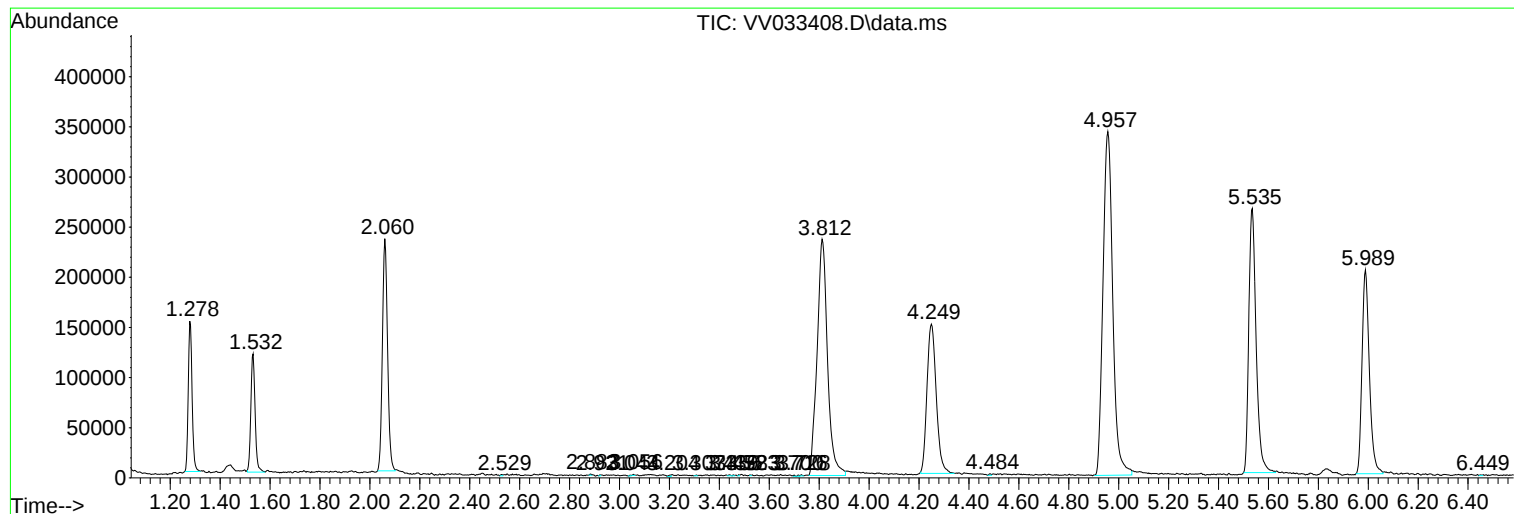

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033408.D
Acq On : 16 Dec 2023 03:41
Operator : SY/MD
Sample : 05802-18DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033408.D
Acq On : 16 Dec 2023 03:41
Operator : SY/MD
Sample : 05802-18DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc