

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033409.D
 Acq On : 16 Dec 2023 04:05
 Operator : SY/MD
 Sample : 05802-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	122956	125132	13.94%	1.734%
2	1.532	146	153	163	rVB	110435	130291	14.51%	1.805%
3	2.060	308	317	334	rVB	226569	326665	36.38%	4.527%
4	2.317	394	397	399	rBV4	1068	804	0.09%	0.011%
5	2.397	420	422	426	rBV5	783	592	0.07%	0.008%
6	2.555	468	471	472	rBV2	1566	781	0.09%	0.011%
7	2.809	548	550	554	rVV3	1200	846	0.09%	0.012%
8	2.831	556	557	561	rVV4	811	556	0.06%	0.008%
9	2.889	567	575	578	rBV7	1586	1859	0.21%	0.026%
10	3.037	616	621	624	rBV7	1165	1369	0.15%	0.019%
11	3.146	652	655	657	rBV4	1133	603	0.07%	0.008%
12	3.201	670	672	675	rVB3	982	522	0.06%	0.007%
13	3.375	724	726	732	rVB7	1420	721	0.08%	0.010%
14	3.397	732	733	737	rBV4	940	540	0.06%	0.007%
15	3.629	801	805	810	rBV7	1535	1517	0.17%	0.021%
16	3.683	819	822	826	rBV6	900	849	0.09%	0.012%
17	3.786	843	854	886	rBV	50900	170442	18.98%	2.362%
18	4.172	970	974	978	rBV5	1433	1199	0.13%	0.017%
19	4.249	985	998	1022	rBV	144150	364604	40.61%	5.052%
20	4.622	1112	1114	1118	rBV4	1185	687	0.08%	0.010%
21	4.732	1145	1148	1151	rBV4	1004	971	0.11%	0.013%
22	4.876	1189	1193	1196	rVB6	1155	811	0.09%	0.011%
23	4.957	1202	1218	1245	rBV4	339160	897804	100.00%	12.441%
24	5.535	1385	1398	1422	rBV	256099	542275	60.40%	7.514%
25	5.838	1480	1492	1512	rBV3	46306	106117	11.82%	1.470%
26	5.989	1527	1539	1562	rBV	196481	409854	45.65%	5.679%
27	6.503	1694	1699	1705	rBV9	1320	2011	0.22%	0.028%
28	6.535	1708	1709	1712	rBV3	770	545	0.06%	0.008%
29	6.632	1736	1739	1742	rBV4	1457	770	0.09%	0.011%
30	6.915	1815	1827	1850	rBV	93001	185437	20.65%	2.570%
31	7.243	1918	1929	1950	rBV	385415	681746	75.93%	9.447%
32	7.555	2018	2026	2039	rBV2	68097	118250	13.17%	1.639%
33	7.828	2108	2111	2114	rVB6	1322	677	0.08%	0.009%
34	7.905	2123	2135	2154	rBV	171458	292825	32.62%	4.058%
35	8.024	2163	2172	2206	rBV	175814	358329	39.91%	4.965%
36	8.458	2304	2307	2310	rVB3	1602	1018	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033409.D
 Acq On : 16 Dec 2023 04:05
 Operator : SY/MD
 Sample : 05802-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.481	2310	2314	2316	rBV3	1028	812	0.09%	0.011%
38	8.786	2396	2409	2431	rBV	426780	713888	79.51%	9.893%
39	8.982	2467	2470	2472	rBV3	1674	880	0.10%	0.012%
40	9.050	2489	2491	2495	rBV6	1271	845	0.09%	0.012%
41	9.291	2562	2566	2569	rBV4	914	711	0.08%	0.010%
42	9.317	2572	2574	2579	rVB5	1279	944	0.11%	0.013%
43	9.429	2606	2609	2614	rBV6	1765	1493	0.17%	0.021%
44	9.468	2618	2621	2625	rVB5	1022	792	0.09%	0.011%
45	9.526	2636	2639	2644	rVB7	1741	1228	0.14%	0.017%
46	9.551	2644	2647	2650	rBV4	1740	1095	0.12%	0.015%
47	9.606	2659	2664	2667	rBV6	2113	2444	0.27%	0.034%
48	9.812	2725	2728	2734	rBV6	1093	1238	0.14%	0.017%
49	9.892	2750	2753	2754	rBV3	915	591	0.07%	0.008%
50	9.928	2762	2764	2768	rVB4	1158	608	0.07%	0.008%
51	9.950	2768	2771	2775	rBV5	1064	921	0.10%	0.013%
52	10.040	2796	2799	2802	rVB2	1528	1122	0.12%	0.016%
53	10.063	2802	2806	2807	rBV2	1183	646	0.07%	0.009%
54	10.153	2824	2834	2849	rBV	271058	428047	47.68%	5.932%
55	10.252	2863	2865	2870	rBV6	949	700	0.08%	0.010%
56	10.317	2882	2885	2888	rBV5	1704	1090	0.12%	0.015%
57	10.336	2888	2891	2894	rVB5	1110	764	0.09%	0.011%
58	10.352	2894	2896	2901	rBV6	972	973	0.11%	0.013%
59	10.609	2973	2976	2978	rBV3	1447	899	0.10%	0.012%
60	10.638	2982	2985	2987	rVB4	1487	751	0.08%	0.010%
61	10.654	2987	2990	2994	rBV6	1006	840	0.09%	0.012%
62	10.673	2994	2996	3000	rVV2	1132	736	0.08%	0.010%
63	10.738	3012	3016	3017	rBV3	1082	732	0.08%	0.010%
64	10.960	3080	3085	3088	rBV5	1152	1091	0.12%	0.015%
65	11.056	3111	3115	3116	rBV3	931	571	0.06%	0.008%
66	11.185	3144	3155	3176	rBV	398642	628188	69.97%	8.705%
67	11.394	3218	3220	3222	rBV3	1159	558	0.06%	0.008%
68	11.442	3232	3235	3237	rBV4	988	578	0.06%	0.008%
69	11.561	3261	3272	3291	rBV	420734	661792	73.71%	9.171%
70	11.725	3321	3323	3331	rVB7	1794	1714	0.19%	0.024%
71	11.786	3337	3342	3344	rBV6	1143	927	0.10%	0.013%
72	11.831	3354	3356	3360	rVB4	1875	877	0.10%	0.012%
73	11.998	3407	3408	3412	rVB3	1054	534	0.06%	0.007%
74	12.108	3439	3442	3447	rBV7	1356	1097	0.12%	0.015%
75	12.362	3519	3521	3525	rVB5	1500	702	0.08%	0.010%
76	12.387	3525	3529	3532	rBV4	1320	1193	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033409.D
 Acq On : 16 Dec 2023 04:05
 Operator : SY/MD
 Sample : 05802-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.622	3599	3602	3606	rVB6	1008	664	0.07%	0.009%
78	12.712	3629	3630	3634	rVB4	1027	579	0.06%	0.008%
79	12.837	3667	3669	3671	rBV2	1150	703	0.08%	0.010%
80	13.085	3744	3746	3751	rBV4	903	885	0.10%	0.012%
81	13.236	3789	3793	3797	rBV5	1057	1183	0.13%	0.016%
82	13.445	3854	3858	3860	rBV4	1676	1250	0.14%	0.017%
83	13.545	3885	3889	3891	rBV5	1641	1041	0.12%	0.014%
84	13.580	3899	3900	3903	rBV2	1022	594	0.07%	0.008%
85	13.709	3938	3940	3942	rBV2	1035	671	0.07%	0.009%
86	13.995	4023	4029	4032	rBV7	1434	1309	0.15%	0.018%
87	14.140	4071	4074	4078	rBV6	1251	941	0.10%	0.013%
88	14.304	4120	4125	4127	rBV7	1172	940	0.10%	0.013%
89	14.365	4140	4144	4148	rBV6	1682	1291	0.14%	0.018%
90	14.419	4159	4161	4165	rVV4	1392	919	0.10%	0.013%
91	14.519	4190	4192	4196	rBV5	1347	770	0.09%	0.011%
92	14.564	4204	4206	4210	rVB5	1180	549	0.06%	0.008%
93	14.619	4219	4223	4225	rBV4	1006	594	0.07%	0.008%
94	14.635	4225	4228	4230	rBV4	926	635	0.07%	0.009%
95	15.014	4342	4346	4348	rBV4	813	664	0.07%	0.009%
96	15.111	4374	4376	4381	rVB5	1283	1009	0.11%	0.014%
97	15.239	4413	4416	4419	rBV3	1009	783	0.09%	0.011%
98	15.426	4471	4474	4477	rBV5	1512	1137	0.13%	0.016%
99	15.471	4486	4488	4490	rBV2	1575	795	0.09%	0.011%
100	15.535	4506	4508	4510	rBV3	1451	897	0.10%	0.012%




Sum of corrected areas: 7216434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033409.D
Acq On : 16 Dec 2023 04:05
Operator : SY/MD
Sample : 05802-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

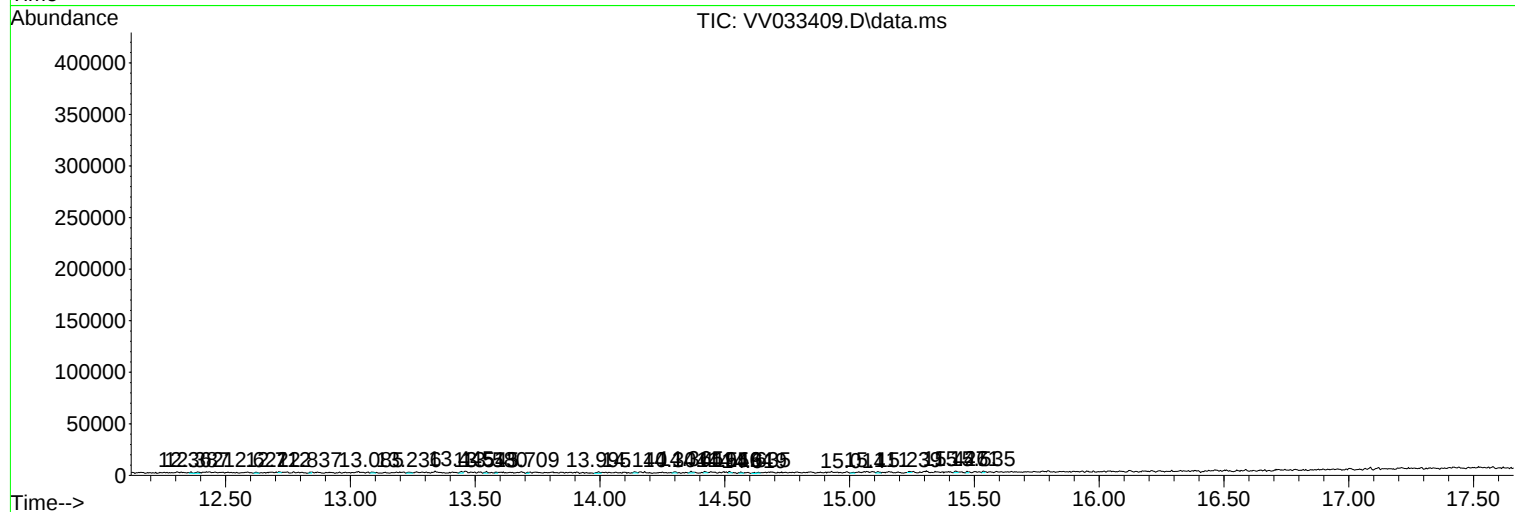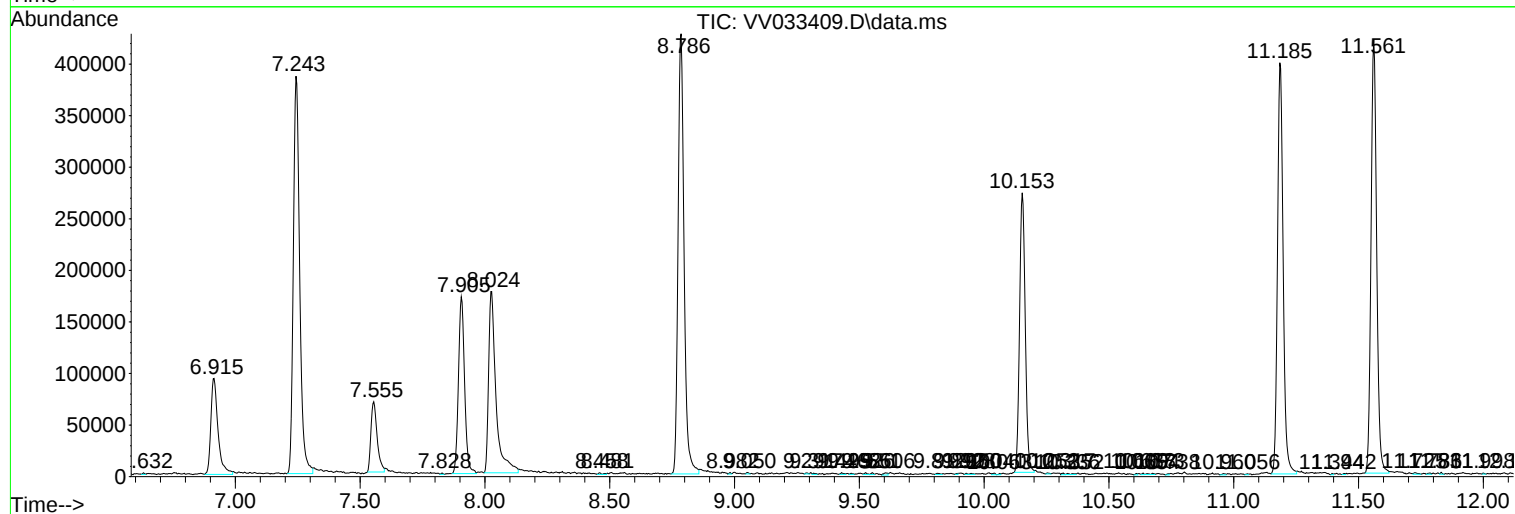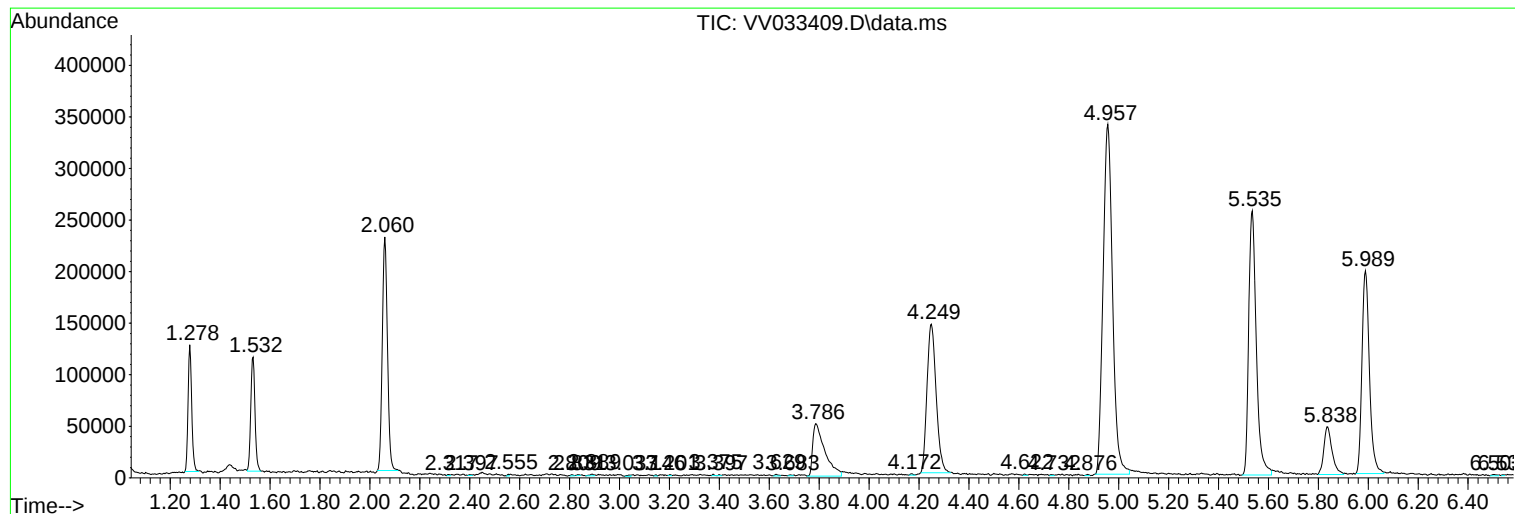

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033409.D
Acq On : 16 Dec 2023 04:05
Operator : SY/MD
Sample : 05802-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033409.D
Acq On : 16 Dec 2023 04:05
Operator : SY/MD
Sample : 05802-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc