

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033410.D
 Acq On : 16 Dec 2023 04:28
 Operator : SY/MD
 Sample : 05802-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VW033410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB2	147645	158849	17.66%	2.145%
2	1.532	146	153	163	rVB	110305	128426	14.28%	1.735%
3	2.060	308	317	335	rVB	228666	330522	36.74%	4.464%
4	2.240	371	373	376	rBV4	1483	997	0.11%	0.013%
5	2.690	510	513	515	rBV2	2012	1381	0.15%	0.019%
6	2.738	524	528	532	rBV7	1431	1213	0.13%	0.016%
7	2.925	584	586	588	rBV3	997	473	0.05%	0.006%
8	3.011	612	613	615	rBV2	936	400	0.04%	0.005%
9	3.114	643	645	648	rVB3	1338	558	0.06%	0.008%
10	3.195	668	670	673	rBV3	1206	580	0.06%	0.008%
11	3.233	680	682	684	rBV4	786	450	0.05%	0.006%
12	3.317	706	708	713	rBV6	1301	1027	0.11%	0.014%
13	3.339	713	715	716	rBV	856	349	0.04%	0.005%
14	3.478	757	758	759	rBV	997	333	0.04%	0.004%
15	3.732	835	837	842	rBV4	1100	658	0.07%	0.009%
16	3.812	846	862	887	rBV2	226688	651084	72.38%	8.794%
17	4.249	984	998	1025	rBV	145675	374194	41.60%	5.054%
18	4.683	1132	1133	1137	rVB4	1142	678	0.08%	0.009%
19	4.838	1179	1181	1183	rVB3	1254	395	0.04%	0.005%
20	4.957	1202	1218	1241	rBV2	336819	899578	100.00%	12.150%
21	5.391	1351	1353	1355	rBV2	1476	834	0.09%	0.011%
22	5.535	1386	1398	1425	rBV	258168	541927	60.24%	7.319%
23	5.989	1527	1539	1562	rBV	195240	407640	45.31%	5.506%
24	6.346	1648	1650	1653	rBV4	1402	691	0.08%	0.009%
25	6.523	1699	1705	1706	rBV5	1206	966	0.11%	0.013%
26	6.629	1735	1738	1739	rBV3	1009	544	0.06%	0.007%
27	6.680	1751	1754	1756	rBV4	1745	1140	0.13%	0.015%
28	6.741	1771	1773	1775	rBV3	917	437	0.05%	0.006%
29	6.786	1786	1787	1792	rVB4	1663	1208	0.13%	0.016%
30	6.812	1792	1795	1797	rBV4	1459	899	0.10%	0.012%
31	6.915	1816	1827	1844	rBV	93244	179119	19.91%	2.419%
32	7.121	1889	1891	1895	rVB3	1476	792	0.09%	0.011%
33	7.191	1908	1913	1915	rBV5	1024	1049	0.12%	0.014%
34	7.243	1919	1929	1949	rBV	381451	672247	74.73%	9.079%
35	7.555	2017	2026	2043	rBV	68170	127006	14.12%	1.715%
36	7.992	2160	2162	2163	rBV2	1349	545	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033410.D
 Acq On : 16 Dec 2023 04:28
 Operator : SY/MD
 Sample : 05802-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.027	2164	2173	2193	rBV	167069	328873	36.56%	4.442%
38	8.683	2375	2377	2381	rBV5	1002	723	0.08%	0.010%
39	8.786	2398	2409	2436	rBV	429746	733534	81.54%	9.907%
40	8.953	2459	2461	2463	rBV3	1437	568	0.06%	0.008%
41	9.233	2546	2548	2550	rVB4	1508	560	0.06%	0.008%
42	9.490	2626	2628	2631	rBV4	1110	601	0.07%	0.008%
43	9.510	2631	2634	2638	rVB5	2365	1939	0.22%	0.026%
44	9.532	2638	2641	2643	rBV4	1311	824	0.09%	0.011%
45	9.616	2666	2667	2670	rVB2	1598	498	0.06%	0.007%
46	9.632	2670	2672	2675	rBV5	1215	644	0.07%	0.009%
47	9.661	2678	2681	2684	rBV3	1431	1010	0.11%	0.014%
48	9.809	2722	2727	2729	rBV5	1551	1419	0.16%	0.019%
49	9.866	2741	2745	2746	rBV3	1059	645	0.07%	0.009%
50	10.153	2823	2834	2853	rVB	267264	423265	47.05%	5.717%
51	10.413	2912	2915	2916	rBV3	1621	863	0.10%	0.012%
52	10.529	2948	2951	2954	rBV6	1492	1075	0.12%	0.015%
53	10.677	2993	2997	2999	rBV4	1088	954	0.11%	0.013%
54	10.741	3015	3017	3018	rBV2	1064	398	0.04%	0.005%
55	10.796	3031	3034	3038	rVB5	1939	1745	0.19%	0.024%
56	10.825	3038	3043	3046	rBV5	1785	1919	0.21%	0.026%
57	11.021	3102	3104	3108	rBV4	1290	1006	0.11%	0.014%
58	11.075	3119	3121	3124	rBV3	1225	671	0.07%	0.009%
59	11.124	3127	3136	3144	rBV2	13004	21724	2.41%	0.293%
60	11.185	3145	3155	3180	rVB	406182	665636	73.99%	8.990%
61	11.468	3242	3243	3245	rBV2	720	372	0.04%	0.005%
62	11.561	3261	3272	3292	rBV	425436	691885	76.91%	9.345%
63	11.931	3383	3387	3388	rBV4	1199	962	0.11%	0.013%
64	12.136	3450	3451	3454	rVB3	1500	584	0.06%	0.008%
65	12.262	3487	3490	3492	rBV4	1538	1091	0.12%	0.015%
66	12.317	3503	3507	3511	rBV6	1191	1324	0.15%	0.018%
67	12.625	3601	3603	3606	rBV3	1046	653	0.07%	0.009%
68	12.683	3619	3621	3623	rBV3	758	403	0.04%	0.005%
69	12.722	3632	3633	3636	rBV3	838	465	0.05%	0.006%
70	12.805	3657	3659	3662	rBV3	1185	949	0.11%	0.013%
71	12.850	3671	3673	3675	rBV3	1088	572	0.06%	0.008%
72	12.918	3692	3694	3696	rBV3	832	534	0.06%	0.007%
73	13.091	3744	3748	3752	rBV6	1335	1154	0.13%	0.016%
74	13.162	3768	3770	3771	rBV2	983	448	0.05%	0.006%
75	13.207	3781	3784	3787	rBV5	1567	1201	0.13%	0.016%
76	13.281	3805	3807	3810	rBV4	711	331	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033410.D
 Acq On : 16 Dec 2023 04:28
 Operator : SY/MD
 Sample : 05802-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.329	3820	3822	3826	rBV6	781	474	0.05%	0.006%
78	13.435	3854	3855	3858	rBV2	1205	603	0.07%	0.008%
79	13.455	3858	3861	3862	rBV3	1183	707	0.08%	0.010%
80	13.693	3932	3935	3940	rBV8	1599	1551	0.17%	0.021%
81	13.808	3967	3971	3973	rBV5	1243	866	0.10%	0.012%
82	13.873	3989	3991	3993	rBV3	1068	543	0.06%	0.007%
83	13.898	3997	3999	4000	rBV2	964	441	0.05%	0.006%
84	13.927	4006	4008	4014	rVB6	1537	1187	0.13%	0.016%
85	14.014	4033	4035	4038	rVB3	1369	652	0.07%	0.009%
86	14.037	4038	4042	4044	rBV5	1311	960	0.11%	0.013%
87	14.197	4090	4092	4096	rBV4	1280	1054	0.12%	0.014%
88	14.297	4121	4123	4126	rBV4	1044	496	0.06%	0.007%
89	14.500	4184	4186	4187	rBV2	1065	543	0.06%	0.007%
90	14.541	4195	4199	4200	rBV3	1262	924	0.10%	0.012%
91	14.599	4212	4217	4219	rBV5	2285	1613	0.18%	0.022%
92	14.635	4226	4228	4232	rVB5	1898	1212	0.13%	0.016%
93	14.728	4255	4257	4259	rBV3	1150	482	0.05%	0.007%
94	14.889	4302	4307	4308	rBV3	1156	738	0.08%	0.010%
95	15.014	4343	4346	4348	rBV3	1597	1205	0.13%	0.016%
96	15.204	4403	4405	4409	rBV4	1014	652	0.07%	0.009%
97	15.252	4416	4420	4422	rBV4	965	755	0.08%	0.010%
98	15.313	4436	4439	4444	rBV5	1442	1514	0.17%	0.020%
99	15.342	4446	4448	4449	rBV2	1199	546	0.06%	0.007%
100	15.757	4574	4577	4579	rBV3	1601	1082	0.12%	0.015%




Sum of corrected areas: 7404011

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033410.D
Acq On : 16 Dec 2023 04:28
Operator : SY/MD
Sample : 05802-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

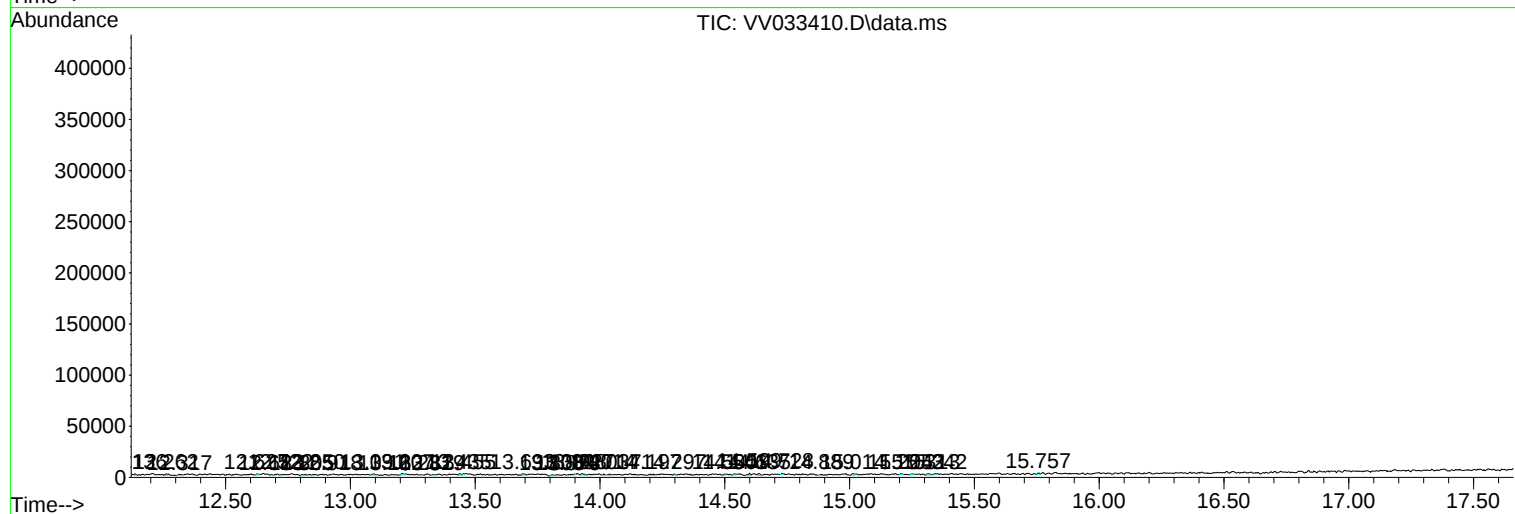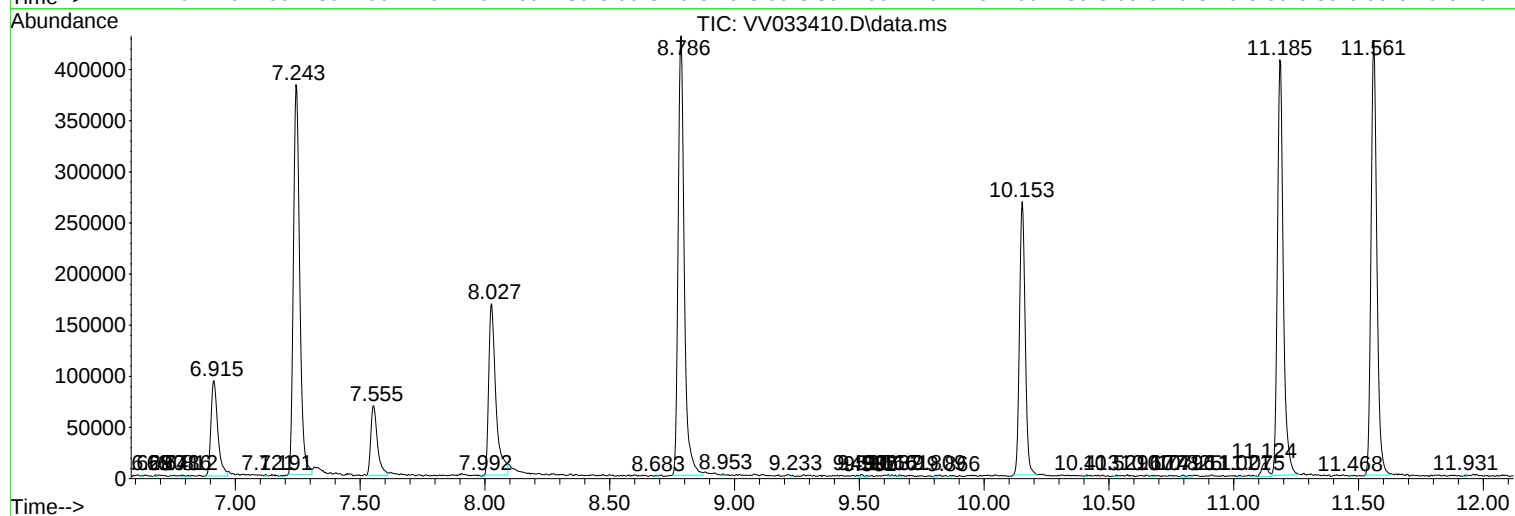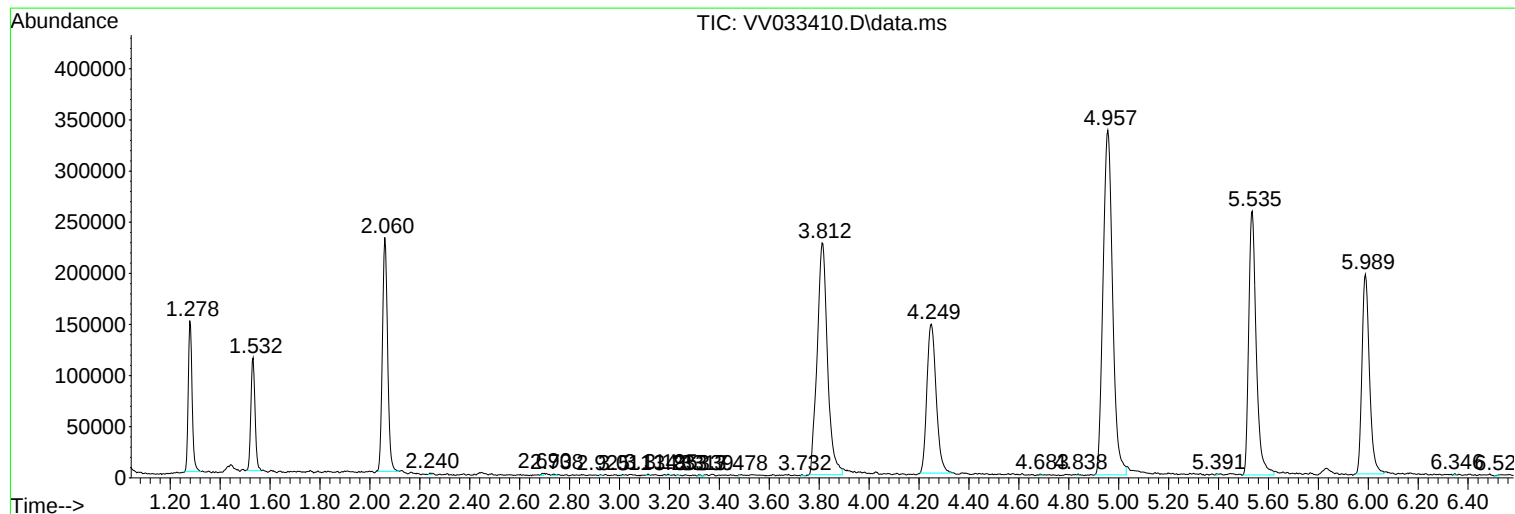

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033410.D
Acq On : 16 Dec 2023 04:28
Operator : SY/MD
Sample : 05802-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033410.D
Acq On : 16 Dec 2023 04:28
Operator : SY/MD
Sample : 05802-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc