

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033412.D
 Acq On : 16 Dec 2023 05:14
 Operator : SY/MD
 Sample : 05802-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	121365	123943	14.04%	1.759%
2	1.532	146	153	164	rVB	112293	130672	14.80%	1.855%
3	2.066	308	319	344	rVB3	401581	691783	78.35%	9.819%
4	2.349	404	407	410	rBV4	1762	1244	0.14%	0.018%
5	2.387	417	419	420	rBV3	1590	679	0.08%	0.010%
6	2.442	427	436	437	rBV8	2726	3326	0.38%	0.047%
7	2.629	491	494	497	rBV5	1459	995	0.11%	0.014%
8	2.773	535	539	542	rBV4	1343	908	0.10%	0.013%
9	2.844	558	561	563	rBV4	989	616	0.07%	0.009%
10	2.963	595	598	603	rBV6	1776	1665	0.19%	0.024%
11	3.220	675	678	682	rBV4	829	538	0.06%	0.008%
12	3.246	682	686	688	rBV3	1160	768	0.09%	0.011%
13	3.259	688	690	694	rVB3	1149	503	0.06%	0.007%
14	3.317	706	708	711	rVB4	1209	559	0.06%	0.008%
15	3.349	711	718	720	rBV6	1056	1000	0.11%	0.014%
16	3.506	762	767	769	rBV6	1373	841	0.10%	0.012%
17	3.535	775	776	782	rVB4	1046	911	0.10%	0.013%
18	3.567	782	786	788	rBV4	1205	1073	0.12%	0.015%
19	3.600	793	796	801	rVB6	1306	1040	0.12%	0.015%
20	3.635	804	807	810	rBV5	1038	794	0.09%	0.011%
21	3.664	815	816	820	rVB4	1194	511	0.06%	0.007%
22	3.751	839	843	846	rBV6	1485	1296	0.15%	0.018%
23	3.789	846	855	884	rVV	48759	141753	16.05%	2.012%
24	4.249	981	998	1021	rBV	147009	379750	43.01%	5.390%
25	4.706	1136	1140	1142	rBV5	1484	1163	0.13%	0.017%
26	4.956	1202	1218	1246	rBV2	328646	882986	100.00%	12.533%
27	5.535	1386	1398	1424	rBV2	249610	530023	60.03%	7.523%
28	5.934	1520	1522	1525	rBV4	1104	710	0.08%	0.010%
29	5.989	1528	1539	1562	rVV2	196099	409537	46.38%	5.813%
30	6.310	1635	1639	1643	rVB8	1600	1373	0.16%	0.019%
31	6.336	1643	1647	1649	rBV5	1101	1014	0.11%	0.014%
32	6.452	1680	1683	1685	rBV4	891	592	0.07%	0.008%
33	6.561	1712	1717	1720	rBV4	2159	1898	0.21%	0.027%
34	6.690	1754	1757	1764	rVB8	1613	1355	0.15%	0.019%
35	6.718	1764	1766	1768	rBV3	1025	581	0.07%	0.008%
36	6.763	1777	1780	1783	rVV5	1537	1047	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033412.D
 Acq On : 16 Dec 2023 05:14
 Operator : SY/MD
 Sample : 05802-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.780	1783	1785	1792	rVV8	1157	954	0.11%	0.014%
38	6.808	1792	1794	1801	rVV7	1004	826	0.09%	0.012%
39	6.860	1804	1810	1812	rBV6	998	1138	0.13%	0.016%
40	6.915	1817	1827	1843	rBV	92397	170099	19.26%	2.414%
41	7.243	1918	1929	1955	rBV	380903	677278	76.70%	9.613%
42	7.554	2017	2026	2043	rBV	68090	121999	13.82%	1.732%
43	7.760	2086	2090	2091	rBV3	1003	491	0.06%	0.007%
44	7.908	2132	2136	2141	rBV8	2099	2334	0.26%	0.033%
45	8.027	2164	2173	2191	rBV	168083	327375	37.08%	4.647%
46	8.445	2302	2303	2306	rBV3	1543	689	0.08%	0.010%
47	8.561	2337	2339	2341	rBV3	1171	565	0.06%	0.008%
48	8.718	2385	2388	2389	rBV3	1776	988	0.11%	0.014%
49	8.786	2395	2409	2428	rBV	414902	693809	78.58%	9.848%
50	9.085	2500	2502	2503	rBV2	1597	653	0.07%	0.009%
51	9.165	2524	2527	2530	rBV5	1180	1071	0.12%	0.015%
52	9.239	2544	2550	2552	rBV6	1604	1497	0.17%	0.021%
53	9.294	2565	2567	2568	rBV2	1223	591	0.07%	0.008%
54	9.435	2608	2611	2614	rVB4	1568	1060	0.12%	0.015%
55	9.455	2614	2617	2620	rBV6	1513	924	0.10%	0.013%
56	9.561	2647	2650	2653	rBV5	1407	783	0.09%	0.011%
57	9.615	2664	2667	2669	rBV3	997	648	0.07%	0.009%
58	9.908	2754	2758	2760	rBV4	1498	1001	0.11%	0.014%
59	9.959	2770	2774	2776	rBV4	1085	667	0.08%	0.009%
60	10.088	2811	2814	2818	rBV6	1575	1360	0.15%	0.019%
61	10.152	2823	2834	2856	rVV	268717	426144	48.26%	6.049%
62	10.255	2863	2866	2867	rBV2	1079	566	0.06%	0.008%
63	10.361	2896	2899	2901	rBV4	1188	684	0.08%	0.010%
64	10.435	2916	2922	2923	rBV5	1679	1674	0.19%	0.024%
65	10.625	2979	2981	2983	rBV	1245	560	0.06%	0.008%
66	10.638	2983	2985	2987	rVB3	1316	629	0.07%	0.009%
67	10.812	3036	3039	3040	rBV3	1659	923	0.10%	0.013%
68	10.879	3056	3060	3062	rBV4	1279	847	0.10%	0.012%
69	11.017	3099	3103	3104	rBV3	1444	682	0.08%	0.010%
70	11.075	3117	3121	3123	rBV3	1610	1275	0.14%	0.018%
71	11.185	3145	3155	3178	rBV	381663	605231	68.54%	8.591%
72	11.426	3228	3230	3233	rBV4	965	609	0.07%	0.009%
73	11.561	3261	3272	3294	rBV	418787	653386	74.00%	9.274%
74	12.146	3450	3454	3456	rBV3	1551	1100	0.12%	0.016%
75	12.265	3488	3491	3493	rBV3	952	572	0.06%	0.008%
76	12.371	3522	3524	3528	rVB4	1091	504	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033412.D
 Acq On : 16 Dec 2023 05:14
 Operator : SY/MD
 Sample : 05802-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.393	3528	3531	3533	rBV3	995	793	0.09%	0.011%
78	12.709	3626	3629	3632	rBV5	1086	773	0.09%	0.011%
79	12.879	3674	3682	3685	rBV9	2190	3062	0.35%	0.043%
80	13.082	3739	3745	3751	rBV8	1444	2118	0.24%	0.030%
81	13.181	3774	3776	3779	rVB3	1392	732	0.08%	0.010%
82	13.246	3793	3796	3799	rBV5	1327	1018	0.12%	0.014%
83	13.390	3839	3841	3845	rVV3	1026	568	0.06%	0.008%
84	13.525	3881	3883	3887	rBV4	1027	577	0.07%	0.008%
85	13.551	3887	3891	3895	rBV6	688	608	0.07%	0.009%
86	13.622	3911	3913	3917	rVB4	1401	660	0.07%	0.009%
87	13.754	3951	3954	3956	rVB4	1473	937	0.11%	0.013%
88	13.766	3956	3958	3960	rBV2	1286	685	0.08%	0.010%
89	13.831	3975	3978	3980	rBV4	1193	893	0.10%	0.013%
90	13.860	3984	3987	3991	rVB6	901	680	0.08%	0.010%
91	14.027	4036	4039	4043	rBV6	1547	1154	0.13%	0.016%
92	14.069	4050	4052	4055	rVB4	1438	778	0.09%	0.011%
93	14.361	4141	4143	4148	rBV5	919	725	0.08%	0.010%
94	14.413	4155	4159	4160	rBV3	1070	937	0.11%	0.013%
95	14.535	4194	4197	4198	rBV2	1228	685	0.08%	0.010%
96	14.824	4285	4287	4290	rBV4	1203	813	0.09%	0.012%
97	14.876	4301	4303	4305	rBV3	1273	768	0.09%	0.011%
98	15.165	4390	4393	4394	rBV3	981	631	0.07%	0.009%
99	15.438	4476	4478	4480	rBV3	1236	549	0.06%	0.008%
100	15.647	4540	4543	4544	rBV2	1043	501	0.06%	0.007%




Sum of corrected areas: 7045278

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033412.D
Acq On : 16 Dec 2023 05:14
Operator : SY/MD
Sample : 05802-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

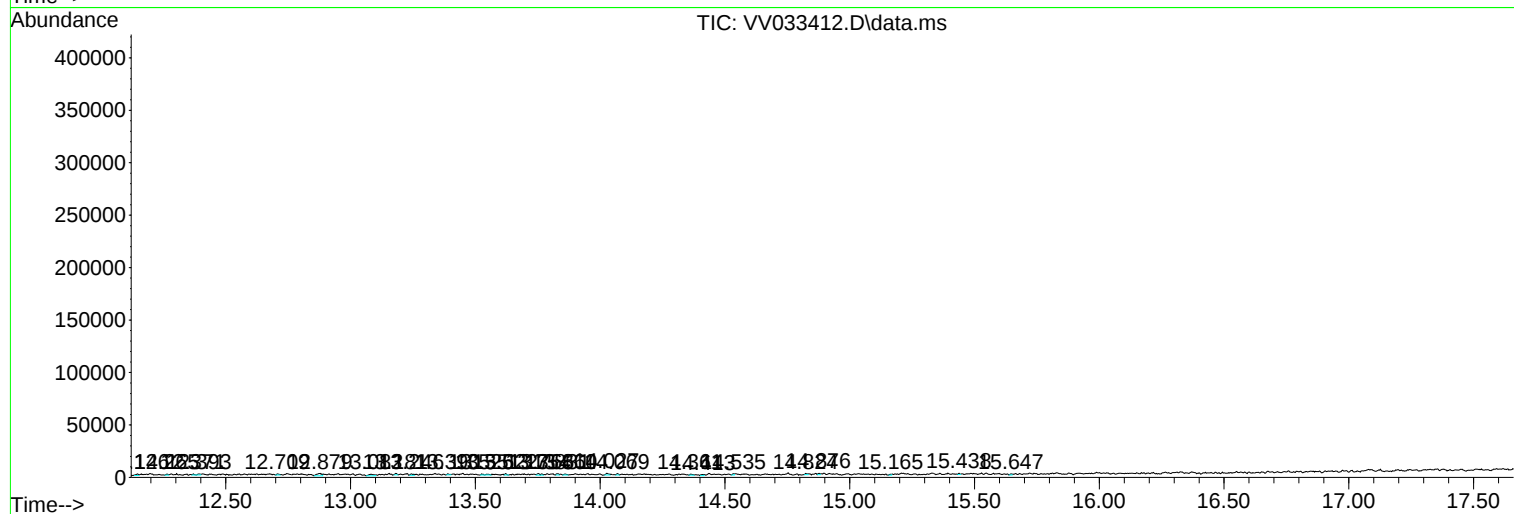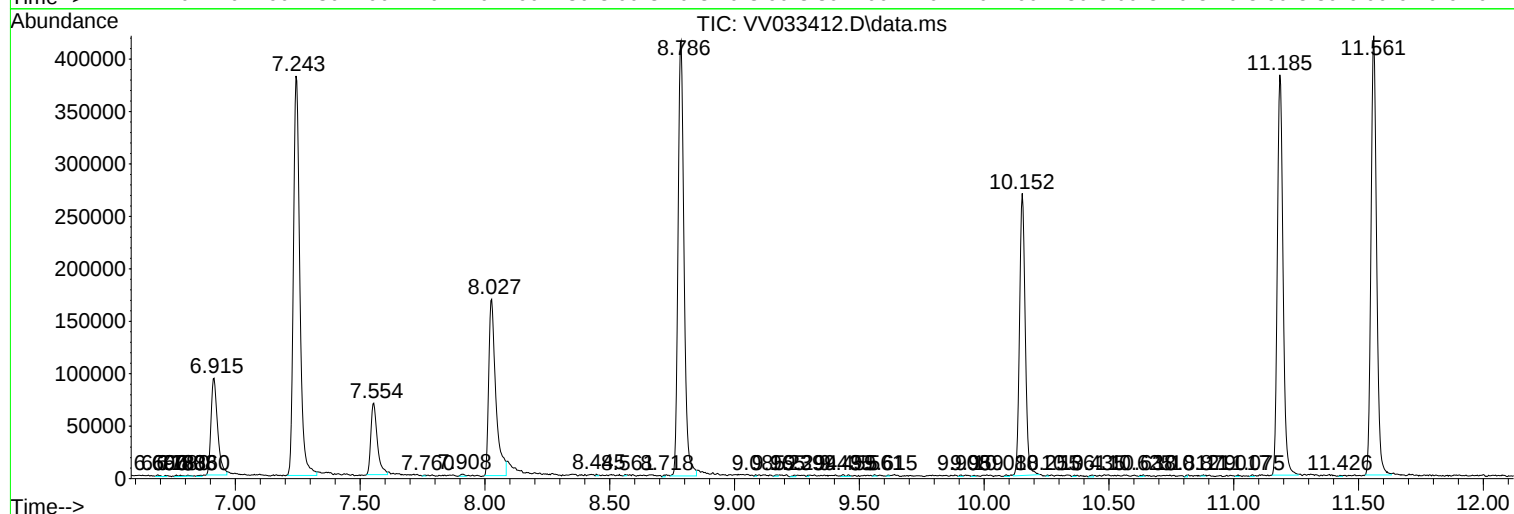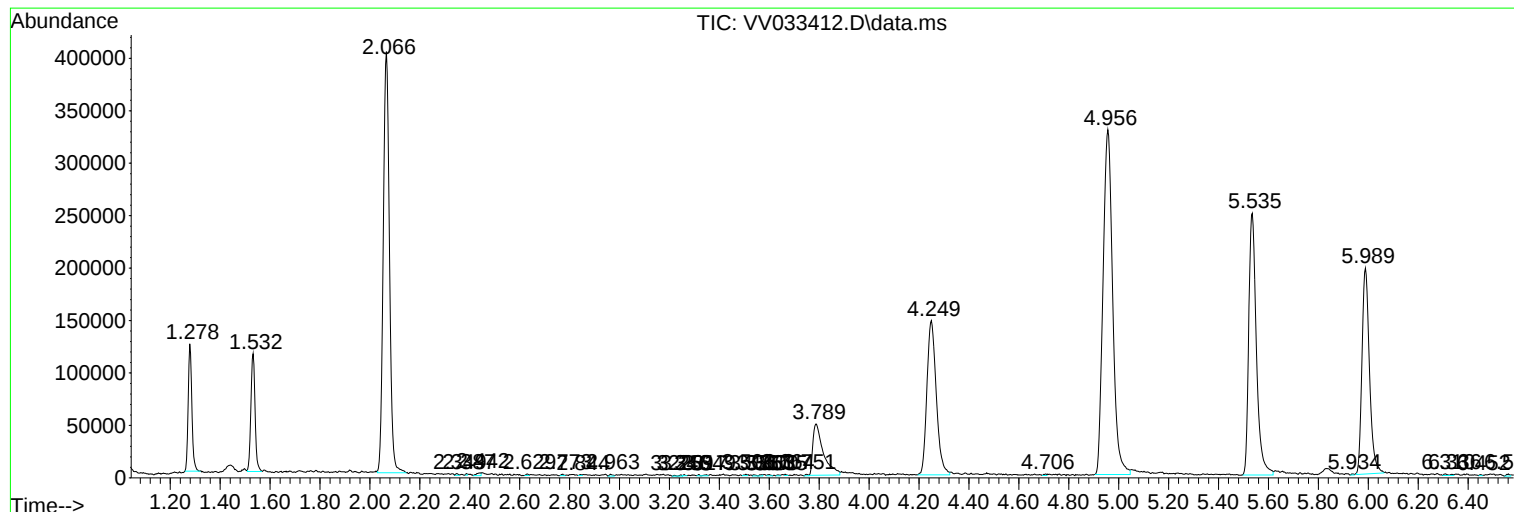

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033412.D
Acq On : 16 Dec 2023 05:14
Operator : SY/MD
Sample : 05802-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033412.D
Acq On : 16 Dec 2023 05:14
Operator : SY/MD
Sample : 05802-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------