

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033413.D
 Acq On : 16 Dec 2023 05:37
 Operator : SY/MD
 Sample : 05802-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	122721	128554	14.60%	1.936%
2	1.532	146	153	164	rVB	111584	127131	14.44%	1.914%
3	2.060	308	317	329	rBV	223006	318048	36.12%	4.789%
4	2.310	391	395	397	rBV5	1527	1104	0.13%	0.017%
5	2.368	411	413	415	rBV2	878	438	0.05%	0.007%
6	2.603	483	486	489	rBV4	1175	624	0.07%	0.009%
7	2.632	492	495	498	rBV3	1134	830	0.09%	0.012%
8	2.783	540	542	546	rVB4	1841	1152	0.13%	0.017%
9	2.818	546	553	556	rBV6	1381	1666	0.19%	0.025%
10	2.970	595	600	601	rBV5	1132	786	0.09%	0.012%
11	3.063	626	629	632	rBV4	1215	753	0.09%	0.011%
12	3.079	632	634	636	rBV3	1164	675	0.08%	0.010%
13	3.159	656	659	662	rBV5	545	406	0.05%	0.006%
14	3.172	662	663	666	rBV4	815	446	0.05%	0.007%
15	3.320	707	709	711	rBV3	1091	440	0.05%	0.007%
16	3.442	742	747	750	rBV7	1772	1563	0.18%	0.024%
17	3.490	760	762	763	rBV2	1111	504	0.06%	0.008%
18	3.539	771	777	779	rBV6	1462	1447	0.16%	0.022%
19	3.568	785	786	789	rVB2	1166	498	0.06%	0.007%
20	3.584	789	791	792	rBV2	794	317	0.04%	0.005%
21	3.593	792	794	796	rVV3	809	332	0.04%	0.005%
22	3.606	796	798	799	rVV2	1400	496	0.06%	0.007%
23	3.629	802	805	809	rBV6	1285	1251	0.14%	0.019%
24	3.648	809	811	813	rBV3	1050	514	0.06%	0.008%
25	3.786	846	854	879	rBV	48668	136220	15.47%	2.051%
26	4.169	969	973	977	rBV6	1242	1421	0.16%	0.021%
27	4.246	984	997	1026	rVB2	144683	368895	41.89%	5.555%
28	4.574	1097	1099	1102	rVB4	1473	759	0.09%	0.011%
29	4.957	1202	1218	1243	rBV2	330359	880607	100.00%	13.261%
30	5.535	1386	1398	1421	rBV	253332	527424	59.89%	7.942%
31	5.989	1528	1539	1558	rBV	190179	394385	44.79%	5.939%
32	6.362	1654	1655	1656	rBV2	763	148	0.02%	0.002%
33	6.375	1656	1659	1661	rBV4	1092	550	0.06%	0.008%
34	6.497	1695	1697	1700	rBV5	1012	496	0.06%	0.007%
35	6.523	1700	1705	1706	rBV5	1175	794	0.09%	0.012%
36	6.555	1712	1715	1719	rBV6	1040	948	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033413.D
 Acq On : 16 Dec 2023 05:37
 Operator : SY/MD
 Sample : 05802-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.658	1744	1747	1749	rBV4	1948	1374	0.16%	0.021%
38	6.748	1773	1775	1776	rVB2	1315	319	0.04%	0.005%
39	6.818	1795	1797	1799	rVB3	1136	344	0.04%	0.005%
40	6.915	1816	1827	1848	rBV	92799	180806	20.53%	2.723%
41	7.133	1892	1895	1896	rBV3	1349	924	0.10%	0.014%
42	7.243	1918	1929	1949	rBV	379519	670848	76.18%	10.102%
43	7.555	2017	2026	2044	rBV	67455	121086	13.75%	1.823%
44	7.754	2083	2088	2090	rBV6	1739	1628	0.18%	0.025%
45	8.024	2163	2172	2206	rBV	167982	346691	39.37%	5.221%
46	8.616	2353	2356	2358	rBV4	947	774	0.09%	0.012%
47	8.786	2398	2409	2427	rBV	425946	697265	79.18%	10.500%
48	9.185	2531	2533	2534	rBV2	825	366	0.04%	0.006%
49	9.403	2597	2601	2603	rBV4	1412	1047	0.12%	0.016%
50	9.426	2606	2608	2609	rBV2	865	302	0.03%	0.005%
51	9.709	2692	2696	2698	rVB4	1577	1057	0.12%	0.016%
52	10.021	2792	2793	2794	rBB	565	109	0.01%	0.002%
53	10.085	2810	2813	2815	rBV2	1090	782	0.09%	0.012%
54	10.153	2823	2834	2853	rBV	268257	422967	48.03%	6.369%
55	10.410	2912	2914	2918	rVB5	1557	823	0.09%	0.012%
56	10.590	2965	2970	2971	rBV4	1074	755	0.09%	0.011%
57	10.718	3008	3010	3013	rBV4	971	530	0.06%	0.008%
58	10.735	3013	3015	3018	rBV4	882	595	0.07%	0.009%
59	10.770	3024	3026	3028	rBV3	1059	676	0.08%	0.010%
60	10.841	3046	3048	3051	rBV4	1472	1066	0.12%	0.016%
61	10.937	3075	3078	3081	rBV4	606	413	0.05%	0.006%
62	10.950	3081	3082	3085	rBV3	698	289	0.03%	0.004%
63	10.969	3085	3088	3089	rBV	792	483	0.05%	0.007%
64	11.011	3099	3101	3104	rBV3	1159	515	0.06%	0.008%
65	11.027	3104	3106	3107	rVV2	642	199	0.02%	0.003%
66	11.108	3128	3131	3132	rBV3	1060	603	0.07%	0.009%
67	11.185	3145	3155	3171	rBV	392706	615738	69.92%	9.272%
68	11.342	3202	3204	3206	rBV3	1168	445	0.05%	0.007%
69	11.477	3244	3246	3249	rBV3	719	395	0.04%	0.006%
70	11.561	3261	3272	3292	rBV	418481	645701	73.32%	9.723%
71	11.870	3366	3368	3372	rVB6	1309	816	0.09%	0.012%
72	11.899	3375	3377	3379	rBV2	1106	443	0.05%	0.007%
73	11.998	3404	3408	3411	rBV6	1797	1707	0.19%	0.026%
74	12.133	3448	3450	3451	rBV3	673	188	0.02%	0.003%
75	12.471	3553	3555	3556	rBV2	435	138	0.02%	0.002%
76	12.625	3600	3603	3607	rVB6	1448	1129	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033413.D
 Acq On : 16 Dec 2023 05:37
 Operator : SY/MD
 Sample : 05802-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.657	3607	3613	3616	rBV8	1199	1445	0.16%	0.022%
78	12.689	3621	3623	3625	rVB3	698	228	0.03%	0.003%
79	12.706	3625	3628	3629	rBV3	954	528	0.06%	0.008%
80	12.924	3694	3696	3699	rBV3	764	489	0.06%	0.007%
81	13.040	3730	3732	3733	rBV2	948	363	0.04%	0.005%
82	13.091	3743	3748	3751	rBV6	1691	1344	0.15%	0.020%
83	13.181	3773	3776	3780	rBV5	1221	1252	0.14%	0.019%
84	13.590	3901	3903	3905	rBV3	1158	485	0.06%	0.007%
85	13.860	3985	3987	3989	rBV3	831	419	0.05%	0.006%
86	13.908	4000	4002	4005	rBV4	780	418	0.05%	0.006%
87	13.940	4010	4012	4014	rBV	934	344	0.04%	0.005%
88	13.953	4014	4016	4018	rBV2	881	401	0.05%	0.006%
89	14.226	4097	4101	4103	rBV4	846	550	0.06%	0.008%
90	14.400	4153	4155	4159	rVB4	914	533	0.06%	0.008%
91	14.490	4181	4183	4184	rBV2	640	162	0.02%	0.002%
92	14.554	4201	4203	4206	rBV4	1226	726	0.08%	0.011%
93	14.603	4217	4218	4220	rVB2	775	192	0.02%	0.003%
94	14.712	4247	4252	4253	rBV4	1063	744	0.08%	0.011%
95	14.815	4282	4284	4286	rBV2	984	590	0.07%	0.009%
96	15.136	4381	4384	4388	rBV6	1728	1402	0.16%	0.021%
97	15.355	4448	4452	4453	rBV3	1549	1114	0.13%	0.017%
98	15.619	4532	4534	4537	rBV4	1301	768	0.09%	0.012%
99	15.763	4577	4579	4583	rBV5	1777	1212	0.14%	0.018%




Sum of corrected areas: 6640667

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033413.D
Acq On : 16 Dec 2023 05:37
Operator : SY/MD
Sample : 05802-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

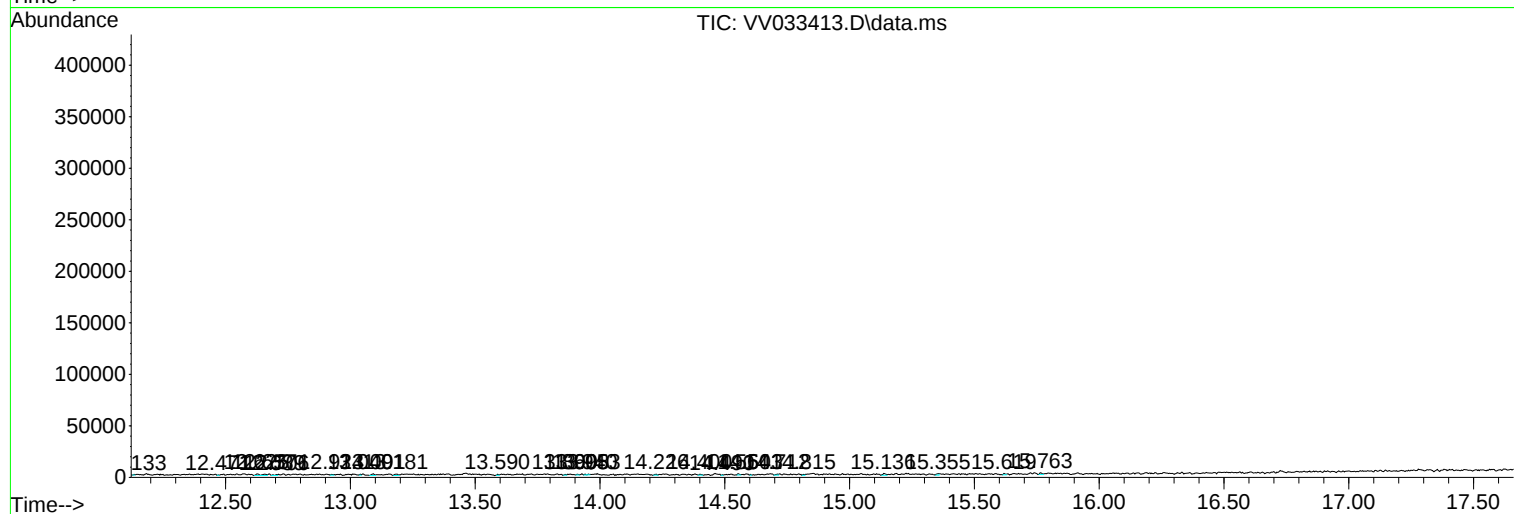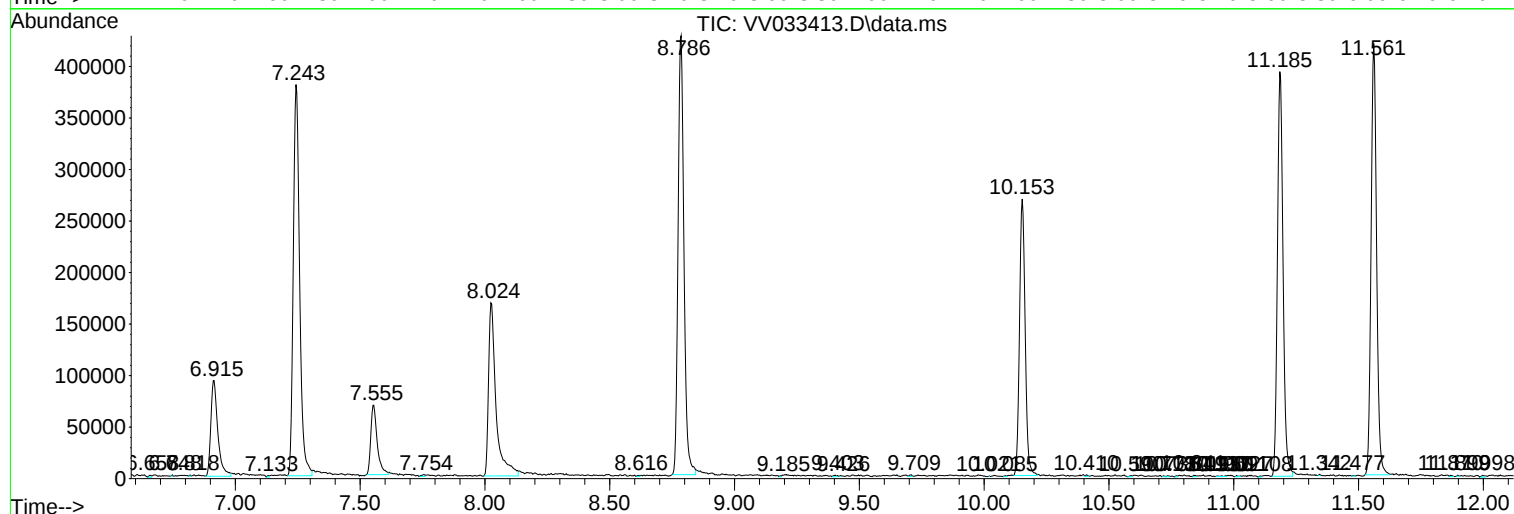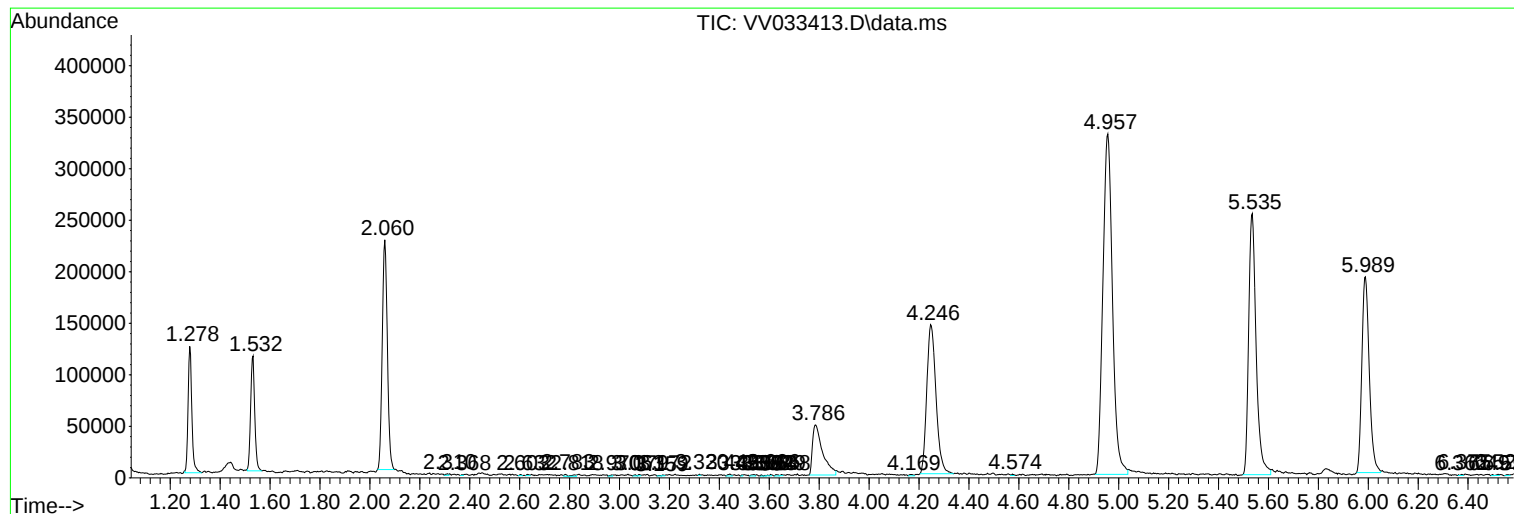

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033413.D
Acq On : 16 Dec 2023 05:37
Operator : SY/MD
Sample : 05802-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033413.D
Acq On : 16 Dec 2023 05:37
Operator : SY/MD
Sample : 05802-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------