

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033414.D
 Acq On : 16 Dec 2023 06:01
 Operator : SY/MD
 Sample : 05802-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	120776	124292	13.55%	1.740%
2	1.529	146	152	167	rVB	108788	129946	14.17%	1.819%
3	2.066	308	319	340	rVB3	375669	646032	70.44%	9.043%
4	2.301	389	392	396	rVB6	2003	1367	0.15%	0.019%
5	2.320	396	398	400	rBV3	1309	661	0.07%	0.009%
6	2.850	558	563	564	rBV3	1859	1246	0.14%	0.017%
7	2.915	580	583	586	rBV4	1261	927	0.10%	0.013%
8	3.027	615	618	621	rBV4	1282	723	0.08%	0.010%
9	3.105	638	642	645	rBV5	1532	1581	0.17%	0.022%
10	3.214	674	676	678	rBV3	890	431	0.05%	0.006%
11	3.249	685	687	690	rBV3	1235	620	0.07%	0.009%
12	3.342	712	716	717	rBV3	1040	696	0.08%	0.010%
13	3.391	727	731	732	rBV3	1238	852	0.09%	0.012%
14	3.455	748	751	753	rVB3	1260	705	0.08%	0.010%
15	3.596	792	795	800	rBV6	1194	1107	0.12%	0.015%
16	3.638	807	808	810	rBV2	637	195	0.02%	0.003%
17	3.648	810	811	812	rBV	853	304	0.03%	0.004%
18	3.706	827	829	831	rVB3	1147	405	0.04%	0.006%
19	3.783	844	853	873	rBV	50000	131041	14.29%	1.834%
20	4.143	963	965	966	rBV3	1029	369	0.04%	0.005%
21	4.249	982	998	1019	rBV2	148457	384888	41.97%	5.388%
22	4.670	1125	1129	1131	rBV4	1387	1183	0.13%	0.017%
23	4.844	1179	1183	1185	rBV4	1265	1000	0.11%	0.014%
24	4.957	1201	1218	1247	rBV2	339136	917077	100.00%	12.837%
25	5.490	1381	1384	1385	rBV2	1055	569	0.06%	0.008%
26	5.535	1385	1398	1416	rBV	262291	545908	59.53%	7.642%
27	5.989	1527	1539	1561	rBV	198134	416375	45.40%	5.828%
28	6.317	1637	1641	1645	rBV8	1502	1330	0.15%	0.019%
29	6.391	1662	1664	1666	rBV3	1580	866	0.09%	0.012%
30	6.657	1743	1747	1753	rBV7	1367	1301	0.14%	0.018%
31	6.812	1793	1795	1796	rBV2	1216	607	0.07%	0.008%
32	6.870	1810	1813	1814	rBV3	875	449	0.05%	0.006%
33	6.915	1817	1827	1847	rVV	92488	177954	19.40%	2.491%
34	7.243	1918	1929	1957	rBV	387501	689487	75.18%	9.651%
35	7.551	2017	2025	2046	rBV2	70092	125655	13.70%	1.759%
36	7.908	2131	2136	2138	rBV5	1287	1297	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033414.D
 Acq On : 16 Dec 2023 06:01
 Operator : SY/MD
 Sample : 05802-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.963	2151	2153	2154	rBV2	964	438	0.05%	0.006%
38	8.024	2163	2172	2205	rBV	167237	347103	37.85%	4.859%
39	8.786	2398	2409	2430	rBV	447084	724450	79.00%	10.141%
40	9.342	2580	2582	2583	rBV	949	290	0.03%	0.004%
41	9.493	2626	2629	2632	rBV3	1356	1157	0.13%	0.016%
42	9.947	2768	2770	2772	rBV3	909	469	0.05%	0.007%
43	10.152	2823	2834	2848	rBV	273778	432655	47.18%	6.056%
44	10.455	2926	2928	2930	rBV3	1181	485	0.05%	0.007%
45	10.635	2981	2984	2986	rBV3	1012	603	0.07%	0.008%
46	10.844	3045	3049	3050	rBV4	1230	734	0.08%	0.010%
47	10.860	3052	3054	3056	rVV2	987	388	0.04%	0.005%
48	10.937	3075	3078	3079	rBV2	930	464	0.05%	0.006%
49	10.950	3079	3082	3085	rVB4	1695	1128	0.12%	0.016%
50	11.059	3114	3116	3120	rBV5	1015	786	0.09%	0.011%
51	11.185	3144	3155	3179	rBV	406262	637866	69.55%	8.929%
52	11.349	3202	3206	3211	rBV7	1258	1575	0.17%	0.022%
53	11.410	3222	3225	3227	rBV4	1773	1316	0.14%	0.018%
54	11.561	3261	3272	3288	rBV	415296	659636	71.93%	9.234%
55	12.024	3415	3416	3417	rBV	712	208	0.02%	0.003%
56	12.049	3421	3424	3428	rVV5	1705	1155	0.13%	0.016%
57	12.117	3442	3445	3448	rBV4	1144	931	0.10%	0.013%
58	12.342	3511	3515	3517	rBV4	1828	1027	0.11%	0.014%
59	12.361	3517	3521	3524	rBV6	996	781	0.09%	0.011%
60	12.525	3568	3572	3574	rBV5	1717	1224	0.13%	0.017%
61	12.564	3582	3584	3587	rBV3	1060	858	0.09%	0.012%
62	12.847	3668	3672	3675	rBV4	1311	1278	0.14%	0.018%
63	12.866	3675	3678	3680	rVV3	954	513	0.06%	0.007%
64	13.085	3744	3746	3751	rBV4	1158	817	0.09%	0.011%
65	13.184	3774	3777	3781	rBV4	2391	1796	0.20%	0.025%
66	13.532	3884	3885	3888	rVB3	1143	410	0.04%	0.006%
67	13.548	3888	3890	3891	rBV	740	246	0.03%	0.003%
68	13.564	3891	3895	3896	rVV3	622	437	0.05%	0.006%
69	13.580	3898	3900	3905	rVB4	1195	767	0.08%	0.011%
70	13.744	3948	3951	3955	rVB5	1339	809	0.09%	0.011%
71	13.856	3982	3986	3989	rBV5	890	597	0.07%	0.008%
72	14.008	4030	4033	4035	rBV3	1017	717	0.08%	0.010%
73	14.046	4044	4045	4046	rBV2	751	259	0.03%	0.004%
74	14.123	4063	4069	4071	rBV7	1570	1387	0.15%	0.019%
75	14.168	4081	4083	4086	rBV3	914	451	0.05%	0.006%
76	14.188	4088	4089	4091	rBV	1340	439	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033414.D
Acq On : 16 Dec 2023 06:01
Operator : SY/MD
Sample : 05802-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B29

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis

77	14.268	4112	4114	4117	rVB4	1145	449	0.05%	0.006%
78	14.339	4133	4136	4140	rBV4	1152	773	0.08%	0.011%
79	14.496	4182	4185	4188	rBV3	1365	738	0.08%	0.010%
80	14.747	4260	4263	4264	rBV2	1411	818	0.09%	0.011%
81	14.885	4299	4306	4309	rBV6	2080	2471	0.27%	0.035%
82	15.082	4365	4367	4370	rBV3	1257	525	0.06%	0.007%




Sum of corrected areas: 7143870

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033414.D
Acq On : 16 Dec 2023 06:01
Operator : SY/MD
Sample : 05802-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

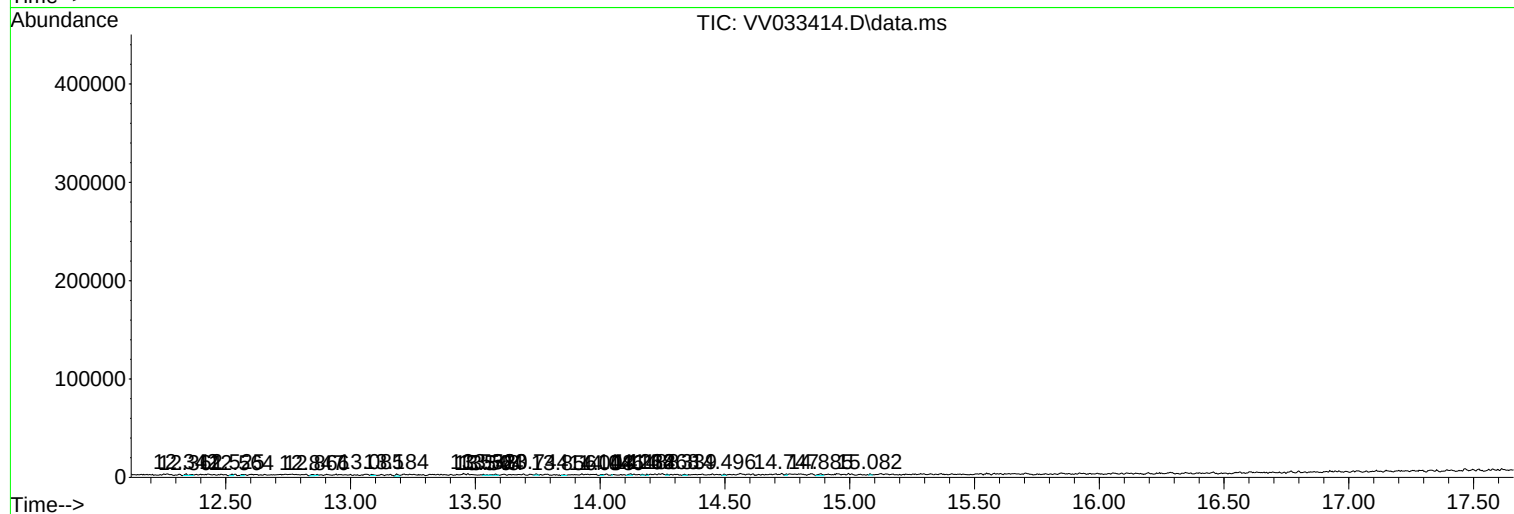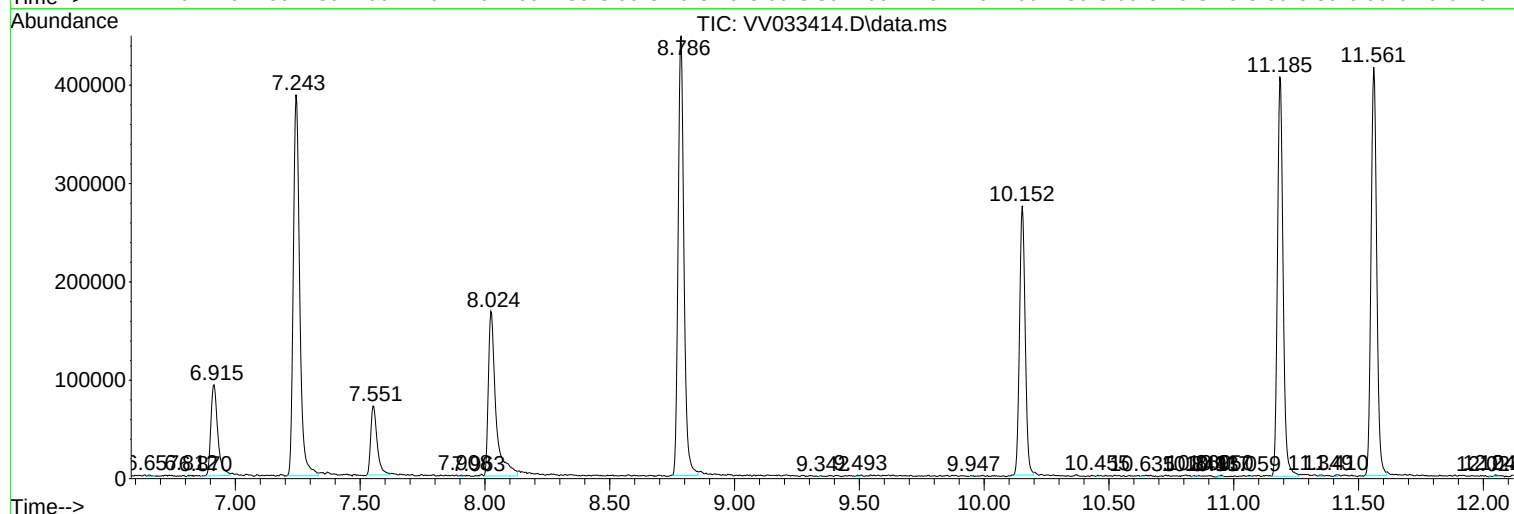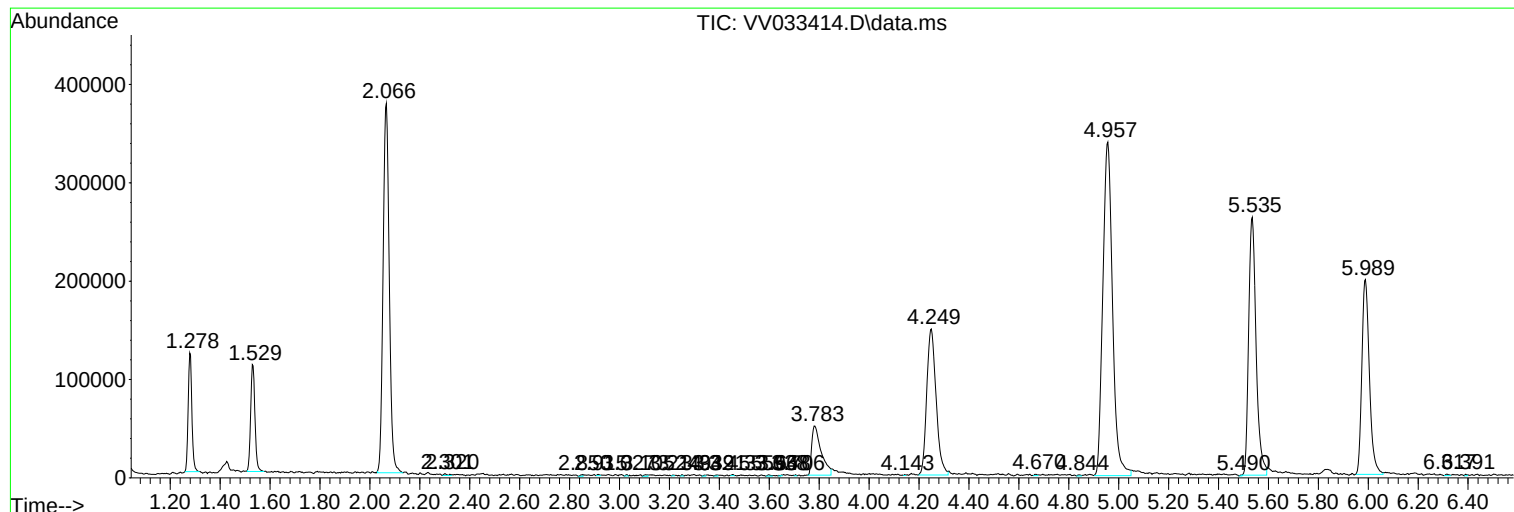

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033414.D
Acq On : 16 Dec 2023 06:01
Operator : SY/MD
Sample : 05802-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033414.D
Acq On : 16 Dec 2023 06:01
Operator : SY/MD
Sample : 05802-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------