

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033415.D
 Acq On : 16 Dec 2023 06:24
 Operator : SY/MD
 Sample : 05802-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	46	55	56	rBV9	2625	3105	0.35%	0.047%
2	1.278	68	74	86	rBV	116398	120183	13.62%	1.829%
3	1.529	146	152	170	rVB	108066	131870	14.94%	2.007%
4	2.060	307	317	336	rBV	218621	322240	36.51%	4.904%
5	2.368	411	413	415	rBV3	1158	652	0.07%	0.010%
6	2.400	421	423	427	rVB5	1661	961	0.11%	0.015%
7	2.436	431	434	435	rBV3	1873	958	0.11%	0.015%
8	2.609	485	488	492	rBV5	890	778	0.09%	0.012%
9	2.754	530	533	536	rBV6	1006	793	0.09%	0.012%
10	2.783	539	542	545	rBV4	1492	1151	0.13%	0.018%
11	2.857	560	565	570	rBV10	1403	1632	0.18%	0.025%
12	2.892	573	576	580	rVB3	1054	693	0.08%	0.011%
13	3.326	708	711	715	rBB4	1156	844	0.10%	0.013%
14	3.445	744	748	752	rVB7	1394	809	0.09%	0.012%
15	3.468	752	755	758	rBV4	902	780	0.09%	0.012%
16	3.590	789	793	796	rVB5	1879	1557	0.18%	0.024%
17	3.645	806	810	814	rBV5	1393	1496	0.17%	0.023%
18	3.786	843	854	878	rBV	49458	140635	15.94%	2.140%
19	4.072	940	943	946	rBV5	1228	1057	0.12%	0.016%
20	4.178	971	976	980	rBV6	1361	1205	0.14%	0.018%
21	4.249	985	998	1028	rVB	144268	374241	42.41%	5.695%
22	4.796	1165	1168	1171	rBV6	906	910	0.10%	0.014%
23	4.957	1201	1218	1246	rBV2	329010	882536	100.00%	13.430%
24	5.535	1387	1398	1422	rBV	246821	510984	57.90%	7.776%
25	5.989	1528	1539	1564	rVB2	194346	397271	45.01%	6.046%
26	6.497	1694	1697	1698	rBV2	1491	678	0.08%	0.010%
27	6.526	1703	1706	1710	rVB5	1315	736	0.08%	0.011%
28	6.593	1724	1727	1729	rBV3	1149	854	0.10%	0.013%
29	6.805	1791	1793	1798	rBV6	1457	1144	0.13%	0.017%
30	6.828	1798	1800	1804	rBV4	900	713	0.08%	0.011%
31	6.870	1809	1813	1815	rBV5	1215	814	0.09%	0.012%
32	6.915	1817	1827	1847	rVV	88790	169174	19.17%	2.574%
33	7.243	1919	1929	1952	rBV	371907	663255	75.15%	10.093%
34	7.555	2018	2026	2044	rBV	66387	115245	13.06%	1.754%
35	7.841	2113	2115	2120	rVB6	815	779	0.09%	0.012%
36	7.866	2120	2123	2125	rBV4	862	656	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033415.D
 Acq On : 16 Dec 2023 06:24
 Operator : SY/MD
 Sample : 05802-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.947	2145	2148	2152	rBV5	992	919	0.10%	0.014%
38	8.024	2163	2172	2189	rBV	163516	314879	35.68%	4.792%
39	8.786	2398	2409	2426	rBV	414206	685669	77.69%	10.434%
40	9.066	2495	2496	2500	rBV4	1309	925	0.10%	0.014%
41	9.310	2568	2572	2574	rBV5	1200	771	0.09%	0.012%
42	9.345	2580	2583	2585	rBV4	1348	882	0.10%	0.013%
43	9.464	2617	2620	2623	rBV5	1863	1337	0.15%	0.020%
44	9.480	2623	2625	2628	rVV3	1060	682	0.08%	0.010%
45	9.532	2636	2641	2642	rBV5	1032	705	0.08%	0.011%
46	9.648	2674	2677	2681	rBV5	876	691	0.08%	0.011%
47	9.741	2702	2706	2713	rBV7	1368	1531	0.17%	0.023%
48	9.783	2713	2719	2722	rVB6	1106	877	0.10%	0.013%
49	9.841	2734	2737	2741	rBV5	1354	997	0.11%	0.015%
50	9.934	2763	2766	2770	rVB5	1368	944	0.11%	0.014%
51	9.956	2770	2773	2775	rBV3	1210	635	0.07%	0.010%
52	10.005	2785	2788	2790	rBV3	996	656	0.07%	0.010%
53	10.152	2823	2834	2850	rBV	264098	417797	47.34%	6.358%
54	10.259	2864	2867	2874	rVB9	1660	1670	0.19%	0.025%
55	10.397	2906	2910	2915	rBV6	1261	1657	0.19%	0.025%
56	10.448	2923	2926	2929	rVB5	1180	762	0.09%	0.012%
57	10.464	2929	2931	2933	rBV2	1064	671	0.08%	0.010%
58	10.558	2957	2960	2962	rBV3	1223	777	0.09%	0.012%
59	10.648	2985	2988	2990	rBV4	1131	636	0.07%	0.010%
60	10.664	2990	2993	2996	rBV4	1394	1013	0.11%	0.015%
61	10.837	3044	3047	3049	rBV4	1265	754	0.09%	0.011%
62	10.857	3049	3053	3057	rVB7	1051	1078	0.12%	0.016%
63	10.995	3094	3096	3098	rBV3	1154	636	0.07%	0.010%
64	11.033	3105	3108	3111	rBV3	1455	1141	0.13%	0.017%
65	11.069	3116	3119	3120	rBV3	1157	663	0.08%	0.010%
66	11.133	3137	3139	3142	rBV4	1559	1019	0.12%	0.016%
67	11.185	3145	3155	3179	rVV	381863	597411	67.69%	9.091%
68	11.355	3205	3208	3212	rBV5	1181	880	0.10%	0.013%
69	11.561	3259	3272	3290	rBV	410356	646435	73.25%	9.837%
70	11.734	3324	3326	3329	rVB3	1707	889	0.10%	0.014%
71	12.210	3469	3474	3475	rBV5	1060	754	0.09%	0.011%
72	12.468	3551	3554	3556	rBV4	1435	792	0.09%	0.012%
73	12.541	3573	3577	3579	rBV5	1319	887	0.10%	0.013%
74	12.696	3623	3625	3629	rBV4	1225	961	0.11%	0.015%
75	12.754	3638	3643	3648	rBV8	999	1214	0.14%	0.018%
76	12.795	3654	3656	3659	rBV3	1619	1073	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033415.D
 Acq On : 16 Dec 2023 06:24
 Operator : SY/MD
 Sample : 05802-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.934	3697	3699	3701	rBV2	947	643	0.07%	0.010%
78	13.011	3719	3723	3725	rBV5	965	686	0.08%	0.010%
79	13.046	3731	3734	3737	rBV5	1422	1160	0.13%	0.018%
80	13.107	3751	3753	3756	rVV4	1402	760	0.09%	0.012%
81	13.255	3793	3799	3802	rVB6	1316	1127	0.13%	0.017%
82	13.275	3802	3805	3807	rBV4	1254	900	0.10%	0.014%
83	13.477	3864	3868	3871	rVB4	1698	1502	0.17%	0.023%
84	13.496	3871	3874	3876	rBV2	2017	1274	0.14%	0.019%
85	13.686	3928	3933	3937	rBV6	1631	1577	0.18%	0.024%
86	14.094	4058	4060	4062	rBV2	1488	791	0.09%	0.012%
87	14.255	4105	4110	4112	rBV4	908	787	0.09%	0.012%
88	14.332	4131	4134	4137	rVB5	1136	813	0.09%	0.012%
89	14.358	4139	4142	4144	rBV3	1036	805	0.09%	0.012%
90	14.564	4203	4206	4210	rVB4	1094	823	0.09%	0.013%
91	14.657	4232	4235	4238	rVB3	1445	860	0.10%	0.013%
92	14.699	4243	4248	4249	rBV3	1307	876	0.10%	0.013%
93	14.750	4261	4264	4268	rBV4	1319	1237	0.14%	0.019%
94	14.863	4296	4299	4302	rVB4	2065	1186	0.13%	0.018%
95	14.882	4302	4305	4309	rBV6	1478	1259	0.14%	0.019%
96	15.226	4410	4412	4414	rBV3	1364	748	0.08%	0.011%
97	15.432	4475	4476	4479	rVB3	1244	668	0.08%	0.010%
98	15.474	4485	4489	4493	rBV5	1174	1013	0.11%	0.015%
99	15.516	4500	4502	4505	rBV4	1181	702	0.08%	0.011%
100	16.181	4707	4709	4711	rBV3	1897	1030	0.12%	0.016%



Sum of corrected areas: 6571286

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033415.D
Acq On : 16 Dec 2023 06:24
Operator : SY/MD
Sample : 05802-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

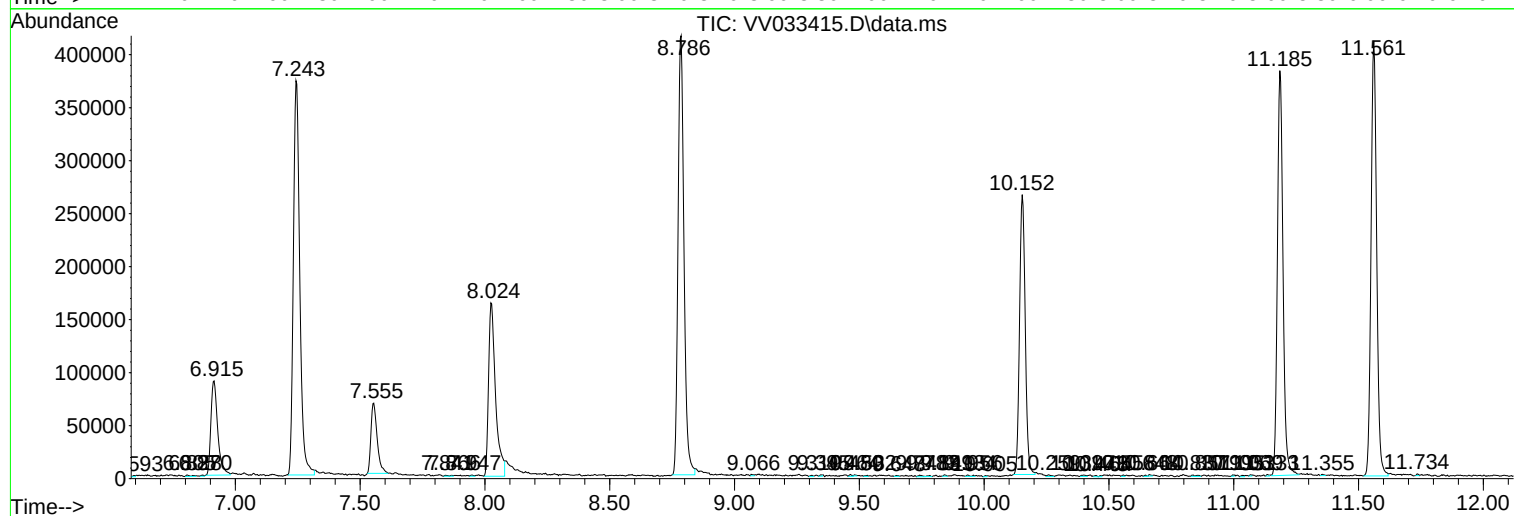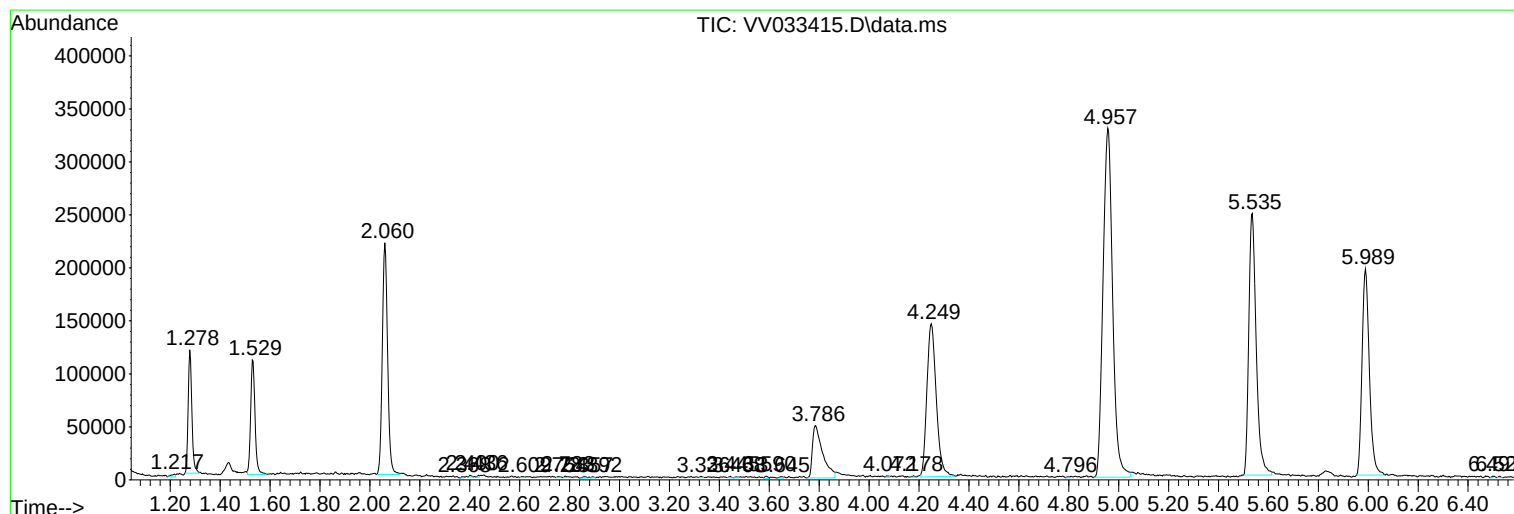

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033415.D
Acq On : 16 Dec 2023 06:24
Operator : SY/MD
Sample : 05802-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033415.D
Acq On : 16 Dec 2023 06:24
Operator : SY/MD
Sample : 05802-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------