

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033421.D
 Acq On : 16 Dec 2023 09:43
 Operator : SY/MD
 Sample : VV1215WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	125547	133090	15.57%	2.017%
2	1.529	146	152	167	rVB	112996	134650	15.75%	2.041%
3	2.060	307	317	332	rBV	222845	326665	38.22%	4.951%
4	2.169	348	351	353	rBV4	1598	891	0.10%	0.014%
5	2.375	412	415	418	rBV5	863	619	0.07%	0.009%
6	2.555	469	471	473	rVB2	1502	565	0.07%	0.009%
7	2.590	479	482	483	rBV3	905	641	0.07%	0.010%
8	2.661	500	504	506	rBV4	752	566	0.07%	0.009%
9	2.683	510	511	517	rVV5	1231	1143	0.13%	0.017%
10	2.744	527	530	531	rBV3	995	603	0.07%	0.009%
11	2.825	552	555	558	rBV4	1237	908	0.11%	0.014%
12	2.966	594	599	601	rBV5	981	938	0.11%	0.014%
13	2.998	605	609	611	rBV3	1281	948	0.11%	0.014%
14	3.079	631	634	635	rBV2	1240	714	0.08%	0.011%
15	3.114	642	645	646	rBV4	1078	601	0.07%	0.009%
16	3.150	652	656	657	rBV4	1135	862	0.10%	0.013%
17	3.227	674	680	683	rBV6	975	879	0.10%	0.013%
18	3.278	692	696	699	rBV4	736	692	0.08%	0.010%
19	3.320	707	709	711	rBV3	1142	610	0.07%	0.009%
20	3.368	722	724	728	rVB3	848	627	0.07%	0.010%
21	3.397	731	733	736	rBV3	1326	809	0.09%	0.012%
22	3.439	744	746	750	rVB5	1302	591	0.07%	0.009%
23	3.622	798	803	807	rBV8	1330	1228	0.14%	0.019%
24	3.732	836	837	841	rVB4	1480	765	0.09%	0.012%
25	3.786	845	854	875	rBV2	45057	127261	14.89%	1.929%
26	4.169	971	973	974	rBV	1451	571	0.07%	0.009%
27	4.246	985	997	1022	rVB	144404	365067	42.71%	5.533%
28	4.513	1077	1080	1081	rBV3	1172	665	0.08%	0.010%
29	4.590	1101	1104	1108	rBV4	1350	1060	0.12%	0.016%
30	4.876	1191	1193	1196	rBV3	1354	773	0.09%	0.012%
31	4.953	1201	1217	1243	rBV2	318958	854685	100.00%	12.954%
32	5.477	1377	1380	1384	rBV5	1333	1353	0.16%	0.021%
33	5.532	1384	1397	1426	rVV	255469	537574	62.90%	8.148%
34	5.985	1526	1538	1559	rBV	188101	396516	46.39%	6.010%
35	6.326	1642	1644	1646	rBV2	1089	609	0.07%	0.009%
36	6.381	1658	1661	1664	rBV5	1338	1093	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033421.D
 Acq On : 16 Dec 2023 09:43
 Operator : SY/MD
 Sample : VV1215WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.413	1667	1671	1674	rBV6	1553	1260	0.15%	0.019%
38	6.455	1682	1684	1686	rBV3	869	591	0.07%	0.009%
39	6.500	1696	1698	1703	rVB5	1025	641	0.07%	0.010%
40	6.674	1749	1752	1753	rBV2	859	558	0.07%	0.008%
41	6.793	1787	1789	1791	rBV2	1000	611	0.07%	0.009%
42	6.838	1798	1803	1805	rBV6	934	823	0.10%	0.012%
43	6.911	1815	1826	1841	rBV	93343	174727	20.44%	2.648%
44	7.243	1918	1929	1954	rBV	364126	642014	75.12%	9.731%
45	7.551	2014	2025	2043	rBV	66938	126180	14.76%	1.912%
46	7.831	2109	2112	2116	rVB6	1549	1334	0.16%	0.020%
47	7.985	2157	2160	2163	rBV5	1746	1216	0.14%	0.018%
48	8.024	2163	2172	2200	rBV	151665	321229	37.58%	4.869%
49	8.783	2398	2408	2431	rBV	432122	719228	84.15%	10.901%
50	9.181	2529	2532	2534	rVB3	1216	616	0.07%	0.009%
51	9.265	2557	2558	2560	rBV2	1180	613	0.07%	0.009%
52	9.490	2625	2628	2629	rBV3	1098	589	0.07%	0.009%
53	9.603	2660	2663	2667	rBV5	1216	1203	0.14%	0.018%
54	9.628	2667	2671	2673	rBV5	1432	1368	0.16%	0.021%
55	9.805	2722	2726	2730	rBV5	1002	1095	0.13%	0.017%
56	9.857	2739	2742	2744	rBV3	1188	579	0.07%	0.009%
57	9.992	2779	2784	2785	rBV4	877	601	0.07%	0.009%
58	10.034	2794	2797	2799	rBV4	930	618	0.07%	0.009%
59	10.098	2811	2817	2818	rBV4	1736	1283	0.15%	0.019%
60	10.153	2823	2834	2853	rVV	254086	406511	47.56%	6.161%
61	10.304	2878	2881	2883	rBV4	1259	630	0.07%	0.010%
62	10.419	2913	2917	2918	rBV4	1168	804	0.09%	0.012%
63	10.525	2946	2950	2953	rBV5	1473	1123	0.13%	0.017%
64	10.651	2986	2989	2990	rBV3	1495	797	0.09%	0.012%
65	10.789	3030	3032	3035	rBV4	1180	588	0.07%	0.009%
66	10.844	3047	3049	3053	rVB4	1254	634	0.07%	0.010%
67	10.989	3092	3094	3097	rBV2	1041	602	0.07%	0.009%
68	11.040	3107	3110	3114	rBV5	1120	1124	0.13%	0.017%
69	11.185	3145	3155	3176	rBV	400242	623262	72.92%	9.447%
70	11.561	3261	3272	3294	rBV	404163	636413	74.46%	9.646%
71	11.741	3324	3328	3332	rBV7	1332	1406	0.16%	0.021%
72	11.876	3368	3370	3375	rVB6	2069	1261	0.15%	0.019%
73	12.384	3526	3528	3531	rBV4	1009	647	0.08%	0.010%
74	12.525	3570	3572	3574	rBV3	1196	791	0.09%	0.012%
75	12.567	3581	3585	3588	rBV5	1153	706	0.08%	0.011%
76	12.583	3588	3590	3592	rBV3	1357	887	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033421.D
 Acq On : 16 Dec 2023 09:43
 Operator : SY/MD
 Sample : VV1215WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.654	3609	3612	3615	rBV3	995	612	0.07%	0.009%
78	12.805	3656	3659	3665	rVB5	1023	1067	0.12%	0.016%
79	12.924	3693	3696	3700	rBV4	1317	1000	0.12%	0.015%
80	12.963	3706	3708	3709	rBV2	1117	565	0.07%	0.009%
81	13.053	3733	3736	3739	rBV5	1223	903	0.11%	0.014%
82	13.162	3768	3770	3772	rBV2	1068	696	0.08%	0.011%
83	13.207	3779	3784	3788	rBV7	2485	2431	0.28%	0.037%
84	13.313	3815	3817	3819	rBV3	1102	563	0.07%	0.009%
85	13.525	3880	3883	3887	rBV4	1490	855	0.10%	0.013%
86	13.567	3892	3896	3898	rVB5	1108	774	0.09%	0.012%
87	13.660	3919	3925	3927	rBV6	2025	1818	0.21%	0.028%
88	13.763	3955	3957	3959	rBV2	1099	610	0.07%	0.009%
89	14.262	4108	4112	4113	rBV3	1518	954	0.11%	0.014%
90	14.377	4146	4148	4152	rBV4	1354	695	0.08%	0.011%
91	14.686	4242	4244	4248	rBV4	953	797	0.09%	0.012%
92	14.728	4253	4257	4258	rBV3	1848	1082	0.13%	0.016%
93	14.828	4285	4288	4289	rBV2	975	614	0.07%	0.009%
94	14.911	4312	4314	4319	rVB5	1345	883	0.10%	0.013%
95	14.934	4319	4321	4324	rBV2	805	561	0.07%	0.009%
96	15.313	4436	4439	4440	rBV3	1348	626	0.07%	0.009%
97	15.455	4481	4483	4485	rBV3	1432	621	0.07%	0.009%
98	15.628	4534	4537	4540	rBV4	1396	1232	0.14%	0.019%
99	15.692	4555	4557	4561	rBV7	1115	791	0.09%	0.012%
100	16.512	4809	4812	4816	rVB5	2627	1974	0.23%	0.030%




Sum of corrected areas: 6597719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033421.D
Acq On : 16 Dec 2023 09:43
Operator : SY/MD
Sample : VV1215WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

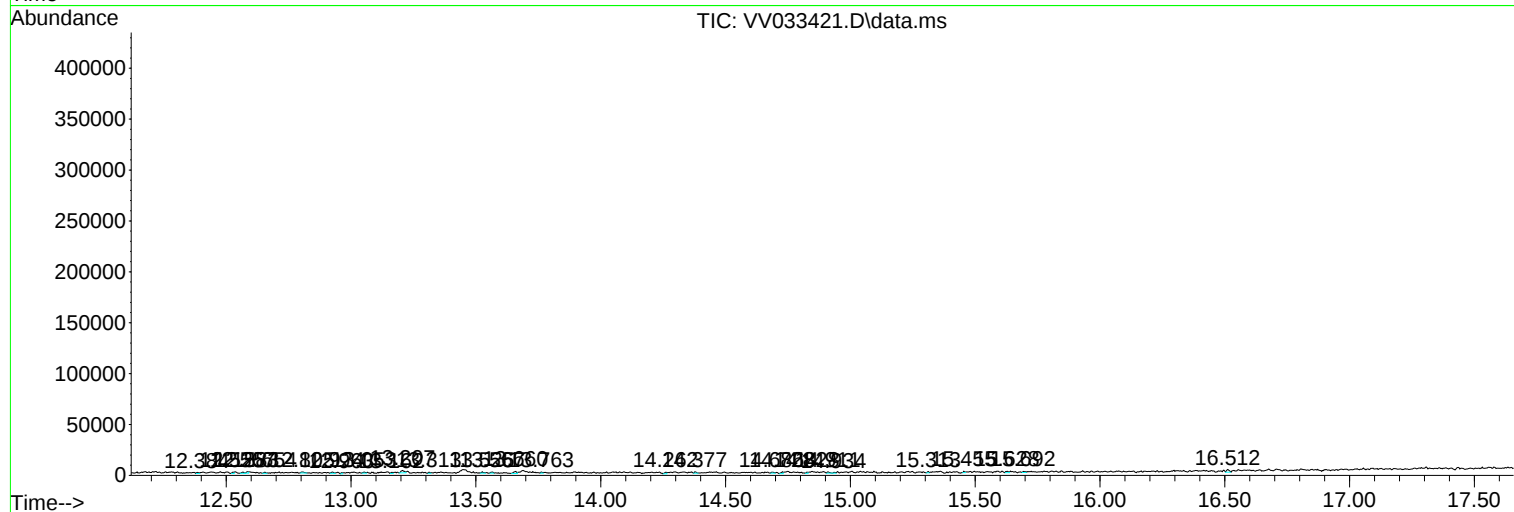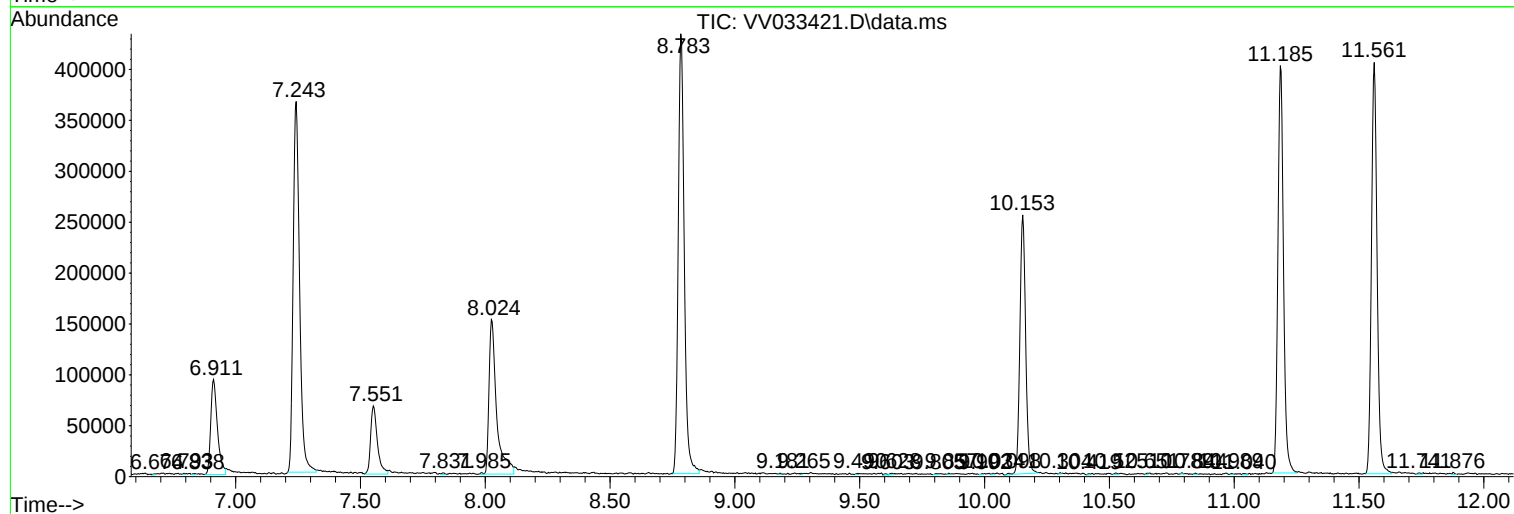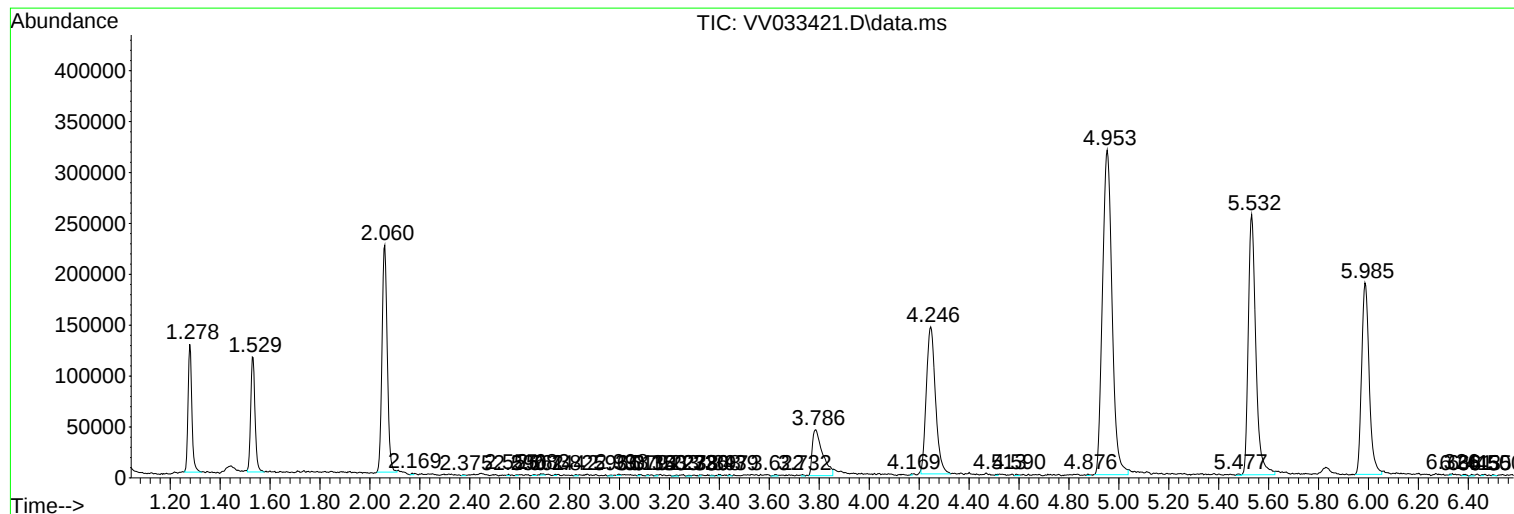

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033421.D
Acq On : 16 Dec 2023 09:43
Operator : SY/MD
Sample : VV1215WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033421.D
Acq On : 16 Dec 2023 09:43
Operator : SY/MD
Sample : VV1215WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------