

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033423.D
 Acq On : 16 Dec 2023 10:38
 Operator : SY/MD
 Sample : 05846-15DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	121264	128838	14.22%	1.810%
2	1.532	146	153	165	rVB	110491	129386	14.28%	1.818%
3	2.063	308	318	347	rVB3	356127	634748	70.05%	8.920%
4	2.507	453	456	459	rVB5	1413	769	0.08%	0.011%
5	2.703	513	517	521	rVB6	1600	1531	0.17%	0.022%
6	2.938	587	590	593	rBV4	750	618	0.07%	0.009%
7	3.011	609	613	618	rBV7	1592	1411	0.16%	0.020%
8	3.060	626	628	633	rVB5	1025	821	0.09%	0.012%
9	3.121	636	647	655	rVV3	5059	10345	1.14%	0.145%
10	3.198	668	671	672	rBV4	1270	614	0.07%	0.009%
11	3.449	744	749	750	rBV4	1546	1266	0.14%	0.018%
12	3.491	758	762	764	rBV4	1524	1353	0.15%	0.019%
13	3.545	777	779	782	rVB3	1169	651	0.07%	0.009%
14	3.581	786	790	792	rBV4	1185	872	0.10%	0.012%
15	3.648	807	811	813	rBV4	833	819	0.09%	0.012%
16	3.703	822	828	830	rBV6	1241	1082	0.12%	0.015%
17	3.783	844	853	879	rBV	54859	184141	20.32%	2.588%
18	4.249	985	998	1022	rVB	145835	368846	40.71%	5.183%
19	4.667	1123	1128	1132	rBV7	1461	1653	0.18%	0.023%
20	4.725	1143	1146	1148	rBV3	1157	614	0.07%	0.009%
21	4.761	1153	1157	1159	rBV4	1179	835	0.09%	0.012%
22	4.847	1178	1184	1188	rBV7	1048	1284	0.14%	0.018%
23	4.957	1196	1218	1242	rBV2	334207	906091	100.00%	12.732%
24	5.497	1382	1386	1387	rBV3	1515	1214	0.13%	0.017%
25	5.535	1387	1398	1422	rVV	253236	532653	58.79%	7.485%
26	5.989	1527	1539	1564	rBV	196692	410455	45.30%	5.768%
27	6.336	1644	1647	1650	rBV4	1360	819	0.09%	0.012%
28	6.362	1652	1655	1657	rBV2	995	672	0.07%	0.009%
29	6.545	1701	1712	1714	rBV10	1917	2945	0.33%	0.041%
30	6.789	1786	1788	1791	rBV3	985	702	0.08%	0.010%
31	6.912	1816	1826	1845	rBV2	96486	181391	20.02%	2.549%
32	7.143	1896	1898	1902	rBV5	1679	1222	0.13%	0.017%
33	7.243	1918	1929	1953	rBV	379979	670384	73.99%	9.420%
34	7.555	2017	2026	2043	rBV	69073	127307	14.05%	1.789%
35	7.905	2132	2135	2137	rBV3	2037	1345	0.15%	0.019%
36	7.976	2154	2157	2159	rBV3	1198	653	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033423.D
 Acq On : 16 Dec 2023 10:38
 Operator : SY/MD
 Sample : 05846-15DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.024	2163	2172	2199	rVV	166031	338731	37.38%	4.760%
38	8.584	2341	2346	2351	rBV7	2063	2102	0.23%	0.030%
39	8.715	2382	2387	2389	rBV7	1707	1391	0.15%	0.020%
40	8.783	2393	2408	2432	rBV	425628	718234	79.27%	10.093%
41	9.050	2488	2491	2495	rBV7	1355	1255	0.14%	0.018%
42	9.137	2515	2518	2520	rBV4	1313	646	0.07%	0.009%
43	9.149	2520	2522	2525	rBV4	1155	944	0.10%	0.013%
44	9.307	2567	2571	2575	rBV6	1396	1342	0.15%	0.019%
45	9.352	2582	2585	2586	rBV3	1234	634	0.07%	0.009%
46	9.432	2605	2610	2611	rBV5	1313	1023	0.11%	0.014%
47	9.612	2663	2666	2668	rBV3	1122	665	0.07%	0.009%
48	9.677	2684	2686	2692	rVB6	1868	1547	0.17%	0.022%
49	9.918	2756	2761	2765	rBV6	630	813	0.09%	0.011%
50	9.966	2774	2776	2778	rBV3	1542	952	0.11%	0.013%
51	10.153	2823	2834	2855	rVB	272879	434042	47.90%	6.099%
52	10.484	2934	2937	2941	rVB5	1294	771	0.09%	0.011%
53	10.522	2945	2949	2954	rBV7	1996	1911	0.21%	0.027%
54	10.715	3007	3009	3013	rVB3	1353	791	0.09%	0.011%
55	10.741	3013	3017	3020	rBV5	920	811	0.09%	0.011%
56	10.886	3057	3062	3064	rVB5	1547	1017	0.11%	0.014%
57	10.931	3073	3076	3081	rVB6	946	751	0.08%	0.011%
58	10.989	3085	3094	3096	rBV8	1209	1367	0.15%	0.019%
59	11.185	3145	3155	3177	rBV	386709	609785	67.30%	8.569%
60	11.423	3227	3229	3233	rBV5	1186	872	0.10%	0.012%
61	11.458	3237	3240	3244	rBV6	1133	877	0.10%	0.012%
62	11.561	3261	3272	3295	rBV	404130	641518	70.80%	9.015%
63	11.786	3337	3342	3346	rBV6	1638	1395	0.15%	0.020%
64	11.863	3363	3366	3370	rBV5	1338	1019	0.11%	0.014%
65	11.982	3399	3403	3404	rBV4	1140	811	0.09%	0.011%
66	12.014	3409	3413	3418	rBV7	993	1193	0.13%	0.017%
67	12.127	3443	3448	3450	rBV5	1637	1453	0.16%	0.020%
68	12.201	3468	3471	3474	rVB6	1173	861	0.10%	0.012%
69	12.307	3501	3504	3511	rVB8	1450	1203	0.13%	0.017%
70	12.490	3557	3561	3563	rBV5	1207	996	0.11%	0.014%
71	12.529	3569	3573	3574	rBV3	1012	679	0.07%	0.010%
72	12.554	3577	3581	3588	rVB7	1422	1486	0.16%	0.021%
73	12.583	3588	3590	3592	rBV3	1373	949	0.10%	0.013%
74	12.625	3601	3603	3608	rVB4	1209	821	0.09%	0.012%
75	12.664	3613	3615	3618	rBV3	935	657	0.07%	0.009%
76	12.799	3653	3657	3659	rBV4	1219	826	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033423.D
 Acq On : 16 Dec 2023 10:38
 Operator : SY/MD
 Sample : 05846-15DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.895	3684	3687	3690	rBV4	1228	909	0.10%	0.013%
78	12.931	3694	3698	3700	rBV4	866	615	0.07%	0.009%
79	13.098	3747	3750	3754	rBV6	1231	1125	0.12%	0.016%
80	13.169	3766	3772	3773	rBV6	942	841	0.09%	0.012%
81	13.207	3782	3784	3786	rBV3	1225	716	0.08%	0.010%
82	13.413	3844	3848	3851	rBV6	1053	1079	0.12%	0.015%
83	13.452	3857	3860	3864	rBV5	1852	1685	0.19%	0.024%
84	13.571	3892	3897	3898	rBV5	1331	964	0.11%	0.014%
85	13.670	3926	3928	3932	rVV4	2135	1349	0.15%	0.019%
86	13.689	3932	3934	3938	rVB4	1620	1114	0.12%	0.016%
87	13.831	3975	3978	3984	rBV6	1108	1119	0.12%	0.016%
88	13.876	3990	3992	3996	rVB2	1564	896	0.10%	0.013%
89	13.995	4027	4029	4034	rVB6	1430	890	0.10%	0.013%
90	14.021	4034	4037	4040	rBV4	1254	971	0.11%	0.014%
91	14.088	4053	4058	4060	rBV5	1524	1236	0.14%	0.017%
92	14.497	4182	4185	4189	rBV4	1223	1380	0.15%	0.019%
93	14.551	4199	4202	4205	rBV4	1378	1258	0.14%	0.018%
94	14.599	4212	4217	4218	rBV5	1468	1108	0.12%	0.016%
95	14.898	4304	4310	4311	rBV4	1418	1351	0.15%	0.019%
96	14.908	4311	4313	4320	rVB7	1392	1122	0.12%	0.016%
97	14.998	4339	4341	4347	rBV7	1063	850	0.09%	0.012%
98	15.455	4477	4483	4486	rBV7	1718	1776	0.20%	0.025%
99	15.516	4499	4502	4505	rBV4	1005	744	0.08%	0.010%
100	15.628	4530	4537	4539	rBV7	1776	1805	0.20%	0.025%




Sum of corrected areas: 7116394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033423.D
Acq On : 16 Dec 2023 10:38
Operator : SY/MD
Sample : 05846-15DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

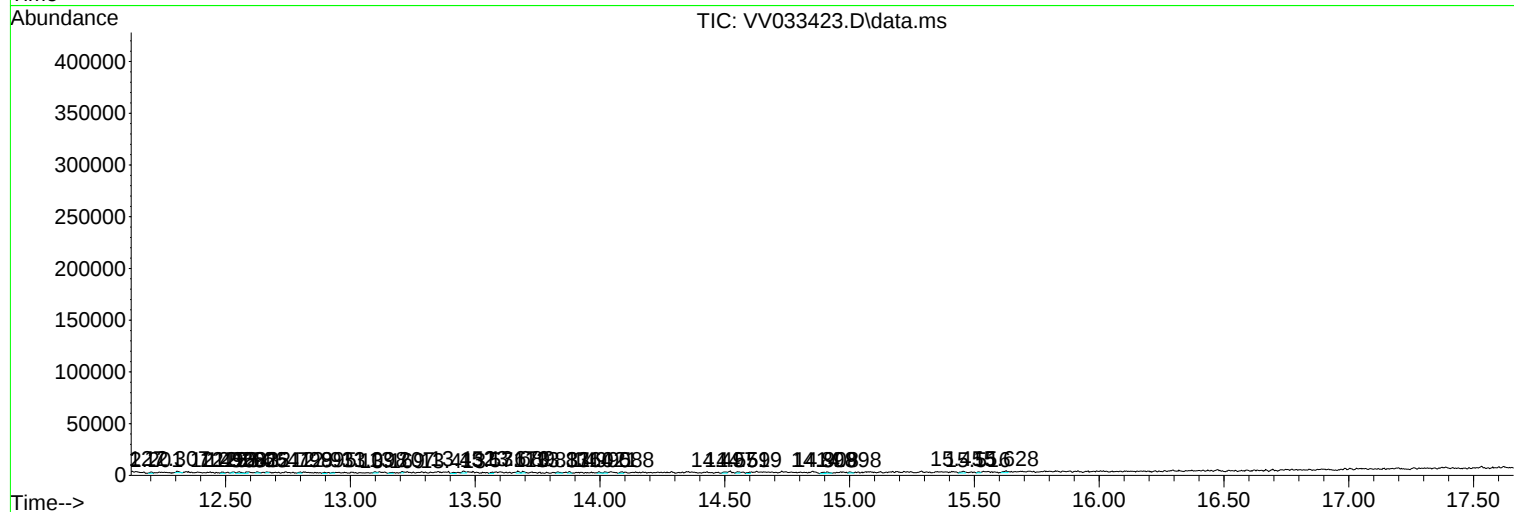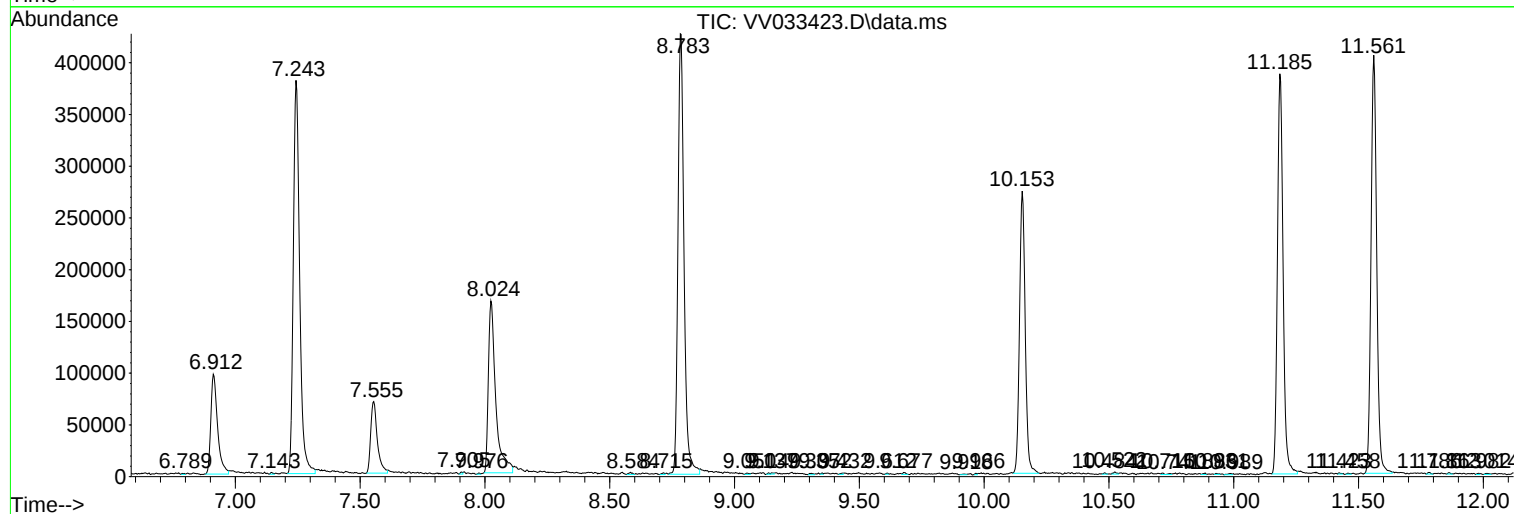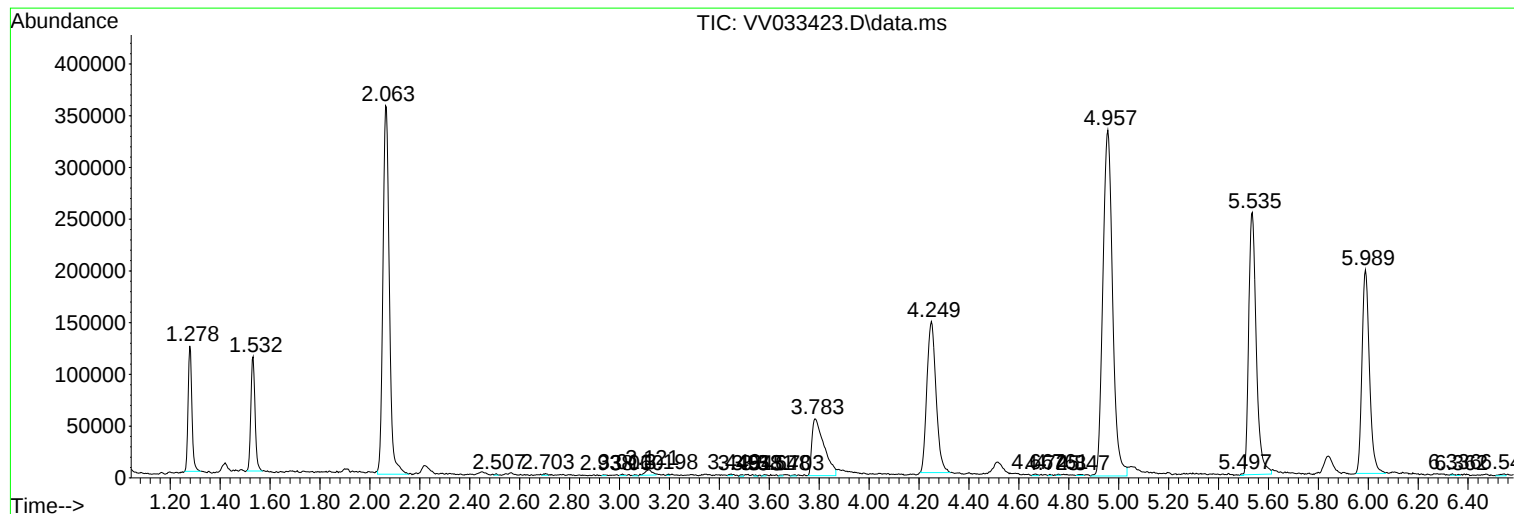

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033423.D
Acq On : 16 Dec 2023 10:38
Operator : SY/MD
Sample : 05846-15DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033423.D
Acq On : 16 Dec 2023 10:38
Operator : SY/MD
Sample : 05846-15DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------