

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033428.D
 Acq On : 16 Dec 2023 12:34
 Operator : SY/MD
 Sample : 05846-12DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	131574	141288	15.35%	1.970%
2	1.532	146	153	168	rVB	108146	132206	14.37%	1.843%
3	2.066	308	319	349	rVB3	401437	702219	76.30%	9.792%
4	2.429	427	432	433	rBV4	1831	1251	0.14%	0.017%
5	2.510	455	457	460	rVB3	1523	678	0.07%	0.009%
6	2.539	463	466	467	rBV3	1237	684	0.07%	0.010%
7	2.706	513	518	521	rBV7	1179	795	0.09%	0.011%
8	2.741	526	529	530	rBV3	1465	739	0.08%	0.010%
9	2.934	586	589	594	rVB7	1724	1268	0.14%	0.018%
10	3.111	632	644	646	rBV2	7975	10863	1.18%	0.151%
11	3.471	749	756	761	rBV8	1127	1504	0.16%	0.021%
12	3.510	766	768	773	rVB5	1461	965	0.10%	0.013%
13	3.542	773	778	782	rBV6	1572	1594	0.17%	0.022%
14	3.648	807	811	814	rBV4	1257	965	0.10%	0.013%
15	3.664	814	816	820	rBV5	907	710	0.08%	0.010%
16	3.709	826	830	833	rBV5	1372	986	0.11%	0.014%
17	3.783	844	853	877	rBV	57194	165315	17.96%	2.305%
18	4.072	941	943	949	rBV6	871	976	0.11%	0.014%
19	4.114	954	956	959	rBV4	1460	833	0.09%	0.012%
20	4.249	981	998	1019	rBV2	147008	387777	42.14%	5.407%
21	4.879	1190	1194	1195	rBV4	985	632	0.07%	0.009%
22	4.957	1201	1218	1248	rBV2	341980	920315	100.00%	12.833%
23	5.346	1337	1339	1344	rBV5	1391	1226	0.13%	0.017%
24	5.535	1386	1398	1422	rBV	236862	498437	54.16%	6.950%
25	5.947	1523	1526	1527	rBV3	1498	1024	0.11%	0.014%
26	5.989	1528	1539	1557	rVV	204749	414850	45.08%	5.785%
27	6.596	1725	1728	1731	rBV4	994	798	0.09%	0.011%
28	6.757	1774	1778	1780	rBV4	2020	1577	0.17%	0.022%
29	6.915	1816	1827	1848	rBV2	99321	189043	20.54%	2.636%
30	7.053	1868	1870	1874	rBV5	1495	722	0.08%	0.010%
31	7.243	1919	1929	1957	rBV	388226	684309	74.36%	9.542%
32	7.555	2017	2026	2048	rBV	72504	129771	14.10%	1.809%
33	7.834	2111	2113	2115	rBV3	1285	718	0.08%	0.010%
34	8.024	2163	2172	2208	rVV	184217	380662	41.36%	5.308%
35	8.423	2293	2296	2300	rBV6	1295	1116	0.12%	0.016%
36	8.786	2398	2409	2426	rBV	394991	655604	71.24%	9.142%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033428.D
 Acq On : 16 Dec 2023 12:34
 Operator : SY/MD
 Sample : 05846-12DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.214	2538	2542	2544	rBV4	1327	954	0.10%	0.013%
38	9.407	2599	2602	2605	rBV5	1035	727	0.08%	0.010%
39	9.423	2605	2607	2611	rVV4	1595	1026	0.11%	0.014%
40	9.487	2620	2627	2630	rVB7	2263	2005	0.22%	0.028%
41	9.526	2630	2639	2640	rBV6	1679	1725	0.19%	0.024%
42	9.625	2668	2670	2675	rBV4	1508	1464	0.16%	0.020%
43	9.809	2722	2727	2729	rBV4	1235	849	0.09%	0.012%
44	9.928	2761	2764	2768	rVB6	1130	840	0.09%	0.012%
45	9.998	2778	2786	2788	rBV7	1248	1512	0.16%	0.021%
46	10.153	2819	2834	2854	rBV	283456	455393	49.48%	6.350%
47	10.313	2881	2884	2886	rBV4	1356	787	0.09%	0.011%
48	10.374	2900	2903	2907	rBV4	1096	1217	0.13%	0.017%
49	10.484	2933	2937	2939	rBV5	1444	928	0.10%	0.013%
50	10.519	2942	2948	2952	rBV10	1637	2081	0.23%	0.029%
51	10.770	3023	3026	3028	rBV3	1421	915	0.10%	0.013%
52	10.873	3052	3058	3062	rVB6	1671	1639	0.18%	0.023%
53	11.005	3097	3099	3103	rVV3	1280	842	0.09%	0.012%
54	11.056	3111	3115	3120	rBV7	1132	1547	0.17%	0.022%
55	11.188	3144	3156	3171	rBV	359690	564388	61.33%	7.870%
56	11.342	3201	3204	3207	rVB4	1351	892	0.10%	0.012%
57	11.400	3217	3222	3224	rBV6	1144	1104	0.12%	0.015%
58	11.419	3226	3228	3233	rVB4	1434	911	0.10%	0.013%
59	11.561	3261	3272	3291	rBV	415909	652661	70.92%	9.101%
60	11.834	3355	3357	3362	rVB4	1369	1090	0.12%	0.015%
61	12.027	3414	3417	3420	rBV5	1382	1088	0.12%	0.015%
62	12.194	3466	3469	3474	rVB6	1593	1688	0.18%	0.024%
63	12.246	3482	3485	3488	rVV4	1276	734	0.08%	0.010%
64	12.410	3532	3536	3539	rVV5	840	682	0.07%	0.010%
65	12.442	3542	3546	3550	rVB5	922	937	0.10%	0.013%
66	12.525	3570	3572	3575	rVB5	1156	638	0.07%	0.009%
67	12.612	3593	3599	3600	rVB4	1135	844	0.09%	0.012%
68	12.815	3656	3662	3665	rBV6	1495	1269	0.14%	0.018%
69	12.902	3686	3689	3692	rBV4	1832	1386	0.15%	0.019%
70	13.011	3719	3723	3726	rBV5	1015	918	0.10%	0.013%
71	13.079	3739	3744	3746	rBV5	1324	1114	0.12%	0.016%
72	13.339	3821	3825	3828	rBV6	1719	1639	0.18%	0.023%
73	13.403	3840	3845	3846	rBV3	915	637	0.07%	0.009%
74	13.580	3896	3900	3902	rBV6	1189	846	0.09%	0.012%
75	13.606	3905	3908	3914	rBV7	1303	1363	0.15%	0.019%
76	13.670	3923	3928	3930	rBV5	1894	1687	0.18%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033428.D
 Acq On : 16 Dec 2023 12:34
 Operator : SY/MD
 Sample : 05846-12DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.773	3957	3960	3961	rBV3	1163	663	0.07%	0.009%
78	13.808	3967	3971	3973	rBV4	1113	749	0.08%	0.010%
79	13.857	3985	3986	3990	rBV4	1011	736	0.08%	0.010%
80	13.889	3990	3996	3999	rBV7	1453	1670	0.18%	0.023%
81	13.985	4023	4026	4029	rVV5	1767	1448	0.16%	0.020%
82	14.008	4031	4033	4039	rVB4	1251	1043	0.11%	0.015%
83	14.149	4073	4077	4078	rBV4	1150	737	0.08%	0.010%
84	14.239	4103	4105	4109	rVB5	1556	1105	0.12%	0.015%
85	14.300	4122	4124	4128	rBV5	918	740	0.08%	0.010%
86	14.377	4146	4148	4152	rBV5	843	687	0.07%	0.010%
87	14.532	4193	4196	4197	rBV3	1345	794	0.09%	0.011%
88	14.606	4217	4219	4221	rBV3	1053	625	0.07%	0.009%
89	14.683	4239	4243	4244	rBV3	1160	945	0.10%	0.013%
90	14.795	4275	4278	4279	rBV3	1595	874	0.09%	0.012%
91	14.841	4287	4292	4293	rBV4	1238	1145	0.12%	0.016%
92	14.966	4327	4331	4334	rBV6	1333	1260	0.14%	0.018%
93	15.168	4391	4394	4396	rBV3	1021	656	0.07%	0.009%
94	15.323	4439	4442	4444	rBV4	1022	725	0.08%	0.010%
95	15.477	4487	4490	4492	rBV3	1616	1141	0.12%	0.016%
96	15.683	4551	4554	4556	rBV4	1348	898	0.10%	0.013%
97	15.725	4565	4567	4569	rBV3	1721	799	0.09%	0.011%
98	15.847	4603	4605	4610	rBV6	1184	965	0.10%	0.013%
99	16.046	4665	4667	4669	rBV3	1428	775	0.08%	0.011%
100	16.098	4680	4683	4685	rBV3	1380	1088	0.12%	0.015%


Sum of corrected areas: 7171655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033428.D
Acq On : 16 Dec 2023 12:34
Operator : SY/MD
Sample : 05846-12DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

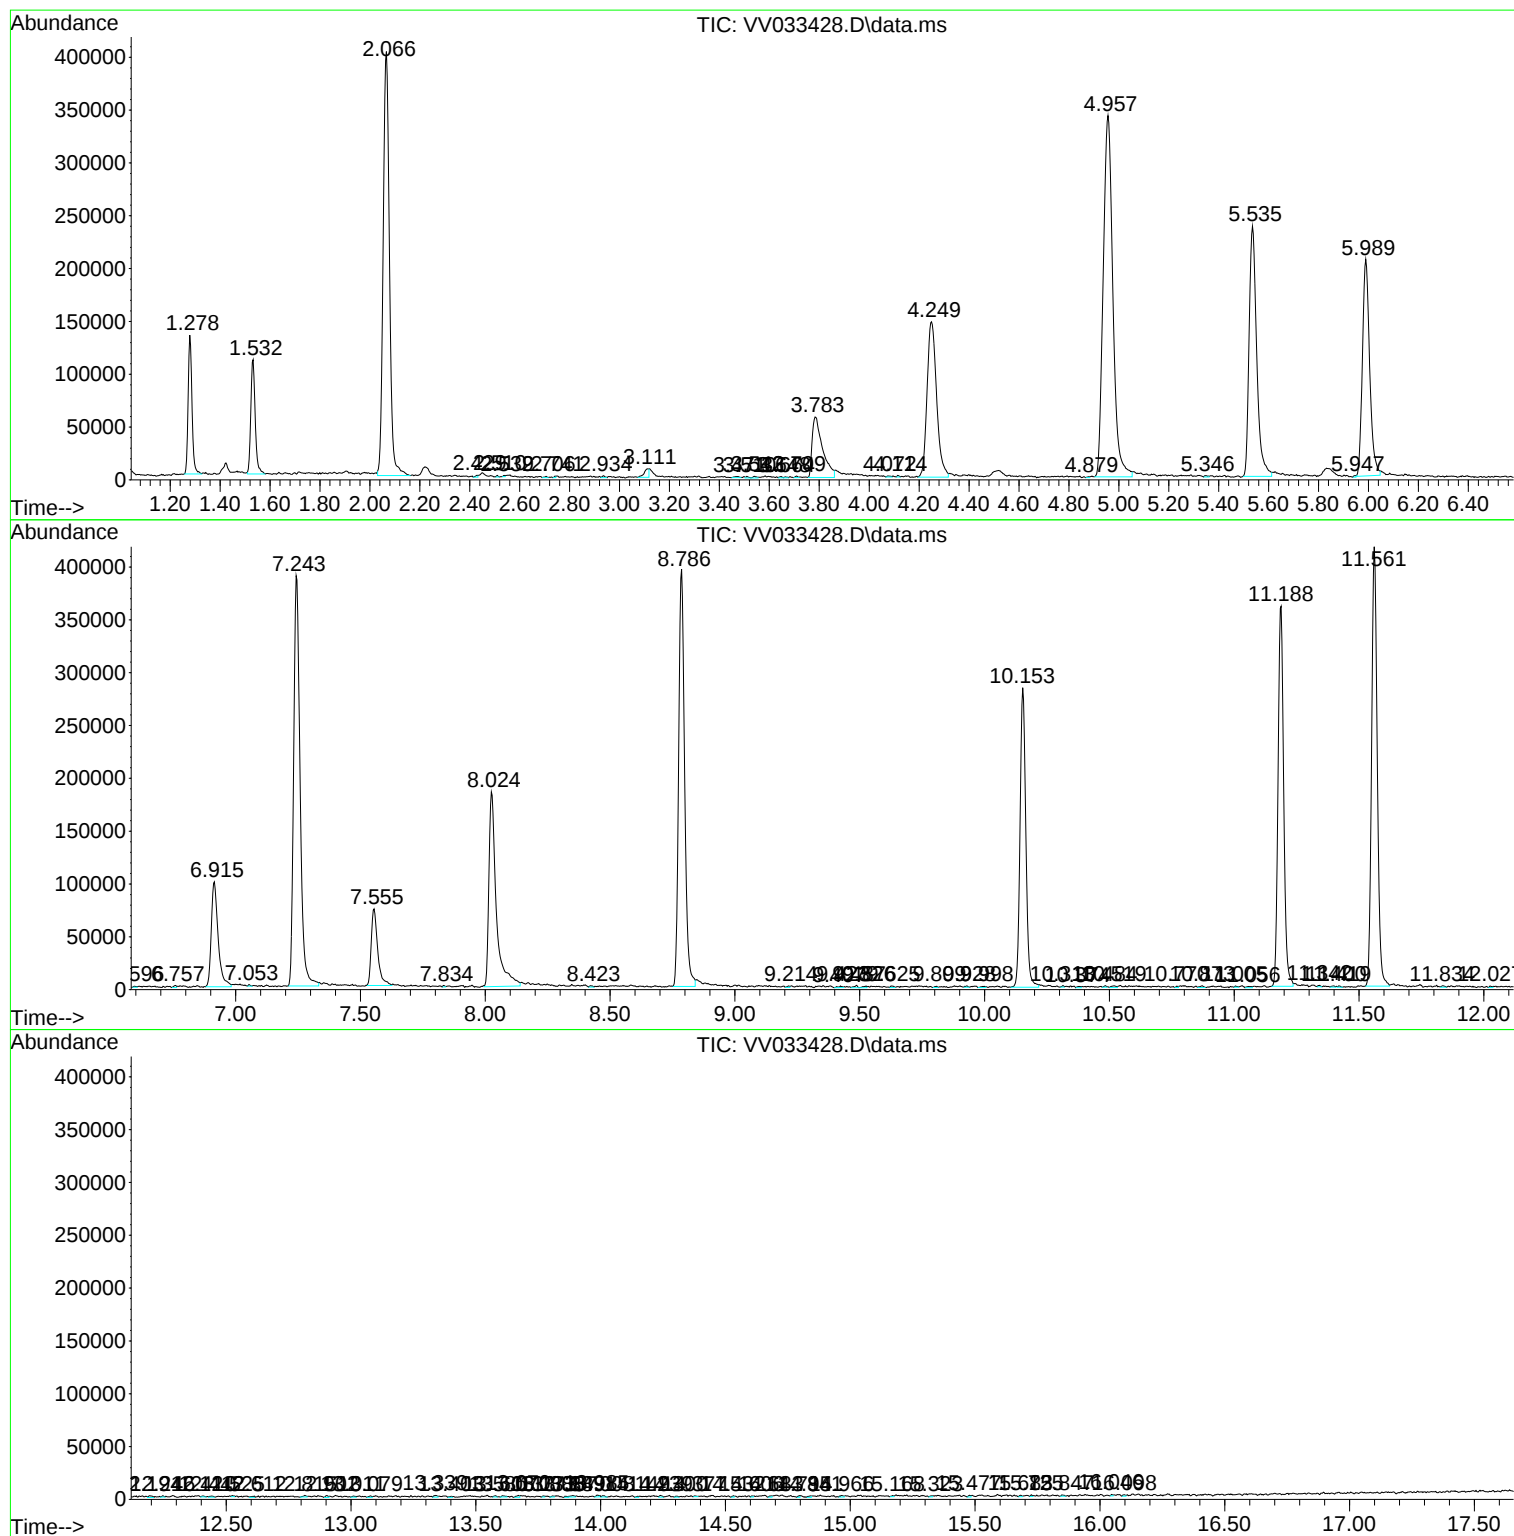

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033428.D
Acq On : 16 Dec 2023 12:34
Operator : SY/MD
Sample : 05846-12DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033428.D
Acq On : 16 Dec 2023 12:34
Operator : SY/MD
Sample : 05846-12DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------