

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033429.D
 Acq On : 16 Dec 2023 12:57
 Operator : SY/MD
 Sample : 05846-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rBV	126309	132484	14.93%	1.837%
2	1.532	146	153	163	rBV	104889	123929	13.97%	1.719%
3	2.066	308	319	346	rVB3	416305	726755	81.92%	10.079%
4	2.442	431	436	437	rBV5	3905	3094	0.35%	0.043%
5	2.545	466	468	471	rVV3	1070	589	0.07%	0.008%
6	2.616	485	490	492	rBV4	776	802	0.09%	0.011%
7	2.670	505	507	510	rVB3	1152	600	0.07%	0.008%
8	2.693	510	514	517	rBV4	1830	1625	0.18%	0.023%
9	2.764	534	536	538	rBV2	1129	814	0.09%	0.011%
10	2.831	555	557	559	rBV2	1389	825	0.09%	0.011%
11	2.937	586	590	592	rBV4	1557	977	0.11%	0.014%
12	2.976	599	602	603	rBV3	911	592	0.07%	0.008%
13	3.079	632	634	636	rVV3	1216	626	0.07%	0.009%
14	3.114	636	645	659	rVB2	9242	19448	2.19%	0.270%
15	3.288	695	699	704	rBV7	1383	1340	0.15%	0.019%
16	3.314	704	707	712	rVV7	1138	1059	0.12%	0.015%
17	3.445	744	748	750	rBV3	1387	959	0.11%	0.013%
18	3.786	841	854	879	rBV	52396	157403	17.74%	2.183%
19	4.249	986	998	1022	rVB	144294	363275	40.95%	5.038%
20	4.426	1050	1053	1054	rBV3	1145	628	0.07%	0.009%
21	4.696	1134	1137	1139	rBV2	1918	1166	0.13%	0.016%
22	4.757	1153	1156	1158	rBV4	1250	838	0.09%	0.012%
23	4.957	1202	1218	1245	rBV3	326121	887156	100.00%	12.304%
24	5.416	1359	1361	1365	rVB4	1175	648	0.07%	0.009%
25	5.535	1387	1398	1423	rBV	261423	545397	61.48%	7.564%
26	5.989	1525	1539	1564	rBV	198817	416165	46.91%	5.772%
27	6.278	1627	1629	1634	rVB6	1895	1285	0.14%	0.018%
28	6.346	1648	1650	1653	rVB3	1396	661	0.07%	0.009%
29	6.452	1681	1683	1686	rVB4	1317	584	0.07%	0.008%
30	6.545	1709	1712	1716	rVB5	1175	657	0.07%	0.009%
31	6.603	1724	1730	1735	rBV8	1825	1886	0.21%	0.026%
32	6.915	1818	1827	1849	rBV	92604	174083	19.62%	2.414%
33	7.127	1891	1893	1896	rBV4	1291	779	0.09%	0.011%
34	7.246	1918	1930	1958	rBV	365645	667158	75.20%	9.253%
35	7.555	2017	2026	2044	rBV	70536	123120	13.88%	1.708%
36	7.847	2115	2117	2120	rBV4	910	587	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033429.D
 Acq On : 16 Dec 2023 12:57
 Operator : SY/MD
 Sample : 05846-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.866	2120	2123	2128	rVB6	1324	983	0.11%	0.014%
38	8.024	2163	2172	2202	rBV	172323	355521	40.07%	4.931%
39	8.419	2291	2295	2298	rBV5	1056	800	0.09%	0.011%
40	8.474	2306	2312	2313	rBV5	1575	1347	0.15%	0.019%
41	8.535	2330	2331	2334	rVB3	1806	711	0.08%	0.010%
42	8.561	2335	2339	2342	rBV5	1655	1169	0.13%	0.016%
43	8.645	2362	2365	2367	rBV4	1099	646	0.07%	0.009%
44	8.680	2372	2376	2378	rBV4	1400	1245	0.14%	0.017%
45	8.786	2396	2409	2431	rBV	443441	733870	82.72%	10.178%
46	9.124	2512	2514	2517	rBV4	1072	769	0.09%	0.011%
47	9.185	2531	2533	2535	rVB3	1166	586	0.07%	0.008%
48	9.207	2535	2540	2544	rBV7	1179	1200	0.14%	0.017%
49	9.493	2627	2629	2633	rVB4	1130	620	0.07%	0.009%
50	9.628	2668	2671	2672	rBV3	1249	691	0.08%	0.010%
51	9.722	2698	2700	2704	rVB3	1086	703	0.08%	0.010%
52	10.152	2824	2834	2855	rVB	275691	436159	49.16%	6.049%
53	10.535	2946	2953	2956	rBV5	1993	1988	0.22%	0.028%
54	10.664	2990	2993	2996	rVB5	991	646	0.07%	0.009%
55	10.757	3018	3022	3025	rBV5	1420	1003	0.11%	0.014%
56	10.792	3025	3033	3039	rVB5	1555	2360	0.27%	0.033%
57	10.863	3052	3055	3057	rBV4	1598	1022	0.12%	0.014%
58	10.921	3071	3073	3076	rBV4	1375	900	0.10%	0.012%
59	10.995	3094	3096	3099	rVB4	1241	583	0.07%	0.008%
60	11.098	3125	3128	3132	rBV5	1070	860	0.10%	0.012%
61	11.117	3132	3134	3137	rVV3	1050	704	0.08%	0.010%
62	11.185	3144	3155	3175	rBV	391905	630306	71.05%	8.742%
63	11.419	3221	3228	3229	rBV8	1273	1432	0.16%	0.020%
64	11.561	3258	3272	3292	rBV	400656	634931	71.57%	8.806%
65	11.776	3337	3339	3346	rVB7	2170	1472	0.17%	0.020%
66	11.876	3368	3370	3376	rBV6	1087	644	0.07%	0.009%
67	12.021	3411	3415	3417	rBV5	672	583	0.07%	0.008%
68	12.117	3443	3445	3448	rBV3	871	691	0.08%	0.010%
69	12.233	3476	3481	3485	rBV6	1265	1566	0.18%	0.022%
70	12.278	3492	3495	3499	rBV7	1463	1512	0.17%	0.021%
71	12.455	3548	3550	3553	rVB2	1396	789	0.09%	0.011%
72	12.477	3553	3557	3561	rBV6	1341	959	0.11%	0.013%
73	12.699	3622	3626	3629	rBV5	1175	1283	0.14%	0.018%
74	12.757	3642	3644	3647	rBV4	1203	709	0.08%	0.010%
75	12.776	3647	3650	3653	rBV3	1323	987	0.11%	0.014%
76	12.879	3679	3682	3686	rVB6	2149	1793	0.20%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033429.D
 Acq On : 16 Dec 2023 12:57
 Operator : SY/MD
 Sample : 05846-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHD4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.127	3757	3759	3761	rBV3	1112	641	0.07%	0.009%
78	13.268	3801	3803	3807	rVB4	1323	710	0.08%	0.010%
79	13.291	3807	3810	3814	rBV6	1415	1173	0.13%	0.016%
80	13.310	3814	3816	3821	rVB5	1335	796	0.09%	0.011%
81	13.416	3846	3849	3852	rBV5	1033	699	0.08%	0.010%
82	13.500	3871	3875	3877	rBV4	1197	915	0.10%	0.013%
83	13.551	3886	3891	3898	rVB8	1091	1130	0.13%	0.016%
84	13.673	3927	3929	3931	rVV3	1424	869	0.10%	0.012%
85	13.857	3983	3986	3990	rVB5	1290	1052	0.12%	0.015%
86	13.882	3991	3994	3995	rBV3	1260	607	0.07%	0.008%
87	13.972	4017	4022	4024	rBV5	1573	1051	0.12%	0.015%
88	14.021	4035	4037	4041	rBV4	1009	734	0.08%	0.010%
89	14.094	4057	4060	4062	rBV4	1740	1234	0.14%	0.017%
90	14.159	4078	4080	4083	rBV3	1338	753	0.08%	0.010%
91	14.217	4093	4098	4103	rVB6	1539	1642	0.19%	0.023%
92	14.246	4103	4107	4108	rBV4	1082	812	0.09%	0.011%
93	14.397	4151	4154	4156	rBV3	907	620	0.07%	0.009%
94	14.471	4175	4177	4182	rVB7	932	881	0.10%	0.012%
95	14.718	4250	4254	4256	rVB5	898	699	0.08%	0.010%
96	15.291	4430	4432	4439	rVB7	1467	1203	0.14%	0.017%
97	15.953	4635	4638	4641	rBV5	2203	1421	0.16%	0.020%
98	16.004	4649	4654	4655	rBV4	1604	1261	0.14%	0.017%
99	16.075	4674	4676	4677	rBV	1566	654	0.07%	0.009%
100	16.506	4805	4810	4811	rBV5	2416	2029	0.23%	0.028%




Sum of corrected areas: 7210323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033429.D
Acq On : 16 Dec 2023 12:57
Operator : SY/MD
Sample : 05846-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

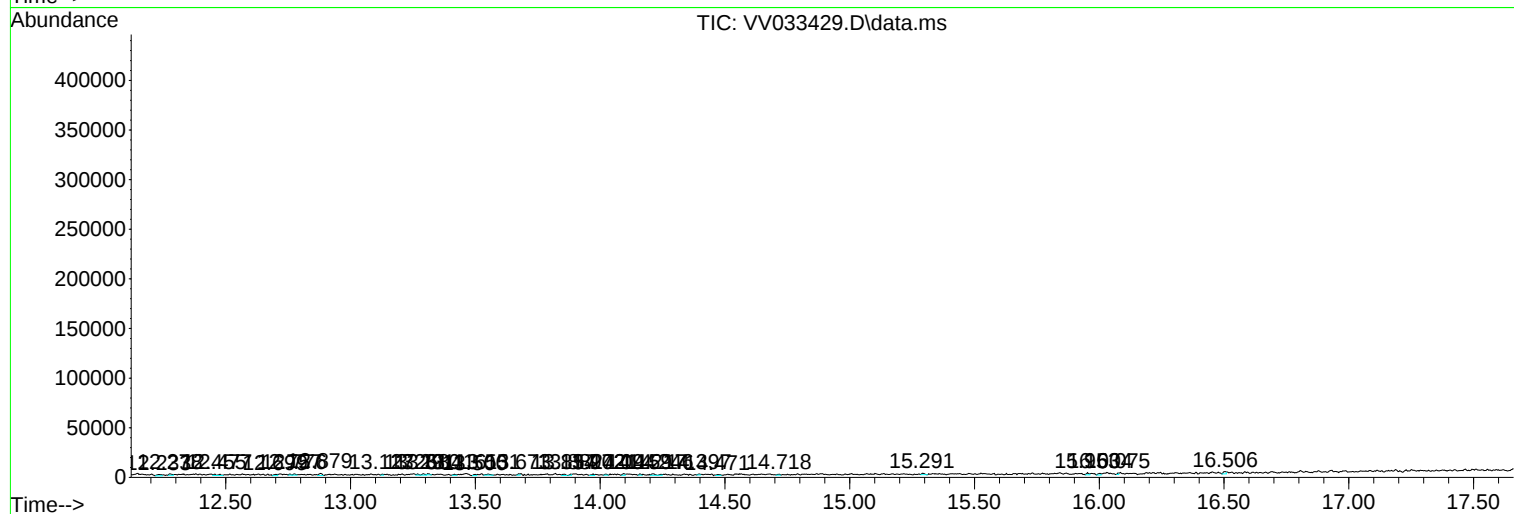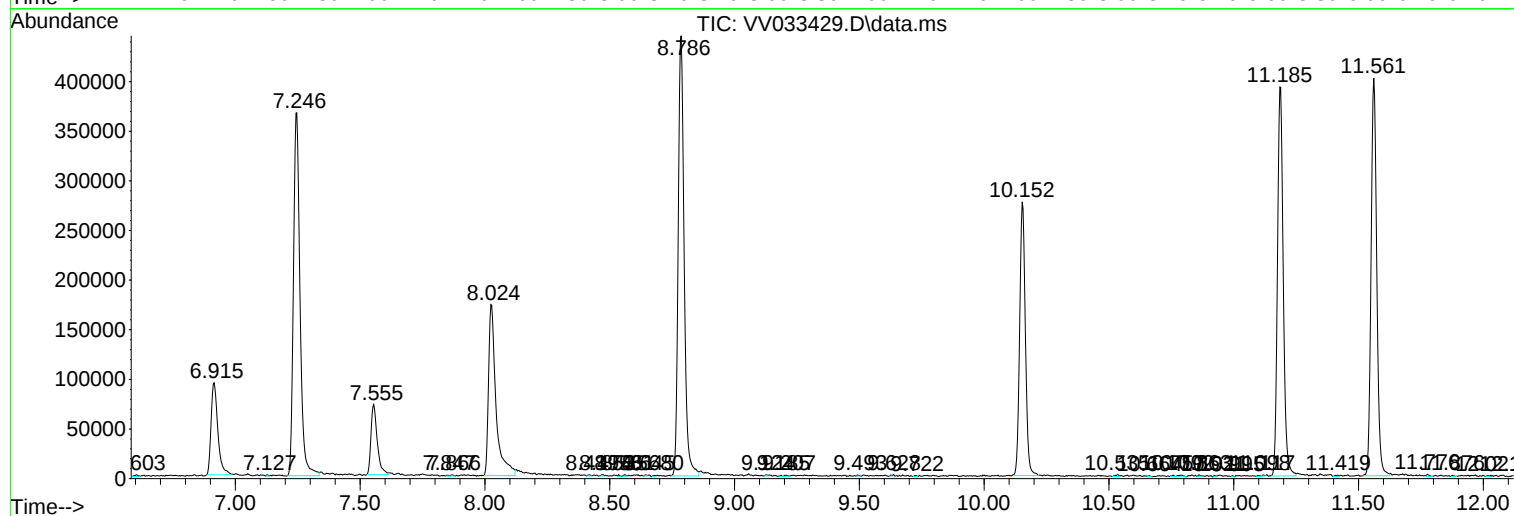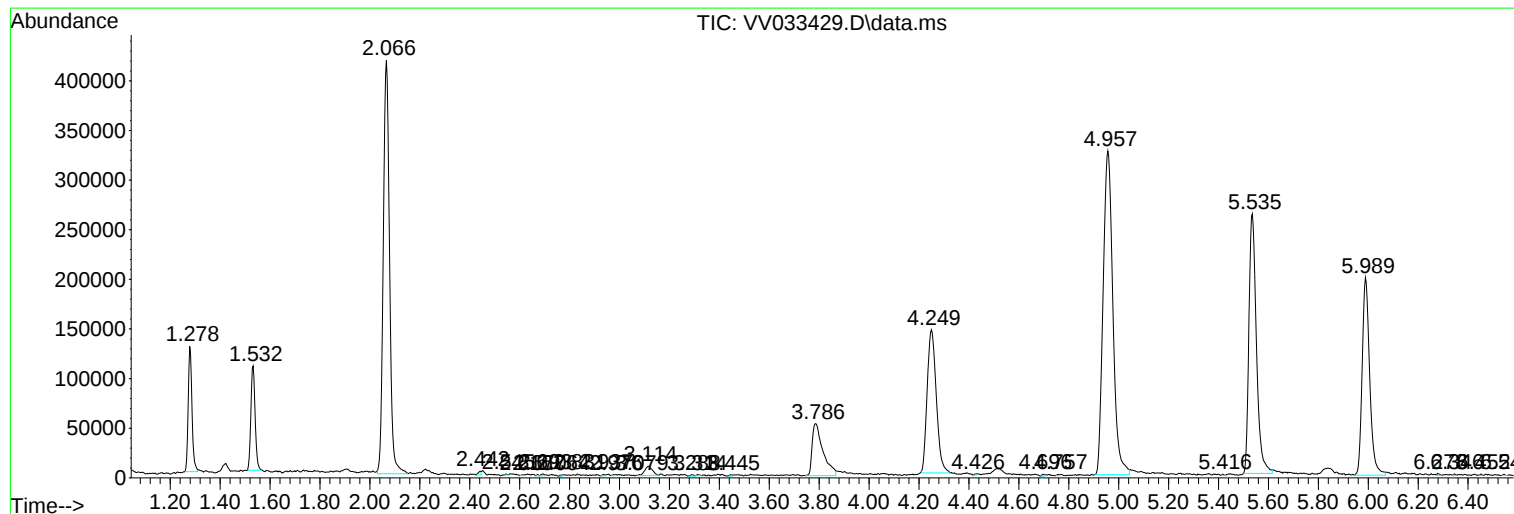

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033429.D
Acq On : 16 Dec 2023 12:57
Operator : SY/MD
Sample : 05846-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033429.D
Acq On : 16 Dec 2023 12:57
Operator : SY/MD
Sample : 05846-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------