

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033433.D
 Acq On : 16 Dec 2023 14:30
 Operator : SY/MD
 Sample : 05802-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	110881	115072	11.64%	1.582%
2	1.532	146	153	167	rVB	105086	125273	12.68%	1.723%
3	2.060	308	317	338	rVB	212731	309022	31.27%	4.249%
4	2.314	393	396	398	rBV4	1663	1185	0.12%	0.016%
5	2.481	445	448	452	rBV5	1598	1036	0.10%	0.014%
6	2.568	472	475	477	rBV3	1435	794	0.08%	0.011%
7	2.667	503	506	512	rBV5	1219	1191	0.12%	0.016%
8	3.066	624	630	634	rVB9	1619	1225	0.12%	0.017%
9	3.352	714	719	723	rBV5	1435	1383	0.14%	0.019%
10	3.735	832	838	840	rBV5	1258	1155	0.12%	0.016%
11	3.786	845	854	877	rBV	47710	133134	13.47%	1.831%
12	3.989	915	917	919	rBV2	1619	790	0.08%	0.011%
13	4.108	951	954	956	rBV3	1112	772	0.08%	0.011%
14	4.182	972	977	979	rBV4	1174	944	0.10%	0.013%
15	4.249	985	998	1030	rVB	142545	361783	36.61%	4.975%
16	4.497	1073	1075	1078	rVV5	1254	617	0.06%	0.008%
17	4.603	1104	1108	1110	rBV5	893	671	0.07%	0.009%
18	4.687	1130	1134	1135	rBV3	1186	805	0.08%	0.011%
19	4.957	1202	1218	1248	rBV2	318700	857874	86.80%	11.797%
20	5.240	1302	1306	1307	rBV4	1397	1065	0.11%	0.015%
21	5.272	1314	1316	1321	rVB5	1711	939	0.10%	0.013%
22	5.535	1387	1398	1425	rVV	215888	450273	45.56%	6.192%
23	5.725	1454	1457	1459	rVB3	1555	709	0.07%	0.010%
24	5.831	1477	1490	1511	rBV	497534	988341	100.00%	13.591%
25	5.989	1529	1539	1559	rVB	193677	386446	39.10%	5.314%
26	6.339	1644	1648	1650	rBV4	1769	1253	0.13%	0.017%
27	6.516	1700	1703	1705	rBV4	1325	956	0.10%	0.013%
28	6.677	1751	1753	1758	rVB6	1210	979	0.10%	0.013%
29	6.731	1768	1770	1772	rBV3	1341	763	0.08%	0.010%
30	6.850	1806	1807	1809	rBV2	1395	665	0.07%	0.009%
31	6.873	1812	1814	1816	rVV3	1883	885	0.09%	0.012%
32	6.915	1817	1827	1848	rVV	92964	177296	17.94%	2.438%
33	7.117	1887	1890	1891	rBV3	1415	963	0.10%	0.013%
34	7.246	1918	1930	1953	rVV	352791	638621	64.62%	8.782%
35	7.555	2017	2026	2046	rBV	69349	125583	12.71%	1.727%
36	7.828	2108	2111	2117	rBV6	1420	1573	0.16%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033433.D
 Acq On : 16 Dec 2023 14:30
 Operator : SY/MD
 Sample : 05802-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.857	2117	2120	2122	rBV5	1530	1122	0.11%	0.015%
38	7.908	2133	2136	2138	rBV4	1485	952	0.10%	0.013%
39	8.024	2162	2172	2202	rBV	164284	341176	34.52%	4.692%
40	8.307	2258	2260	2265	rBV6	1438	1204	0.12%	0.017%
41	8.423	2293	2296	2301	rBV5	1500	1075	0.11%	0.015%
42	8.445	2301	2303	2305	rBV3	1068	617	0.06%	0.008%
43	8.506	2319	2322	2325	rVB4	1321	866	0.09%	0.012%
44	8.786	2399	2409	2433	rBV	365272	600057	60.71%	8.252%
45	9.091	2500	2504	2506	rBV4	1745	1038	0.11%	0.014%
46	9.162	2524	2526	2532	rVB6	1196	803	0.08%	0.011%
47	9.204	2537	2539	2543	rBV6	979	642	0.06%	0.009%
48	9.349	2582	2584	2587	rBV3	963	665	0.07%	0.009%
49	9.423	2603	2607	2610	rBV5	1524	1327	0.13%	0.018%
50	9.583	2655	2657	2661	rVB4	1612	993	0.10%	0.014%
51	9.603	2661	2663	2667	rBV5	1353	1102	0.11%	0.015%
52	9.908	2755	2758	2761	rVB3	1007	615	0.06%	0.008%
53	9.927	2761	2764	2766	rBV3	1468	1014	0.10%	0.014%
54	10.153	2821	2834	2851	rBV	275456	438367	44.35%	6.028%
55	10.461	2927	2930	2933	rBV5	1120	726	0.07%	0.010%
56	10.480	2933	2936	2940	rBV6	1468	1165	0.12%	0.016%
57	10.500	2940	2942	2944	rBV3	1152	614	0.06%	0.008%
58	10.587	2967	2969	2972	rVB4	1264	607	0.06%	0.008%
59	10.622	2978	2980	2985	rVV6	1337	869	0.09%	0.012%
60	10.683	2997	2999	3006	rVB7	892	974	0.10%	0.013%
61	10.715	3006	3009	3010	rBV2	1057	598	0.06%	0.008%
62	10.863	3051	3055	3059	rBV6	1751	1672	0.17%	0.023%
63	11.062	3113	3117	3118	rBV3	1225	865	0.09%	0.012%
64	11.188	3145	3156	3175	rBV	330579	519522	52.57%	7.144%
65	11.419	3226	3228	3231	rBV4	1569	822	0.08%	0.011%
66	11.493	3246	3251	3252	rBV5	1721	1160	0.12%	0.016%
67	11.561	3258	3272	3294	rBV	394081	627670	63.51%	8.631%
68	11.837	3355	3358	3361	rVB5	1093	628	0.06%	0.009%
69	11.869	3361	3368	3369	rVB5	848	695	0.07%	0.010%
70	11.898	3374	3377	3380	rBV4	1556	1306	0.13%	0.018%
71	11.940	3386	3390	3393	rVB6	1434	993	0.10%	0.014%
72	11.963	3393	3397	3398	rBV4	1122	791	0.08%	0.011%
73	12.262	3487	3490	3494	rBV6	1311	824	0.08%	0.011%
74	12.484	3556	3559	3562	rBV5	1029	808	0.08%	0.011%
75	12.622	3598	3602	3604	rVV4	987	643	0.07%	0.009%
76	12.641	3604	3608	3610	rVB5	885	614	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033433.D
 Acq On : 16 Dec 2023 14:30
 Operator : SY/MD
 Sample : 05802-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.744	3636	3640	3643	rBV5	1141	1038	0.11%	0.014%
78	12.770	3646	3648	3653	rVV5	1370	1060	0.11%	0.015%
79	13.078	3739	3744	3747	rVB4	1321	1213	0.12%	0.017%
80	13.095	3747	3749	3751	rBV3	1034	691	0.07%	0.010%
81	13.207	3781	3784	3789	rBV4	1000	763	0.08%	0.010%
82	13.259	3796	3800	3803	rBV5	1878	1345	0.14%	0.018%
83	13.365	3829	3833	3838	rBV6	1648	1779	0.18%	0.024%
84	13.426	3849	3852	3855	rVB4	1212	698	0.07%	0.010%
85	13.487	3868	3871	3875	rVB4	1602	1050	0.11%	0.014%
86	13.506	3875	3877	3880	rBV4	1083	680	0.07%	0.009%
87	13.873	3988	3991	3994	rVB4	980	693	0.07%	0.010%
88	13.895	3994	3998	4001	rBV5	867	736	0.07%	0.010%
89	14.271	4113	4115	4119	rVB5	1651	813	0.08%	0.011%
90	14.664	4234	4237	4241	rBV6	1281	1029	0.10%	0.014%
91	14.725	4252	4256	4260	rVV6	1340	971	0.10%	0.013%
92	14.821	4282	4286	4291	rBV7	1040	894	0.09%	0.012%
93	14.866	4295	4300	4301	rBV5	1058	874	0.09%	0.012%
94	14.905	4308	4312	4313	rBV3	1129	805	0.08%	0.011%
95	15.020	4346	4348	4352	rVB5	1839	928	0.09%	0.013%
96	15.053	4354	4358	4362	rBV6	1067	843	0.09%	0.012%
97	15.078	4362	4366	4367	rBV4	1195	759	0.08%	0.010%
98	15.172	4393	4395	4398	rBV4	1169	737	0.07%	0.010%
99	15.464	4484	4486	4487	rBV2	1275	662	0.07%	0.009%
100	15.734	4568	4570	4572	rBV2	1676	722	0.07%	0.010%

Sum of corrected areas: 7272020




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033433.D
Acq On : 16 Dec 2023 14:30
Operator : SY/MD
Sample : 05802-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

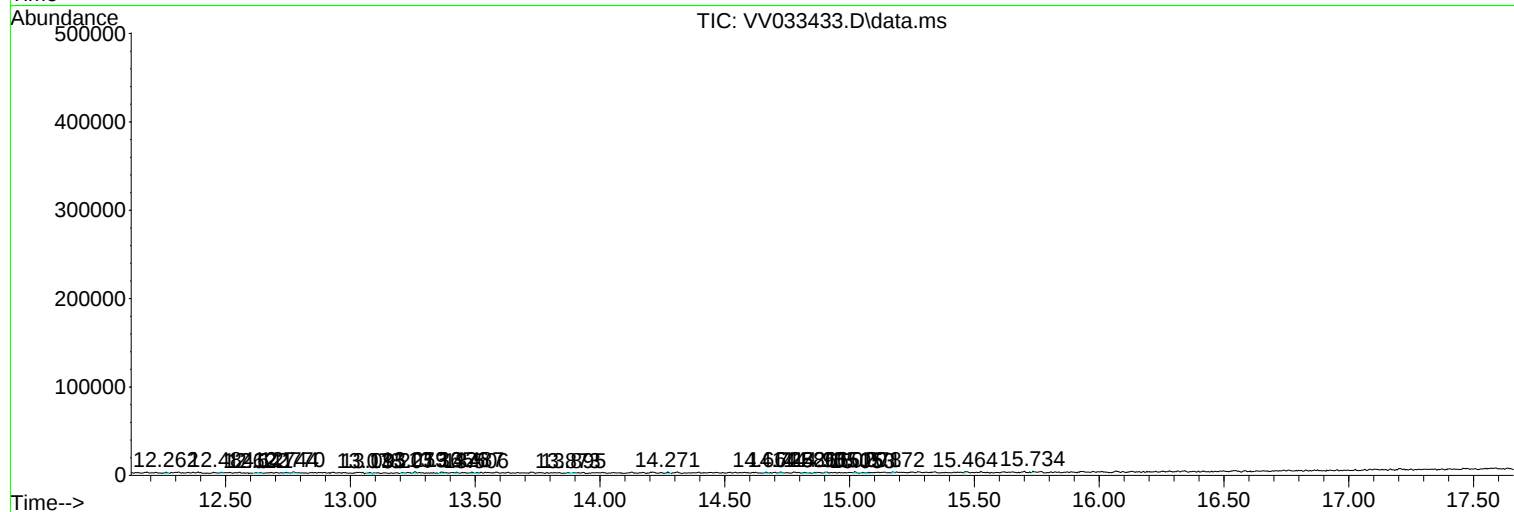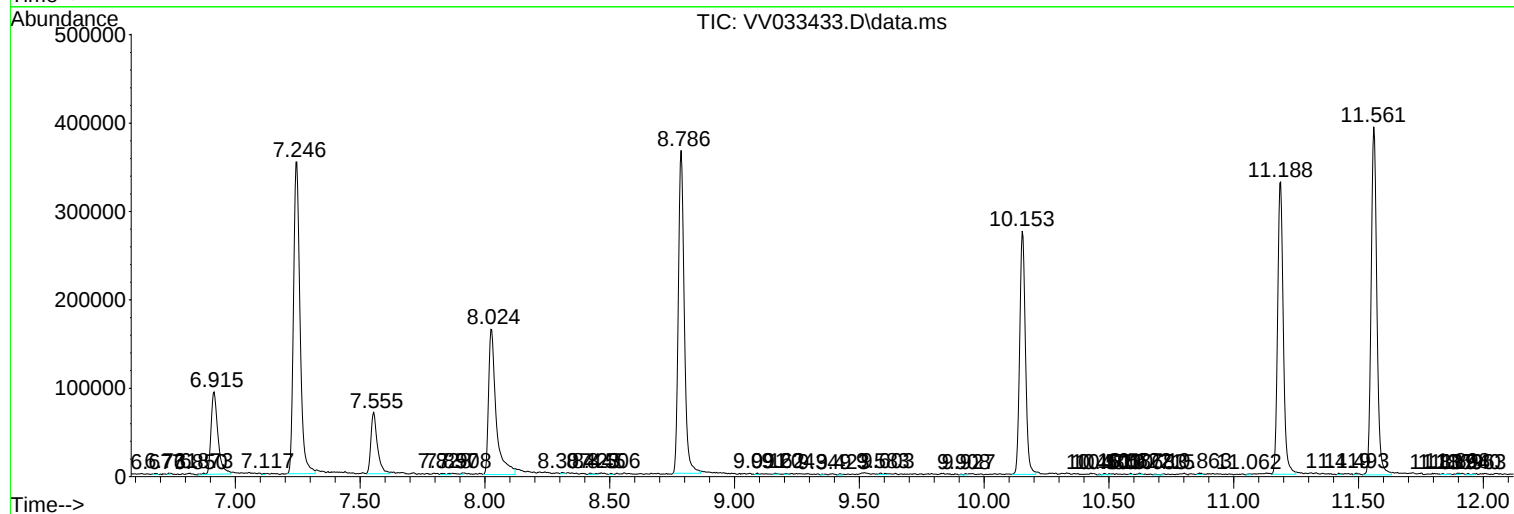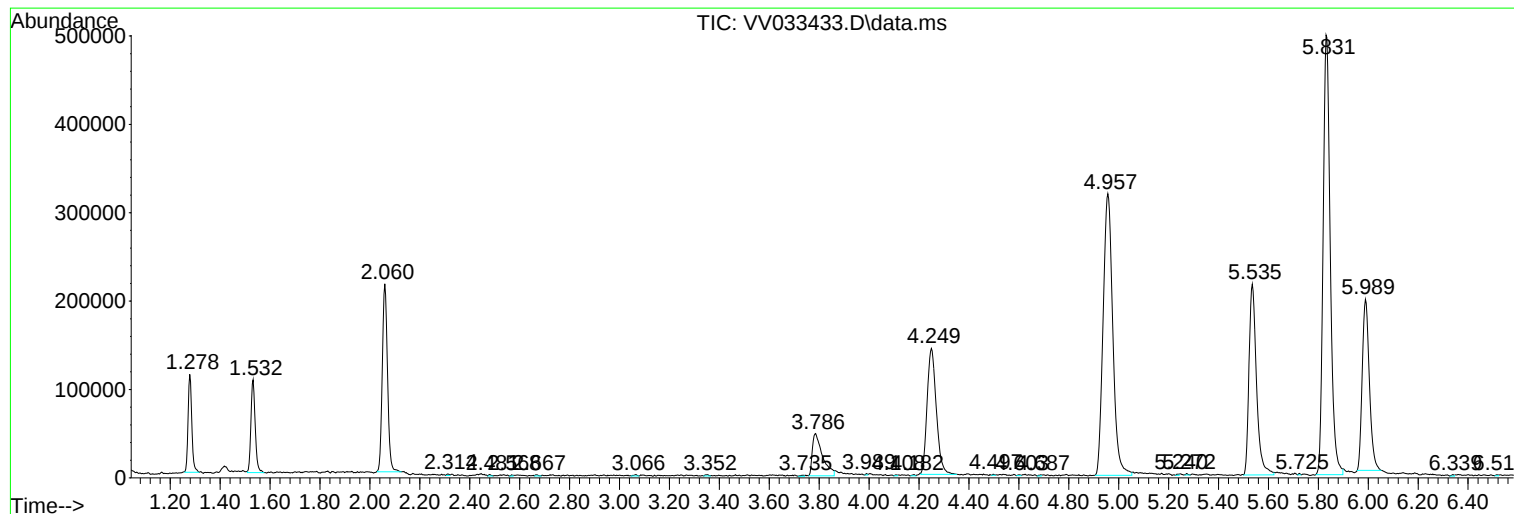

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033433.D
Acq On : 16 Dec 2023 14:30
Operator : SY/MD
Sample : 05802-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033433.D
Acq On : 16 Dec 2023 14:30
Operator : SY/MD
Sample : 05802-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc