

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033435.D
 Acq On : 16 Dec 2023 15:16
 Operator : SY/MD
 Sample : 05802-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VW033435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	112295	114526	13.72%	1.790%
2	1.532	146	153	165	rVB	101757	120460	14.43%	1.883%
3	2.060	309	317	335	rVB	204608	298030	35.71%	4.658%
4	2.532	460	464	465	rBV2	1246	721	0.09%	0.011%
5	2.700	513	516	520	rBV5	1178	948	0.11%	0.015%
6	2.847	560	562	564	rBV3	933	538	0.06%	0.008%
7	2.921	583	585	587	rBV3	1153	571	0.07%	0.009%
8	2.973	596	601	604	rBV6	1799	1257	0.15%	0.020%
9	3.047	620	624	626	rBV5	915	722	0.09%	0.011%
10	3.262	686	691	698	rBV9	1435	2165	0.26%	0.034%
11	3.310	704	706	707	rBV2	1225	597	0.07%	0.009%
12	3.381	723	728	729	rBV4	747	745	0.09%	0.012%
13	3.394	729	732	735	rVB4	1269	852	0.10%	0.013%
14	3.445	745	748	752	rBV5	1325	1099	0.13%	0.017%
15	3.510	765	768	770	rBV3	1452	870	0.10%	0.014%
16	3.564	782	785	789	rBV5	1089	844	0.10%	0.013%
17	3.584	789	791	794	rVB3	1180	639	0.08%	0.010%
18	3.642	805	809	812	rBV4	926	846	0.10%	0.013%
19	3.674	814	819	821	rBV6	1400	867	0.10%	0.014%
20	3.783	844	853	873	rBV	59155	156451	18.74%	2.445%
21	4.249	981	998	1018	rBV2	142074	366557	43.92%	5.729%
22	4.561	1093	1095	1096	rBV2	1691	680	0.08%	0.011%
23	4.834	1176	1180	1185	rBV6	1472	1348	0.16%	0.021%
24	4.957	1202	1218	1242	rBV2	312251	834663	100.00%	13.044%
25	5.416	1358	1361	1364	rBV4	1440	1345	0.16%	0.021%
26	5.535	1387	1398	1420	rBV	229479	469980	56.31%	7.345%
27	5.989	1525	1539	1563	rBV	189062	398674	47.76%	6.231%
28	6.352	1649	1652	1656	rBV5	1465	1331	0.16%	0.021%
29	6.638	1734	1741	1743	rBV8	1285	1317	0.16%	0.021%
30	6.703	1758	1761	1768	rBV9	1257	1067	0.13%	0.017%
31	6.818	1795	1797	1800	rBV3	1414	873	0.10%	0.014%
32	6.915	1817	1827	1848	rBV	86977	164115	19.66%	2.565%
33	7.079	1876	1878	1882	rBV4	1161	698	0.08%	0.011%
34	7.175	1904	1908	1910	rBV4	791	705	0.08%	0.011%
35	7.246	1918	1930	1951	rBV	343395	621248	74.43%	9.709%
36	7.555	2017	2026	2047	rBV	65246	118285	14.17%	1.849%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033435.D
 Acq On : 16 Dec 2023 15:16
 Operator : SY/MD
 Sample : 05802-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.841	2111	2115	2116	rBV4	1067	872	0.10%	0.014%
38	7.950	2146	2149	2156	rVB8	2015	2134	0.26%	0.033%
39	7.989	2156	2161	2163	rBV5	1354	1164	0.14%	0.018%
40	8.024	2163	2172	2209	rBV	218153	436746	52.33%	6.826%
41	8.445	2299	2303	2305	rBV6	1571	1188	0.14%	0.019%
42	8.609	2351	2354	2357	rBV4	1033	776	0.09%	0.012%
43	8.744	2392	2396	2398	rBV5	1728	1416	0.17%	0.022%
44	8.786	2399	2409	2427	rVV	385704	628589	75.31%	9.824%
45	9.162	2523	2526	2531	rBV7	1349	1352	0.16%	0.021%
46	9.329	2574	2578	2580	rBV4	1178	939	0.11%	0.015%
47	9.432	2608	2610	2615	rVB5	778	574	0.07%	0.009%
48	9.465	2615	2620	2623	rBV6	1268	1333	0.16%	0.021%
49	9.532	2638	2641	2642	rBV3	1132	698	0.08%	0.011%
50	9.619	2665	2668	2670	rBV4	1122	816	0.10%	0.013%
51	9.731	2700	2703	2705	rBV4	964	598	0.07%	0.009%
52	9.789	2719	2721	2726	rVB5	1444	1151	0.14%	0.018%
53	9.812	2726	2728	2732	rBV3	1318	850	0.10%	0.013%
54	9.873	2743	2747	2748	rBV4	1160	758	0.09%	0.012%
55	9.924	2760	2763	2765	rBV5	1315	925	0.11%	0.014%
56	9.947	2768	2770	2773	rBV4	1083	760	0.09%	0.012%
57	10.153	2823	2834	2855	rVB	282317	451278	54.07%	7.053%
58	10.227	2855	2857	2861	rBV4	1606	832	0.10%	0.013%
59	10.683	2996	2999	3003	rBV4	1056	706	0.08%	0.011%
60	10.764	3022	3024	3026	rBV3	1077	605	0.07%	0.009%
61	11.140	3139	3141	3144	rVB4	1604	676	0.08%	0.011%
62	11.185	3144	3155	3176	rBV	341181	547252	65.57%	8.553%
63	11.355	3206	3208	3210	rBV3	1226	709	0.08%	0.011%
64	11.416	3224	3227	3229	rBV3	1021	761	0.09%	0.012%
65	11.519	3256	3259	3260	rBV3	1505	748	0.09%	0.012%
66	11.561	3261	3272	3288	rVV	372678	592157	70.95%	9.254%
67	11.763	3333	3335	3338	rBV4	1153	615	0.07%	0.010%
68	12.487	3555	3560	3565	rBV8	1854	2196	0.26%	0.034%
69	12.529	3571	3573	3575	rBV3	1132	719	0.09%	0.011%
70	12.606	3595	3597	3600	rBV4	1674	852	0.10%	0.013%
71	12.751	3639	3642	3644	rBV4	877	584	0.07%	0.009%
72	12.796	3654	3656	3663	rVB8	1336	1194	0.14%	0.019%
73	12.837	3666	3669	3670	rBV3	923	581	0.07%	0.009%
74	13.333	3820	3823	3825	rBV3	1107	821	0.10%	0.013%
75	13.397	3842	3843	3848	rBV4	1107	725	0.09%	0.011%
76	13.451	3857	3860	3863	rBV3	1375	915	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033435.D
 Acq On : 16 Dec 2023 15:16
 Operator : SY/MD
 Sample : 05802-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.493	3870	3873	3877	rBV6	1444	1331	0.16%	0.021%
78	13.538	3884	3887	3890	rBV4	1508	745	0.09%	0.012%
79	13.564	3890	3895	3899	rBV4	1267	1396	0.17%	0.022%
80	13.625	3912	3914	3918	rVB4	1342	759	0.09%	0.012%
81	13.648	3918	3921	3922	rBV2	869	587	0.07%	0.009%
82	13.696	3928	3936	3940	rBV10	1443	1998	0.24%	0.031%
83	13.741	3945	3950	3952	rVV6	1222	936	0.11%	0.015%
84	13.783	3960	3963	3968	rVB7	1007	669	0.08%	0.010%
85	13.902	3996	4000	4002	rBV4	1122	740	0.09%	0.012%
86	13.947	4011	4014	4017	rVB4	1344	958	0.11%	0.015%
87	13.969	4019	4021	4024	rBV3	929	573	0.07%	0.009%
88	14.085	4054	4057	4061	rBV5	1165	1114	0.13%	0.017%
89	14.146	4074	4076	4081	rBV6	1445	1368	0.16%	0.021%
90	14.181	4084	4087	4089	rBV2	1069	817	0.10%	0.013%
91	14.223	4095	4100	4101	rBV4	1504	1110	0.13%	0.017%
92	14.249	4106	4108	4112	rVV4	1718	1169	0.14%	0.018%
93	14.287	4116	4120	4123	rBV5	1429	1547	0.19%	0.024%
94	14.387	4149	4151	4153	rBV3	1354	634	0.08%	0.010%
95	14.503	4185	4187	4190	rBV3	1034	606	0.07%	0.009%
96	14.763	4265	4268	4272	rBV4	1367	930	0.11%	0.015%
97	14.808	4280	4282	4285	rBV4	1136	806	0.10%	0.013%
98	14.992	4336	4339	4340	rBV3	927	633	0.08%	0.010%
99	15.381	4457	4460	4461	rBV3	1169	668	0.08%	0.010%
100	15.947	4632	4636	4639	rBV5	1395	1339	0.16%	0.021%




Sum of corrected areas: 6398632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033435.D
Acq On : 16 Dec 2023 15:16
Operator : SY/MD
Sample : 05802-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

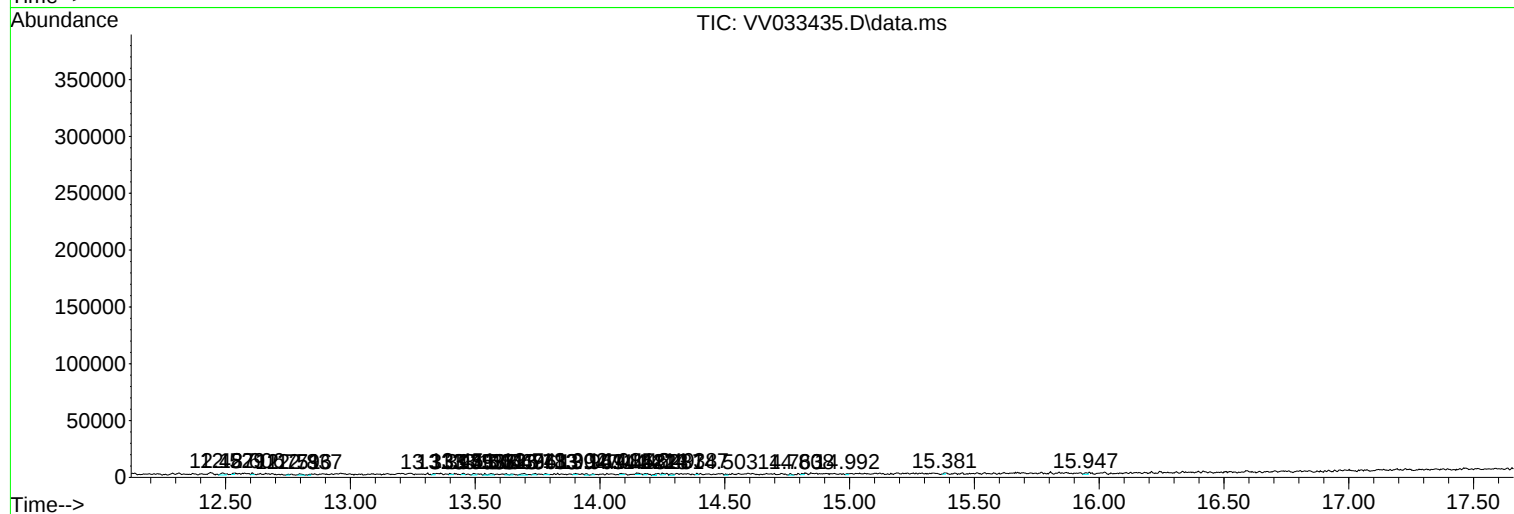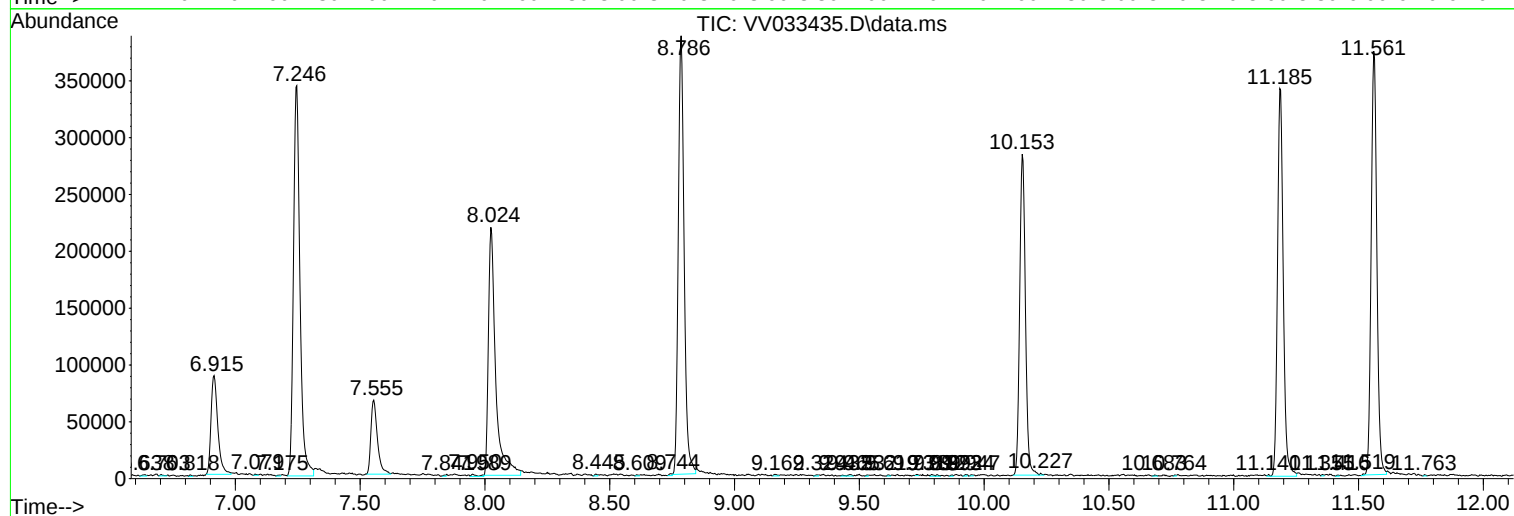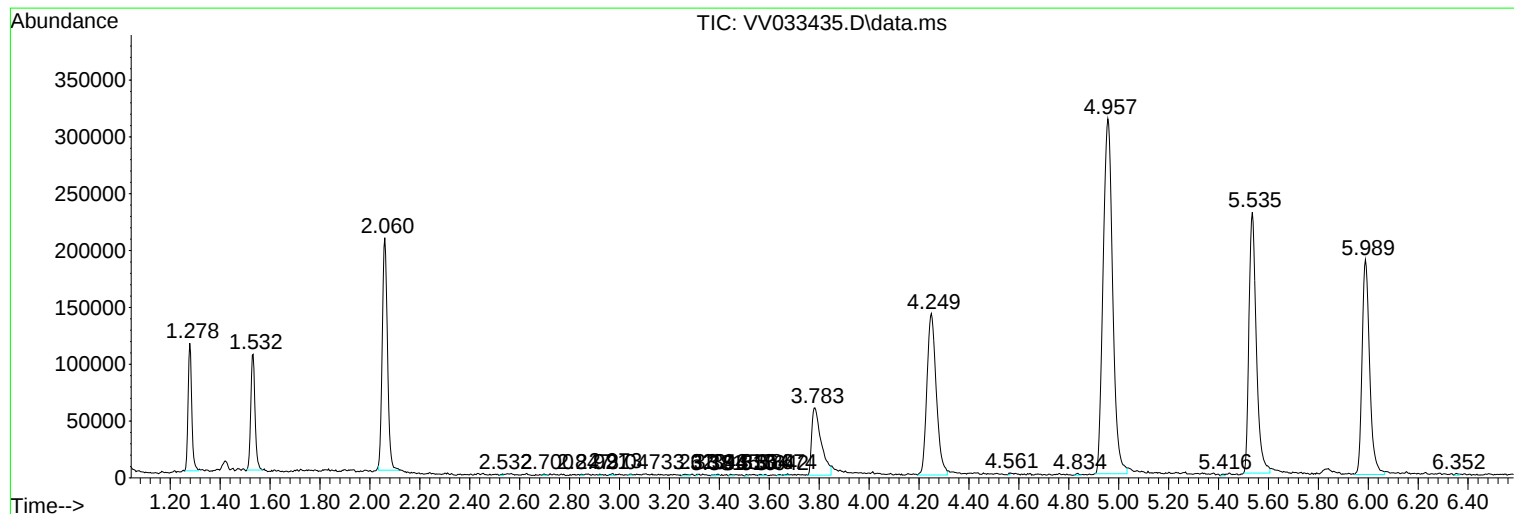

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033435.D
Acq On : 16 Dec 2023 15:16
Operator : SY/MD
Sample : 05802-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033435.D
Acq On : 16 Dec 2023 15:16
Operator : SY/MD
Sample : 05802-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc