

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033436.D
 Acq On : 16 Dec 2023 15:40
 Operator : SY/MD
 Sample : 05802-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	111755	114639	13.72%	1.777%
2	1.532	146	153	163	rVB	102330	118524	14.18%	1.837%
3	2.060	308	317	333	rBV	206496	303804	36.35%	4.709%
4	2.507	454	456	458	rVB3	1563	505	0.06%	0.008%
5	2.613	487	489	492	rBV4	949	544	0.07%	0.008%
6	2.683	509	511	514	rBV3	1048	635	0.08%	0.010%
7	2.793	543	545	547	rBV3	1210	529	0.06%	0.008%
8	2.828	554	556	561	rVB5	893	647	0.08%	0.010%
9	2.864	565	567	571	rBV4	1383	996	0.12%	0.015%
10	3.288	695	699	703	rBV7	1772	1770	0.21%	0.027%
11	3.372	723	725	729	rVV6	836	528	0.06%	0.008%
12	3.433	741	744	745	rBV3	1084	596	0.07%	0.009%
13	3.619	798	802	805	rBV5	853	544	0.07%	0.008%
14	3.667	814	817	820	rVB5	1485	790	0.09%	0.012%
15	3.741	835	840	843	rBV4	1299	1140	0.14%	0.018%
16	3.786	845	854	879	rBV2	50629	140865	16.85%	2.183%
17	4.249	985	998	1026	rVB2	140622	353972	42.35%	5.486%
18	4.375	1035	1037	1039	rBV3	1500	721	0.09%	0.011%
19	4.503	1076	1077	1080	rBV3	865	589	0.07%	0.009%
20	4.590	1101	1104	1105	rBV2	981	621	0.07%	0.010%
21	4.622	1112	1114	1116	rBV2	1158	524	0.06%	0.008%
22	4.764	1154	1158	1161	rBV6	1305	1159	0.14%	0.018%
23	4.889	1195	1197	1200	rBV3	643	547	0.07%	0.008%
24	4.957	1202	1218	1240	rBV3	312834	835796	100.00%	12.954%
25	5.535	1386	1398	1420	rBV	249726	523175	62.60%	8.109%
26	5.989	1528	1539	1565	rBV	188513	390129	46.68%	6.047%
27	6.275	1624	1628	1629	rBV4	1556	921	0.11%	0.014%
28	6.336	1646	1647	1651	rBV5	1059	511	0.06%	0.008%
29	6.468	1686	1688	1690	rBV3	1181	505	0.06%	0.008%
30	6.494	1694	1696	1698	rBV3	997	529	0.06%	0.008%
31	6.516	1701	1703	1706	rBV3	894	539	0.06%	0.008%
32	6.558	1712	1716	1719	rBV5	1250	1039	0.12%	0.016%
33	6.619	1731	1735	1738	rBV5	1597	1402	0.17%	0.022%
34	6.680	1751	1754	1755	rBV3	1211	717	0.09%	0.011%
35	6.815	1791	1796	1800	rBV7	1379	1504	0.18%	0.023%
36	6.915	1817	1827	1848	rBV	89000	173688	20.78%	2.692%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033436.D
 Acq On : 16 Dec 2023 15:40
 Operator : SY/MD
 Sample : 05802-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.105	1884	1886	1891	rBV5	1099	815	0.10%	0.013%
38	7.130	1891	1894	1897	rBV4	1345	1074	0.13%	0.017%
39	7.198	1911	1915	1917	rBV5	1894	1554	0.19%	0.024%
40	7.246	1918	1930	1949	rVV	346915	618160	73.96%	9.581%
41	7.555	2016	2026	2042	rBV2	67747	122652	14.67%	1.901%
42	7.751	2084	2087	2088	rBV3	1747	709	0.08%	0.011%
43	7.812	2103	2106	2109	rBV4	1277	643	0.08%	0.010%
44	8.024	2160	2172	2205	rBV	172133	359636	43.03%	5.574%
45	8.603	2349	2352	2354	rBV3	1643	1291	0.15%	0.020%
46	8.667	2369	2372	2374	rBV3	1045	578	0.07%	0.009%
47	8.706	2378	2384	2386	rBV6	1478	1610	0.19%	0.025%
48	8.786	2398	2409	2429	rBV	416045	684690	81.92%	10.612%
49	9.214	2540	2542	2544	rBV3	1386	706	0.08%	0.011%
50	9.252	2552	2554	2555	rBV2	1380	588	0.07%	0.009%
51	9.278	2559	2562	2566	rBV6	1471	1034	0.12%	0.016%
52	9.336	2577	2580	2582	rBV5	1197	694	0.08%	0.011%
53	9.458	2613	2618	2624	rVB9	1323	1604	0.19%	0.025%
54	9.487	2626	2627	2632	rVB5	1132	731	0.09%	0.011%
55	9.529	2637	2640	2643	rBV5	1431	902	0.11%	0.014%
56	9.783	2717	2719	2722	rVB4	1130	530	0.06%	0.008%
57	9.902	2754	2756	2760	rVB5	878	596	0.07%	0.009%
58	9.924	2760	2763	2767	rBV4	1947	1448	0.17%	0.022%
59	9.947	2767	2770	2774	rBV7	1119	1014	0.12%	0.016%
60	10.043	2795	2800	2801	rBV5	770	680	0.08%	0.011%
61	10.153	2823	2834	2853	rBV	276236	435466	52.10%	6.749%
62	10.397	2904	2910	2912	rBV7	1425	1256	0.15%	0.019%
63	10.680	2996	2998	3000	rVB2	1211	546	0.07%	0.008%
64	10.731	3008	3014	3018	rBV8	937	854	0.10%	0.013%
65	10.754	3018	3021	3024	rBV5	941	515	0.06%	0.008%
66	10.828	3040	3044	3046	rBV5	1091	828	0.10%	0.013%
67	10.860	3051	3054	3056	rBV4	1016	526	0.06%	0.008%
68	10.931	3074	3076	3079	rBV4	1145	625	0.07%	0.010%
69	10.979	3089	3091	3093	rBV3	945	499	0.06%	0.008%
70	11.188	3145	3156	3173	rBV	371137	590557	70.66%	9.153%
71	11.561	3261	3272	3290	rBV	385735	614885	73.57%	9.530%
72	11.953	3392	3394	3396	rBV2	967	535	0.06%	0.008%
73	12.069	3428	3430	3432	rVB4	1617	567	0.07%	0.009%
74	12.124	3445	3447	3449	rBV3	938	510	0.06%	0.008%
75	12.252	3484	3487	3489	rBV4	1316	775	0.09%	0.012%
76	12.397	3529	3532	3533	rBV2	937	577	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033436.D
 Acq On : 16 Dec 2023 15:40
 Operator : SY/MD
 Sample : 05802-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.722	3631	3633	3639	rVB5	1051	795	0.10%	0.012%
78	12.792	3652	3655	3657	rVB3	1197	644	0.08%	0.010%
79	12.831	3663	3667	3671	rVV7	1465	1213	0.15%	0.019%
80	12.902	3687	3689	3693	rVB4	1429	943	0.11%	0.015%
81	12.924	3693	3696	3698	rBV3	1260	737	0.09%	0.011%
82	13.005	3716	3721	3723	rBV5	1083	1088	0.13%	0.017%
83	13.130	3756	3760	3762	rBV4	1299	1123	0.13%	0.017%
84	13.291	3807	3810	3814	rBV6	1546	1492	0.18%	0.023%
85	13.378	3832	3837	3838	rBV3	1524	1261	0.15%	0.020%
86	13.426	3849	3852	3855	rBV3	1379	908	0.11%	0.014%
87	13.452	3858	3860	3862	rBV3	1376	833	0.10%	0.013%
88	13.638	3916	3918	3920	rBV3	1306	852	0.10%	0.013%
89	13.802	3965	3969	3971	rBV3	1499	1208	0.14%	0.019%
90	13.985	4024	4026	4028	rBV3	942	496	0.06%	0.008%
91	14.156	4074	4079	4080	rBV5	1255	1104	0.13%	0.017%
92	14.242	4103	4106	4108	rBV4	1138	772	0.09%	0.012%
93	14.288	4116	4120	4124	rBV7	1864	1793	0.21%	0.028%
94	14.606	4217	4219	4221	rBV3	1111	701	0.08%	0.011%
95	14.773	4269	4271	4274	rBV4	1234	605	0.07%	0.009%
96	14.847	4291	4294	4295	rBV2	1459	557	0.07%	0.009%
97	15.014	4344	4346	4352	rBV7	1377	1280	0.15%	0.020%
98	15.107	4374	4375	4379	rVB4	1580	711	0.09%	0.011%
99	15.689	4554	4556	4559	rVB4	1538	680	0.08%	0.011%
100	15.705	4559	4561	4564	rBV4	1309	976	0.12%	0.015%


Sum of corrected areas: 6451876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033436.D
Acq On : 16 Dec 2023 15:40
Operator : SY/MD
Sample : 05802-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 67 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

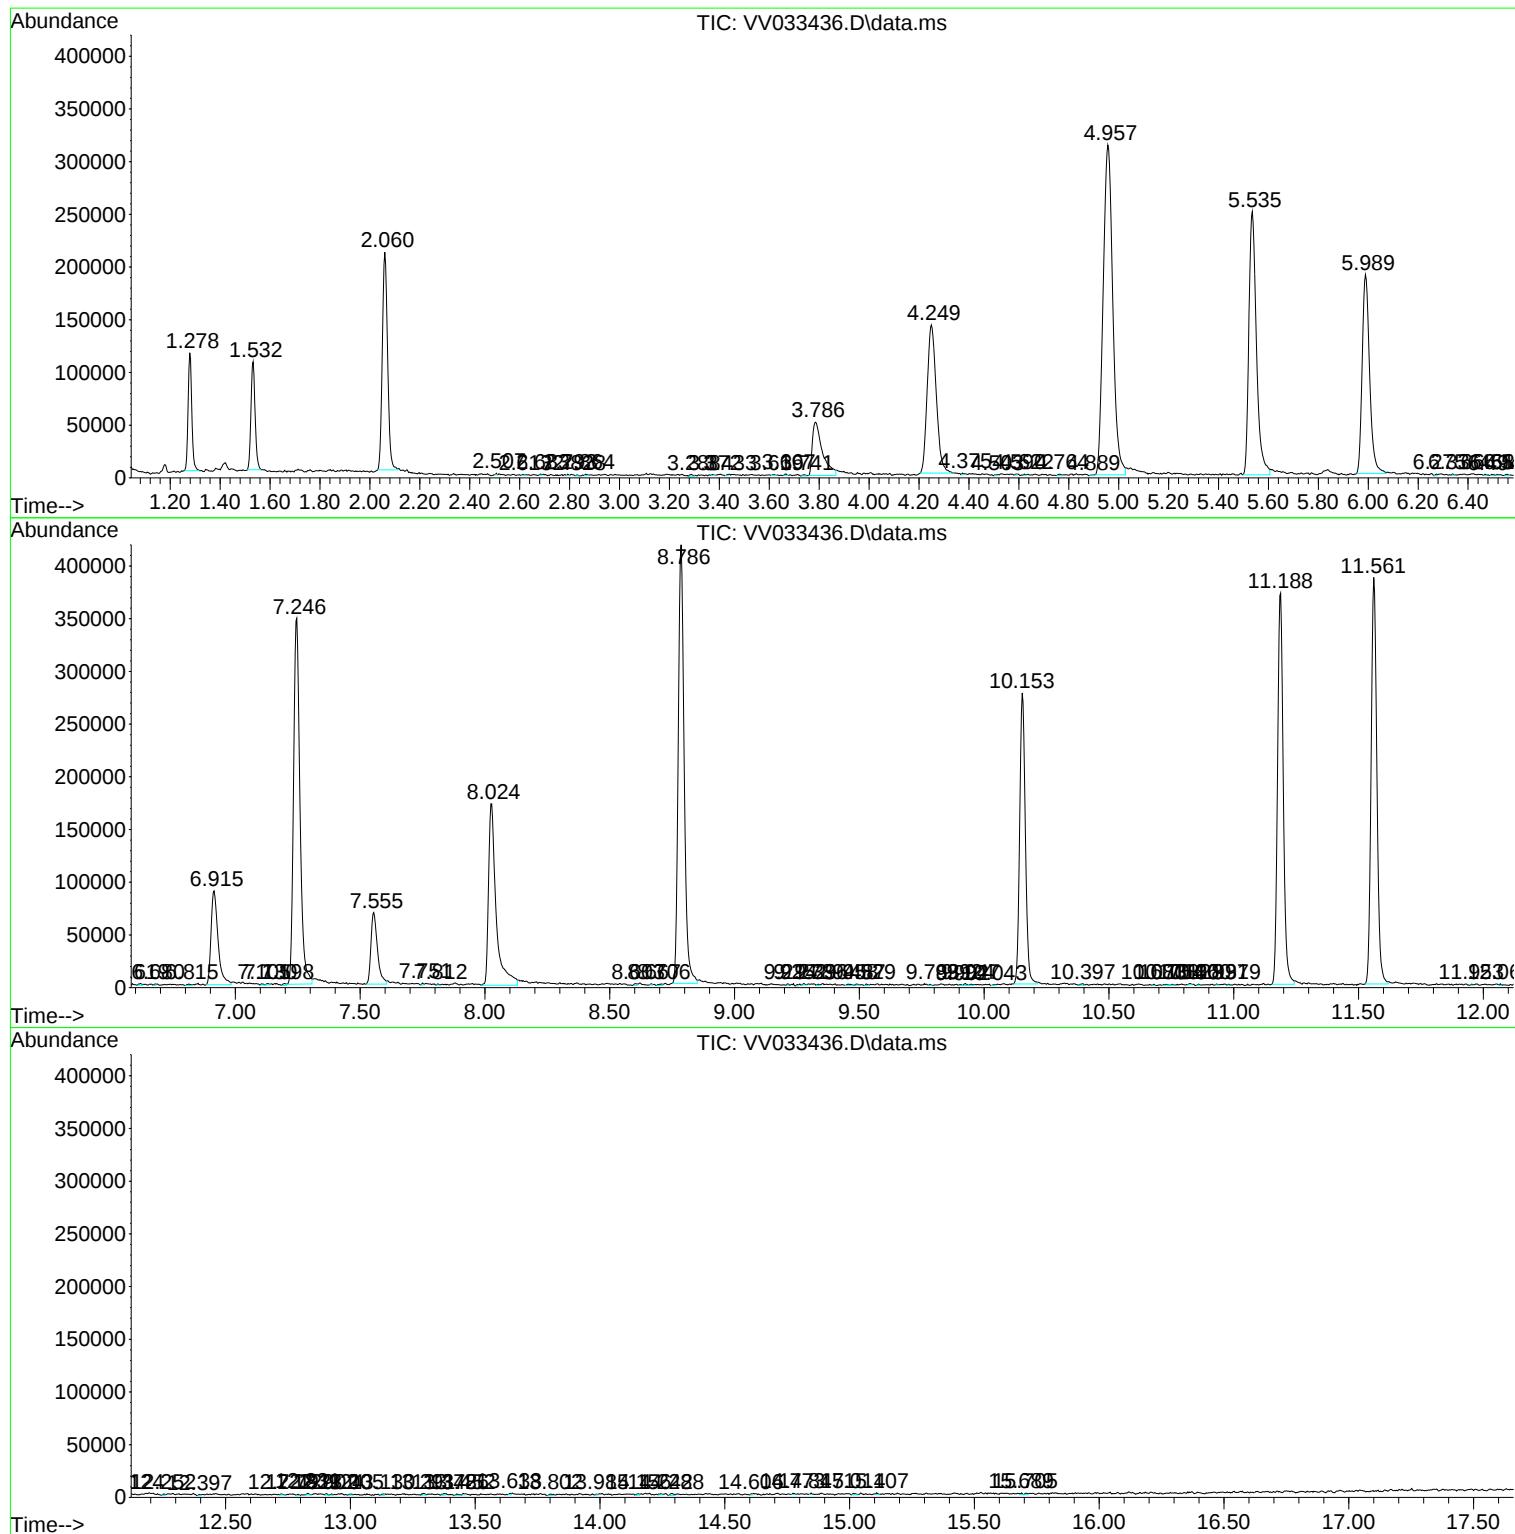

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033436.D
Acq On : 16 Dec 2023 15:40
Operator : SY/MD
Sample : 05802-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 67 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033436.D
Acq On : 16 Dec 2023 15:40
Operator : SY/MD
Sample : 05802-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 67 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------