

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033437.D
 Acq On : 16 Dec 2023 16:03
 Operator : SY/MD
 Sample : 05802-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	111873	114905	13.49%	1.864%
2	1.532	146	153	162	rBV	100907	118090	13.86%	1.916%
3	2.060	308	317	329	rBV	209338	300238	35.24%	4.870%
4	2.272	381	383	386	rBV3	1070	683	0.08%	0.011%
5	2.378	415	416	418	rBV2	1317	487	0.06%	0.008%
6	2.526	458	462	463	rBV3	1250	922	0.11%	0.015%
7	2.606	486	487	491	rBV4	897	501	0.06%	0.008%
8	2.680	507	510	512	rBV4	995	597	0.07%	0.010%
9	2.748	525	531	533	rBV6	1778	1716	0.20%	0.028%
10	2.876	568	571	574	rBV5	1081	665	0.08%	0.011%
11	2.915	581	583	585	rBV3	1041	590	0.07%	0.010%
12	2.928	585	587	590	rVV4	1586	772	0.09%	0.013%
13	3.137	650	652	653	rBV3	1132	520	0.06%	0.008%
14	3.185	664	667	669	rBV3	851	551	0.06%	0.009%
15	3.207	669	674	679	rBV7	1724	2224	0.26%	0.036%
16	3.291	697	700	702	rVB2	1194	514	0.06%	0.008%
17	3.320	704	709	710	rBV5	1461	1071	0.13%	0.017%
18	3.346	714	717	722	rBV5	1092	1184	0.14%	0.019%
19	3.397	730	733	737	rBV6	1769	1305	0.15%	0.021%
20	3.487	757	761	767	rVB8	1851	1673	0.20%	0.027%
21	3.526	767	773	775	rBV6	1232	987	0.12%	0.016%
22	3.613	797	800	805	rVB7	1310	1256	0.15%	0.020%
23	3.751	839	843	845	rBV4	930	807	0.09%	0.013%
24	3.786	845	854	881	rBV	46653	132258	15.52%	2.145%
25	4.159	968	970	971	rBV2	1205	569	0.07%	0.009%
26	4.249	985	998	1021	rVB2	142051	355435	41.71%	5.766%
27	4.519	1080	1082	1084	rBV3	1052	504	0.06%	0.008%
28	4.590	1100	1104	1106	rBV5	883	699	0.08%	0.011%
29	4.641	1117	1120	1122	rBV3	1359	869	0.10%	0.014%
30	4.767	1156	1159	1162	rBV4	727	629	0.07%	0.010%
31	4.883	1191	1195	1199	rBV7	1135	908	0.11%	0.015%
32	4.957	1202	1218	1245	rBV2	318187	852058	100.00%	13.822%
33	5.535	1387	1398	1424	rBV	215324	451467	52.99%	7.324%
34	5.989	1527	1539	1560	rBV	191135	394579	46.31%	6.401%
35	6.616	1732	1734	1738	rBV3	1190	863	0.10%	0.014%
36	6.693	1756	1758	1761	rBV3	745	585	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033437.D
 Acq On : 16 Dec 2023 16:03
 Operator : SY/MD
 Sample : 05802-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.748	1772	1775	1780	rBV5	1163	1076	0.13%	0.017%
38	6.915	1816	1827	1849	rBV	90197	173206	20.33%	2.810%
39	7.201	1914	1916	1918	rBV2	1523	751	0.09%	0.012%
40	7.246	1918	1930	1954	rVV	348240	628961	73.82%	10.203%
41	7.555	2016	2026	2041	rBV2	67988	123060	14.44%	1.996%
42	8.024	2163	2172	2190	rBV	162510	316845	37.19%	5.140%
43	8.574	2341	2343	2346	rBV3	1151	656	0.08%	0.011%
44	8.648	2364	2366	2373	rVB5	1895	1735	0.20%	0.028%
45	8.786	2398	2409	2434	rBV	360040	594061	69.72%	9.637%
46	9.220	2540	2544	2546	rBV5	820	594	0.07%	0.010%
47	9.243	2547	2551	2554	rBV5	1227	1086	0.13%	0.018%
48	9.455	2614	2617	2620	rBV4	1558	1179	0.14%	0.019%
49	9.522	2632	2638	2640	rBV7	1355	1326	0.16%	0.022%
50	9.882	2748	2750	2754	rVB5	1294	512	0.06%	0.008%
51	9.927	2760	2764	2766	rVB5	1269	838	0.10%	0.014%
52	9.960	2766	2774	2778	rVB10	1292	1307	0.15%	0.021%
53	9.985	2778	2782	2784	rBV4	949	576	0.07%	0.009%
54	10.040	2795	2799	2801	rBV4	1274	871	0.10%	0.014%
55	10.050	2801	2802	2805	rVV4	990	506	0.06%	0.008%
56	10.153	2823	2834	2851	rBV	267143	427905	50.22%	6.941%
57	10.307	2879	2882	2883	rBV3	1493	762	0.09%	0.012%
58	10.503	2941	2943	2947	rBV4	1309	1109	0.13%	0.018%
59	10.667	2990	2994	2995	rBV4	1214	889	0.10%	0.014%
60	10.677	2995	2997	3000	rVV4	1583	1005	0.12%	0.016%
61	10.796	3030	3034	3040	rVB8	992	1238	0.15%	0.020%
62	10.831	3040	3045	3048	rBV7	970	1148	0.13%	0.019%
63	10.966	3083	3087	3089	rBV5	1453	846	0.10%	0.014%
64	11.120	3132	3135	3138	rBV4	1336	1170	0.14%	0.019%
65	11.185	3145	3155	3176	rBV	317121	503878	59.14%	8.174%
66	11.371	3211	3213	3216	rBV3	1007	751	0.09%	0.012%
67	11.561	3261	3272	3293	rBV	383679	603330	70.81%	9.787%
68	12.005	3407	3410	3411	rBV3	1053	527	0.06%	0.009%
69	12.159	3454	3458	3459	rBV3	1087	841	0.10%	0.014%
70	12.191	3466	3468	3472	rBV5	824	511	0.06%	0.008%
71	12.519	3567	3570	3572	rVB4	1083	526	0.06%	0.009%
72	12.545	3572	3578	3582	rBV8	2001	2520	0.30%	0.041%
73	12.609	3596	3598	3600	rBV2	960	595	0.07%	0.010%
74	12.638	3605	3607	3609	rBV3	1012	536	0.06%	0.009%
75	12.686	3620	3622	3624	rBV2	1166	698	0.08%	0.011%
76	12.857	3673	3675	3678	rBV4	1108	905	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033437.D
 Acq On : 16 Dec 2023 16:03
 Operator : SY/MD
 Sample : 05802-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.959	3705	3707	3712	rBV5	619	604	0.07%	0.010%
78	13.043	3731	3733	3736	rBV4	988	502	0.06%	0.008%
79	13.191	3776	3779	3781	rBV4	883	605	0.07%	0.010%
80	13.278	3804	3806	3810	rVV4	1048	630	0.07%	0.010%
81	13.313	3815	3817	3821	rBV5	898	789	0.09%	0.013%
82	13.400	3840	3844	3849	rBV7	874	938	0.11%	0.015%
83	13.458	3859	3862	3866	rBV5	1107	817	0.10%	0.013%
84	13.583	3898	3901	3904	rBV3	857	583	0.07%	0.009%
85	13.686	3931	3933	3937	rBV5	941	626	0.07%	0.010%
86	13.831	3973	3978	3983	rVB8	1760	1569	0.18%	0.025%
87	13.850	3983	3984	3989	rBV4	707	568	0.07%	0.009%
88	13.914	4002	4004	4006	rVB3	1074	578	0.07%	0.009%
89	13.972	4019	4022	4029	rVB8	1719	2088	0.25%	0.034%
90	14.001	4029	4031	4033	rBV2	1316	728	0.09%	0.012%
91	14.223	4099	4100	4105	rBV4	921	611	0.07%	0.010%
92	14.255	4108	4110	4113	rVB4	1331	781	0.09%	0.013%
93	14.313	4126	4128	4132	rVB5	857	555	0.07%	0.009%
94	14.345	4136	4138	4143	rBV6	810	630	0.07%	0.010%
95	14.403	4154	4156	4159	rVB3	1744	742	0.09%	0.012%
96	14.519	4188	4192	4195	rBV5	1616	1494	0.18%	0.024%
97	14.557	4200	4204	4205	rBV4	1071	710	0.08%	0.012%
98	14.795	4275	4278	4280	rBV3	1197	867	0.10%	0.014%
99	15.037	4351	4353	4356	rVB3	1280	642	0.08%	0.010%
100	15.927	4628	4630	4634	rBV5	1752	1401	0.16%	0.023%




Sum of corrected areas: 6164575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033437.D
Acq On : 16 Dec 2023 16:03
Operator : SY/MD
Sample : 05802-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

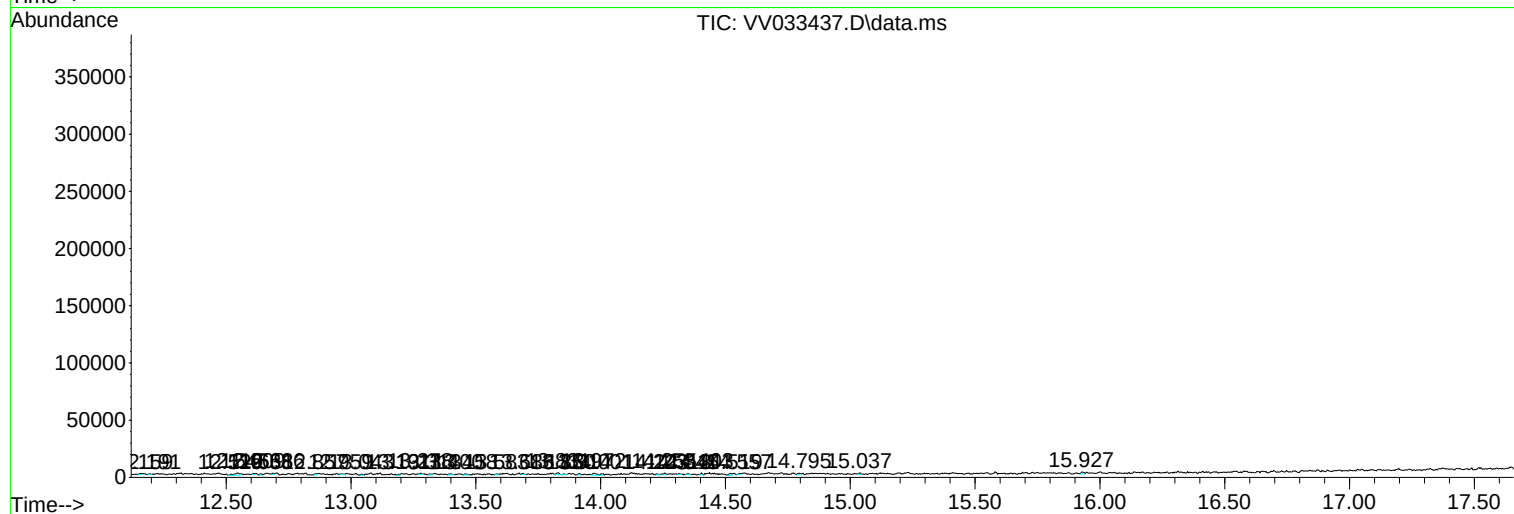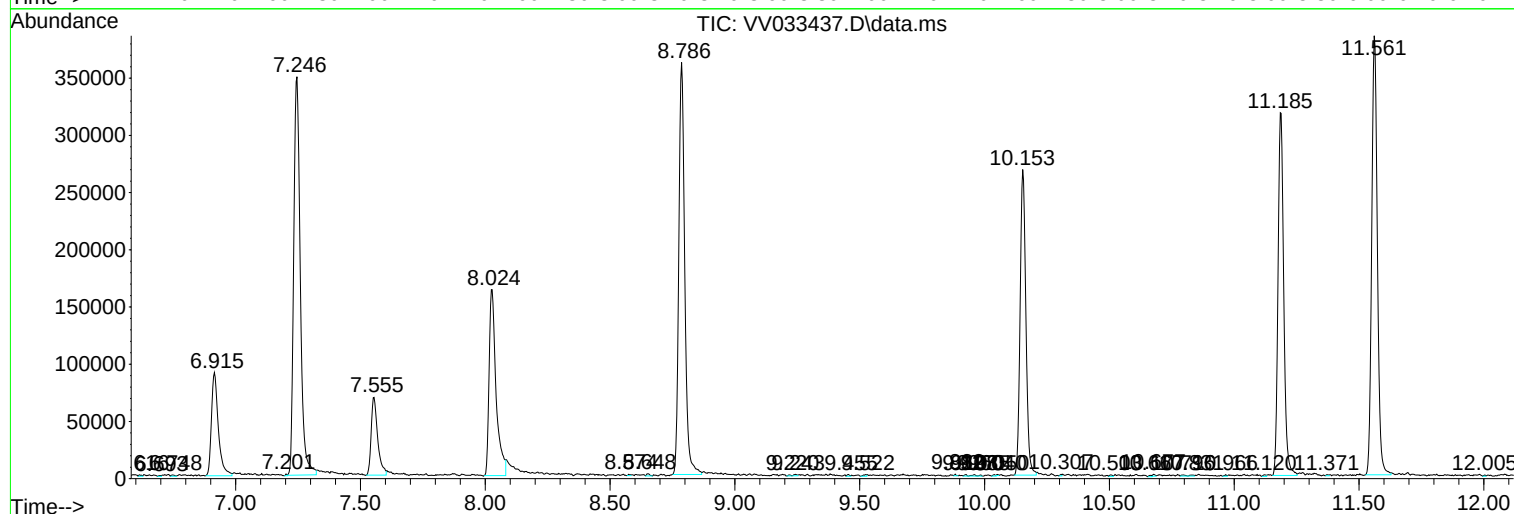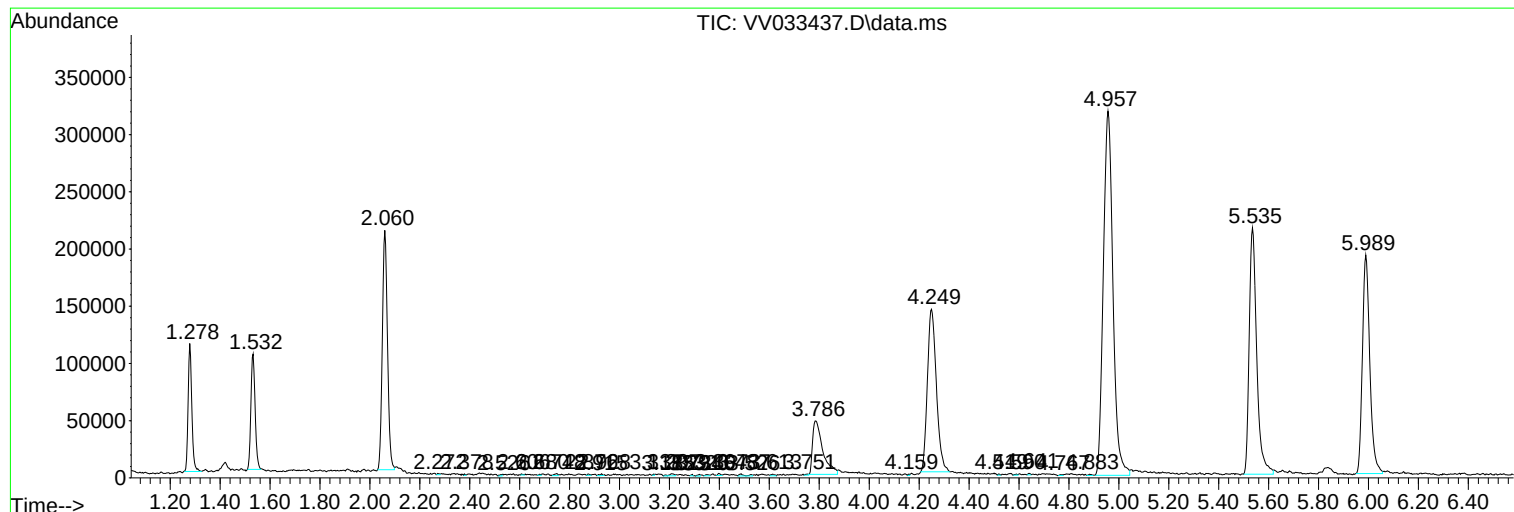

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033437.D
Acq On : 16 Dec 2023 16:03
Operator : SY/MD
Sample : 05802-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033437.D
Acq On : 16 Dec 2023 16:03
Operator : SY/MD
Sample : 05802-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc