

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033438.D
 Acq On : 16 Dec 2023 16:26
 Operator : SY/MD
 Sample : 05802-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	110670	117572	13.84%	1.772%
2	1.532	146	153	163	rVB	99397	116085	13.67%	1.750%
3	2.060	309	317	330	rVB	202290	287926	33.90%	4.339%
4	2.214	363	365	372	rBV6	1482	1493	0.18%	0.023%
5	2.381	415	417	423	rVB7	1507	1373	0.16%	0.021%
6	2.455	438	440	444	rVB5	1441	857	0.10%	0.013%
7	2.529	460	463	464	rBV3	1192	634	0.07%	0.010%
8	2.561	464	473	475	rBV6	4778	6451	0.76%	0.097%
9	2.744	527	530	532	rBV2	1379	820	0.10%	0.012%
10	2.944	589	592	595	rBV5	1174	975	0.11%	0.015%
11	3.027	614	618	619	rBV3	1080	747	0.09%	0.011%
12	3.101	639	641	646	rVB4	820	591	0.07%	0.009%
13	3.127	646	649	652	rBV5	1441	1049	0.12%	0.016%
14	3.272	690	694	696	rBV5	1363	915	0.11%	0.014%
15	3.413	736	738	740	rBV3	1525	774	0.09%	0.012%
16	3.497	761	764	766	rBV4	1222	815	0.10%	0.012%
17	3.574	785	788	791	rBV5	970	774	0.09%	0.012%
18	3.629	802	805	806	rBV3	1208	680	0.08%	0.010%
19	3.661	812	815	817	rBV3	1049	684	0.08%	0.010%
20	3.783	841	853	875	rBV	58213	154697	18.21%	2.331%
21	4.249	984	998	1019	rBV	140640	352853	41.54%	5.318%
22	4.735	1145	1149	1150	rBV3	1053	694	0.08%	0.010%
23	4.828	1176	1178	1181	rBV4	1364	818	0.10%	0.012%
24	4.883	1191	1195	1198	rBV5	1611	1449	0.17%	0.022%
25	4.957	1203	1218	1240	rBV2	316040	849411	100.00%	12.801%
26	5.397	1352	1355	1356	rBV3	1352	806	0.09%	0.012%
27	5.477	1378	1380	1383	rBV4	1244	804	0.09%	0.012%
28	5.535	1387	1398	1421	rBV	250794	513127	60.41%	7.733%
29	5.989	1527	1539	1562	rBV	190160	393916	46.38%	5.937%
30	6.651	1742	1745	1748	rBV5	1703	1112	0.13%	0.017%
31	6.670	1748	1751	1754	rVB3	1331	612	0.07%	0.009%
32	6.754	1775	1777	1784	rVB5	1642	1199	0.14%	0.018%
33	6.796	1784	1790	1795	rBV8	1380	1669	0.20%	0.025%
34	6.915	1816	1827	1846	rBV2	89205	173701	20.45%	2.618%
35	7.246	1919	1930	1953	rVV	357223	626058	73.70%	9.435%
36	7.555	2018	2026	2046	rBV	67592	119597	14.08%	1.802%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033438.D
 Acq On : 16 Dec 2023 16:26
 Operator : SY/MD
 Sample : 05802-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.844	2111	2116	2118	rBV5	1005	890	0.10%	0.013%
38	8.024	2161	2172	2204	rBV	207814	420254	49.48%	6.334%
39	8.609	2352	2354	2359	rVB7	1709	1144	0.13%	0.017%
40	8.677	2372	2375	2379	rVB5	1627	605	0.07%	0.009%
41	8.786	2397	2409	2427	rBV	424340	697089	82.07%	10.506%
42	9.136	2515	2518	2519	rBV3	1387	757	0.09%	0.011%
43	9.243	2549	2551	2553	rBV3	1158	796	0.09%	0.012%
44	9.445	2610	2614	2615	rBV4	1296	824	0.10%	0.012%
45	9.500	2620	2631	2645	rBV2	12296	24788	2.92%	0.374%
46	9.593	2659	2660	2663	rBV3	1048	643	0.08%	0.010%
47	9.963	2773	2775	2779	rBV5	1332	823	0.10%	0.012%
48	9.982	2779	2781	2783	rBV3	1279	650	0.08%	0.010%
49	10.153	2822	2834	2850	rBV	292115	467831	55.08%	7.051%
50	10.249	2861	2864	2867	rBV5	1259	756	0.09%	0.011%
51	10.284	2873	2875	2879	rVB4	1400	801	0.09%	0.012%
52	10.448	2924	2926	2929	rVB3	1167	601	0.07%	0.009%
53	10.468	2929	2932	2938	rBV8	1309	1517	0.18%	0.023%
54	10.603	2971	2974	2977	rVV3	1200	984	0.12%	0.015%
55	10.757	3018	3022	3025	rBV5	1184	960	0.11%	0.014%
56	10.895	3063	3065	3071	rVB5	2118	1433	0.17%	0.022%
57	11.111	3128	3132	3133	rBV4	978	645	0.08%	0.010%
58	11.188	3145	3156	3175	rBV	388823	612680	72.13%	9.234%
59	11.513	3252	3257	3260	rBV5	2043	2037	0.24%	0.031%
60	11.561	3262	3272	3293	rVB	399061	625107	73.59%	9.421%
61	11.738	3323	3327	3328	rBV4	1459	906	0.11%	0.014%
62	11.841	3357	3359	3362	rBV3	1293	800	0.09%	0.012%
63	11.908	3377	3380	3381	rBV3	1328	715	0.08%	0.011%
64	12.021	3411	3415	3416	rBV3	1316	769	0.09%	0.012%
65	12.111	3441	3443	3449	rVB6	2020	1697	0.20%	0.026%
66	12.275	3492	3494	3496	rBV3	1355	623	0.07%	0.009%
67	12.519	3566	3570	3572	rVV4	1511	920	0.11%	0.014%
68	12.535	3572	3575	3579	rVB6	1468	1121	0.13%	0.017%
69	12.590	3590	3592	3593	rBV2	1321	608	0.07%	0.009%
70	12.644	3607	3609	3611	rVB3	1607	602	0.07%	0.009%
71	12.734	3635	3637	3640	rBV3	1428	855	0.10%	0.013%
72	12.799	3655	3657	3660	rVB5	1112	621	0.07%	0.009%
73	12.908	3687	3691	3693	rBV4	1400	1186	0.14%	0.018%
74	13.004	3718	3721	3722	rBV3	1183	727	0.09%	0.011%
75	13.143	3761	3764	3765	rBV3	947	650	0.08%	0.010%
76	13.310	3812	3816	3818	rBV5	1135	887	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VV033438.D
 Acq On : 16 Dec 2023 16:26
 Operator : SY/MD
 Sample : 05802-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.397	3842	3843	3847	rVB3	1488	687	0.08%	0.010%
78	13.493	3869	3873	3876	rVB6	839	705	0.08%	0.011%
79	13.606	3904	3908	3911	rBV5	1592	1388	0.16%	0.021%
80	13.689	3931	3934	3935	rBV2	1502	925	0.11%	0.014%
81	14.040	4040	4043	4045	rBV3	1077	600	0.07%	0.009%
82	14.127	4068	4070	4076	rBV5	864	590	0.07%	0.009%
83	14.152	4076	4078	4081	rVB4	1534	893	0.11%	0.013%
84	14.172	4081	4084	4087	rBV4	1018	854	0.10%	0.013%
85	14.554	4200	4203	4207	rVB5	1983	1491	0.18%	0.022%
86	14.574	4207	4209	4211	rBV3	1483	681	0.08%	0.010%
87	14.638	4226	4229	4230	rBV2	1306	927	0.11%	0.014%
88	14.689	4242	4245	4246	rBV3	1165	595	0.07%	0.009%
89	14.792	4273	4277	4280	rBV5	2082	1549	0.18%	0.023%
90	14.873	4300	4302	4305	rVB4	951	587	0.07%	0.009%
91	14.895	4305	4309	4314	rBV5	1730	2237	0.26%	0.034%
92	14.943	4321	4324	4328	rVV5	992	798	0.09%	0.012%
93	14.966	4328	4331	4337	rVB7	1814	1253	0.15%	0.019%
94	14.995	4337	4340	4342	rBV5	1757	1008	0.12%	0.015%
95	15.053	4354	4358	4362	rBV6	1054	876	0.10%	0.013%
96	15.075	4363	4365	4368	rBV4	1406	768	0.09%	0.012%
97	15.326	4440	4443	4446	rBV4	1418	1042	0.12%	0.016%
98	15.352	4446	4451	4452	rBV4	1337	930	0.11%	0.014%
99	15.815	4592	4595	4597	rBV3	1276	986	0.12%	0.015%
100	15.898	4619	4621	4623	rBV3	1444	846	0.10%	0.013%




Sum of corrected areas: 6635256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033438.D
Acq On : 16 Dec 2023 16:26
Operator : SY/MD
Sample : 05802-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

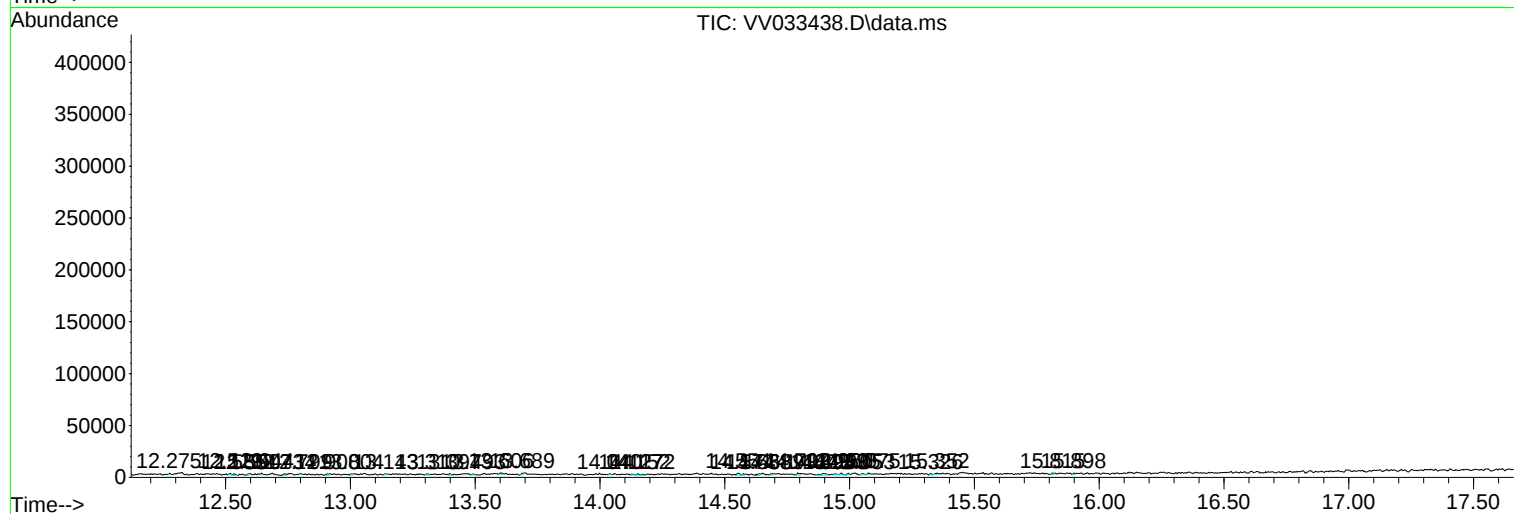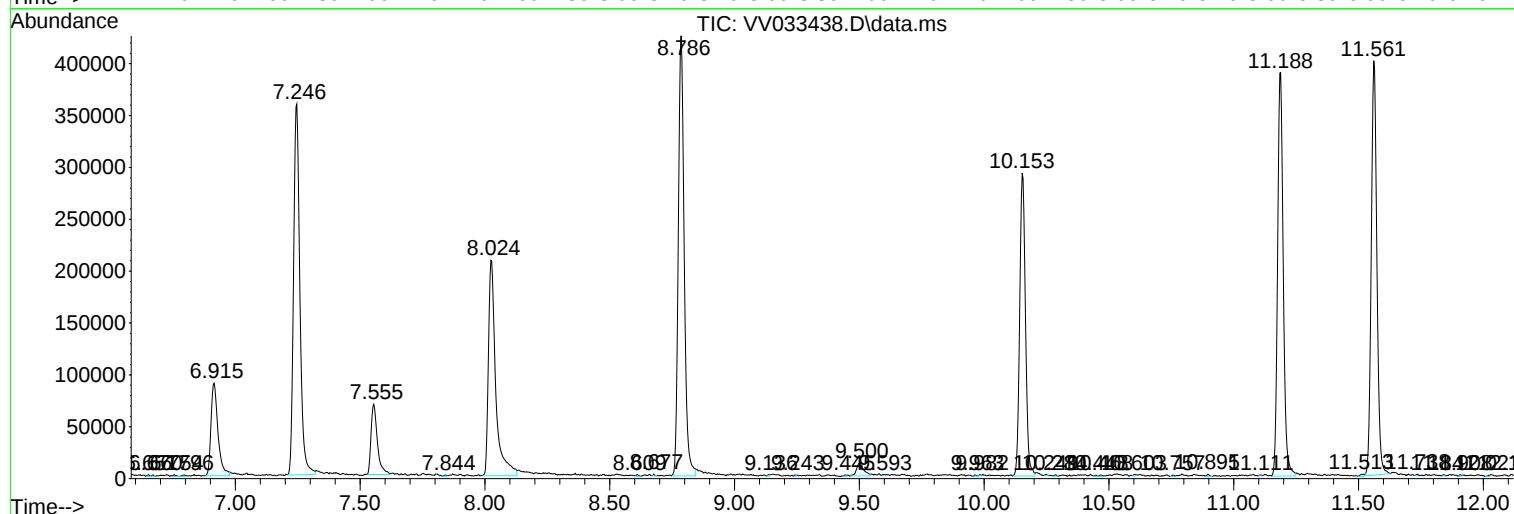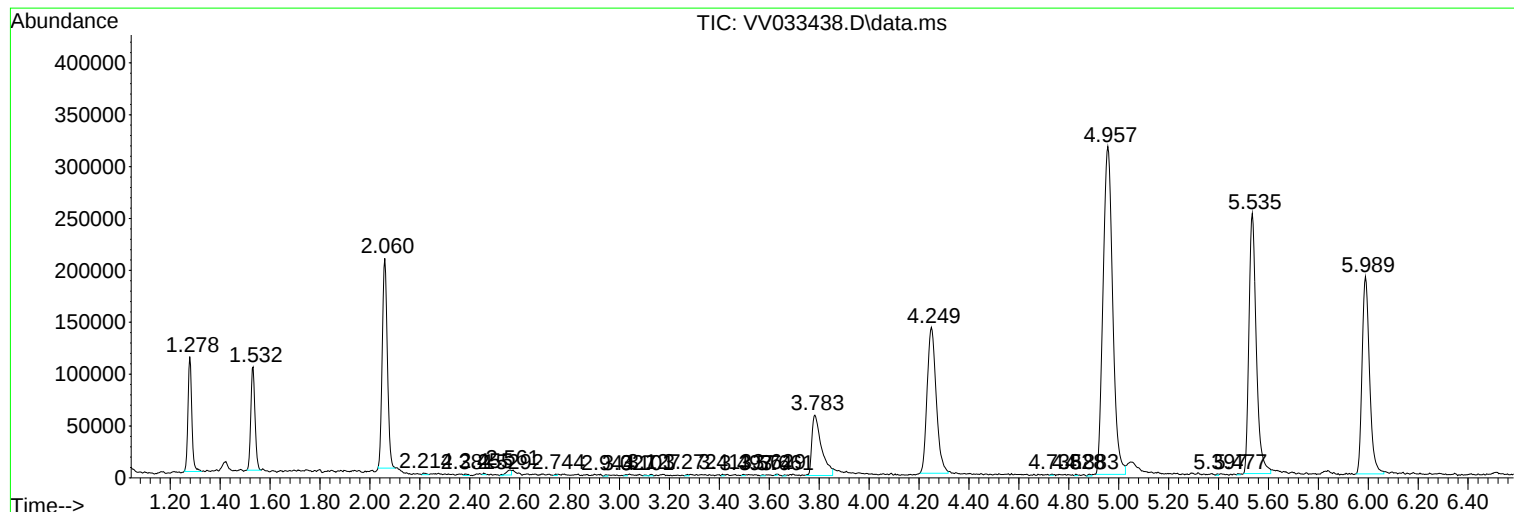

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033438.D
Acq On : 16 Dec 2023 16:26
Operator : SY/MD
Sample : 05802-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033438.D
Acq On : 16 Dec 2023 16:26
Operator : SY/MD
Sample : 05802-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc