

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033439.D
 Acq On : 16 Dec 2023 16:50
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	108710	111704	3.49%	1.195%
2	1.532	146	153	164	rVB	101119	118135	3.69%	1.263%
3	2.060	309	317	330	rVB	203406	287592	8.97%	3.076%
4	2.310	393	395	397	rBV3	1455	838	0.03%	0.009%
5	2.339	402	404	407	rVV4	1186	656	0.02%	0.007%
6	2.375	413	415	417	rBV3	1257	666	0.02%	0.007%
7	2.642	496	498	499	rBV	1305	583	0.02%	0.006%
8	2.735	525	527	530	rBV3	944	615	0.02%	0.007%
9	2.851	562	563	567	rVB4	869	495	0.02%	0.005%
10	2.960	595	597	599	rBV2	1004	506	0.02%	0.005%
11	3.150	653	656	658	rBV5	1088	655	0.02%	0.007%
12	3.172	661	663	665	rVB4	1221	505	0.02%	0.005%
13	3.191	665	669	673	rBV6	950	901	0.03%	0.010%
14	3.272	692	694	697	rBV4	884	493	0.02%	0.005%
15	3.320	705	709	712	rVB4	1632	1038	0.03%	0.011%
16	3.339	712	715	718	rBV3	768	633	0.02%	0.007%
17	3.461	751	753	756	rVB4	1250	722	0.02%	0.008%
18	3.481	756	759	763	rBV6	1094	945	0.03%	0.010%
19	3.571	785	787	791	rVB3	1498	616	0.02%	0.007%
20	3.725	832	835	837	rVB3	896	520	0.02%	0.006%
21	3.783	842	853	880	rBV2	48918	141031	4.40%	1.508%
22	4.249	985	998	1020	rVB	138962	346989	10.83%	3.711%
23	4.436	1054	1056	1059	rBV4	1356	703	0.02%	0.008%
24	4.661	1123	1126	1127	rBV3	1286	742	0.02%	0.008%
25	4.867	1188	1190	1194	rBV5	1062	649	0.02%	0.007%
26	4.957	1202	1218	1252	rBV2	315677	882921	27.55%	9.443%
27	5.535	1386	1398	1426	rBV2	247899	525124	16.39%	5.616%
28	5.902	1509	1512	1514	rBV3	1436	882	0.03%	0.009%
29	5.989	1528	1539	1565	rBV	186501	388856	12.13%	4.159%
30	6.220	1608	1611	1613	rBV4	1493	872	0.03%	0.009%
31	6.368	1655	1657	1659	rBV3	1427	840	0.03%	0.009%
32	6.510	1699	1701	1705	rVB4	1316	661	0.02%	0.007%
33	6.635	1739	1740	1745	rVB3	1370	606	0.02%	0.006%
34	6.686	1754	1756	1759	rBV4	1278	985	0.03%	0.011%
35	6.770	1780	1782	1784	rBV3	801	474	0.01%	0.005%
36	6.915	1813	1827	1840	rBV	90064	169227	5.28%	1.810%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033439.D
 Acq On : 16 Dec 2023 16:50
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.246	1919	1930	1953	rBV	348406	619444	19.33%	6.625%
38	7.555	2017	2026	2044	rBV	67970	120898	3.77%	1.293%
39	7.764	2089	2091	2095	rBV5	1448	1098	0.03%	0.012%
40	7.847	2115	2117	2119	rBV2	1346	664	0.02%	0.007%
41	7.895	2130	2132	2133	rBV2	1060	475	0.01%	0.005%
42	8.024	2163	2172	2200	rBV2	169394	345326	10.78%	3.693%
43	8.506	2320	2322	2325	rBV2	1182	593	0.02%	0.006%
44	8.574	2340	2343	2346	rBV3	1285	969	0.03%	0.010%
45	8.625	2357	2359	2364	rVB5	1636	1367	0.04%	0.015%
46	8.706	2382	2384	2388	rBV5	1230	710	0.02%	0.008%
47	8.786	2397	2409	2415	rBV	445931	757461	23.64%	8.101%
48	9.072	2495	2498	2499	rBV3	1425	753	0.02%	0.008%
49	9.265	2556	2558	2561	rBV3	786	499	0.02%	0.005%
50	9.365	2587	2589	2593	rBV5	1419	1085	0.03%	0.012%
51	9.616	2663	2667	2672	rBV8	1658	1471	0.05%	0.016%
52	9.641	2672	2675	2676	rBV2	1207	701	0.02%	0.007%
53	9.680	2685	2687	2689	rBV3	1083	517	0.02%	0.006%
54	9.718	2697	2699	2703	rBV4	943	530	0.02%	0.006%
55	9.802	2723	2725	2728	rBV2	2147	1103	0.03%	0.012%
56	9.847	2734	2739	2741	rBV6	1478	1453	0.05%	0.016%
57	9.905	2755	2757	2762	rVB5	1515	929	0.03%	0.010%
58	9.934	2764	2766	2769	rBV2	950	577	0.02%	0.006%
59	9.950	2769	2771	2772	rBV2	1154	526	0.02%	0.006%
60	10.046	2796	2801	2803	rBV4	1539	1243	0.04%	0.013%
61	10.153	2822	2834	2851	rBV	275047	438367	13.68%	4.688%
62	10.368	2897	2901	2902	rBV3	1118	813	0.03%	0.009%
63	10.664	2988	2993	2994	rBV5	1456	987	0.03%	0.011%
64	10.747	3017	3019	3024	rVB6	1319	1036	0.03%	0.011%
65	10.776	3024	3028	3030	rBV4	1298	1068	0.03%	0.011%
66	10.818	3038	3041	3043	rBV4	811	534	0.02%	0.006%
67	10.889	3060	3063	3066	rBV4	1297	848	0.03%	0.009%
68	10.918	3068	3072	3075	rBV5	1522	1304	0.04%	0.014%
69	10.989	3089	3094	3098	rBV7	1298	1651	0.05%	0.018%
70	11.046	3109	3112	3115	rBV5	1120	971	0.03%	0.010%
71	11.107	3128	3131	3132	rBV3	2224	1221	0.04%	0.013%
72	11.188	3145	3156	3178	rBV2	400868	823800	25.71%	8.810%
73	11.580	3261	3278	3297	rBV2	1732610	3204740	100.00%	34.274%
74	11.841	3357	3359	3361	rBV3	1541	727	0.02%	0.008%
75	11.966	3396	3398	3403	rVB6	1074	724	0.02%	0.008%
76	12.188	3464	3467	3469	rBV3	1193	751	0.02%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033439.D
 Acq On : 16 Dec 2023 16:50
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.403	3531	3534	3538	rVB4	921	634	0.02%	0.007%
78	12.429	3538	3542	3545	rBV6	1082	756	0.02%	0.008%
79	12.577	3586	3588	3591	rBV3	1025	642	0.02%	0.007%
80	12.612	3595	3599	3602	rBV7	1160	883	0.03%	0.009%
81	12.699	3623	3626	3628	rBV5	756	528	0.02%	0.006%
82	12.966	3704	3709	3710	rBV5	1511	1053	0.03%	0.011%
83	13.037	3728	3731	3734	rBV5	1192	718	0.02%	0.008%
84	13.262	3799	3801	3805	rVB5	1128	627	0.02%	0.007%
85	13.320	3815	3819	3822	rBV5	897	909	0.03%	0.010%
86	13.397	3839	3843	3847	rVB6	1502	1296	0.04%	0.014%
87	13.419	3847	3850	3853	rBV5	1223	941	0.03%	0.010%
88	13.493	3869	3873	3875	rBV5	1318	974	0.03%	0.010%
89	13.522	3879	3882	3886	rBV3	995	1088	0.03%	0.012%
90	13.837	3978	3980	3984	rVB4	1346	671	0.02%	0.007%
91	13.911	4001	4003	4008	rBV5	917	752	0.02%	0.008%
92	14.033	4039	4041	4045	rBV3	684	609	0.02%	0.007%
93	14.249	4105	4108	4109	rBV2	909	481	0.02%	0.005%
94	14.538	4195	4198	4200	rVB4	1243	632	0.02%	0.007%
95	14.773	4267	4271	4276	rBV5	1185	1315	0.04%	0.014%
96	14.905	4309	4312	4313	rBV3	835	541	0.02%	0.006%
97	15.008	4340	4344	4346	rBV5	1107	853	0.03%	0.009%
98	15.217	4407	4409	4414	rVB5	1898	1404	0.04%	0.015%
99	15.284	4427	4430	4432	rBV3	1363	991	0.03%	0.011%
100	15.403	4464	4467	4468	rBV3	1329	829	0.03%	0.009%

Sum of corrected areas: 9350441




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033439.D
Acq On : 16 Dec 2023 16:50
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

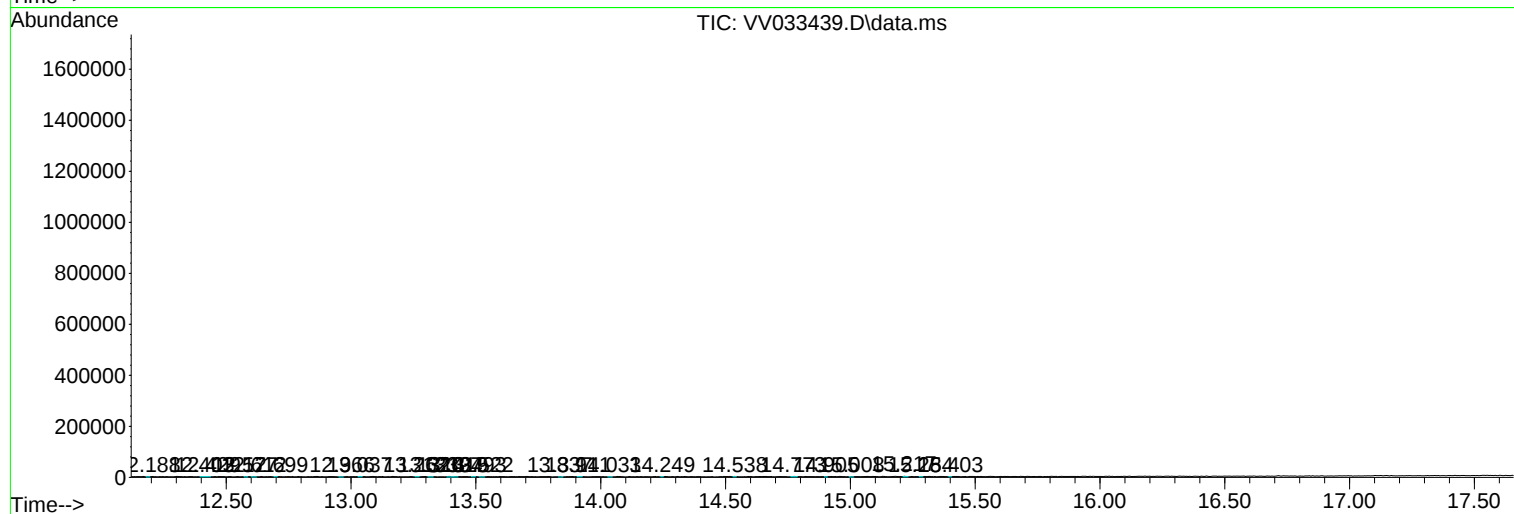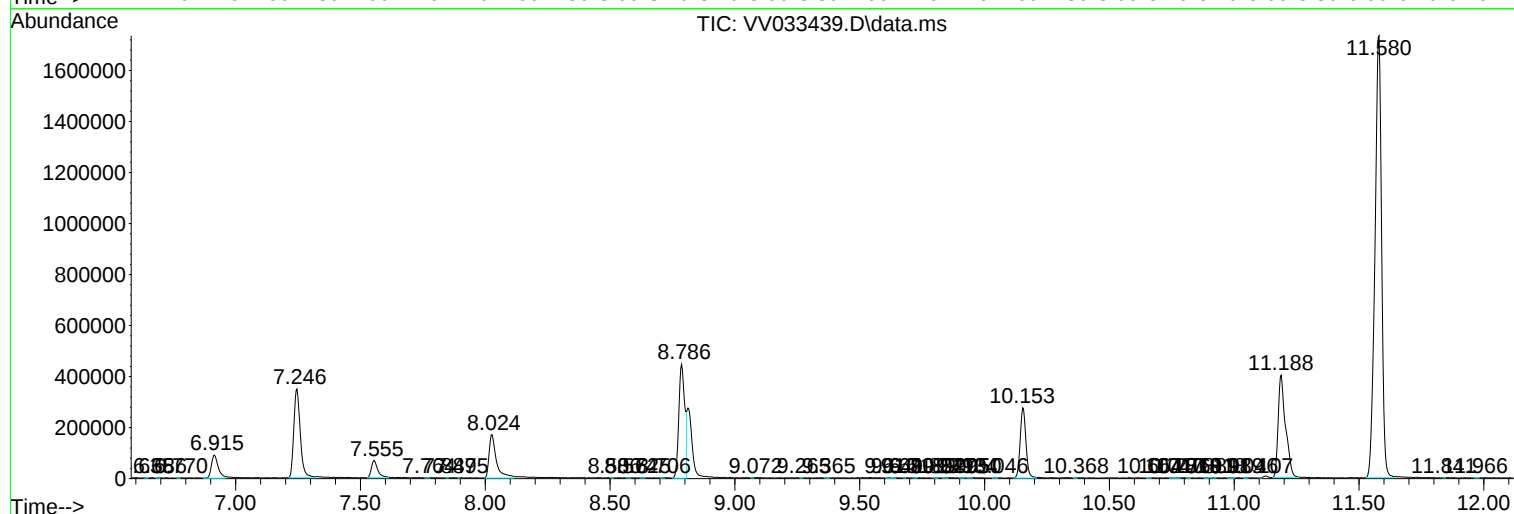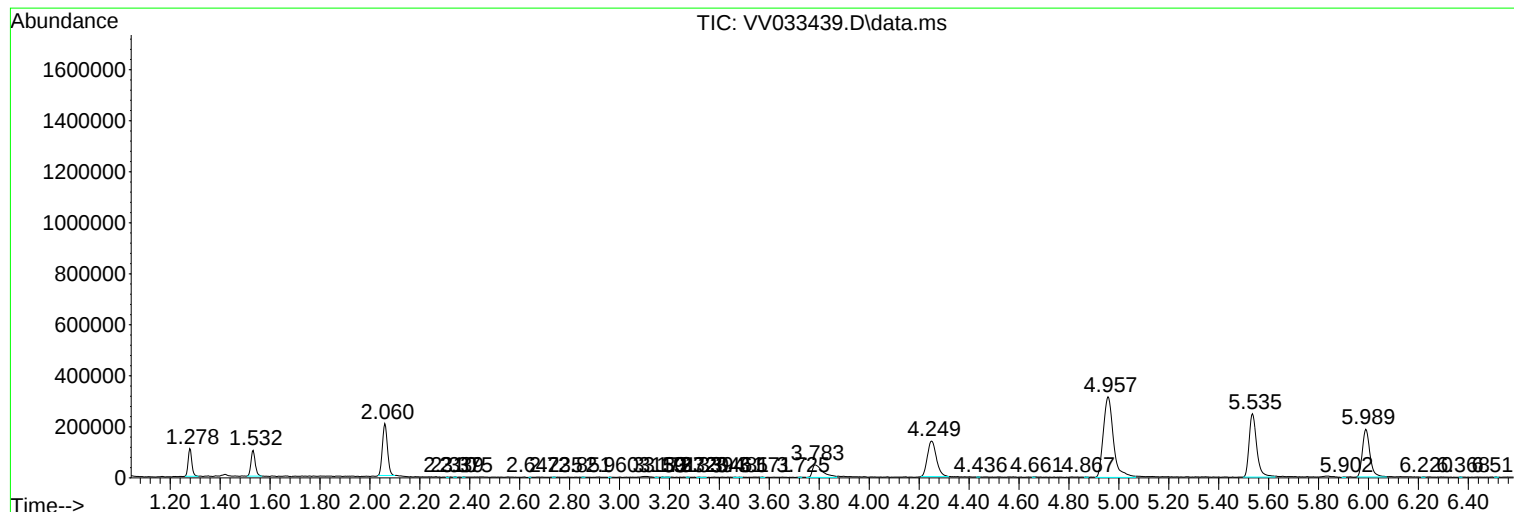

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033439.D
Acq On : 16 Dec 2023 16:50
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033439.D
Acq On : 16 Dec 2023 16:50
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------