

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033440.D
 Acq On : 16 Dec 2023 17:13
 Operator : SY/MD
 Sample : 05834-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	110040	116308	13.89%	1.817%
2	1.532	146	153	166	rVB	102117	119997	14.33%	1.875%
3	2.060	308	317	331	rBV	204982	298192	35.60%	4.660%
4	2.950	591	594	596	rBV4	836	602	0.07%	0.009%
5	3.060	626	628	630	rBV3	773	396	0.05%	0.006%
6	3.111	641	644	648	rBV5	1050	736	0.09%	0.012%
7	3.172	662	663	664	rBV	706	165	0.02%	0.003%
8	3.307	702	705	706	rBV3	1024	490	0.06%	0.008%
9	3.346	715	717	719	rBV3	1330	570	0.07%	0.009%
10	3.429	741	743	745	rBV2	803	437	0.05%	0.007%
11	3.481	755	759	763	rBV7	1377	1273	0.15%	0.020%
12	3.548	777	780	781	rBV3	769	366	0.04%	0.006%
13	3.577	786	789	792	rVB4	1516	970	0.12%	0.015%
14	3.600	792	796	798	rBV5	1362	1001	0.12%	0.016%
15	3.635	803	807	813	rBV7	1358	1429	0.17%	0.022%
16	3.661	813	815	816	rBV	803	280	0.03%	0.004%
17	3.783	845	853	881	rBV	48654	137016	16.36%	2.141%
18	4.249	985	998	1021	rVB	139679	350458	41.84%	5.476%
19	4.780	1159	1163	1164	rBV4	1040	720	0.09%	0.011%
20	4.812	1170	1173	1175	rBV4	1192	678	0.08%	0.011%
21	4.831	1177	1179	1182	rVV4	1240	754	0.09%	0.012%
22	4.863	1187	1189	1191	rBV3	937	407	0.05%	0.006%
23	4.957	1202	1218	1244	rBV3	312592	837518	100.00%	13.087%
24	5.439	1366	1368	1369	rBV2	742	346	0.04%	0.005%
25	5.535	1387	1398	1424	rBV	245664	513042	61.26%	8.017%
26	5.989	1528	1539	1564	rVB	190026	384188	45.87%	6.003%
27	6.452	1682	1683	1686	rBV3	1053	707	0.08%	0.011%
28	6.487	1692	1694	1699	rVB6	1810	1024	0.12%	0.016%
29	6.510	1699	1701	1706	rBV4	1179	999	0.12%	0.016%
30	6.603	1726	1730	1735	rVV7	1923	1762	0.21%	0.028%
31	6.635	1735	1740	1742	rVB5	1327	1191	0.14%	0.019%
32	6.741	1768	1773	1776	rBV6	1416	1382	0.17%	0.022%
33	6.767	1779	1781	1784	rVV2	892	545	0.07%	0.009%
34	6.783	1784	1786	1790	rVB5	1459	959	0.11%	0.015%
35	6.915	1817	1827	1851	rBV	87637	167173	19.96%	2.612%
36	7.063	1870	1873	1874	rBV2	1546	831	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033440.D
 Acq On : 16 Dec 2023 17:13
 Operator : SY/MD
 Sample : 05834-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.146	1895	1899	1900	rBV3	1218	890	0.11%	0.014%
38	7.246	1919	1930	1949	rBV	347656	617436	73.72%	9.648%
39	7.555	2018	2026	2038	rBV	63617	110297	13.17%	1.723%
40	7.728	2078	2080	2081	rBV2	967	387	0.05%	0.006%
41	7.947	2146	2148	2150	rBV3	1035	475	0.06%	0.007%
42	8.027	2163	2173	2212	rBV	162057	347267	41.46%	5.426%
43	8.378	2280	2282	2283	rBV2	1121	458	0.05%	0.007%
44	8.542	2330	2333	2335	rBV3	1707	1128	0.13%	0.018%
45	8.590	2347	2348	2351	rVB2	1722	734	0.09%	0.011%
46	8.606	2351	2353	2354	rBV2	954	453	0.05%	0.007%
47	8.786	2398	2409	2431	rBV	421493	690703	82.47%	10.793%
48	9.310	2569	2572	2573	rBV3	891	501	0.06%	0.008%
49	9.346	2580	2583	2584	rBV2	1131	630	0.08%	0.010%
50	9.423	2603	2607	2613	rBV9	1153	1426	0.17%	0.022%
51	9.542	2639	2644	2647	rBV6	1715	1495	0.18%	0.023%
52	9.641	2672	2675	2679	rBV5	1469	1212	0.14%	0.019%
53	9.674	2679	2685	2687	rBV7	1252	1418	0.17%	0.022%
54	9.744	2705	2707	2708	rBV2	902	296	0.04%	0.005%
55	9.866	2743	2745	2746	rBV2	920	331	0.04%	0.005%
56	10.153	2822	2834	2852	rBV	264854	424423	50.68%	6.632%
57	10.349	2893	2895	2897	rBV2	795	302	0.04%	0.005%
58	10.436	2920	2922	2923	rBV	1491	776	0.09%	0.012%
59	10.461	2928	2930	2931	rBV2	769	321	0.04%	0.005%
60	10.516	2944	2947	2948	rBV2	1152	660	0.08%	0.010%
61	10.635	2982	2984	2986	rVB2	1257	336	0.04%	0.005%
62	10.690	2999	3001	3003	rBV3	1121	529	0.06%	0.008%
63	10.931	3074	3076	3079	rBV3	778	518	0.06%	0.008%
64	11.185	3145	3155	3180	rBV	373952	591055	70.57%	9.236%
65	11.371	3211	3213	3216	rBV4	1223	549	0.07%	0.009%
66	11.419	3226	3228	3231	rBV3	1130	841	0.10%	0.013%
67	11.561	3262	3272	3296	rVB	391450	635854	75.92%	9.936%
68	11.886	3372	3373	3374	rBV	620	185	0.02%	0.003%
69	12.124	3444	3447	3449	rBV4	1228	950	0.11%	0.015%
70	12.268	3490	3492	3495	rBV4	1248	731	0.09%	0.011%
71	12.558	3580	3582	3583	rBV2	1097	439	0.05%	0.007%
72	12.825	3663	3665	3669	rBV5	1200	744	0.09%	0.012%
73	12.940	3697	3701	3702	rBV2	1853	1103	0.13%	0.017%
74	13.095	3748	3749	3751	rBV2	1149	522	0.06%	0.008%
75	13.140	3761	3763	3764	rBV	660	230	0.03%	0.004%
76	13.181	3774	3776	3779	rBV4	834	495	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033440.D
 Acq On : 16 Dec 2023 17:13
 Operator : SY/MD
 Sample : 05834-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.384	3836	3839	3842	rBV5	996	769	0.09%	0.012%
78	13.474	3865	3867	3871	rVB5	2160	1283	0.15%	0.020%
79	13.503	3873	3876	3878	rBV3	1250	725	0.09%	0.011%
80	13.529	3881	3884	3885	rBV3	718	349	0.04%	0.005%
81	13.680	3930	3931	3933	rBV2	943	291	0.03%	0.005%
82	13.754	3952	3954	3958	rBV5	1010	730	0.09%	0.011%
83	13.799	3966	3968	3971	rBV4	984	736	0.09%	0.012%
84	13.918	4003	4005	4008	rBV3	830	403	0.05%	0.006%
85	13.934	4008	4010	4013	rVB3	1646	804	0.10%	0.013%
86	13.956	4016	4017	4020	rBV2	879	354	0.04%	0.006%
87	13.972	4020	4022	4023	rBV	729	310	0.04%	0.005%
88	14.056	4046	4048	4051	rBV4	1304	649	0.08%	0.010%
89	14.230	4100	4102	4104	rBV3	872	469	0.06%	0.007%
90	14.262	4110	4112	4114	rBV3	1004	441	0.05%	0.007%
91	14.352	4137	4140	4142	rBV4	1011	654	0.08%	0.010%
92	14.551	4200	4202	4207	rVB4	1943	1194	0.14%	0.019%
93	14.577	4207	4210	4212	rBV4	890	709	0.08%	0.011%
94	14.632	4224	4227	4229	rBV3	1287	801	0.10%	0.013%
95	14.792	4275	4277	4280	rBV3	1531	1013	0.12%	0.016%
96	15.111	4374	4376	4379	rBV4	1002	576	0.07%	0.009%
97	15.165	4391	4393	4395	rBV2	867	262	0.03%	0.004%
98	15.207	4403	4406	4407	rBV3	1353	713	0.09%	0.011%
99	15.323	4439	4442	4444	rBV4	1515	823	0.10%	0.013%
100	15.416	4469	4471	4473	rBV2	1208	535	0.06%	0.008%




Sum of corrected areas: 6399605

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033440.D
Acq On : 16 Dec 2023 17:13
Operator : SY/MD
Sample : 05834-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

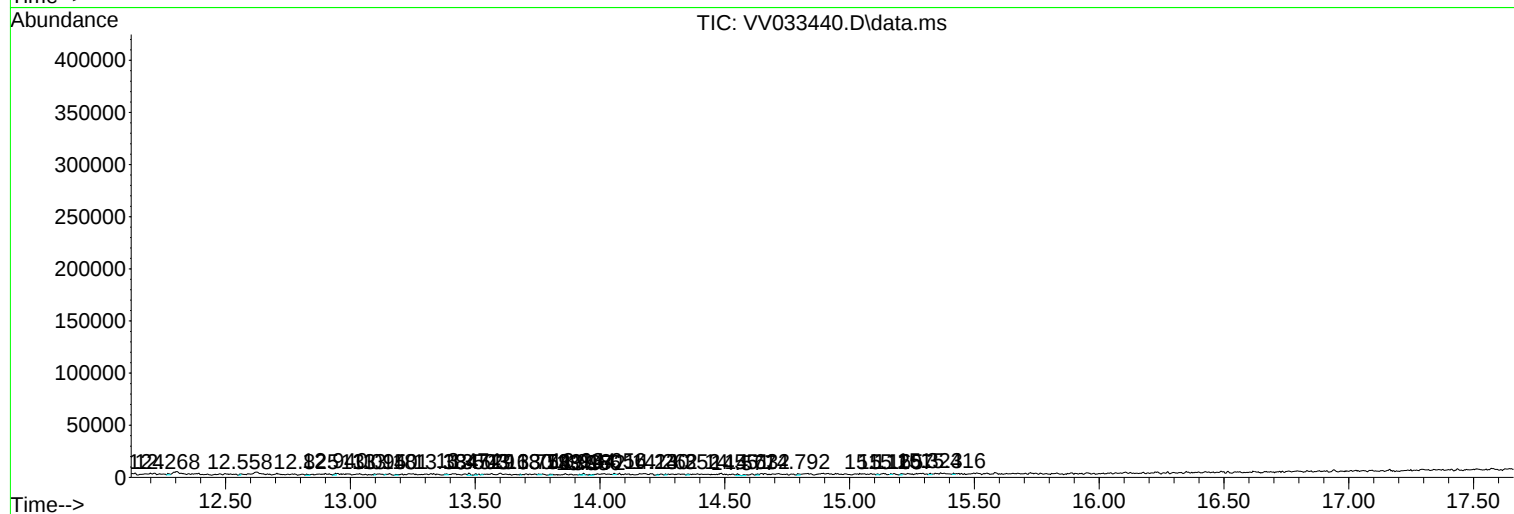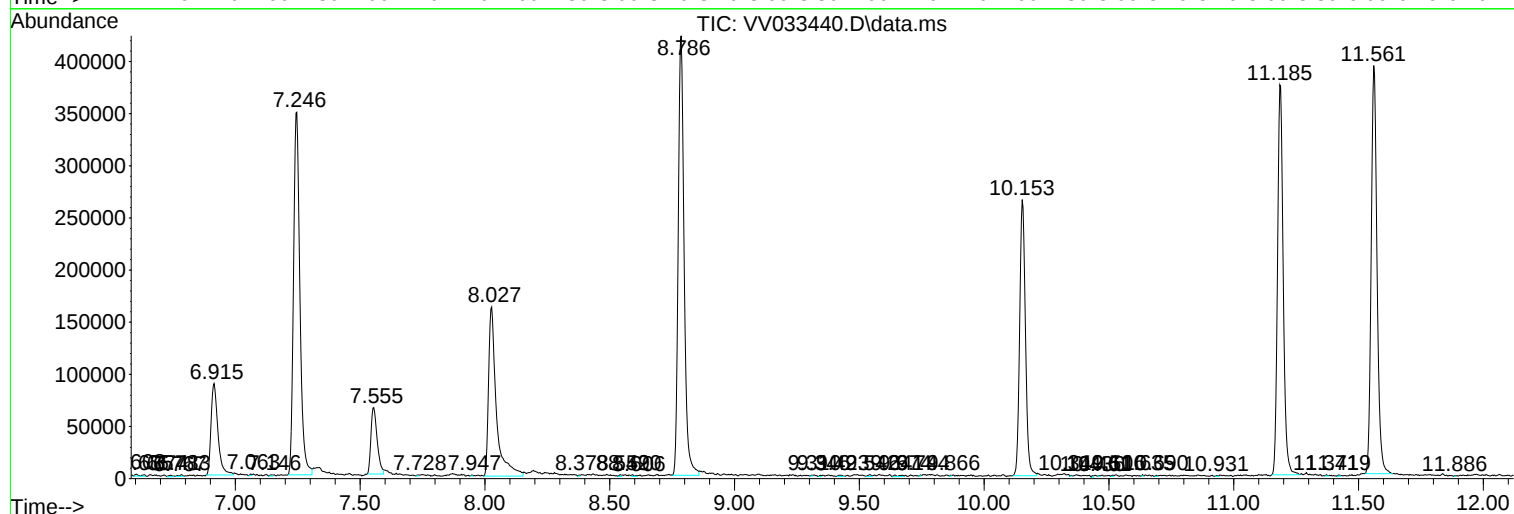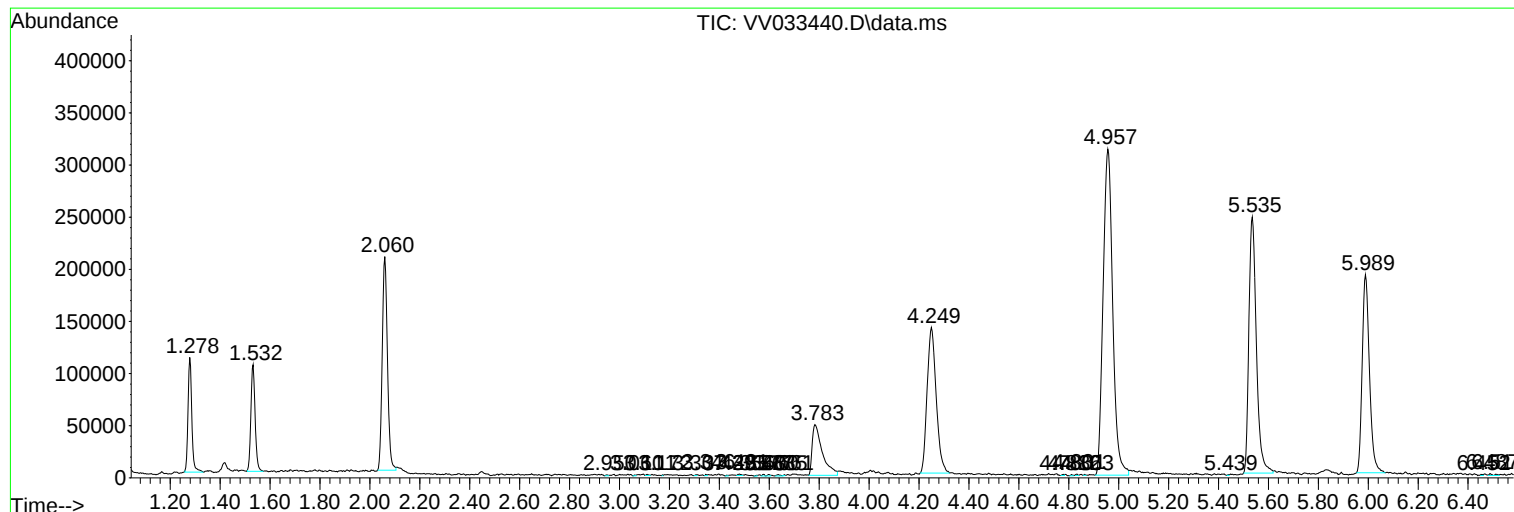

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033440.D
Acq On : 16 Dec 2023 17:13
Operator : SY/MD
Sample : 05834-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033440.D
Acq On : 16 Dec 2023 17:13
Operator : SY/MD
Sample : 05834-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------