

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033441.D
 Acq On : 16 Dec 2023 17:36
 Operator : SY/MD
 Sample : 05834-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	115191	119274	13.40%	1.793%
2	1.532	146	153	167	rVB	107238	126220	14.18%	1.897%
3	2.060	308	317	336	rVB	216885	314987	35.38%	4.734%
4	2.310	391	395	400	rBV7	1865	1880	0.21%	0.028%
5	2.561	470	473	474	rBV3	1270	655	0.07%	0.010%
6	2.600	483	485	487	rBV3	1036	646	0.07%	0.010%
7	2.728	523	525	528	rBV4	1080	655	0.07%	0.010%
8	2.969	597	600	603	rVB4	1578	1144	0.13%	0.017%
9	3.011	611	613	616	rVB3	1508	783	0.09%	0.012%
10	3.076	630	633	637	rBV6	971	890	0.10%	0.013%
11	3.211	673	675	677	rVB2	1427	545	0.06%	0.008%
12	3.294	698	701	704	rVB4	1337	914	0.10%	0.014%
13	3.314	704	707	710	rBV4	1030	984	0.11%	0.015%
14	3.359	718	721	725	rBV5	1341	1008	0.11%	0.015%
15	3.420	735	740	742	rBV6	1284	1024	0.12%	0.015%
16	3.574	785	788	790	rBV2	758	560	0.06%	0.008%
17	3.616	799	801	804	rBV3	1061	633	0.07%	0.010%
18	3.648	807	811	813	rBV5	1043	842	0.09%	0.013%
19	3.722	831	834	836	rVV4	1328	762	0.09%	0.011%
20	3.783	845	853	883	rBV2	52104	142103	15.96%	2.136%
21	3.989	913	917	922	rBV6	1566	1485	0.17%	0.022%
22	4.249	984	998	1022	rBV	149315	372753	41.87%	5.602%
23	4.603	1104	1108	1110	rBV2	1115	973	0.11%	0.015%
24	4.780	1159	1163	1165	rBV4	1549	890	0.10%	0.013%
25	4.892	1196	1198	1200	rBV3	1276	836	0.09%	0.013%
26	4.957	1202	1218	1247	rVV2	329665	890213	100.00%	13.380%
27	5.439	1366	1368	1371	rBV3	887	574	0.06%	0.009%
28	5.535	1385	1398	1425	rBV	247438	522415	58.68%	7.852%
29	5.989	1528	1539	1561	rBV	198027	405220	45.52%	6.090%
30	6.368	1651	1657	1658	rBV5	1303	988	0.11%	0.015%
31	6.542	1708	1711	1715	rBV4	1312	957	0.11%	0.014%
32	6.567	1716	1719	1723	rVV5	2024	1584	0.18%	0.024%
33	6.587	1723	1725	1729	rVB5	1733	1051	0.12%	0.016%
34	6.641	1740	1742	1745	rBV3	1098	676	0.08%	0.010%
35	6.776	1780	1784	1787	rBV5	1574	1188	0.13%	0.018%
36	6.915	1818	1827	1851	rBV	92236	173693	19.51%	2.611%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033441.D
 Acq On : 16 Dec 2023 17:36
 Operator : SY/MD
 Sample : 05834-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.243	1919	1929	1951	rBV	369648	650819	73.11%	9.782%
38	7.554	2018	2026	2045	rBV	68209	119694	13.45%	1.799%
39	8.024	2163	2172	2206	rBV	178020	371459	41.73%	5.583%
40	8.423	2293	2296	2298	rBV3	1445	1005	0.11%	0.015%
41	8.680	2373	2376	2377	rBV3	1348	798	0.09%	0.012%
42	8.725	2384	2390	2393	rBV6	1712	1712	0.19%	0.026%
43	8.786	2398	2409	2427	rBV	419746	682620	76.68%	10.260%
44	9.214	2540	2542	2545	rBV2	1127	716	0.08%	0.011%
45	9.294	2564	2567	2568	rBV3	1153	541	0.06%	0.008%
46	9.345	2580	2583	2585	rVV3	1301	768	0.09%	0.012%
47	9.461	2613	2619	2621	rBV5	1243	1166	0.13%	0.018%
48	9.686	2683	2689	2691	rVV6	1551	1373	0.15%	0.021%
49	9.709	2694	2696	2700	rVB3	1324	839	0.09%	0.013%
50	9.741	2700	2706	2710	rBV7	1238	1332	0.15%	0.020%
51	9.860	2741	2743	2750	rVV8	1082	795	0.09%	0.012%
52	9.934	2764	2766	2770	rBV5	816	546	0.06%	0.008%
53	9.956	2771	2773	2778	rVB4	1095	720	0.08%	0.011%
54	9.992	2780	2784	2786	rBV4	818	575	0.06%	0.009%
55	10.152	2820	2834	2851	rBV	282329	449174	50.46%	6.751%
56	10.487	2936	2938	2942	rVV5	1497	776	0.09%	0.012%
57	10.532	2949	2952	2954	rBV3	1286	821	0.09%	0.012%
58	10.558	2958	2960	2964	rBV5	875	611	0.07%	0.009%
59	10.583	2967	2968	2973	rVB5	1201	839	0.09%	0.013%
60	10.651	2986	2989	2995	rBV5	1338	1179	0.13%	0.018%
61	10.744	3016	3018	3023	rVB6	1010	714	0.08%	0.011%
62	10.789	3030	3032	3033	rBV2	1691	707	0.08%	0.011%
63	10.940	3075	3079	3082	rBV6	1410	1202	0.14%	0.018%
64	10.972	3086	3089	3093	rVV6	1129	879	0.10%	0.013%
65	11.114	3130	3133	3135	rVV4	1120	564	0.06%	0.008%
66	11.188	3145	3156	3175	rBV	372960	595046	66.84%	8.943%
67	11.426	3228	3230	3232	rBV3	1141	645	0.07%	0.010%
68	11.561	3262	3272	3292	rBV	407143	639682	71.86%	9.614%
69	11.824	3351	3354	3359	rBV6	1246	1185	0.13%	0.018%
70	11.876	3364	3370	3373	rVB5	1230	1103	0.12%	0.017%
71	11.892	3373	3375	3377	rBV3	1045	560	0.06%	0.008%
72	12.062	3424	3428	3433	rBV7	1368	1767	0.20%	0.027%
73	12.249	3480	3486	3488	rBV5	1920	1828	0.21%	0.027%
74	12.554	3577	3581	3583	rBV4	1097	732	0.08%	0.011%
75	12.570	3583	3586	3588	rBV4	920	587	0.07%	0.009%
76	12.767	3645	3647	3650	rBV4	817	548	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033441.D
 Acq On : 16 Dec 2023 17:36
 Operator : SY/MD
 Sample : 05834-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.799	3654	3657	3659	rBV4	1439	1037	0.12%	0.016%
78	12.911	3686	3692	3694	rBV7	1140	1222	0.14%	0.018%
79	13.024	3725	3727	3731	rBV4	1558	1163	0.13%	0.017%
80	13.114	3753	3755	3757	rBV3	1159	825	0.09%	0.012%
81	13.165	3769	3771	3775	rVB3	1245	701	0.08%	0.011%
82	13.297	3809	3812	3817	rBV5	1840	1485	0.17%	0.022%
83	13.320	3817	3819	3823	rBV5	919	651	0.07%	0.010%
84	13.439	3852	3856	3858	rBV4	1611	1387	0.16%	0.021%
85	13.471	3864	3866	3868	rBV3	1071	579	0.07%	0.009%
86	13.635	3915	3917	3919	rBV3	1538	557	0.06%	0.008%
87	13.664	3923	3926	3928	rBV3	1149	647	0.07%	0.010%
88	13.754	3951	3954	3956	rBV3	980	665	0.07%	0.010%
89	13.856	3984	3986	3990	rVB5	1003	786	0.09%	0.012%
90	13.975	4021	4023	4026	rBV3	1051	656	0.07%	0.010%
91	14.123	4064	4069	4072	rBV5	1766	1635	0.18%	0.025%
92	14.223	4098	4100	4102	rBV3	1057	589	0.07%	0.009%
93	14.381	4146	4149	4151	rBV2	1205	653	0.07%	0.010%
94	14.442	4165	4168	4173	rBV7	1490	1804	0.20%	0.027%
95	14.490	4180	4183	4184	rBV3	1399	855	0.10%	0.013%
96	14.593	4213	4215	4218	rBV3	1259	817	0.09%	0.012%
97	14.934	4318	4321	4325	rBV5	1192	995	0.11%	0.015%
98	15.194	4400	4402	4405	rVB4	1208	578	0.06%	0.009%
99	15.387	4460	4462	4466	rBV4	1210	891	0.10%	0.013%
100	15.432	4471	4476	4478	rBV7	1601	1656	0.19%	0.025%




Sum of corrected areas: 6653466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033441.D
Acq On : 16 Dec 2023 17:36
Operator : SY/MD
Sample : 05834-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

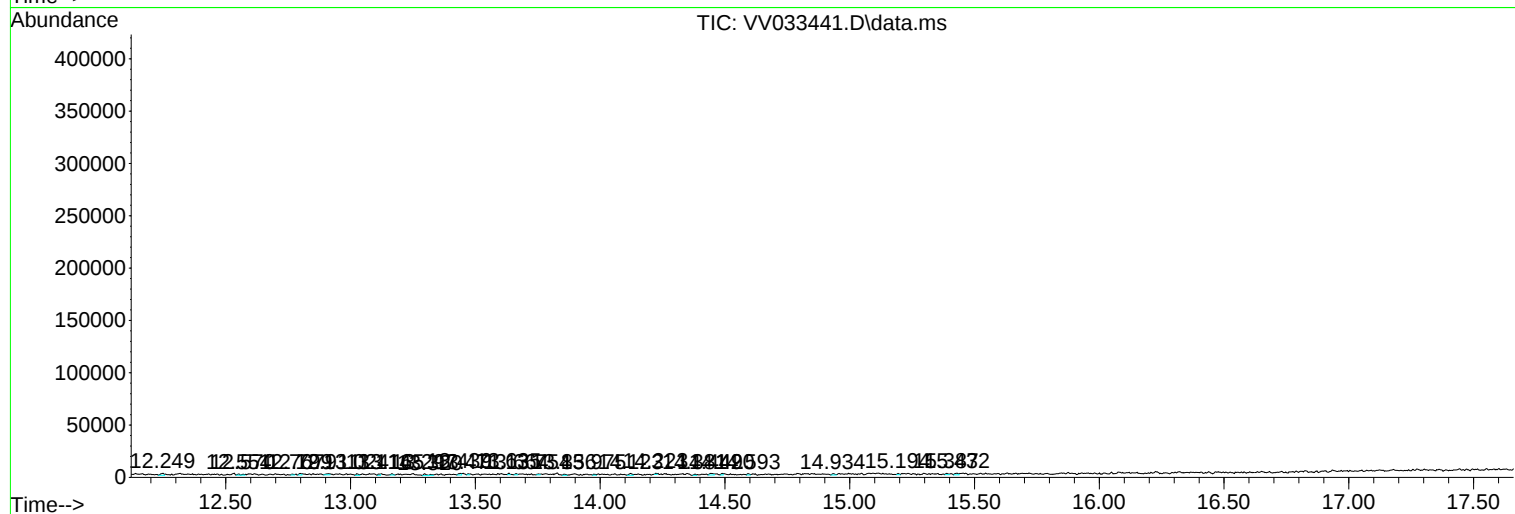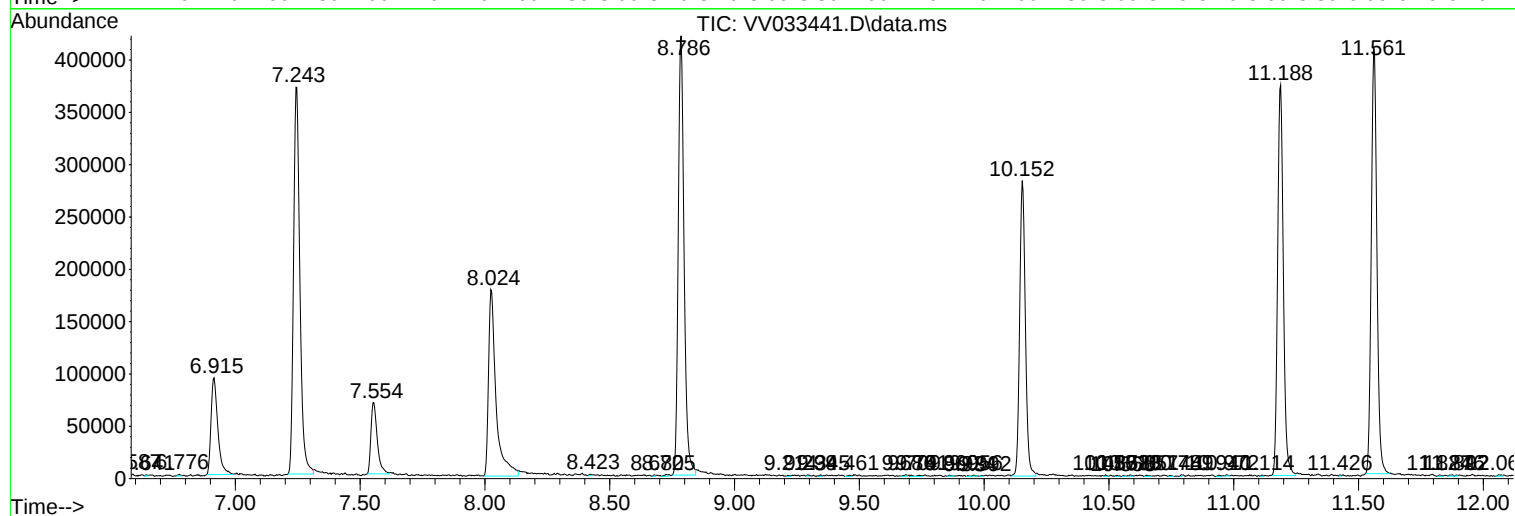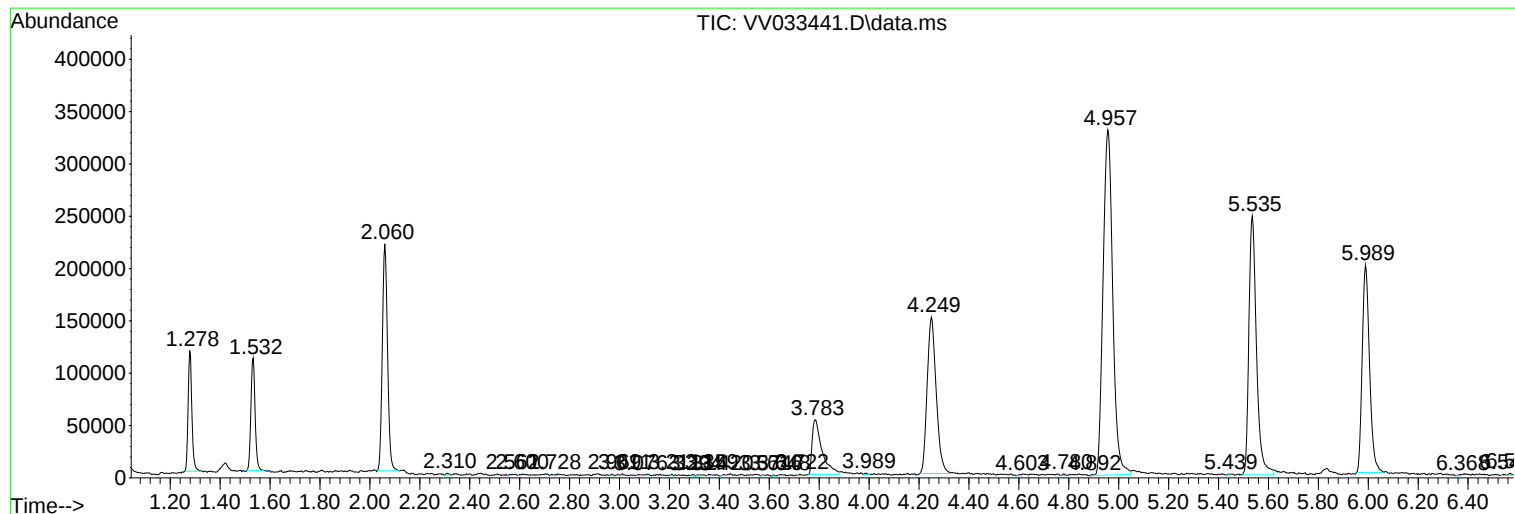

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033441.D
Acq On : 16 Dec 2023 17:36
Operator : SY/MD
Sample : 05834-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033441.D
Acq On : 16 Dec 2023 17:36
Operator : SY/MD
Sample : 05834-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------