

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033442.D
 Acq On : 16 Dec 2023 18:00
 Operator : SY/MD
 Sample : 05846-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	118978	121316	14.05%	1.864%
2	1.532	146	153	168	rVB	102783	123406	14.29%	1.896%
3	2.060	308	317	331	rVB	210835	302625	35.04%	4.649%
4	2.243	370	374	376	rBV3	1494	1303	0.15%	0.020%
5	2.410	423	426	427	rBV3	1412	801	0.09%	0.012%
6	2.442	434	436	443	rBV6	1475	1401	0.16%	0.022%
7	2.790	541	544	547	rBV5	1294	760	0.09%	0.012%
8	2.944	587	592	595	rBV7	1335	1587	0.18%	0.024%
9	3.060	622	628	630	rBV6	1597	1670	0.19%	0.026%
10	3.130	648	650	654	rVB4	1607	1022	0.12%	0.016%
11	3.285	695	698	702	rVB6	1063	717	0.08%	0.011%
12	3.490	760	762	765	rBV4	1312	916	0.11%	0.014%
13	3.571	782	787	790	rBV5	1963	1952	0.23%	0.030%
14	3.680	819	821	826	rVB5	1241	1082	0.13%	0.017%
15	3.719	826	833	836	rBV7	1461	1354	0.16%	0.021%
16	3.748	836	842	843	rBV5	1092	844	0.10%	0.013%
17	3.783	845	853	879	rBV	50962	141663	16.40%	2.176%
18	4.249	985	998	1022	rBV	142612	358251	41.49%	5.504%
19	4.452	1058	1061	1063	rBV4	1132	796	0.09%	0.012%
20	4.574	1096	1099	1102	rBV5	1517	1241	0.14%	0.019%
21	4.703	1135	1139	1142	rBV4	1039	893	0.10%	0.014%
22	4.725	1144	1146	1149	rVB4	1297	715	0.08%	0.011%
23	4.815	1171	1174	1177	rBV3	1000	753	0.09%	0.012%
24	4.854	1183	1186	1189	rVB4	1583	1031	0.12%	0.016%
25	4.873	1189	1192	1195	rBV5	1504	1156	0.13%	0.018%
26	4.957	1202	1218	1243	rBV2	328001	863536	100.00%	13.267%
27	5.310	1325	1328	1329	rBV4	1368	751	0.09%	0.012%
28	5.535	1385	1398	1423	rBV	236570	500614	57.97%	7.691%
29	5.773	1469	1472	1473	rBV2	1149	717	0.08%	0.011%
30	5.989	1528	1539	1561	rBV	192207	397148	45.99%	6.102%
31	6.101	1571	1574	1575	rBV4	1686	871	0.10%	0.013%
32	6.461	1684	1686	1689	rVB3	1853	1125	0.13%	0.017%
33	6.490	1689	1695	1697	rBV4	1328	1312	0.15%	0.020%
34	6.510	1697	1701	1703	rVV4	946	734	0.08%	0.011%
35	6.535	1707	1709	1712	rVB4	1629	818	0.09%	0.013%
36	6.751	1772	1776	1779	rBV5	1339	1094	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121523\
 Data File : VW033442.D
 Acq On : 16 Dec 2023 18:00
 Operator : SY/MD
 Sample : 05846-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.793	1786	1789	1792	rVV5	1120	781	0.09%	0.012%
38	6.841	1801	1804	1809	rVB5	1347	919	0.11%	0.014%
39	6.915	1816	1827	1848	rBV	90196	174092	20.16%	2.675%
40	7.172	1905	1907	1910	rBV4	1578	950	0.11%	0.015%
41	7.246	1917	1930	1948	rBV	358688	637781	73.86%	9.799%
42	7.555	2017	2026	2041	rBV	70189	122815	14.22%	1.887%
43	7.895	2130	2132	2136	rBV4	964	745	0.09%	0.011%
44	7.953	2147	2150	2154	rBV6	1351	812	0.09%	0.012%
45	8.024	2162	2172	2207	rBV	178286	375568	43.49%	5.770%
46	8.329	2265	2267	2270	rVB3	2574	1266	0.15%	0.019%
47	8.346	2270	2272	2274	rBV2	1409	787	0.09%	0.012%
48	8.616	2353	2356	2361	rBV7	1606	1276	0.15%	0.020%
49	8.786	2397	2409	2428	rBV	408972	668583	77.42%	10.272%
50	9.027	2481	2484	2486	rBV3	1501	809	0.09%	0.012%
51	9.307	2568	2571	2578	rVB7	1308	1372	0.16%	0.021%
52	9.506	2627	2633	2639	rVB10	1333	1643	0.19%	0.025%
53	9.542	2639	2644	2648	rBV8	1164	1188	0.14%	0.018%
54	9.854	2737	2741	2744	rBV5	1198	1083	0.13%	0.017%
55	9.931	2761	2765	2766	rBV4	1140	808	0.09%	0.012%
56	9.944	2766	2769	2774	rVV7	969	995	0.12%	0.015%
57	10.153	2824	2834	2848	rVV	277606	440074	50.96%	6.761%
58	10.638	2980	2985	2986	rBV4	1197	730	0.08%	0.011%
59	10.690	2997	3001	3003	rBV4	1026	790	0.09%	0.012%
60	10.889	3058	3063	3065	rBV5	1256	959	0.11%	0.015%
61	10.915	3069	3071	3074	rBV4	1654	1101	0.13%	0.017%
62	10.979	3085	3091	3093	rBV6	851	859	0.10%	0.013%
63	11.143	3138	3142	3144	rBV5	964	739	0.09%	0.011%
64	11.188	3144	3156	3177	rBV	357320	573718	66.44%	8.814%
65	11.445	3233	3236	3239	rBV5	956	773	0.09%	0.012%
66	11.561	3262	3272	3291	rBV	393867	621832	72.01%	9.554%
67	11.780	3337	3340	3342	rBV4	2105	1047	0.12%	0.016%
68	11.825	3349	3354	3355	rBV4	1050	927	0.11%	0.014%
69	11.940	3385	3390	3393	rBV6	850	755	0.09%	0.012%
70	11.960	3393	3396	3398	rBV4	1894	1199	0.14%	0.018%
71	12.030	3416	3418	3423	rBV5	1222	1067	0.12%	0.016%
72	12.082	3432	3434	3438	rVB4	1397	923	0.11%	0.014%
73	12.181	3462	3465	3470	rBV6	1752	1511	0.17%	0.023%
74	12.249	3484	3486	3490	rVV4	1155	874	0.10%	0.013%
75	12.493	3560	3562	3567	rBV7	923	740	0.09%	0.011%
76	12.542	3574	3577	3580	rBV4	1290	932	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
 Data File : VV033442.D
 Acq On : 16 Dec 2023 18:00
 Operator : SY/MD
 Sample : 05846-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.564	3580	3584	3589	rVV7	1818	1951	0.23%	0.030%
78	12.844	3667	3671	3673	rBV5	1268	872	0.10%	0.013%
79	13.059	3735	3738	3742	rVB6	1128	935	0.11%	0.014%
80	13.271	3800	3804	3807	rVB5	1814	1341	0.16%	0.021%
81	13.287	3807	3809	3814	rVB6	1099	996	0.12%	0.015%
82	13.313	3814	3817	3819	rBV3	961	742	0.09%	0.011%
83	13.435	3853	3855	3858	rBV4	1040	736	0.09%	0.011%
84	13.525	3879	3883	3884	rBV3	1220	837	0.10%	0.013%
85	13.702	3933	3938	3939	rBV4	1016	847	0.10%	0.013%
86	13.760	3953	3956	3959	rBV5	1146	702	0.08%	0.011%
87	13.895	3995	3998	4001	rBV3	907	763	0.09%	0.012%
88	13.959	4015	4018	4022	rVB5	976	710	0.08%	0.011%
89	14.066	4049	4051	4054	rVB3	1354	731	0.08%	0.011%
90	14.085	4055	4057	4060	rVB3	1657	815	0.09%	0.013%
91	14.156	4075	4079	4081	rBV3	1331	1112	0.13%	0.017%
92	14.194	4087	4091	4095	rBV5	1586	1503	0.17%	0.023%
93	14.320	4128	4130	4135	rVB4	1507	1232	0.14%	0.019%
94	14.355	4135	4141	4145	rBV9	1607	1720	0.20%	0.026%
95	14.381	4145	4149	4153	rBV6	1796	1483	0.17%	0.023%
96	14.419	4158	4161	4164	rVV5	1326	739	0.09%	0.011%
97	15.149	4384	4388	4392	rVB6	2017	1617	0.19%	0.025%
98	15.236	4411	4415	4416	rBV4	1024	776	0.09%	0.012%
99	15.654	4542	4545	4548	rBV5	1058	833	0.10%	0.013%
100	16.037	4661	4664	4666	rBV4	1716	1043	0.12%	0.016%




Sum of corrected areas: 6508834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033442.D
Acq On : 16 Dec 2023 18:00
Operator : SY/MD
Sample : 05846-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

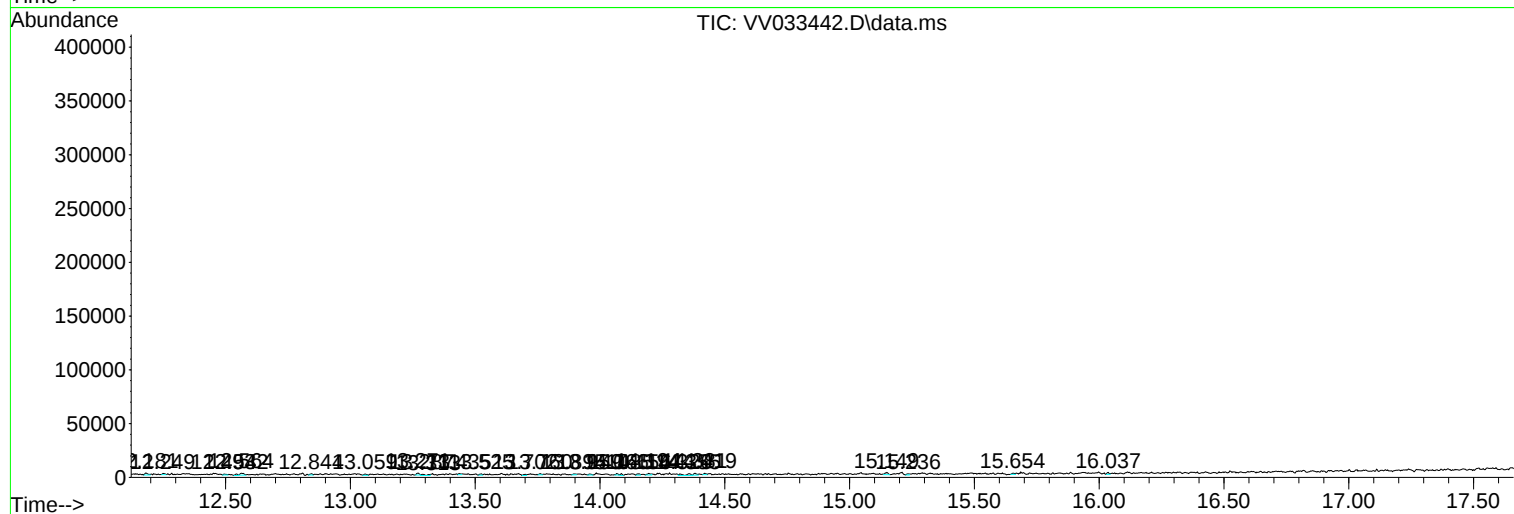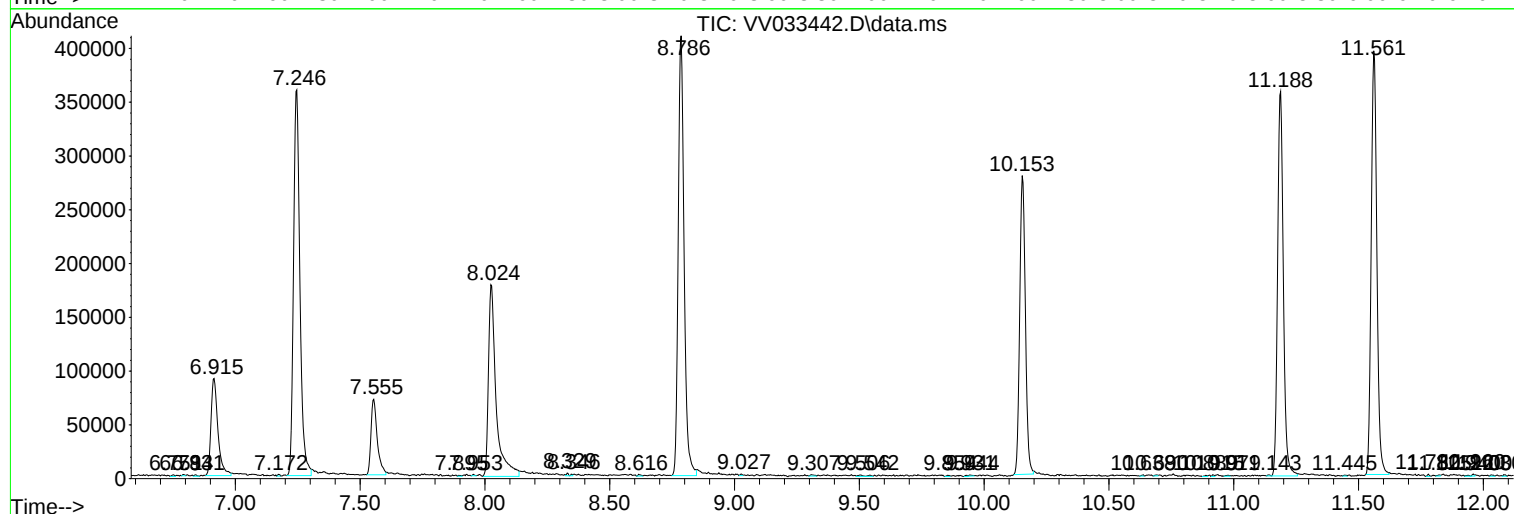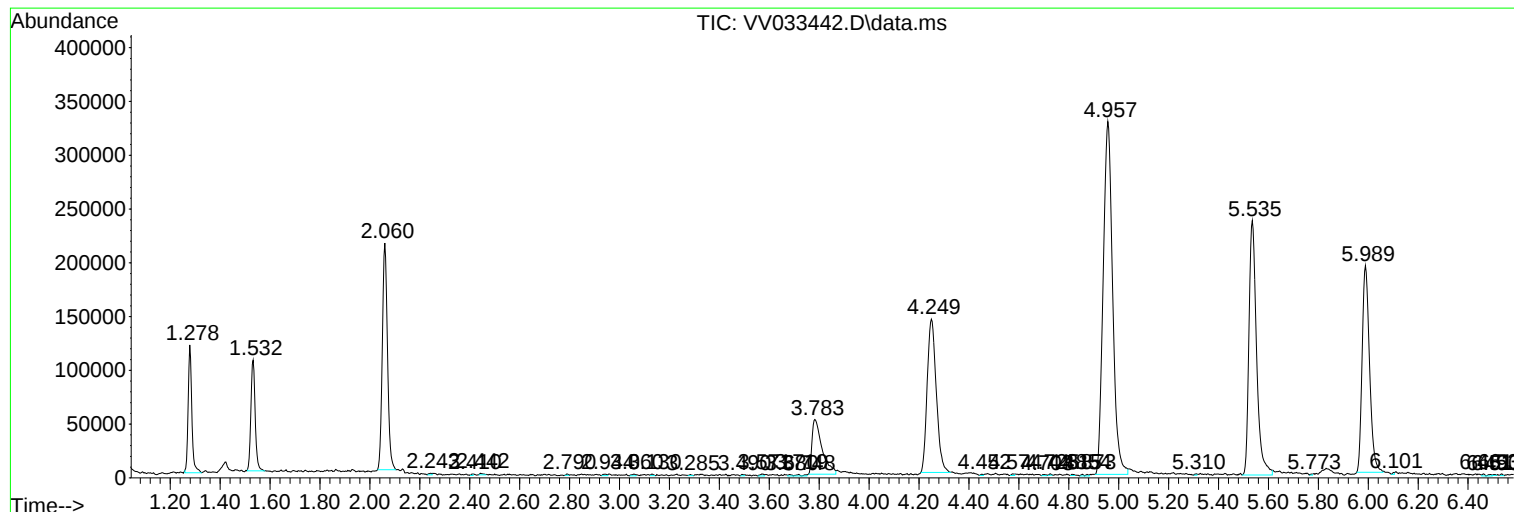

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033442.D
Acq On : 16 Dec 2023 18:00
Operator : SY/MD
Sample : 05846-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033442.D
Acq On : 16 Dec 2023 18:00
Operator : SY/MD
Sample : 05846-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------