
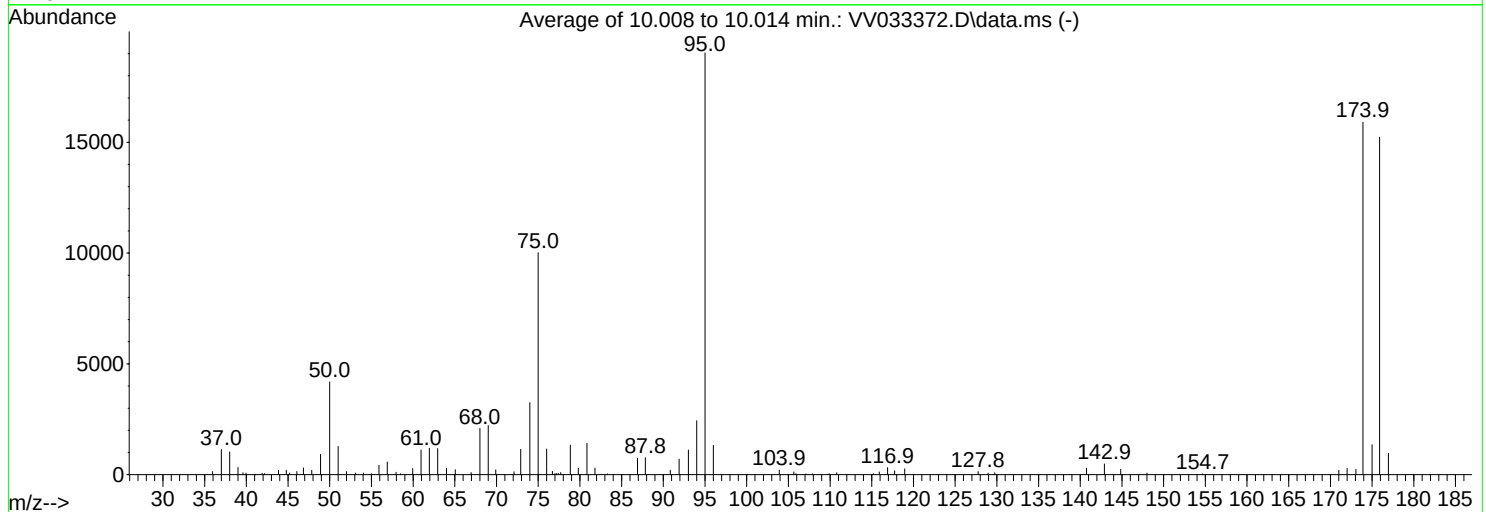


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121523\
Data File : VV033372.D
Acq On : 15 Dec 2023 11:46
Operator : SY/MD
Sample : BFB247
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB247

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis
Last Update : Sat Dec 16 20:24:09 2023

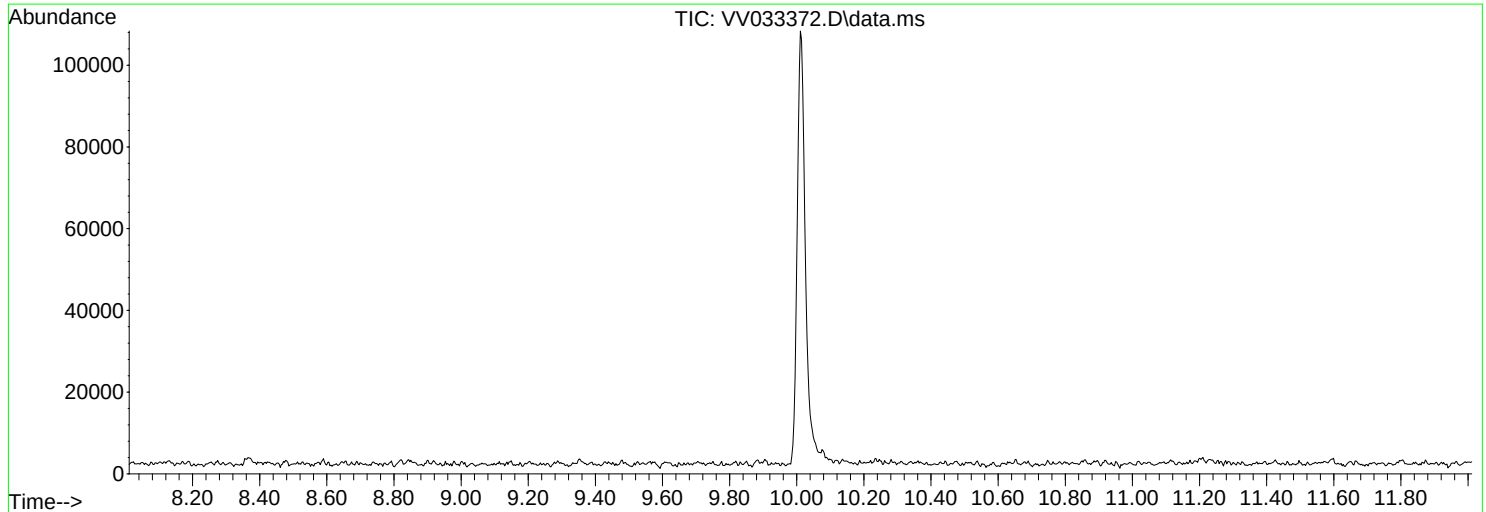

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	4187	PASS
75	95	30	80	52.6	10017	PASS
95	95	100	100	100.0	19037	PASS
96	95	5	9	6.9	1321	PASS
173	174	0.00	2	1.5	235	PASS
174	95	50	120	83.6	15906	PASS
175	174	5	9	8.5	1352	PASS
176	174	95	105	95.7	15227	PASS
177	176	5	10	6.3	964	PASS

m/z	Abundance
35.20	120.0
36.00	159.0
36.70	128.0
37.60	118.0
38.30	103.0
38.90	152.0
39.90	166.0
41.10	130.0
41.90	112.0
42.90	158.0
43.80	253.0
49.20	121.0
50.70	106.0
52.70	125.0
59.10	120.0
63.50	102.0
126.10	109.0
217.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.00	338.0
37.00	1124.0
38.00	996.0
39.10	481.0
40.00	241.0
41.10	141.0
42.00	190.0
43.00	158.0
43.90	463.0
44.80	342.0
46.10	156.0
46.80	322.0
47.80	207.0
48.90	868.0
50.00	4042.0
51.00	1298.0
52.00	114.0
52.70	124.0
53.10	116.0
55.00	103.0
55.90	450.0
56.90	569.0
57.90	108.0
58.50	101.0
59.90	304.0
61.00	1060.0
62.00	1173.0
63.00	1134.0
64.00	284.0
65.00	198.0
67.00	159.0
68.00	2010.0
69.00	1973.0
69.90	180.0
72.90	1039.0
74.00	3250.0
75.00	9789.0
76.00	1026.0
77.00	149.0
77.80	141.0
78.90	1260.0
79.80	255.0
80.80	1379.0
81.80	246.0
86.90	684.0
87.80	732.0
90.90	189.0
91.90	607.0
93.00	1093.0
94.00	2242.0
95.00	18344.0
96.00	1217.0
104.00	203.0
105.60	127.0
105.90	126.0
107.90	118.0
115.20	108.0
115.90	130.0
117.00	302.0
117.80	154.0
119.00	287.0
127.80	102.0
140.80	294.0
142.90	517.0
144.90	251.0
148.10	103.0
154.70	110.0
171.00	182.0
172.00	247.0
173.00	340.0
173.90	14631.0
175.00	1215.0
175.90	13888.0
177.00	960.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.00	289.0
37.00	1162.0
38.00	1040.0
39.00	496.0
40.10	230.0
41.10	164.0
42.00	172.0
43.00	162.0
43.90	448.0
44.80	266.0
46.10	140.0
46.80	318.0
47.80	207.0
48.90	936.0
50.00	4403.0
51.00	1274.0
52.00	141.0
53.10	103.0
54.00	100.0
55.90	444.0
56.90	594.0
57.90	107.0
60.00	290.0
61.00	1150.0
62.00	1212.0
63.00	1208.0
64.00	301.0
65.10	224.0
66.90	123.0
68.00	2124.0
69.00	2333.0
69.90	234.0
72.20	185.0
72.90	1184.0
74.00	3281.0
75.00	10321.0
76.00	1211.0
76.70	219.0
77.20	143.0
77.60	131.0
78.80	1380.0
79.80	293.0
80.90	1501.0
81.80	308.0
86.90	774.0
87.80	819.0
90.90	209.0
91.90	732.0
93.00	1174.0
94.00	2511.0
95.00	19624.0
96.00	1331.0
103.90	209.0
105.60	134.0
107.10	102.0
110.80	109.0
115.90	116.0
116.90	335.0
117.70	185.0
118.90	262.0
127.80	146.0
128.90	102.0
129.80	124.0
140.80	289.0
142.90	500.0
144.80	231.0
147.90	111.0
171.00	190.0
172.00	286.0
173.10	365.0
173.90	16520.0
175.00	1416.0
175.90	15928.0
176.90	973.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
35.90	256.0
37.00	1118.0
38.00	1036.0
39.00	463.0
39.60	262.0
40.10	245.0
41.10	134.0
41.80	148.0
42.20	156.0
42.90	152.0
43.90	429.0
45.20	222.0
46.00	145.0
46.90	281.0
47.90	181.0
48.90	940.0
50.00	4115.0
51.00	1233.0
52.00	150.0
54.10	127.0
55.90	386.0
56.90	553.0
58.00	103.0
60.00	221.0
60.90	1124.0
61.90	1193.0
62.90	1198.0
64.00	276.0
65.10	249.0
68.00	2127.0
69.00	2351.0
69.90	237.0
72.00	198.0
72.90	1192.0
74.00	3211.0
75.00	9942.0
76.00	1228.0
76.70	231.0
77.40	167.0
78.80	1356.0
79.80	299.0
80.90	1360.0
81.80	329.0
83.30	100.0
86.90	749.0
87.90	753.0
90.80	198.0
91.90	769.0
93.00	1078.0
94.00	2542.0
95.00	19144.0
96.00	1414.0
103.80	203.0
105.70	111.0
109.90	109.0
110.80	150.0
115.90	115.0
116.80	327.0
117.70	179.0
118.90	221.0
127.70	153.0
129.00	111.0
129.70	132.0
140.70	297.0
142.90	436.0
144.80	238.0
171.00	204.0
172.00	314.0
173.90	16568.0
175.00	1426.0
175.90	15866.0
176.90	960.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247