
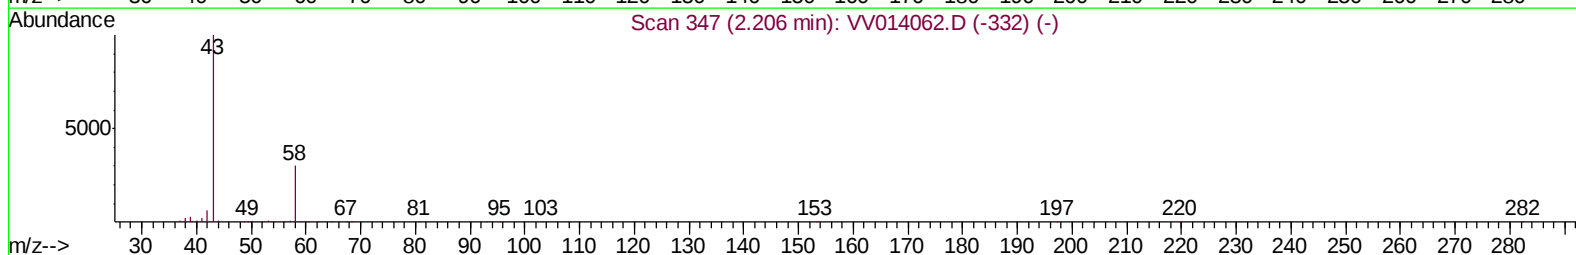
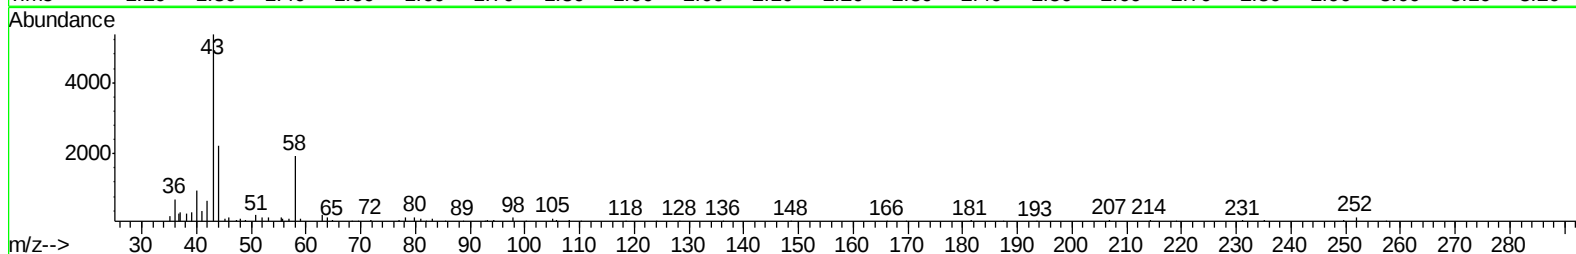


Data File : VV014070.D
Acq On : 16 Dec 2019 14:25
Operator : SY/MD
Sample : K6275-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 17 05:46:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

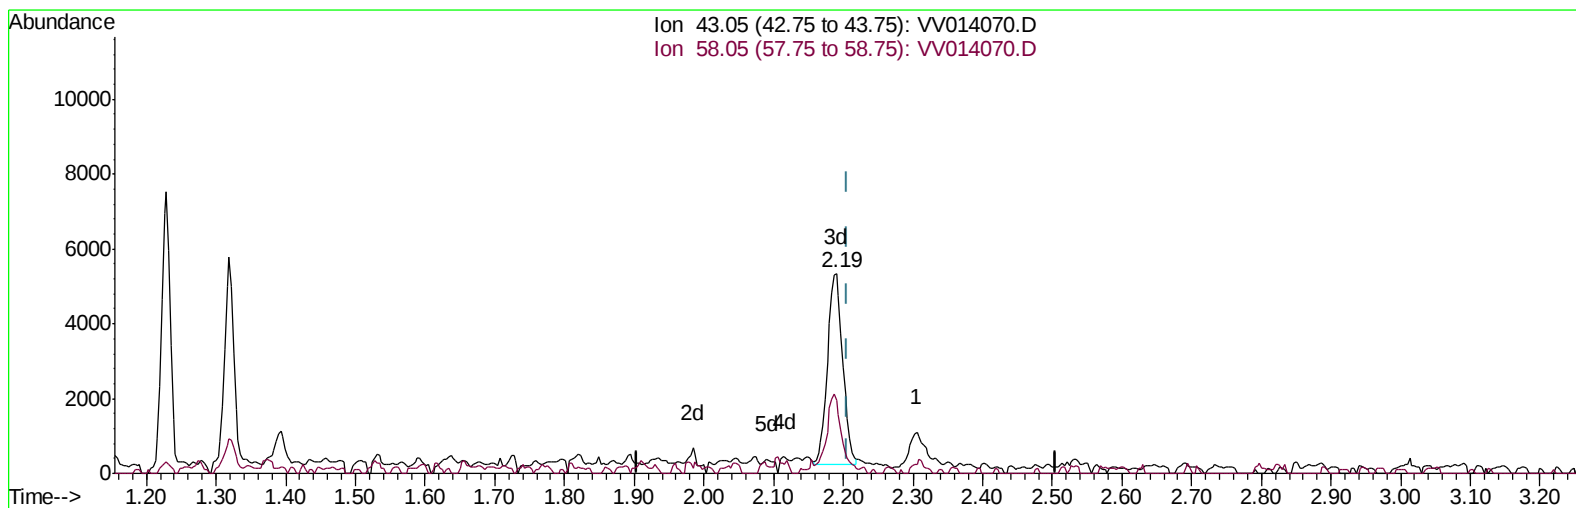

TIC: VV014070.D

(13) Acetone (T)

2.190min (-0.016) 2.29ug/L m

response 7711

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	5.25
0.00	0.00	0.00
0.00	0.00	0.00