
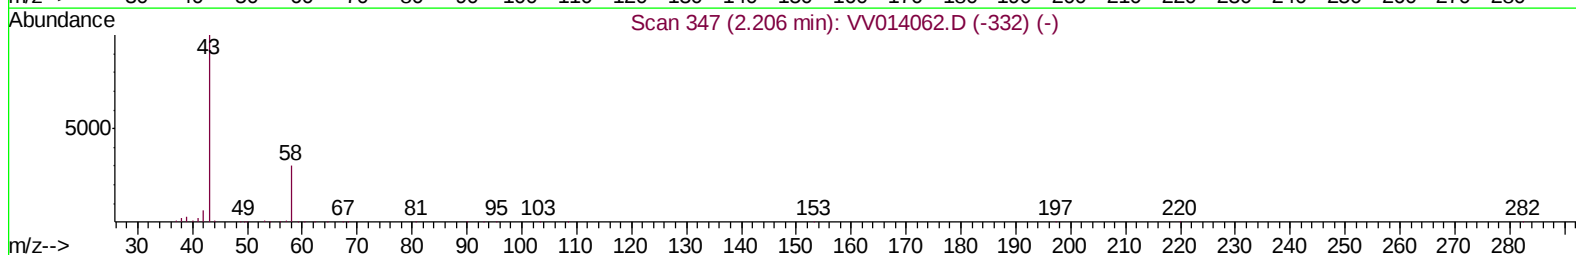
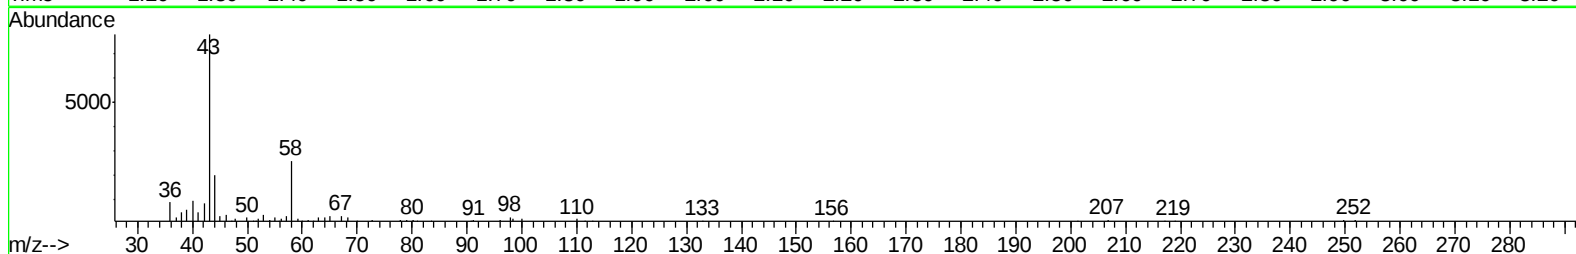


Data File : VV014077.D
Acq On : 16 Dec 2019 17:11
Operator : SY/MD
Sample : K6275-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 17 05:48:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

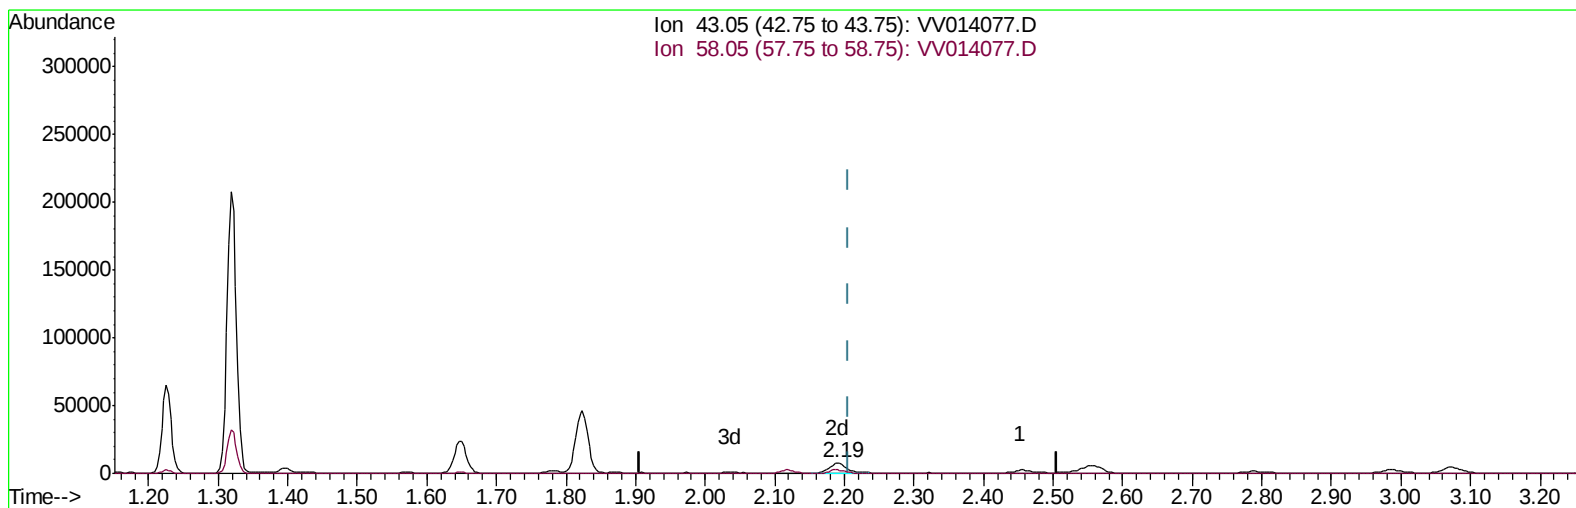

TIC: VV014077.D

(13) Acetone (T)

2.190min (-0.016) 4.04ug/L m

response 13845

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	3.15
0.00	0.00	0.00
0.00	0.00	0.00