


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (QT Reviewed)
Data File : VV014078.D
Acq On : 16 Dec 2019 17:35
Operator : SY/MD
Sample : K6275-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD5

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:43 PM

Quant Time: Dec 17 06:56:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

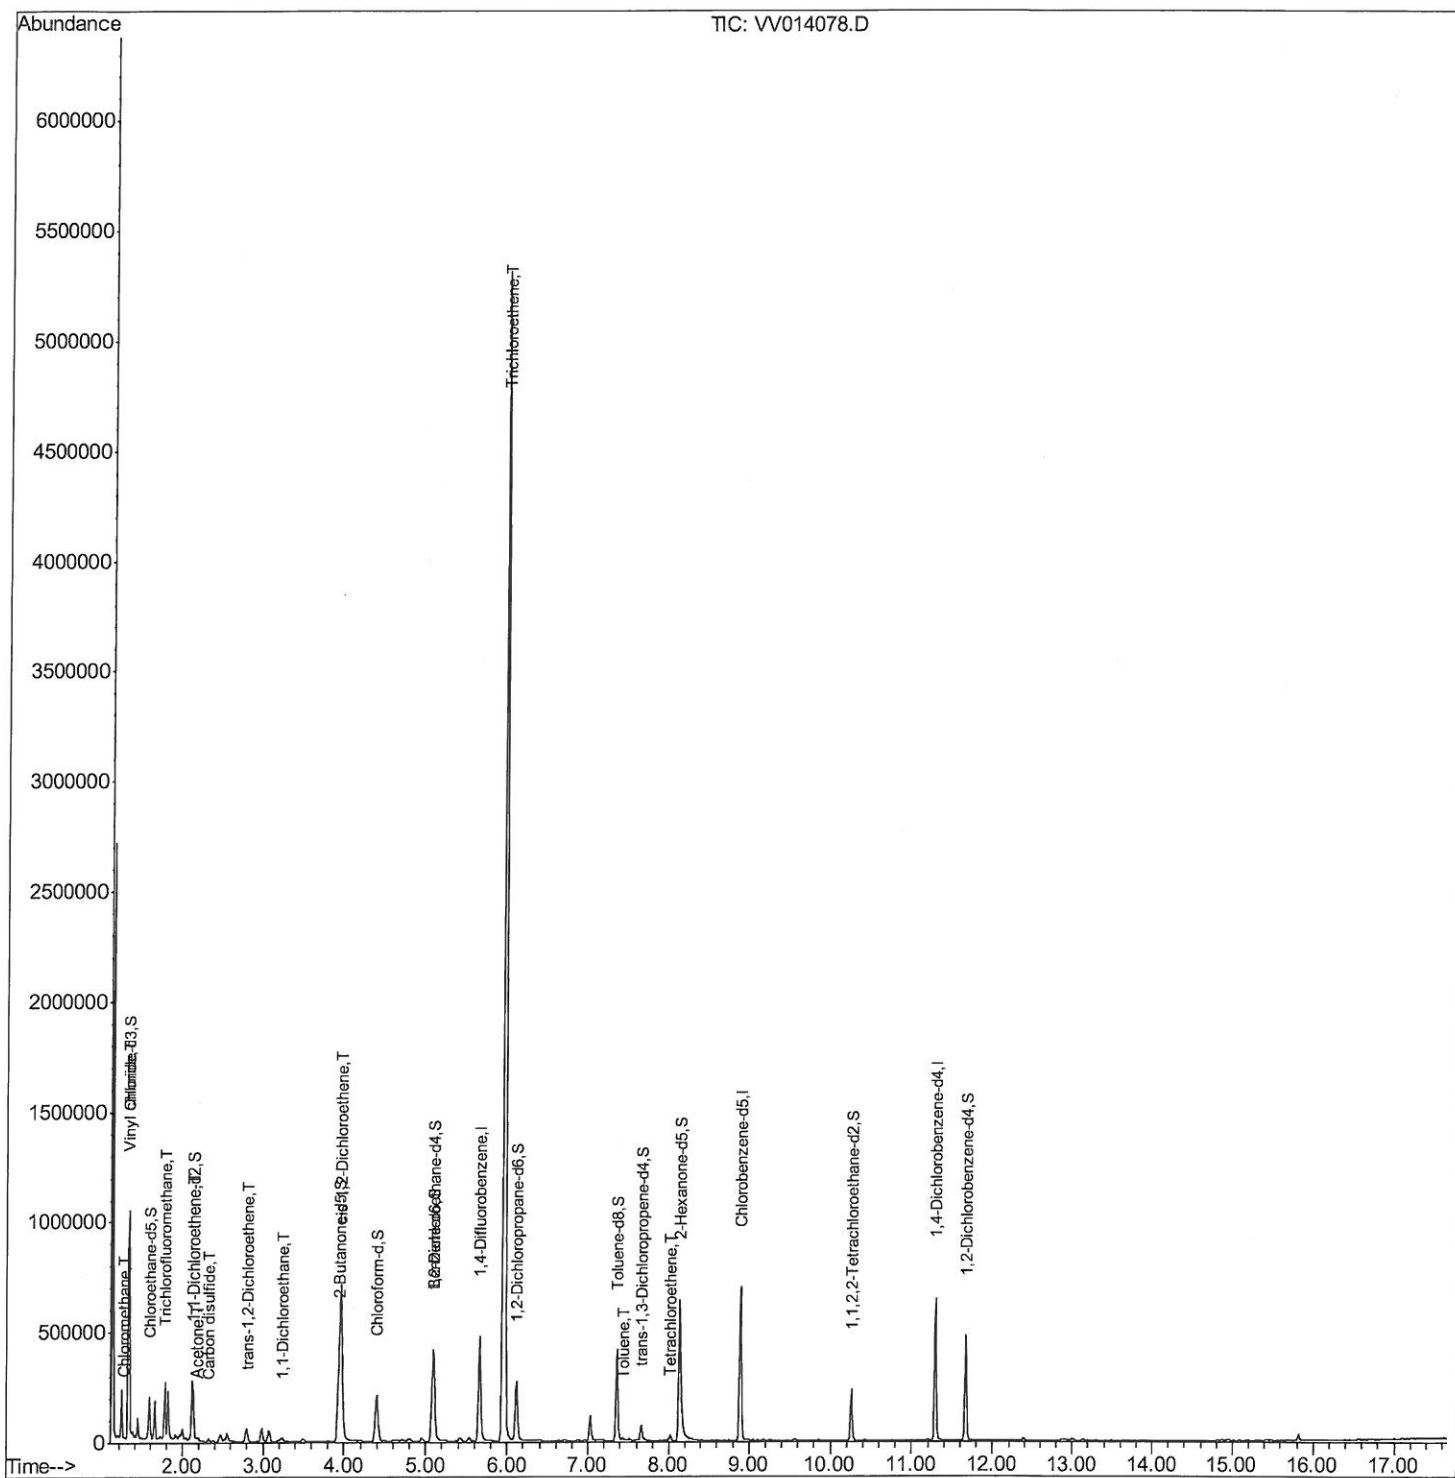

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (Qedit)




Data File : VV014078.D
Acq On : 16 Dec 2019 17:35
Operator : SY/MD
Sample : K6275-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD5

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:43 PM

Quant Time: Dec 17 05:48:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

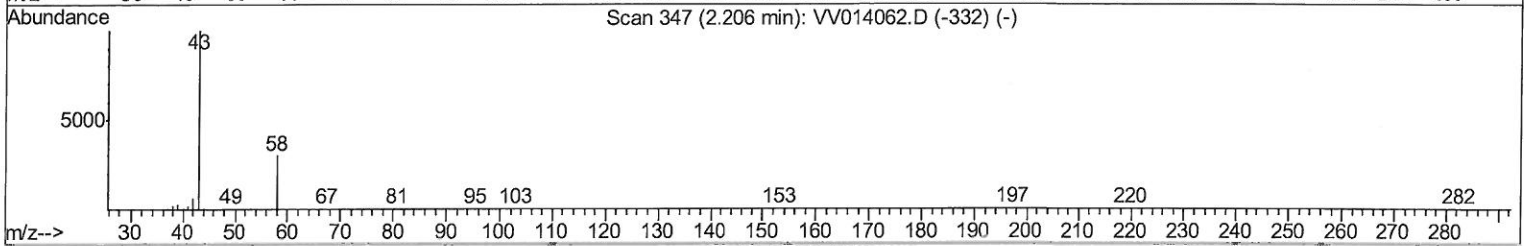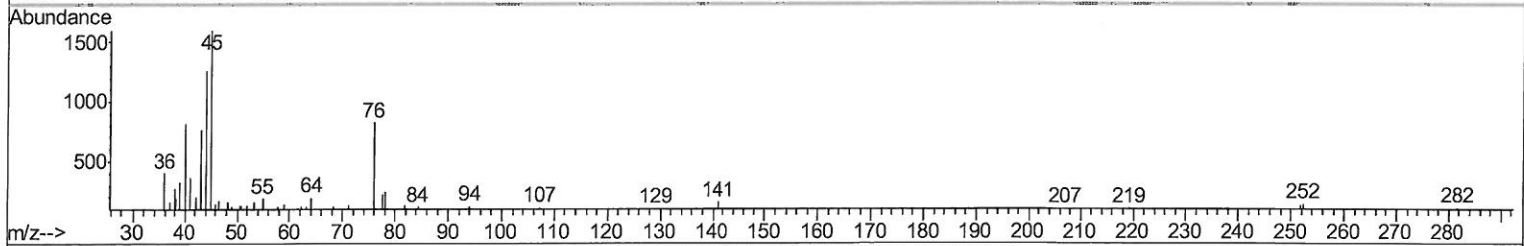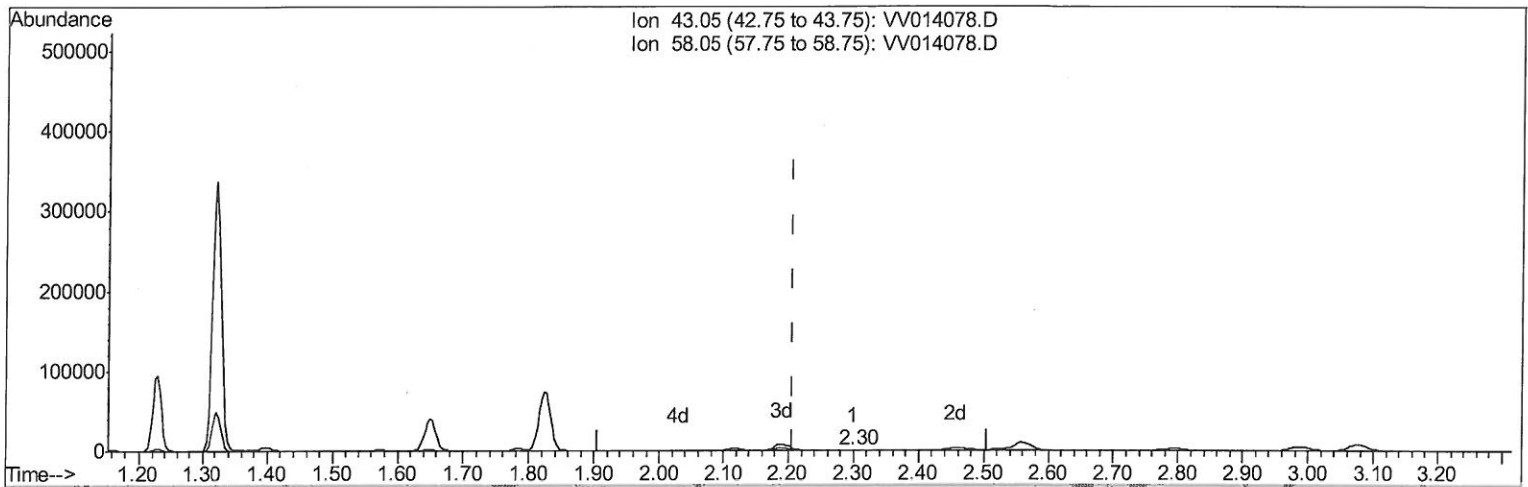

TIC: VV014078.D

(13) Acetone (T)

2.299min (+0.094) 0.19ug/L

response 695

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	21.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (Qedit)




Data File : VV014078.D
Acq On : 16 Dec 2019 17:35
Operator : SY/MD
Sample : K6275-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD5

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:43 PM

Quant Time: Dec 17 05:48:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

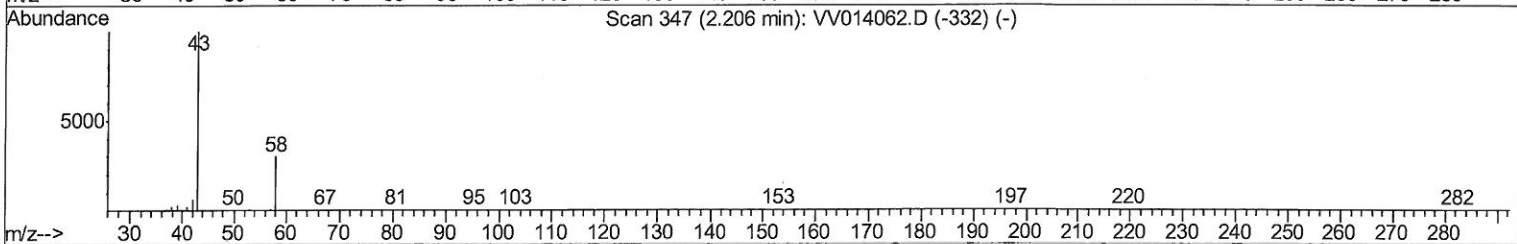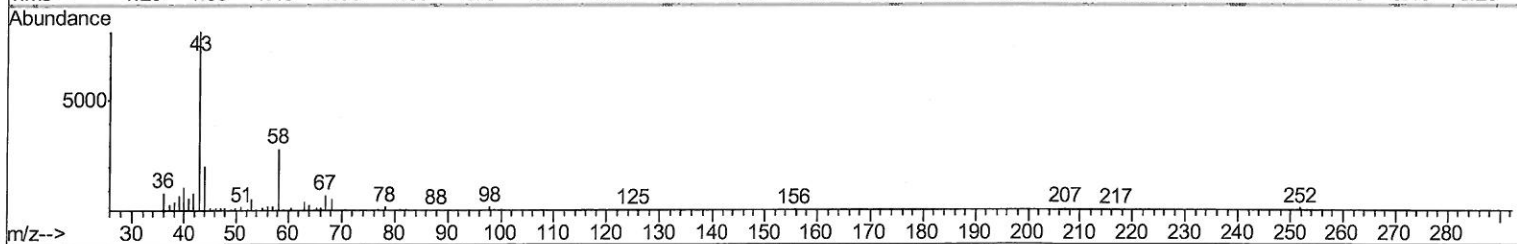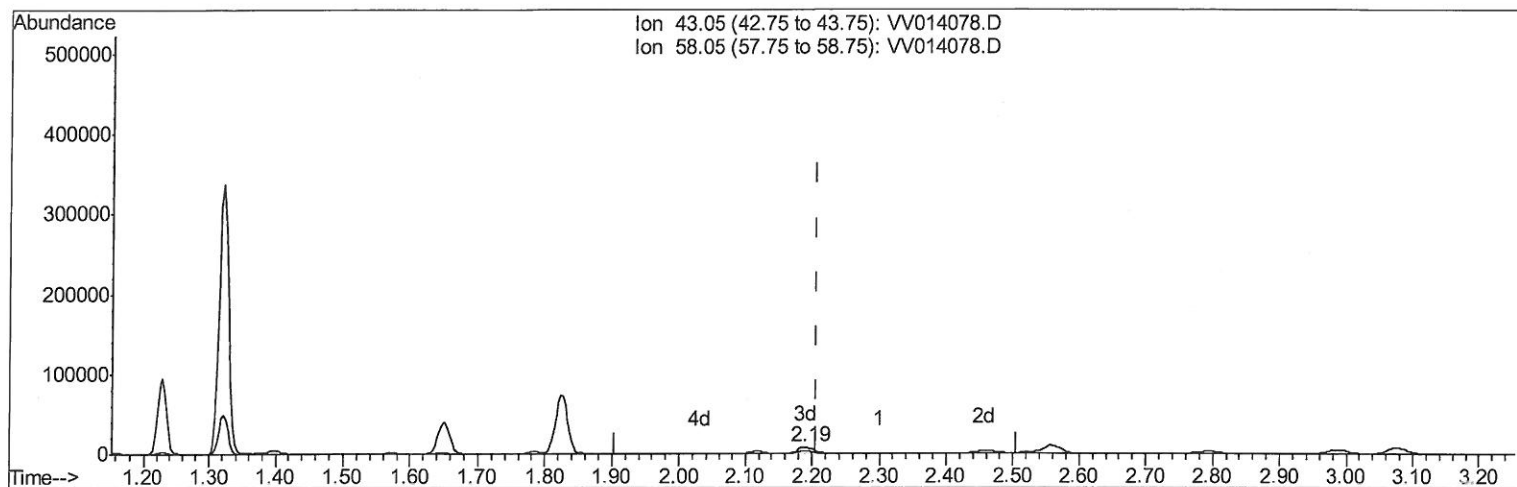

TIC: VV014078.D

(13) Acetone (T)

2.190min (-0.016) 3.71ug/L m

response 13890

Ion Exp% Act%

43.05 100 100

58.05 13.60 1.06

0.00 0.00 0.00

0.00 0.00 0.00

7 MD
12/18/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (QT Reviewed)

Data File : VV014078.D
Acq On : 16 Dec 2019 17:35
Operator : SY/MD
Sample : K6275-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD5

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:43 PM

Quant Time: Dec 17 06:56:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	415766	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	402023	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	179599	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	103709	4.03	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.60%
7) Chloroethane-d5	1.58	69	102871	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.20%
11) 1,1-Dichloroethene-d2	2.13	63	131945	3.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.00%
20) 2-Butanone-d5	3.93	46	323629	60.50	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.00%
24) Chloroform-d	4.40	84	211573	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.60%
26) 1,2-Dichloroethane-d4	5.08	65	110237	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
32) Benzene-d6	5.10	84	372543	3.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.80%
36) 1,2-Dichloropropane-d6	6.12	67	133478	4.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.40%
41) Toluene-d8	7.36	98	284095	2.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	58.40%#
43) trans-1,3-Dichloropropene-	7.66	79	41562	3.45	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.00%
46) 2-Hexanone-d5	8.13	63	237156	53.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.88%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	113493	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	133809	4.22	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.40%

Target Compounds

					Qvalue	
3) Chloromethane	1.25	50	3705	0.152	ug/L	99
5) Vinyl chloride	1.33	62	7153	0.288	ug/L #	51
9) Trichlorofluoromethane	1.77	101	20116	0.522	ug/L	97
12) 1,1-Dichloroethene	2.14	96	11899	0.595	ug/L #	1
13) Acetone	2.19	43	13890m	3.713	ug/L	1
14) Carbon disulfide	2.32	76	10221	0.221	ug/L	95
18) trans-1,2-Dichloroethene	2.79	96	10529	0.466	ug/L	88
19) 1,1-Dichloroethane	3.23	63	13341	0.296	ug/L #	93
22) cis-1,2-Dichloroethene	3.96	96	382667	14.456	ug/L #	97
34) Trichloroethene	5.96	95	1787345	65.702	ug/L	97
42) Toluene	7.43	91	7678	0.073	ug/L	86
47) Tetrachloroethene	8.02	164	6528	0.276	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
12/18/19