

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (QT Reviewed)


Data File : VV014079.D
Acq On : 16 Dec 2019 17:59
Operator : SY/MD
Sample : K6275-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BFD6

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:51 PM

Quant Time: Dec 17 07:00:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

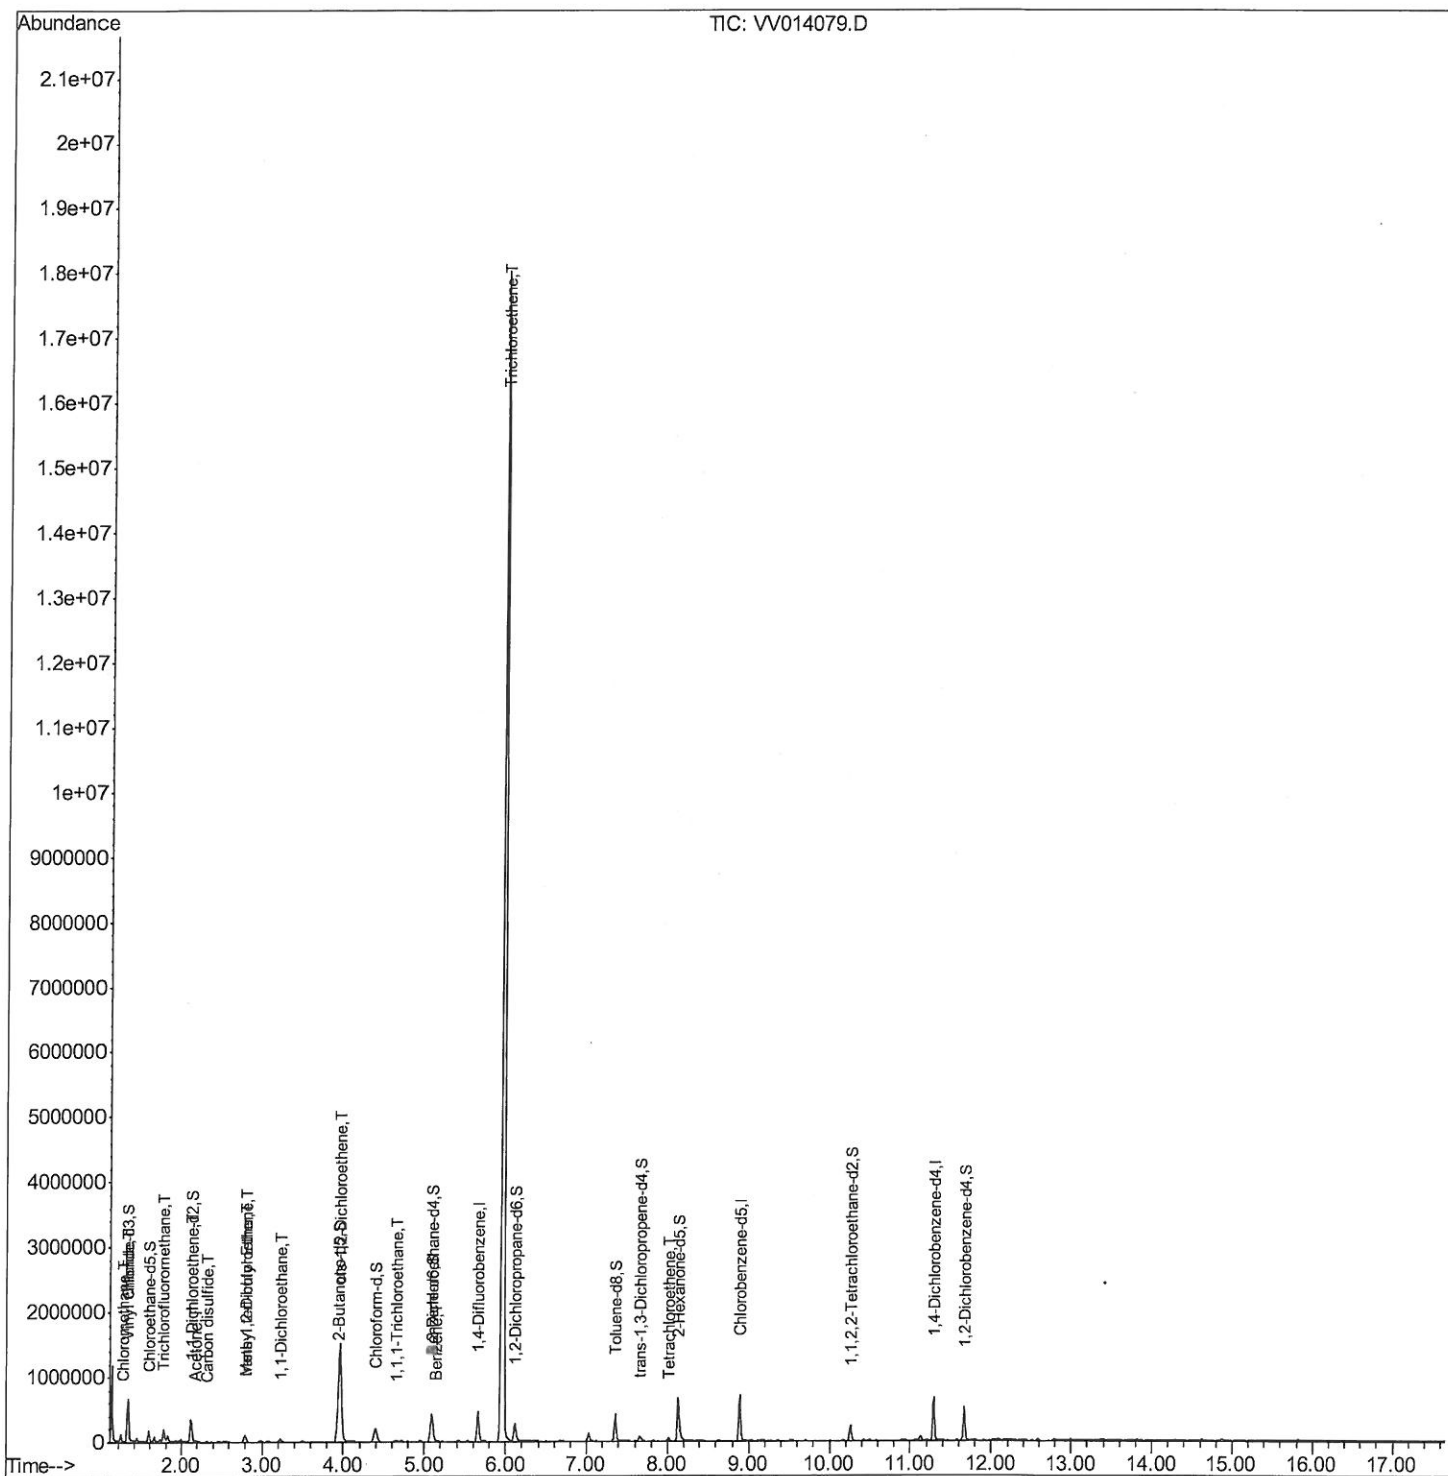

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (Qedit)




Data File : VV014079.D
Acq On : 16 Dec 2019 17:59
Operator : SY/MD
Sample : K6275-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD6

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:51 PM

Quant Time: Dec 17 05:48:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

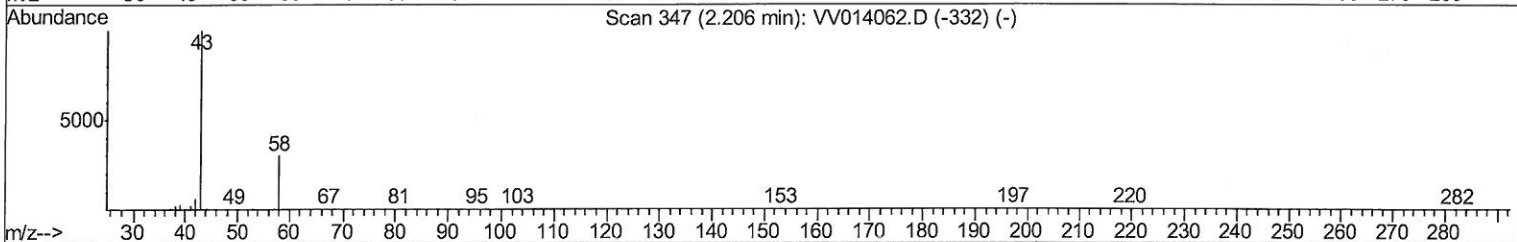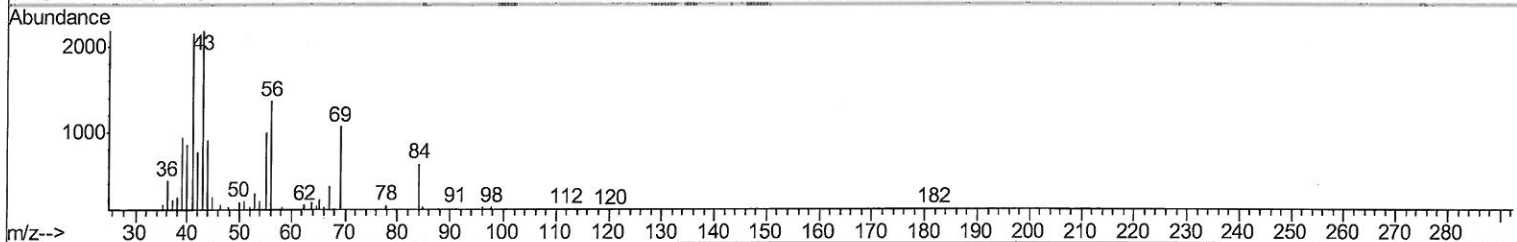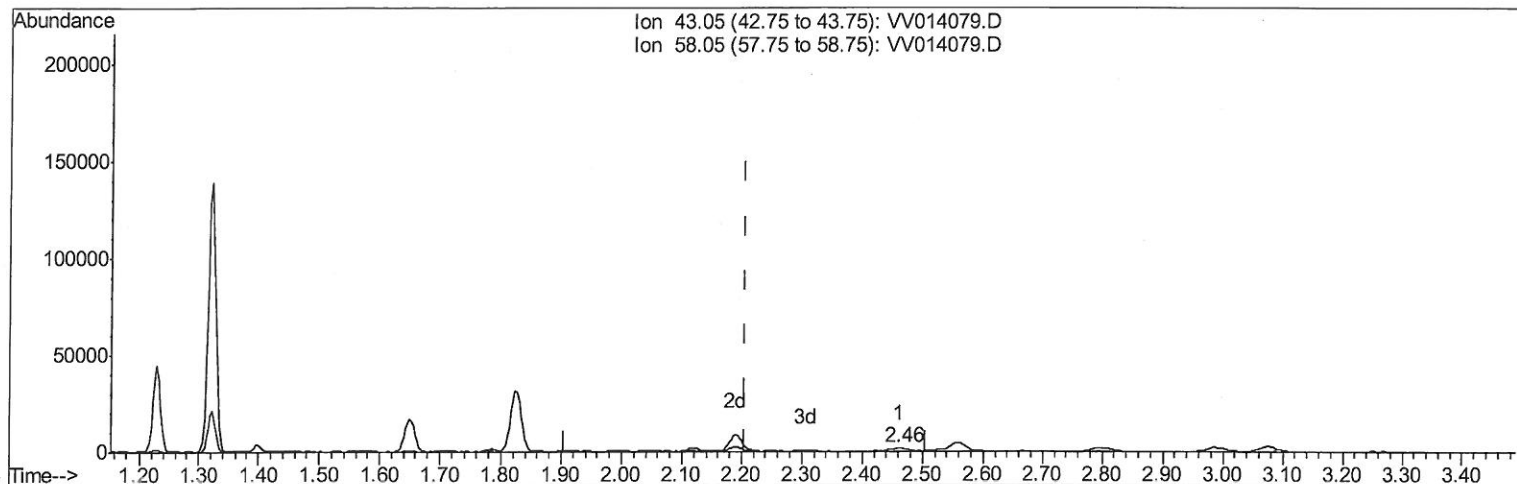

TIC: VV014079.D

(13) Acetone (T)

2.460min (+0.254) 0.81ug/L

response 2973

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	4.98
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (Qedit)




Data File : VV014079.D
Acq On : 16 Dec 2019 17:59
Operator : SY/MD
Sample : K6275-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD6

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:51 PM

Quant Time: Dec 17 05:48:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

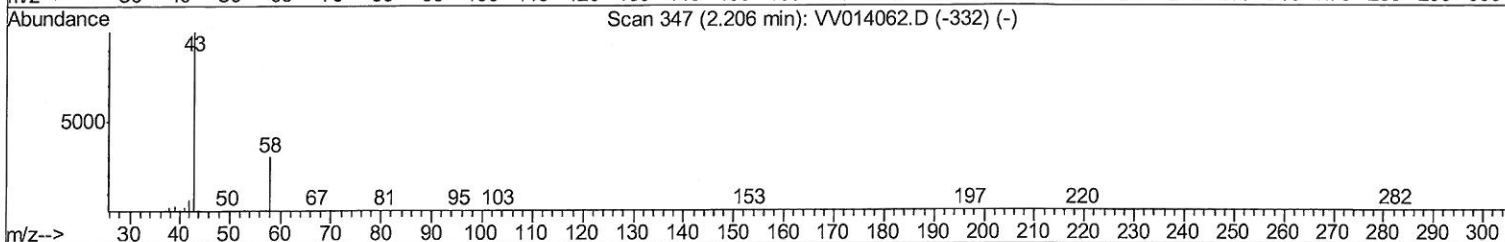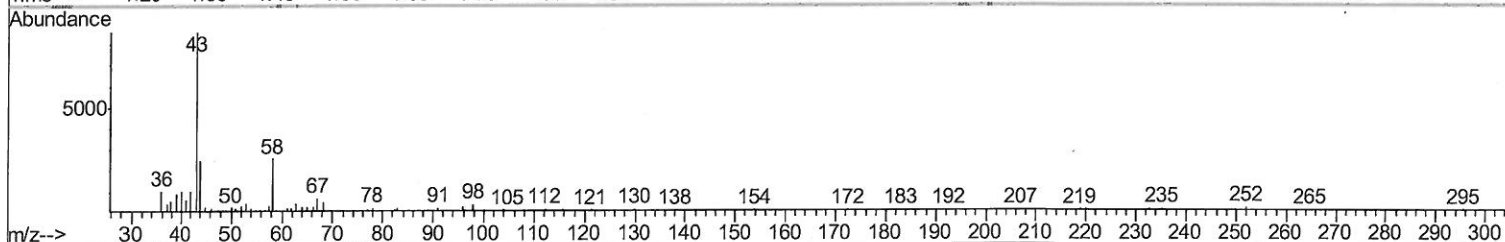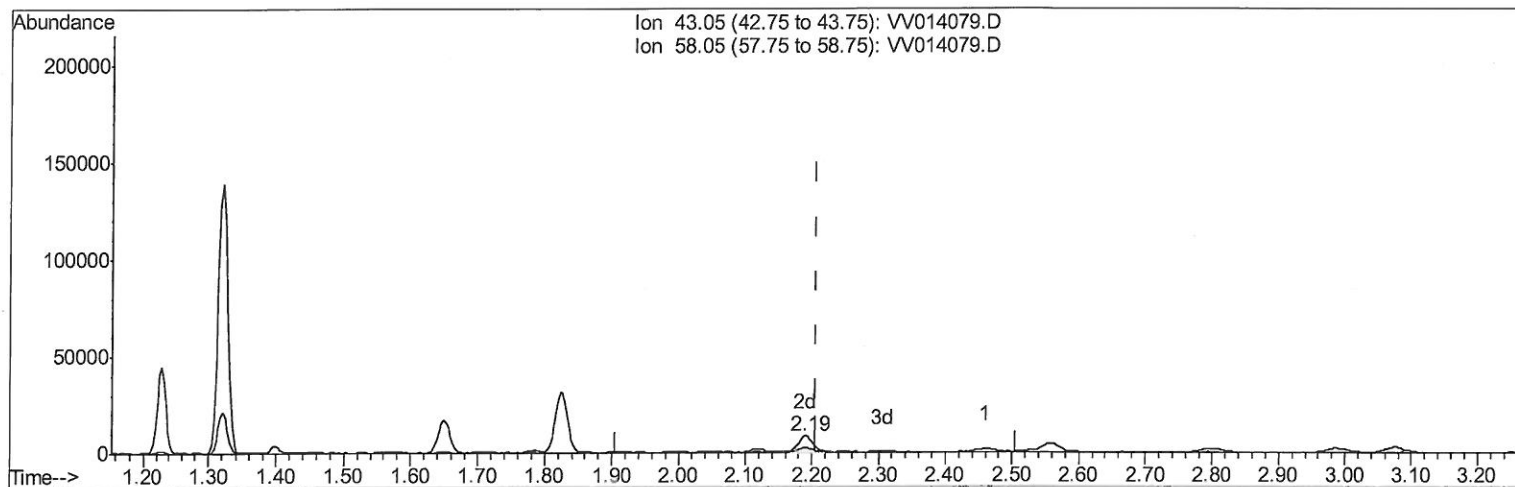

TIC: VV014079.D

(13) Acetone (T)

2.190min (-0.016) 3.88ug/L m

response 14147

MD
12/18/19

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	1.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Quantitation Report (QT Reviewed)

Data File : VV014079.D
Acq On : 16 Dec 2019 17:59
Operator : SY/MD
Sample : K6275-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFDT6

Manual Integrations
APPROVED

apatel
12/17/2019 3:03:51 PM

Quant Time: Dec 17 07:00:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	405754	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	394805	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	188340	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	100425	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.58	69	97413	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.40%
11) 1,1-Dichloroethene-d2	2.13	63	144253	3.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.20%
20) 2-Butanone-d5	3.93	46	329788	63.17	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.34%
24) Chloroform-d	4.40	84	207022	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.80%
26) 1,2-Dichloroethane-d4	5.08	65	106729	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
32) Benzene-d6	5.10	84	370626	3.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.80%
36) 1,2-Dichloropropane-d6	6.12	67	127259	4.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.80%
41) Toluene-d8	7.36	98	285404	2.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	59.80%#
43) trans-1,3-Dichloropropene-	7.66	79	40970	3.47	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.40%
46) 2-Hexanone-d5	8.13	63	246919	56.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	112418	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	141871	4.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.40%

Target Compounds

						Qvalue
3) Chloromethane	1.25	50	2686	0.113	ug/L	83
5) Vinyl chloride	1.32	62	112126	4.626	ug/L	100
9) Trichlorofluoromethane	1.77	101	79303	2.107	ug/L	100
12) 1,1-Dichloroethene	2.14	96	42451	2.176	ug/L	83
13) Acetone	2.19	43	14147m	3.875	ug/L	98
14) Carbon disulfide	2.32	76	8470	0.188	ug/L	98
17) Methyl tert-butyl Ether	2.81	73	9282	0.174	ug/L #	1
18) trans-1,2-Dichloroethene	2.79	96	35617	1.617	ug/L	95
19) 1,1-Dichloroethane	3.23	63	41282	0.939	ug/L	99
22) cis-1,2-Dichloroethene	3.96	96	850271	32.914	ug/L #	98
29) 1,1,1-Trichloroethane	4.65	97	5759	0.143	ug/L #	70
33) Benzene	5.15	78	11442	0.118	ug/L	100
34) Trichloroethene	5.96	95	6074923	227.393	ug/L	98
47) Tetrachloroethene	8.02	164	13456	0.580	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed