

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
 Data File : VV014063.D
 Acq On : 16 Dec 2019 11:28
 Operator : SY/MD
 Sample : VV1216WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK36

Quant Time: Dec 17 05:53:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 17 05:42:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	381083	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	377294	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	169295	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	150259	6.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	127.40%
7) Chloroethane-d5	1.58	69	123044	6.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	122.80%
11) 1,1-Dichloroethene-d2	2.12	63	187481	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.40%
20) 2-Butanone-d5	3.96	46	220151	44.90	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.80%
24) Chloroform-d	4.39	84	225282	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
26) 1,2-Dichloroethane-d4	5.08	65	109560	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.09	84	476194	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.11	67	141665	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.35	98	402121	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
43) trans-1,3-Dichloropropene-	7.66	79	49231	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.14	63	147697	35.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.92%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	84174	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	153031	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%


Target Compounds					Qvalue
16) Methylene chloride	2.53	84	11401	0.454 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Data File : VV014063.D
Acq On : 16 Dec 2019 11:28
Operator : SY/MD
Sample : VV1216WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK36

Quant Time: Dec 17 05:53:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 05:42:45 2019
Response via : Initial Calibration

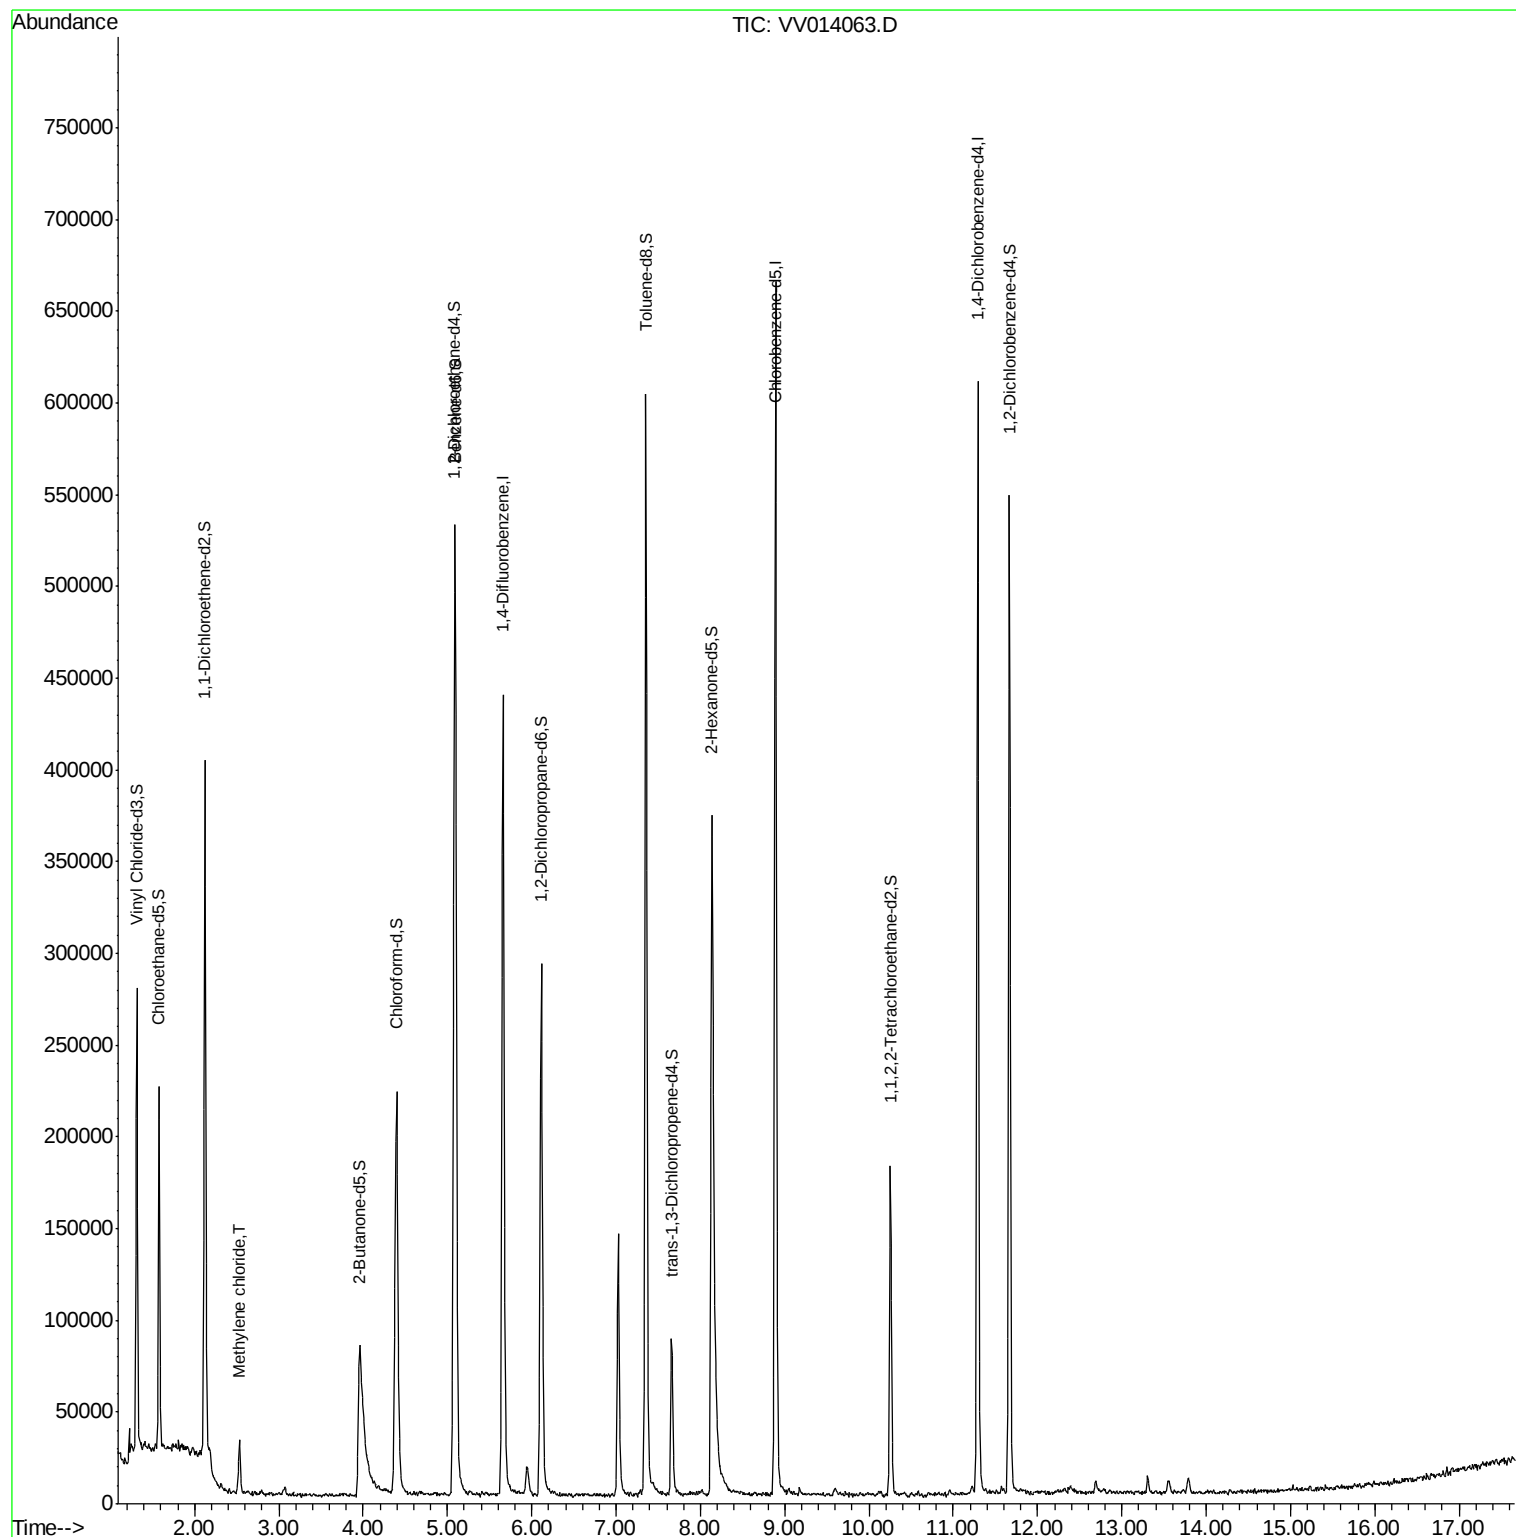

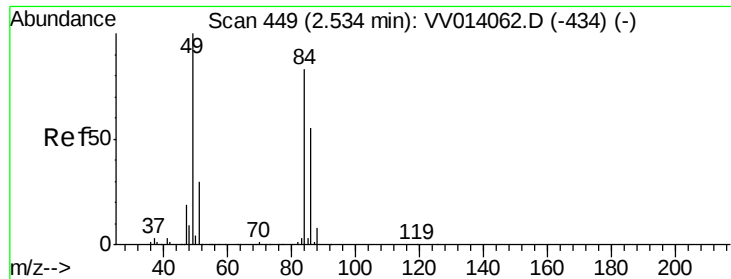

#16
Methylene chloride
Concen: 0.454 ug/L
RT: 2.53 min Scan# 448
Delta R.T. -0.00 min
Lab File: VV014063.D
Acq: 16 Dec 2019 11:28

Instrument :
MSVOA_V
ClientSampleId :
VBLK36

Tgt Ion: 84 Resp: 11401
Ion Ratio Lower Upper
84 100
86 69.3 44.0 81.6
49 120.2 81.5 151.5

