

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121619\
 Data File : VV014067.D
 Acq On : 16 Dec 2019 13:14
 Operator : SY/MD
 Sample : VIBLK45
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK45

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.228	33	43	48	rBV3	24842	35877	2.86%	0.351%
2	1.319	63	71	83	rVB	262445	272667	21.75%	2.667%
3	1.582	145	153	163	rBV	200929	221362	17.66%	2.166%
4	2.129	309	323	334	rBV	372515	535001	42.68%	5.234%
5	2.534	440	449	458	rBV	31861	50848	4.06%	0.497%
6	2.653	475	486	497	rVB	10239	21372	1.70%	0.209%
7	3.926	871	882	918	rBV	143252	428847	34.21%	4.195%
8	4.396	1013	1028	1050	rBV	216124	535919	42.75%	5.243%
9	5.093	1227	1245	1273	rBV2	512352	1253593	100.00%	12.264%
10	5.659	1408	1421	1447	rBV	434301	883572	70.48%	8.644%
11	5.949	1501	1511	1527	rVB4	19021	38691	3.09%	0.379%
12	6.113	1548	1562	1579	rBV2	282975	573945	45.78%	5.615%
13	7.026	1833	1846	1863	rBV	127329	240308	19.17%	2.351%
14	7.357	1936	1949	1967	rBV	561231	970025	77.38%	9.490%
15	7.659	2032	2043	2063	rBV	77494	142992	11.41%	1.399%
16	8.132	2177	2190	2226	rBV3	365194	907047	72.36%	8.874%
17	8.891	2410	2426	2447	rBV	652906	1081446	86.27%	10.580%
18	10.257	2839	2851	2867	rBV	172779	275013	21.94%	2.690%
19	10.421	2893	2902	2912	rVB3	9143	16545	1.32%	0.162%
20	11.289	3158	3172	3187	rBV	574822	908214	72.45%	8.885%
21	11.665	3277	3289	3306	rBV	517176	828656	66.10%	8.107%


Sum of corrected areas: 10221940

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121619\
Data File : VV014067.D
Acq On : 16 Dec 2019 13:14
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

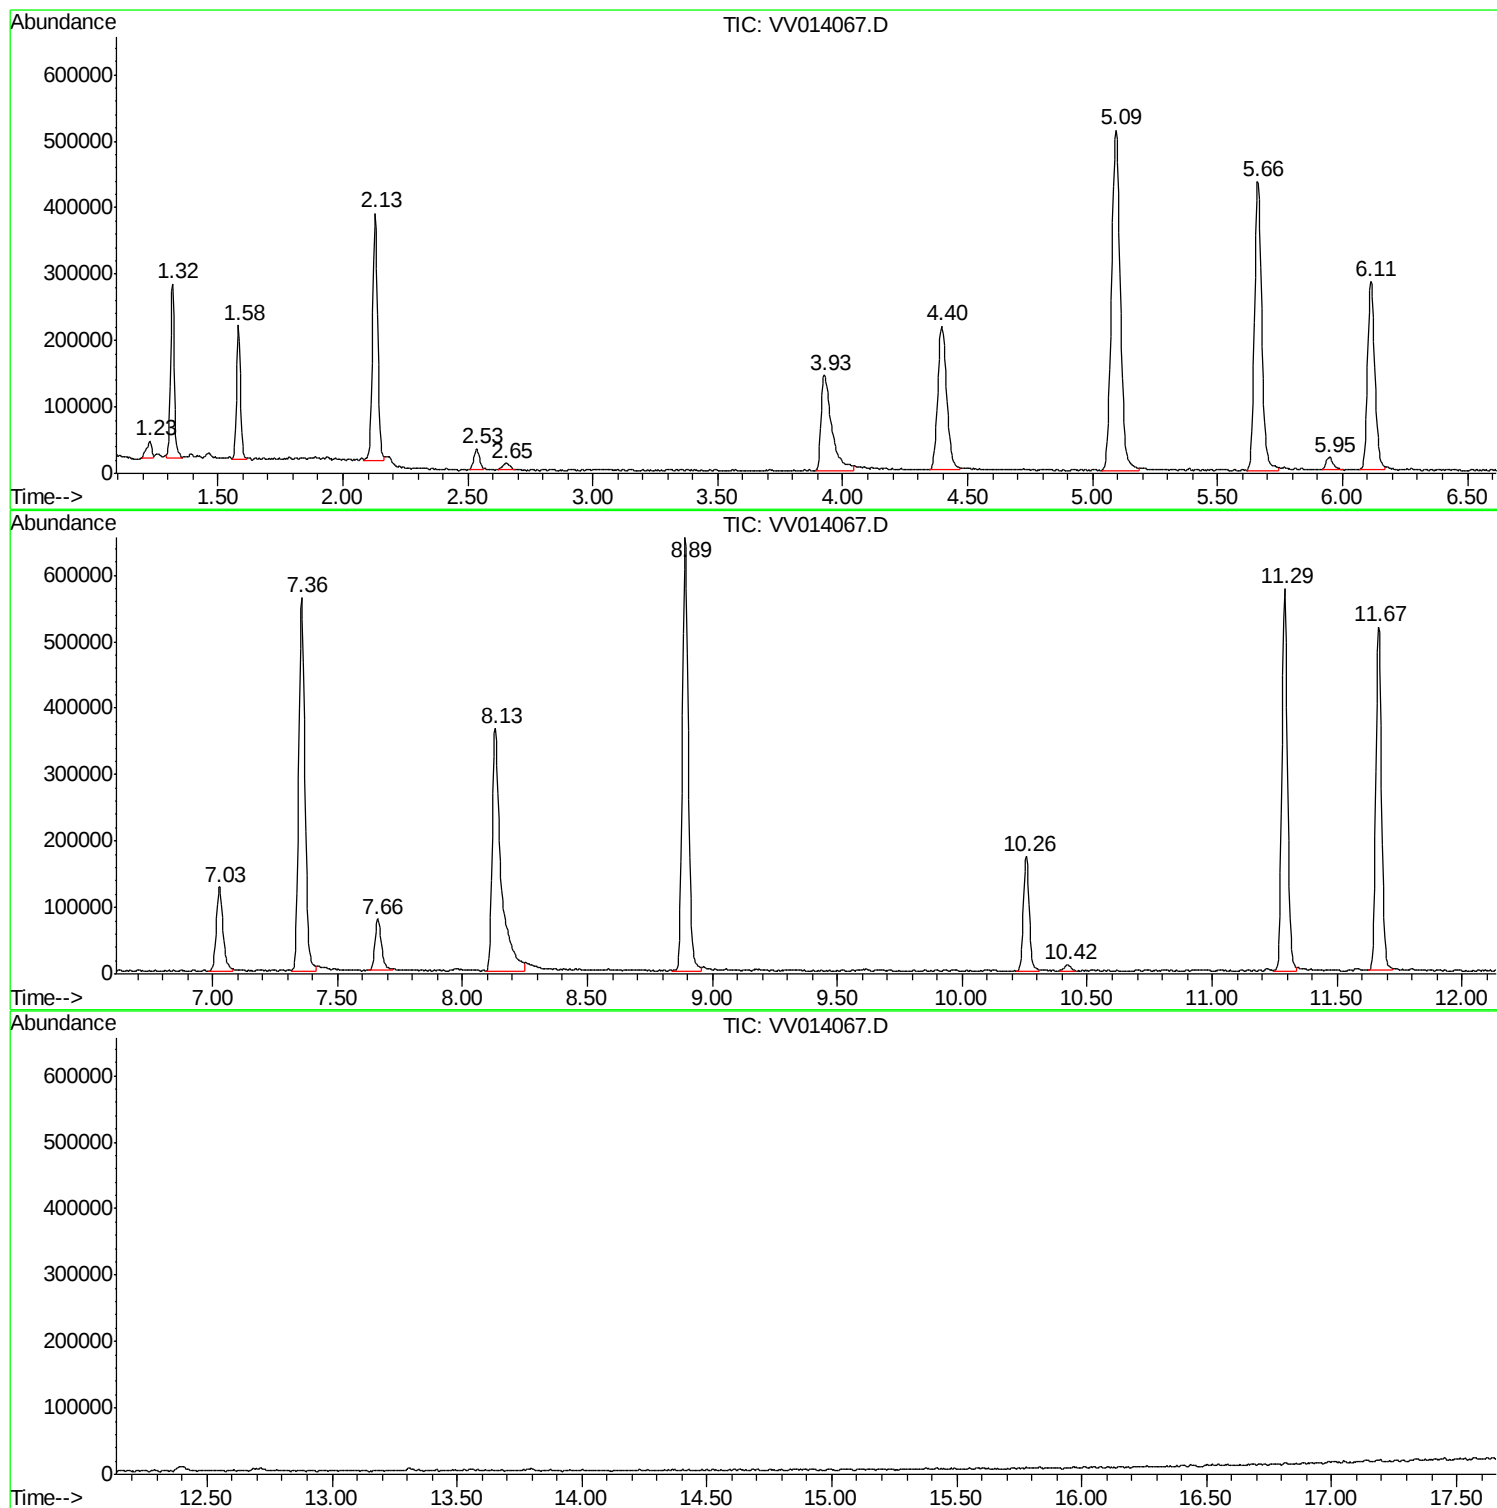

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Data File : VV014067.D
Acq On : 16 Dec 2019 13:14
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121619\
Data File : VV014067.D
Acq On : 16 Dec 2019 13:14
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK45

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc